

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE013120\
 Data File : FE031264.D
 Signal(s) : FID1B.CH
 Acq On : 31 Jan 2020 15:57
 Operator : DD\AJ
 Sample : L1310-02 2X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 31 23:32:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012920.M
 Quant Title :
 QLast Update : Thu Jan 30 04:09:51 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.615	2484698	7.641 ug/ml
Target Compounds			
4) N-TETRADECANE	8.120	654331	1.807 ug/ml
7) N-EICOSANE	12.571f	1359811	3.661 ug/ml
10) N-TETRACOSANE	14.799	594163	1.587 ug/ml
12) N-OCTACOSANE	16.798	469185	1.252 ug/ml
13) N-TRIACONTANE	17.684	979785	2.619 ug/ml
14) N-DOTRIACONTANE	18.517	784973	2.218 ug/ml
15) N-TETRATRIACONTANE	19.306	315747	1.033 ug/ml
16) N-HEXATRIACONTANE	20.051	638538	2.518 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE013120\
Data File : FE031264.D
Signal(s) : FID1B.CH
Acq On : 31 Jan 2020 15:57
Operator : DD\AJ
Sample : L1310-02 2X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 31 23:32:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012920.M
Quant Title :
QLast Update : Thu Jan 30 04:09:51 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

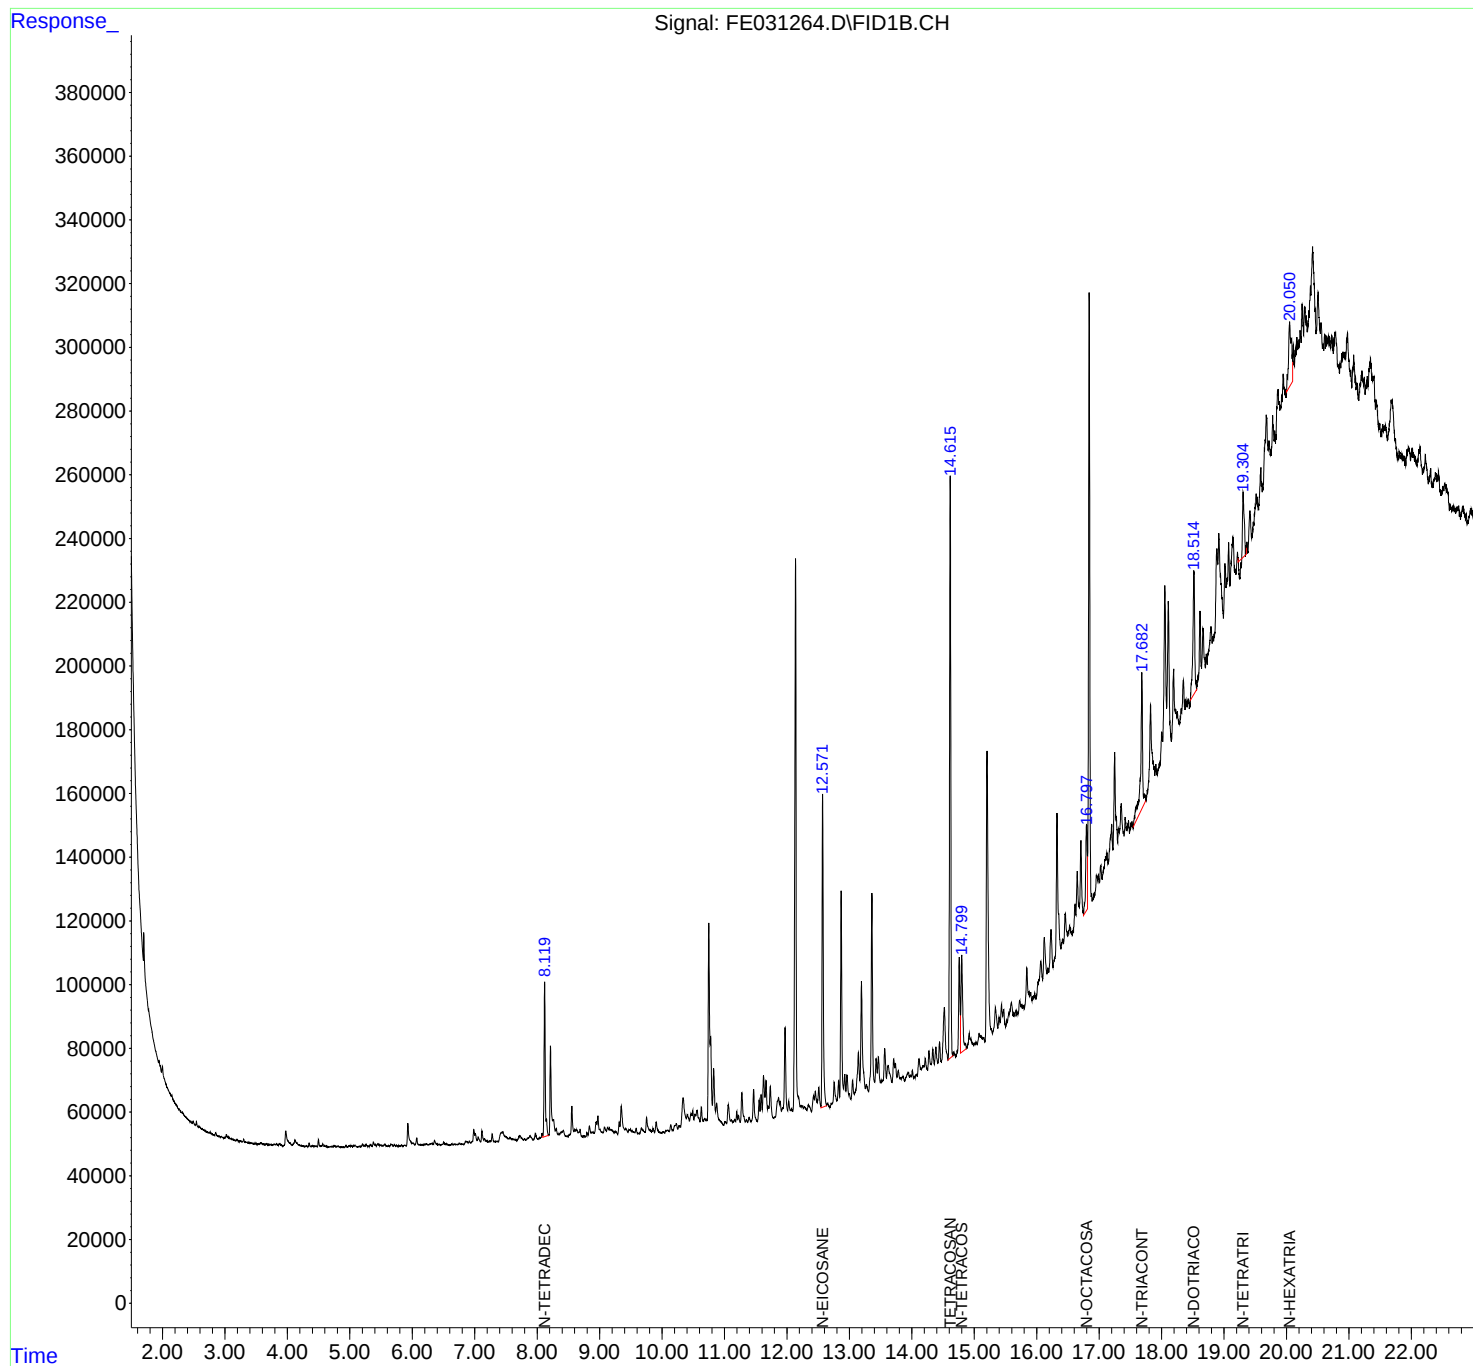


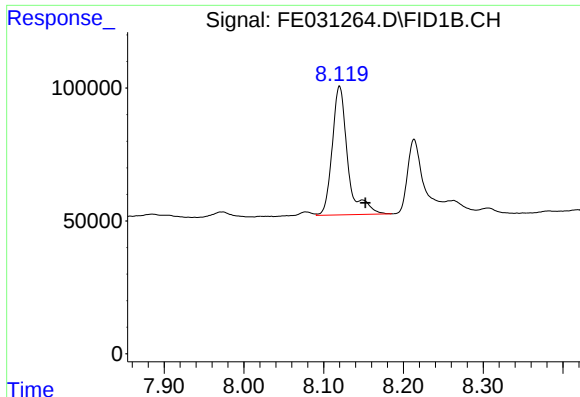

#4 N-TETRADECANE


R.T.: 8.120 min
Delta R.T.: -0.032 min
Response: 654331
Conc: 1.81 ug/ml

Instrument :
FID_E
ClientSampleId :

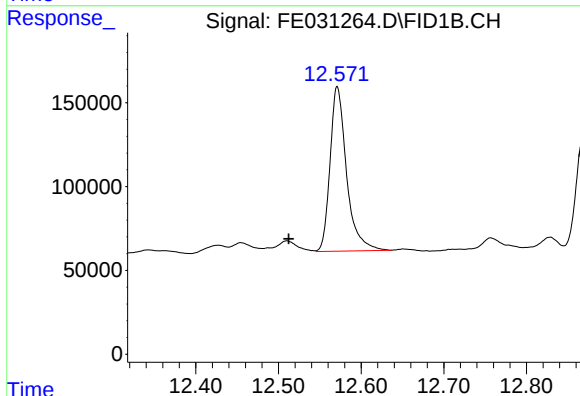


#7 N-EICOSANE

R.T.: 12.571 min
Delta R.T.: 0.059 min
Response: 1359811
Conc: 3.66 ug/ml

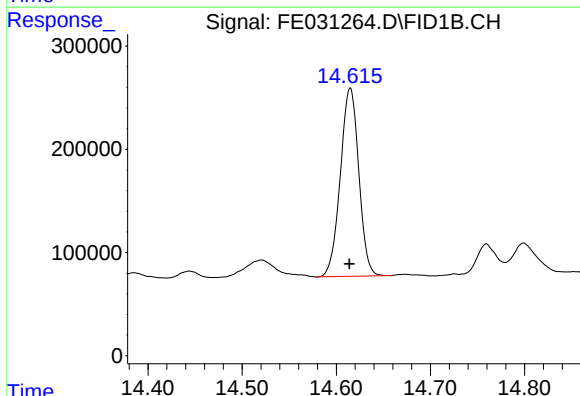


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.615 min
Delta R.T.: 0.000 min
Response: 2484698
Conc: 7.64 ug/ml

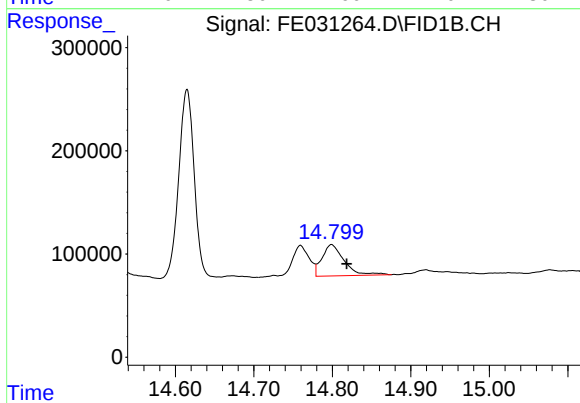

#10 N-TETRACOSANE


R.T.: 14.799 min
Delta R.T.: -0.019 min
Response: 594163
Conc: 1.59 ug/ml

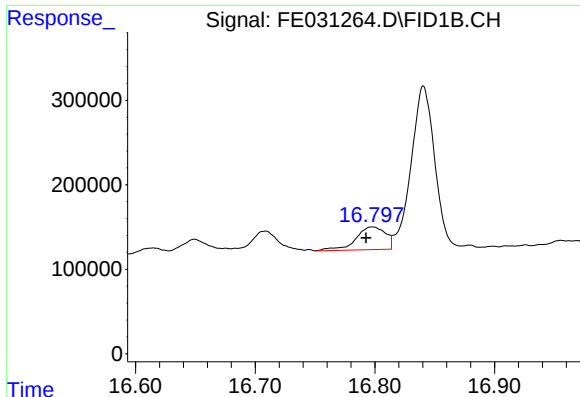

#12 N-OCTACOSANE


R.T.: 16.798 min
Delta R.T.: 0.005 min
Response: 469185
Conc: 1.25 ug/ml

Instrument :
FID_E
ClientSampleId :

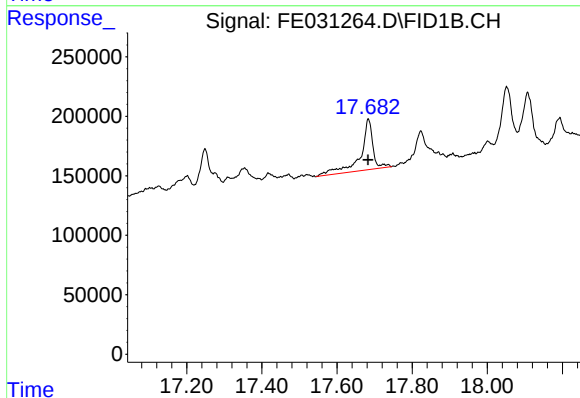


#13 N-TRIACONTANE

R.T.: 17.684 min
Delta R.T.: 0.001 min
Response: 979785
Conc: 2.62 ug/ml

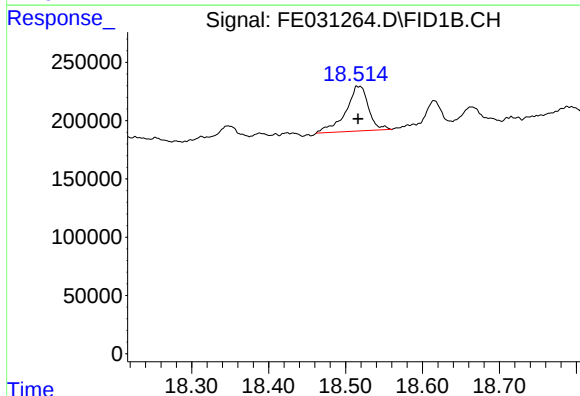


#14 N-DOTRIACONTANE

R.T.: 18.517 min
Delta R.T.: 0.000 min
Response: 784973
Conc: 2.22 ug/ml

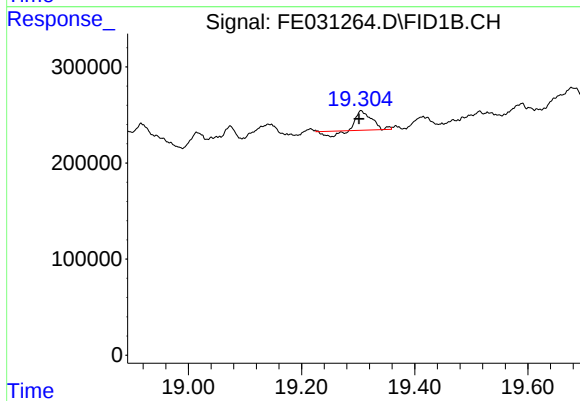

#15 N-TETRATRIACONTANE

R.T.: 19.306 min
Delta R.T.: 0.004 min
Response: 315747
Conc: 1.03 ug/ml

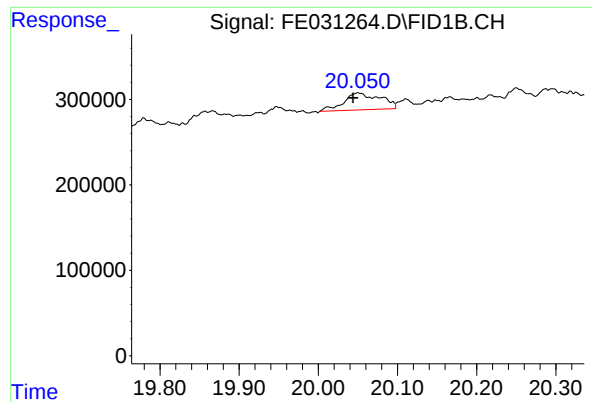

#16 N-HEXATRIACONTANE

R.T.: 20.051 min
Delta R.T.: 0.007 min
Response: 638538
Conc: 2.52 ug/ml

Instrument :
FID_E
ClientSampleId :