

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE013120\
 Data File : FE031265.D
 Signal(s) : FID1B.CH
 Acq On : 31 Jan 2020 16:30
 Operator : DD\AJ
 Sample : L1310-03 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 31 23:32:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012920.M
 Quant Title :
 QLast Update : Thu Jan 30 04:09:51 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.614	2097237	6.449 ug/ml
Target Compounds			
4) N-TETRADECANE	8.214f	366547	1.012 ug/ml
7) N-EICOSANE	12.572f	981489	2.642 ug/ml
10) N-TETRACOSANE	14.802	410925	1.097 ug/ml
12) N-OCTACOSANE	16.797	377204	1.007 ug/ml
13) N-TRIACONTANE	17.682	663191	1.773 ug/ml
14) N-DOTRIACONTANE	18.517	633938	1.792 ug/ml
15) N-TETRATRIACONTANE	19.305	272885	0.893 ug/ml
16) N-HEXATRIACONTANE	20.050	649662	2.562 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE013120\
Data File : FE031265.D
Signal(s) : FID1B.CH
Acq On : 31 Jan 2020 16:30
Operator : DD\AJ
Sample : L1310-03 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 31 23:32:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012920.M
Quant Title :
QLast Update : Thu Jan 30 04:09:51 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

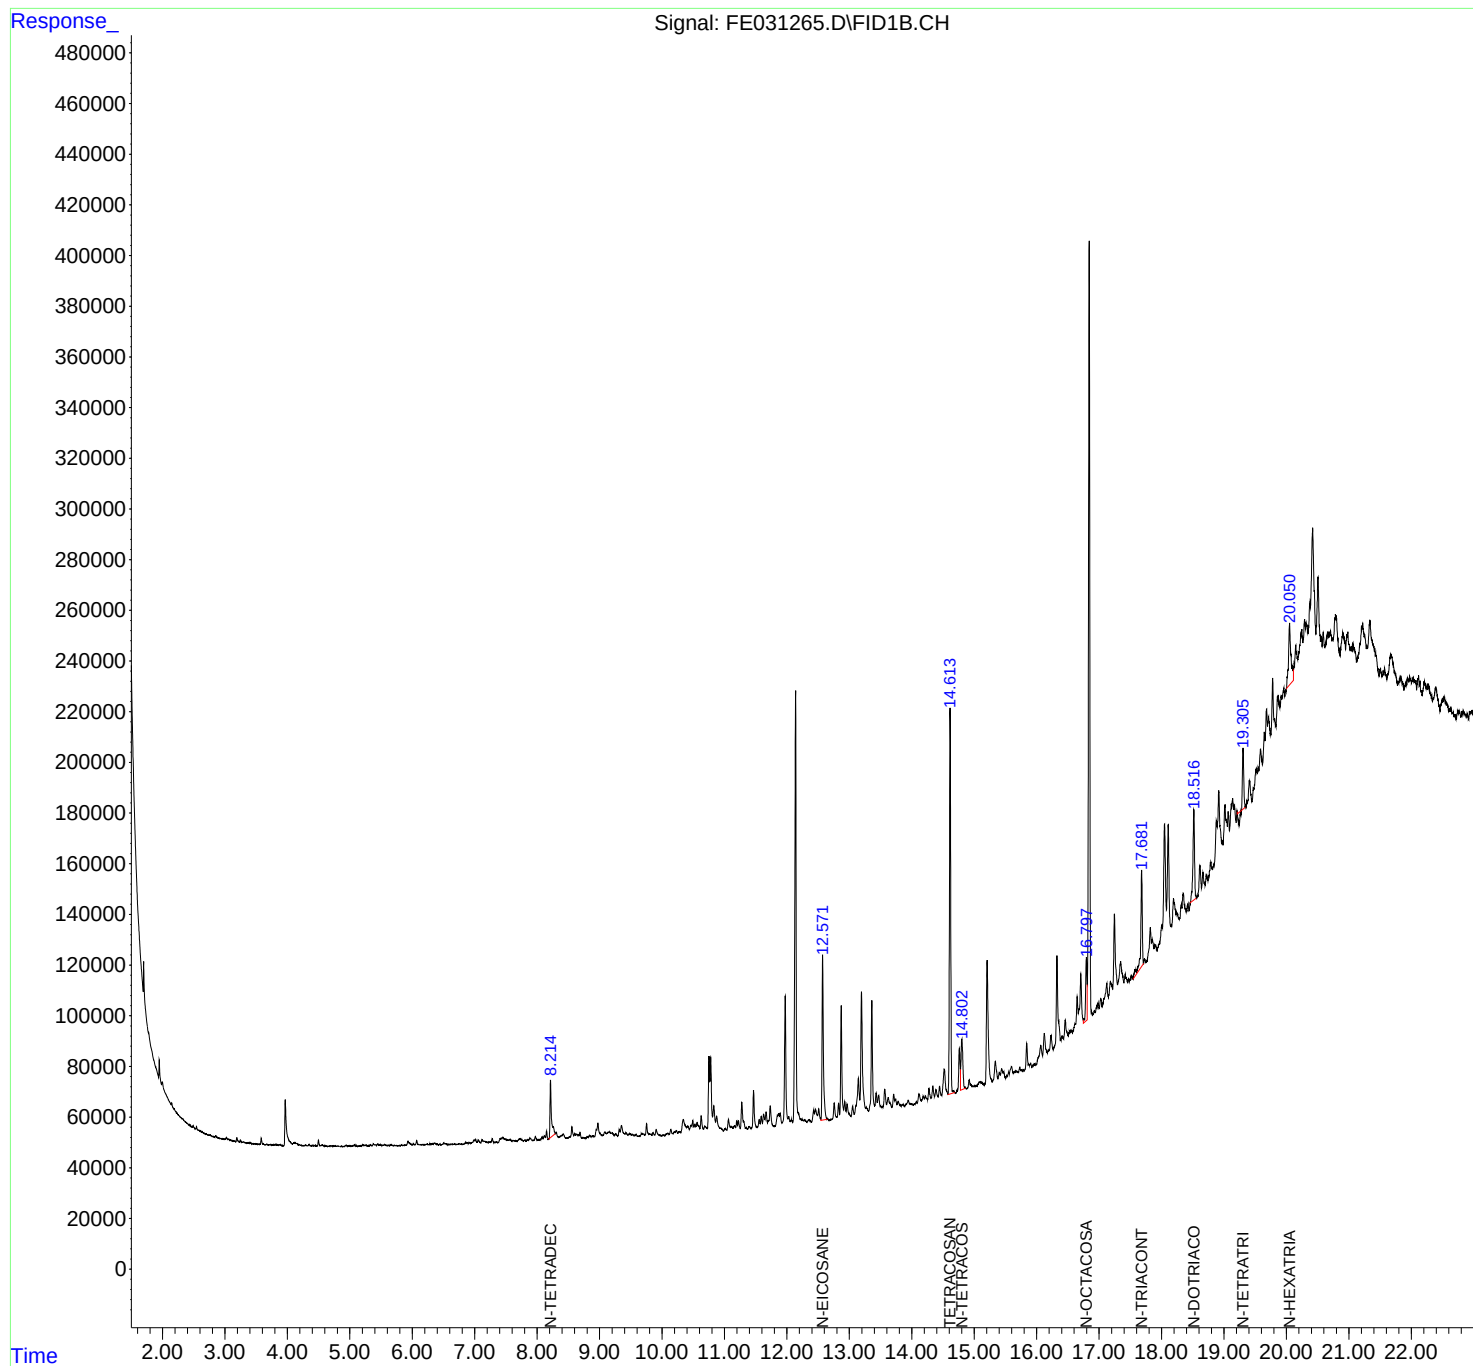


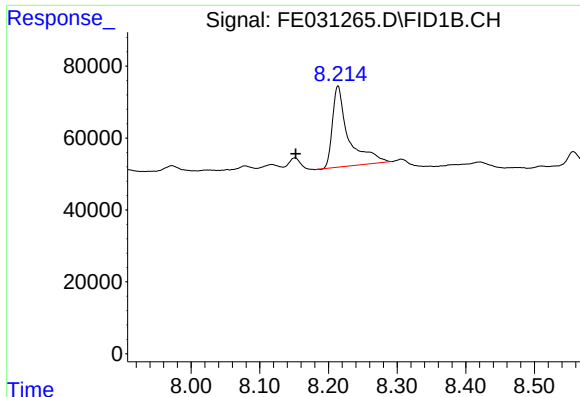

#4 N-TETRADECANE


R.T.: 8.214 min
Delta R.T.: 0.062 min
Response: 366547
Conc: 1.01 ug/ml

Instrument :
FID_E
ClientSampleId :

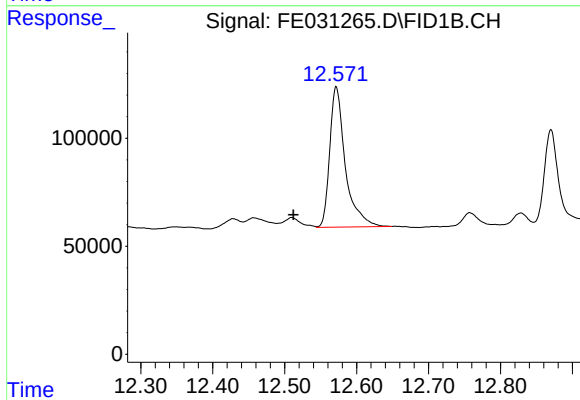


#7 N-EICOSANE

R.T.: 12.572 min
Delta R.T.: 0.060 min
Response: 981489
Conc: 2.64 ug/ml

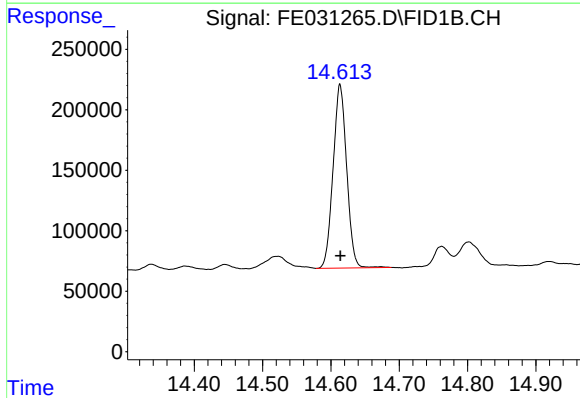


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.614 min
Delta R.T.: 0.000 min
Response: 2097237
Conc: 6.45 ug/ml

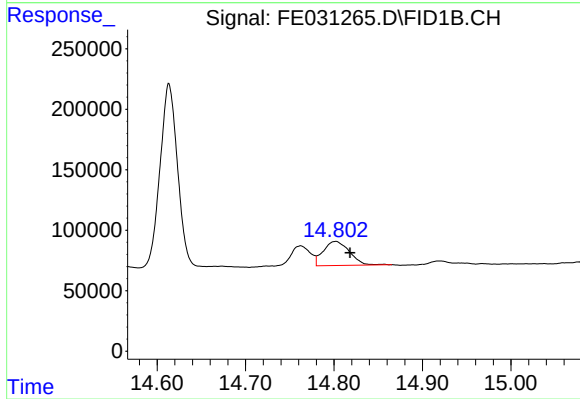

#10 N-TETRACOSANE


R.T.: 14.802 min
Delta R.T.: -0.017 min
Response: 410925
Conc: 1.10 ug/ml

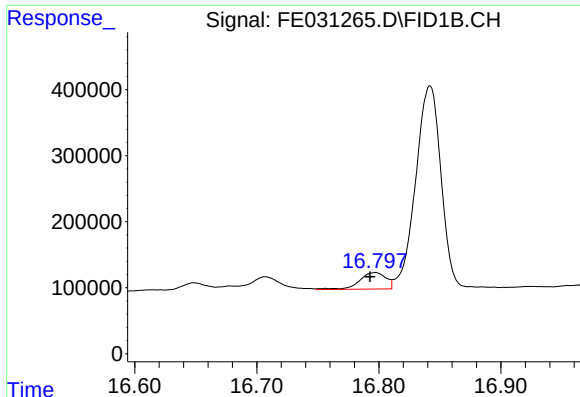

#12 N-OCTACOSANE


R.T.: 16.797 min
Delta R.T.: 0.004 min
Response: 377204
Conc: 1.01 ug/ml

Instrument :
FID_E
ClientSampleId :

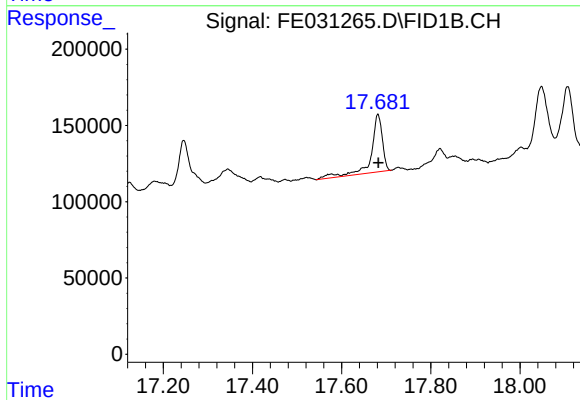


#13 N-TRIACONTANE

R.T.: 17.682 min
Delta R.T.: 0.000 min
Response: 663191
Conc: 1.77 ug/ml

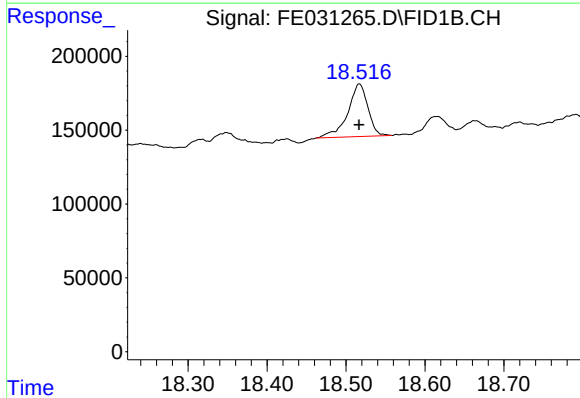


#14 N-DOTRIACONTANE

R.T.: 18.517 min
Delta R.T.: 0.000 min
Response: 633938
Conc: 1.79 ug/ml

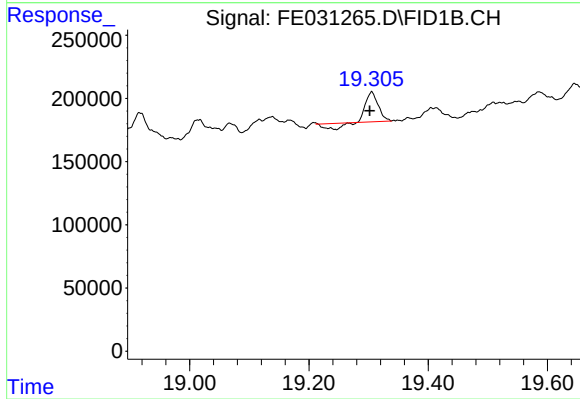

#15 N-TETRATRIACONTANE

R.T.: 19.305 min
Delta R.T.: 0.003 min
Response: 272885
Conc: 0.89 ug/ml

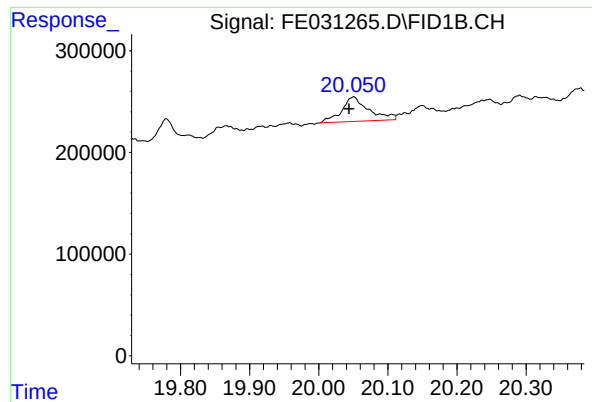

#16 N-HEXATRIACONTANE

R.T.: 20.050 min
Delta R.T.: 0.006 min
Response: 649662
Conc: 2.56 ug/ml

Instrument :
FID_E
ClientSampleId :