

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE013120\  
Data File : FE031265.D  
Signal(s) : FID1B.CH  
Acq On : 31 Jan 2020 16:30  
Operator : DD\AJ  
Sample : L1310-03 2X  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
CTY-SB-10102-0-80

Integration File: autoint1.e  
Quant Time: Jan 31 23:32:52 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE012920.M  
Quant Title :  
QLast Update : Thu Jan 30 04:09:51 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units  |
|-------------------------------|--------|----------|-------------|
| -----                         |        |          |             |
| System Monitoring Compounds   |        |          |             |
| 9) S TETRACOSANE-d50 (SURR... | 14.614 | 2097237  | 6.449 ug/ml |
| Target Compounds              |        |          |             |
| -----                         |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE013120\  
Data File : FE031265.D  
Signal(s) : FID1B.CH  
Acq On : 31 Jan 2020 16:30  
Operator : DD\AJ  
Sample : L1310-03 2X  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
CTY-SB-10102-0-80

Integration File: autoint1.e  
Quant Time: Jan 31 23:32:52 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE012920.M  
Quant Title :  
QLast Update : Thu Jan 30 04:09:51 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

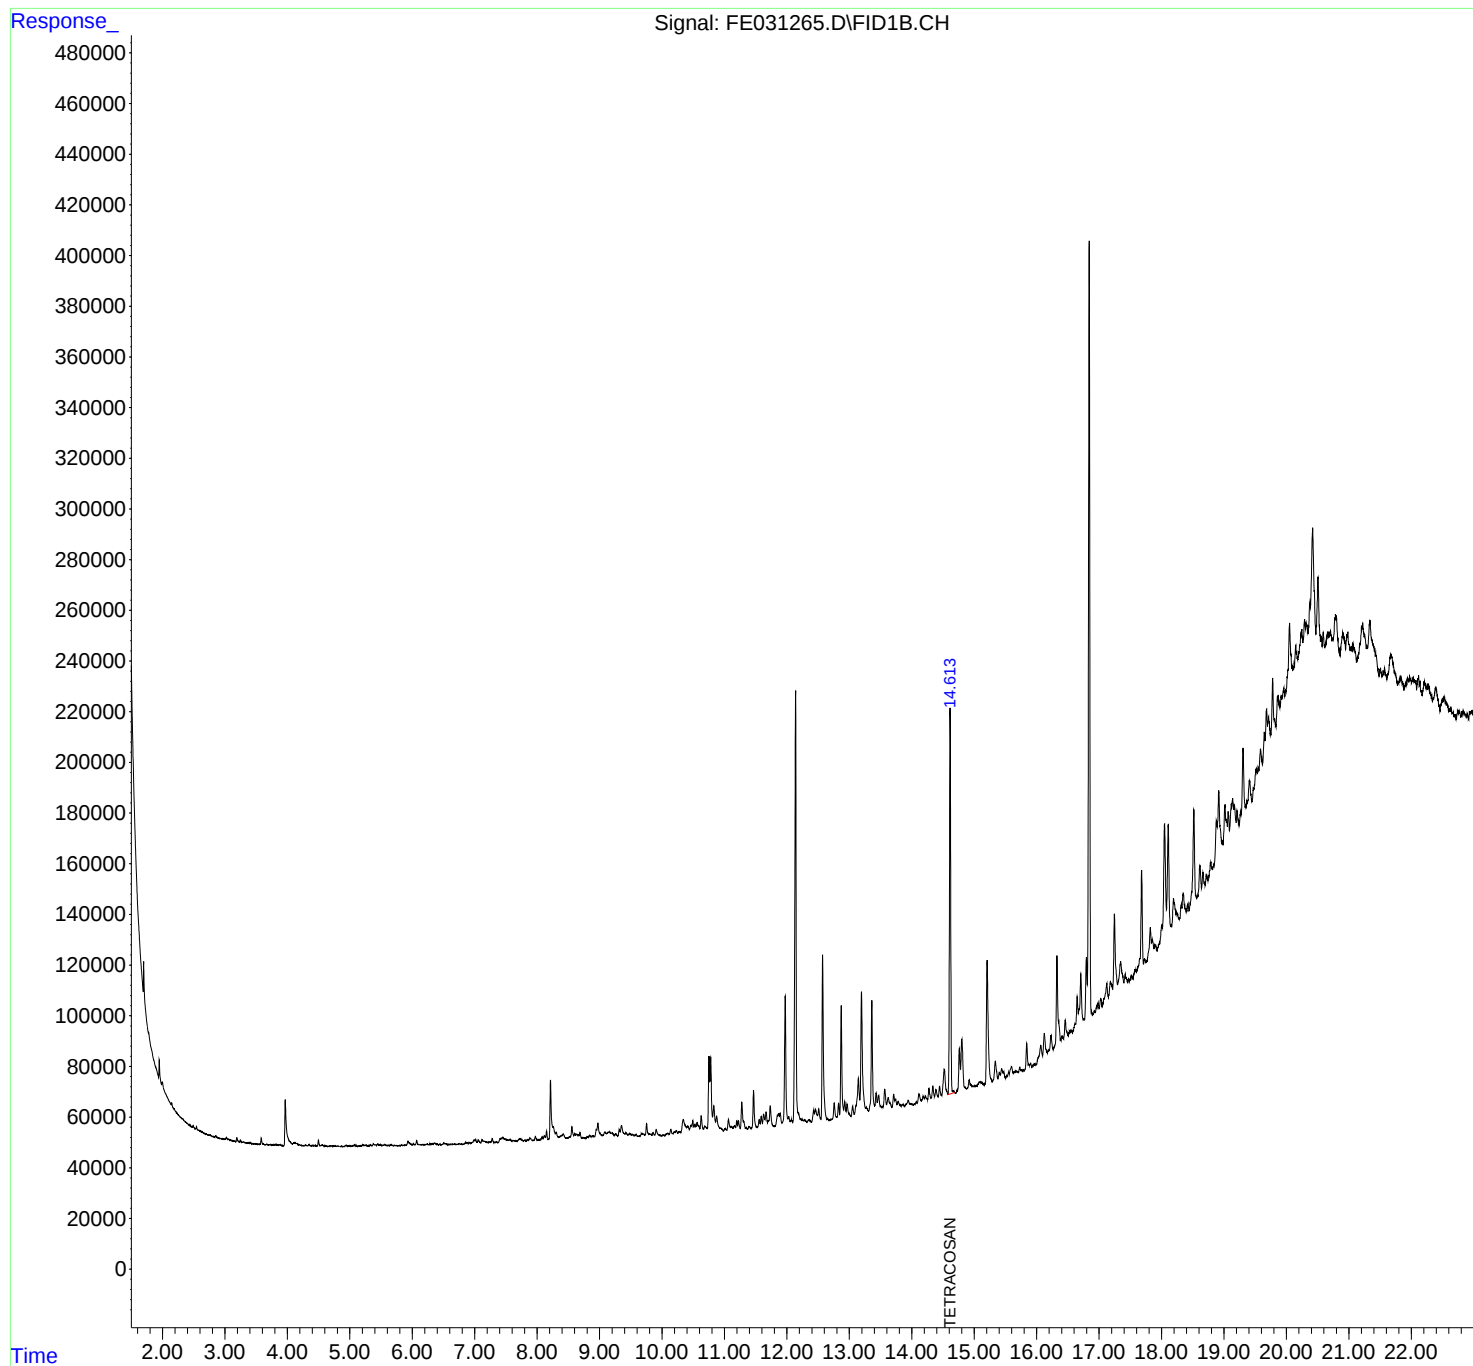

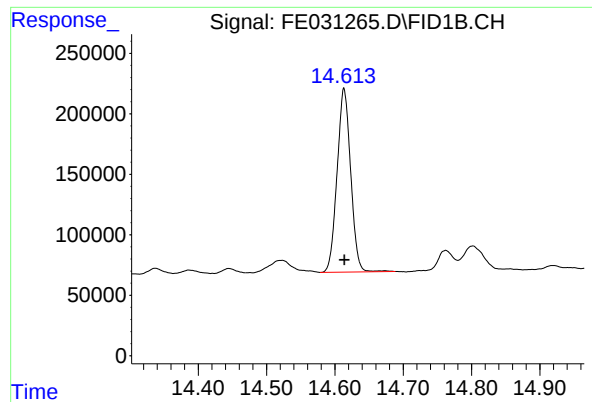

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.614 min  
Delta R.T.: 0.000 min  
Response: 2097237  
Conc: 6.45 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
CTY-SB-10102-0-80