

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE013125\
Data File : FE052166.D
Signal(s) : FID1B.ch
Acq On : 31 Jan 2025 09:26
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 03 00:06:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
Quant Title :
QLast Update : Fri Jan 24 03:06:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	19.153	20413	0.195 ug/ml
15)	N-TETRATRIACONTANE	19.938	32985	0.351 ug/ml
16)	N-HEXATRIACONTANE	20.663	52405	0.649 ug/ml
17)	N-OCTATRIACONTANE	21.456	75694	1.015 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE013125\
Data File : FE052166.D
Signal(s) : FID1B.ch
Acq On : 31 Jan 2025 09:26
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 03 00:06:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
Quant Title :
QLast Update : Fri Jan 24 03:06:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

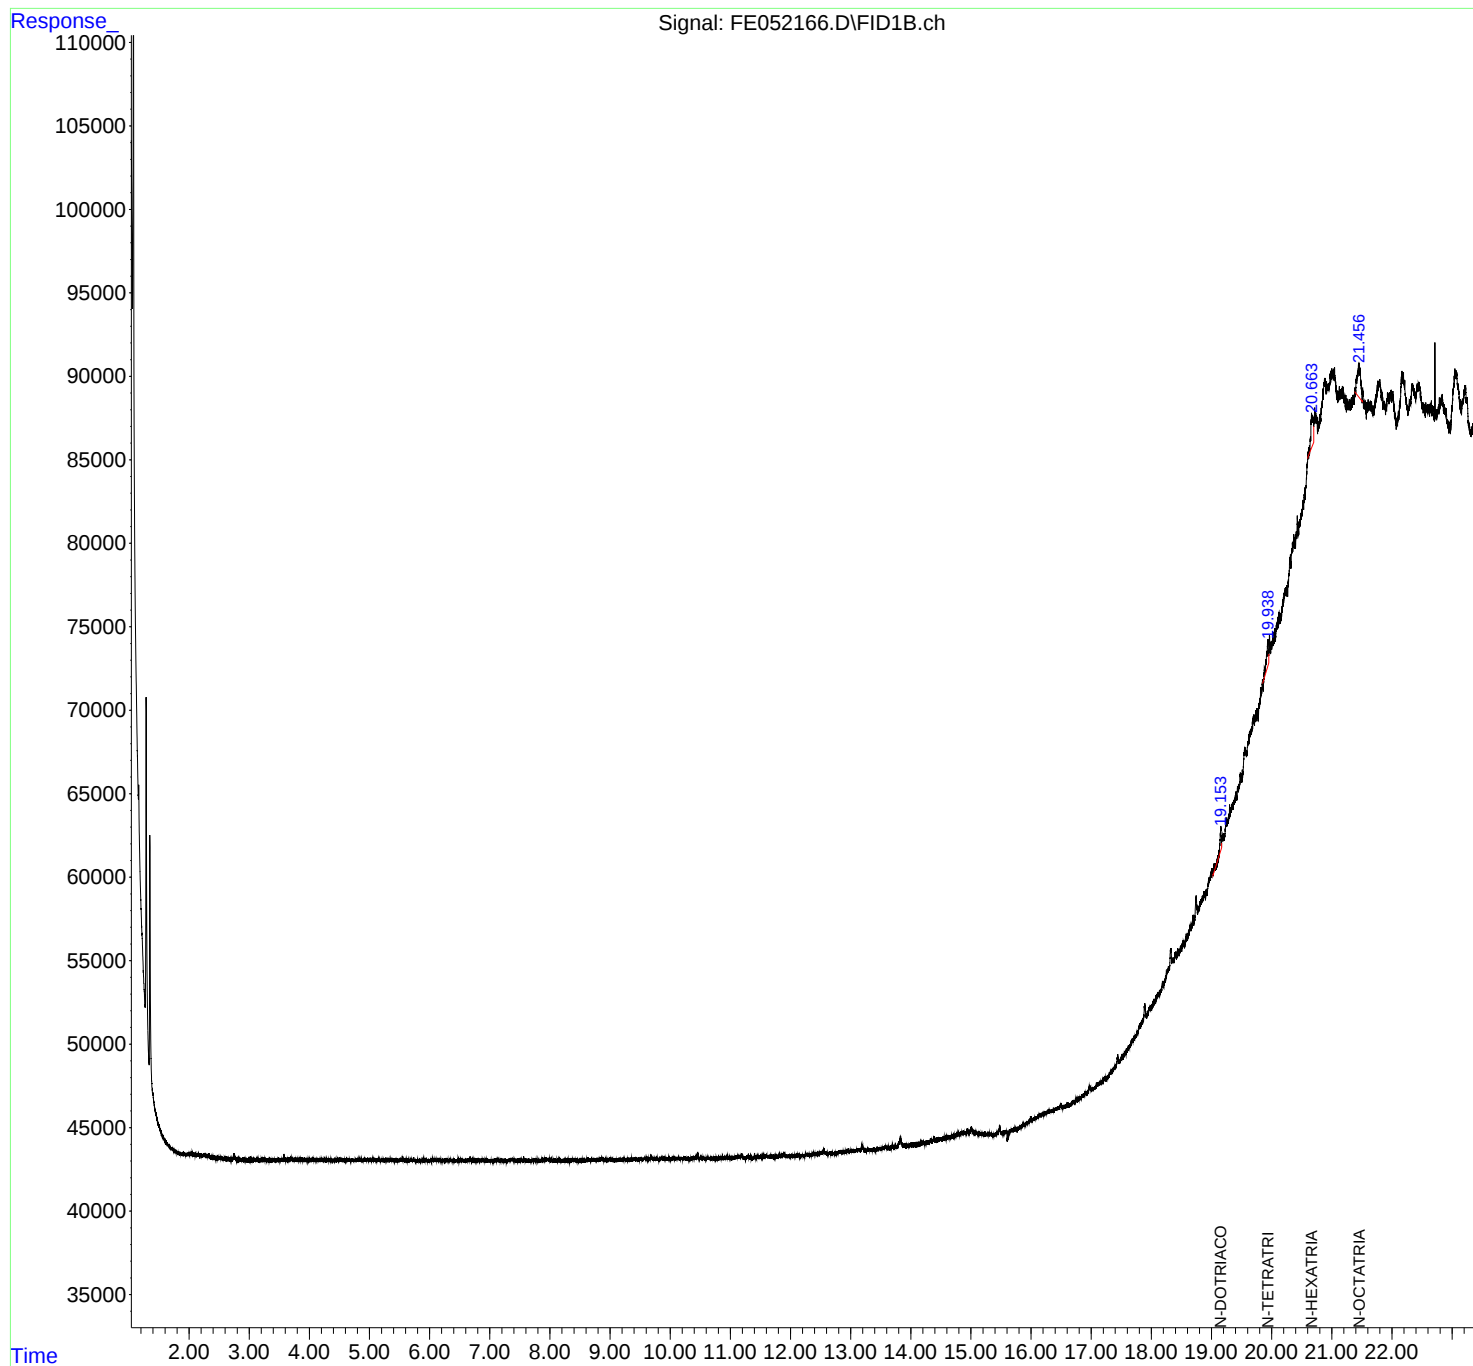


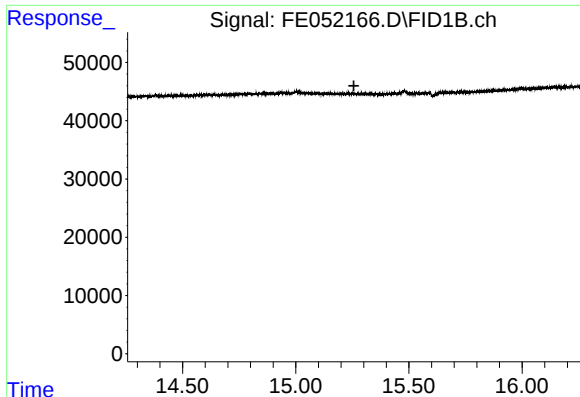

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.257 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

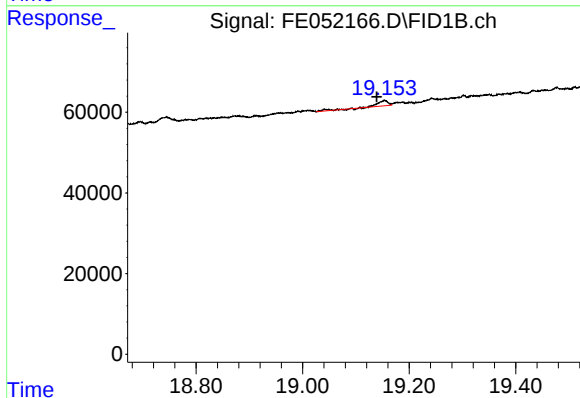


#14 N-DOTRIACONTANE

R.T.: 19.153 min
Delta R.T.: 0.015 min
Response: 20413
Conc: 0.20 ug/ml

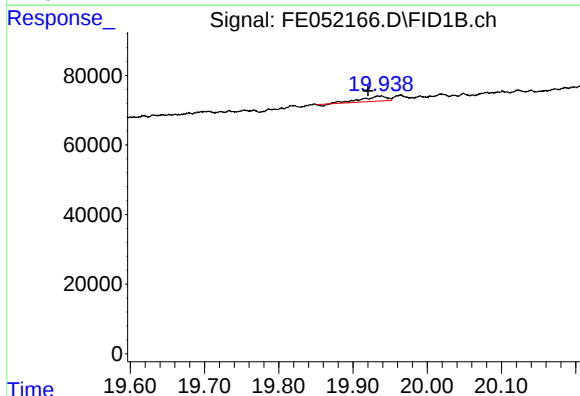


#15 N-TETRATRIACONTANE

R.T.: 19.938 min
Delta R.T.: 0.018 min
Response: 32985
Conc: 0.35 ug/ml

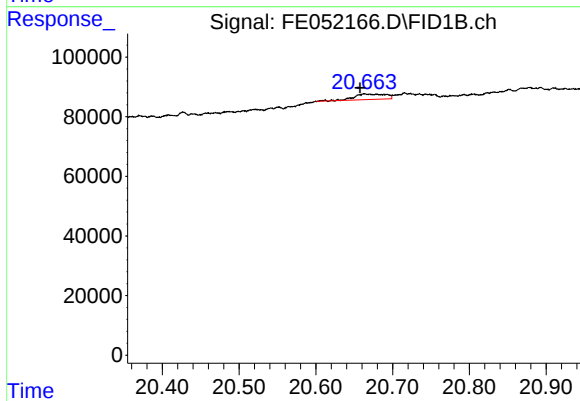

#16 N-HEXATRIACONTANE

R.T.: 20.663 min
Delta R.T.: 0.006 min
Response: 52405
Conc: 0.65 ug/ml

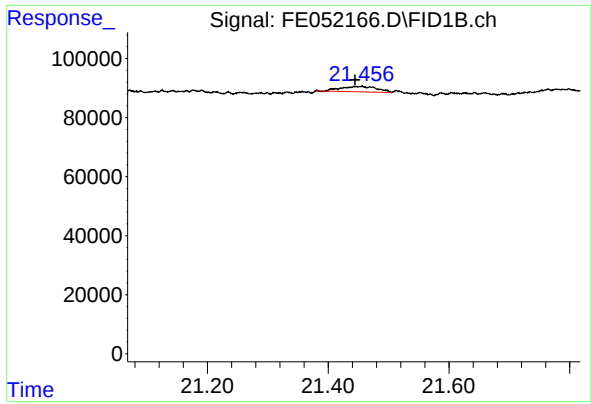

#17 N-OCTATRIACONTANE

R.T.: 21.456 min
Delta R.T.: 0.012 min
Response: 75694
Conc: 1.01 ug/ml

Instrument :
FID_E
ClientSampleId :