

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE013125\  
 Data File : FE052185.D  
 Signal(s) : FID1B.ch  
 Acq On : 31 Jan 2025 19:11  
 Operator : YP\AJ  
 Sample : Q1241-09 10X  
 Misc :  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 JPP-5.2-013025

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 02/03/2025  
 Supervised By :Ankita Jodhani 02/03/2025

Integration File: autoint1.e  
 Quant Time: Feb 03 00:13:21 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE012325.M  
 Quant Title :  
 QLast Update : Fri Jan 24 03:06:38 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 15.231 | 105253   | 1.057 ug/mlm |
| Target Compounds              |        |          |              |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE013125\  
Data File : FE052185.D  
Signal(s) : FID1B.ch  
Acq On : 31 Jan 2025 19:11  
Operator : YP\AJ  
Sample : Q1241-09 10X  
Misc :  
ALS Vial : 24 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
JPP-5.2-013025


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 02/03/2025  
Supervised By :Ankita Jodhani 02/03/2025

Integration File: autoint1.e  
Quant Time: Feb 03 00:13:21 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE012325.M  
Quant Title :  
QLast Update : Fri Jan 24 03:06:38 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

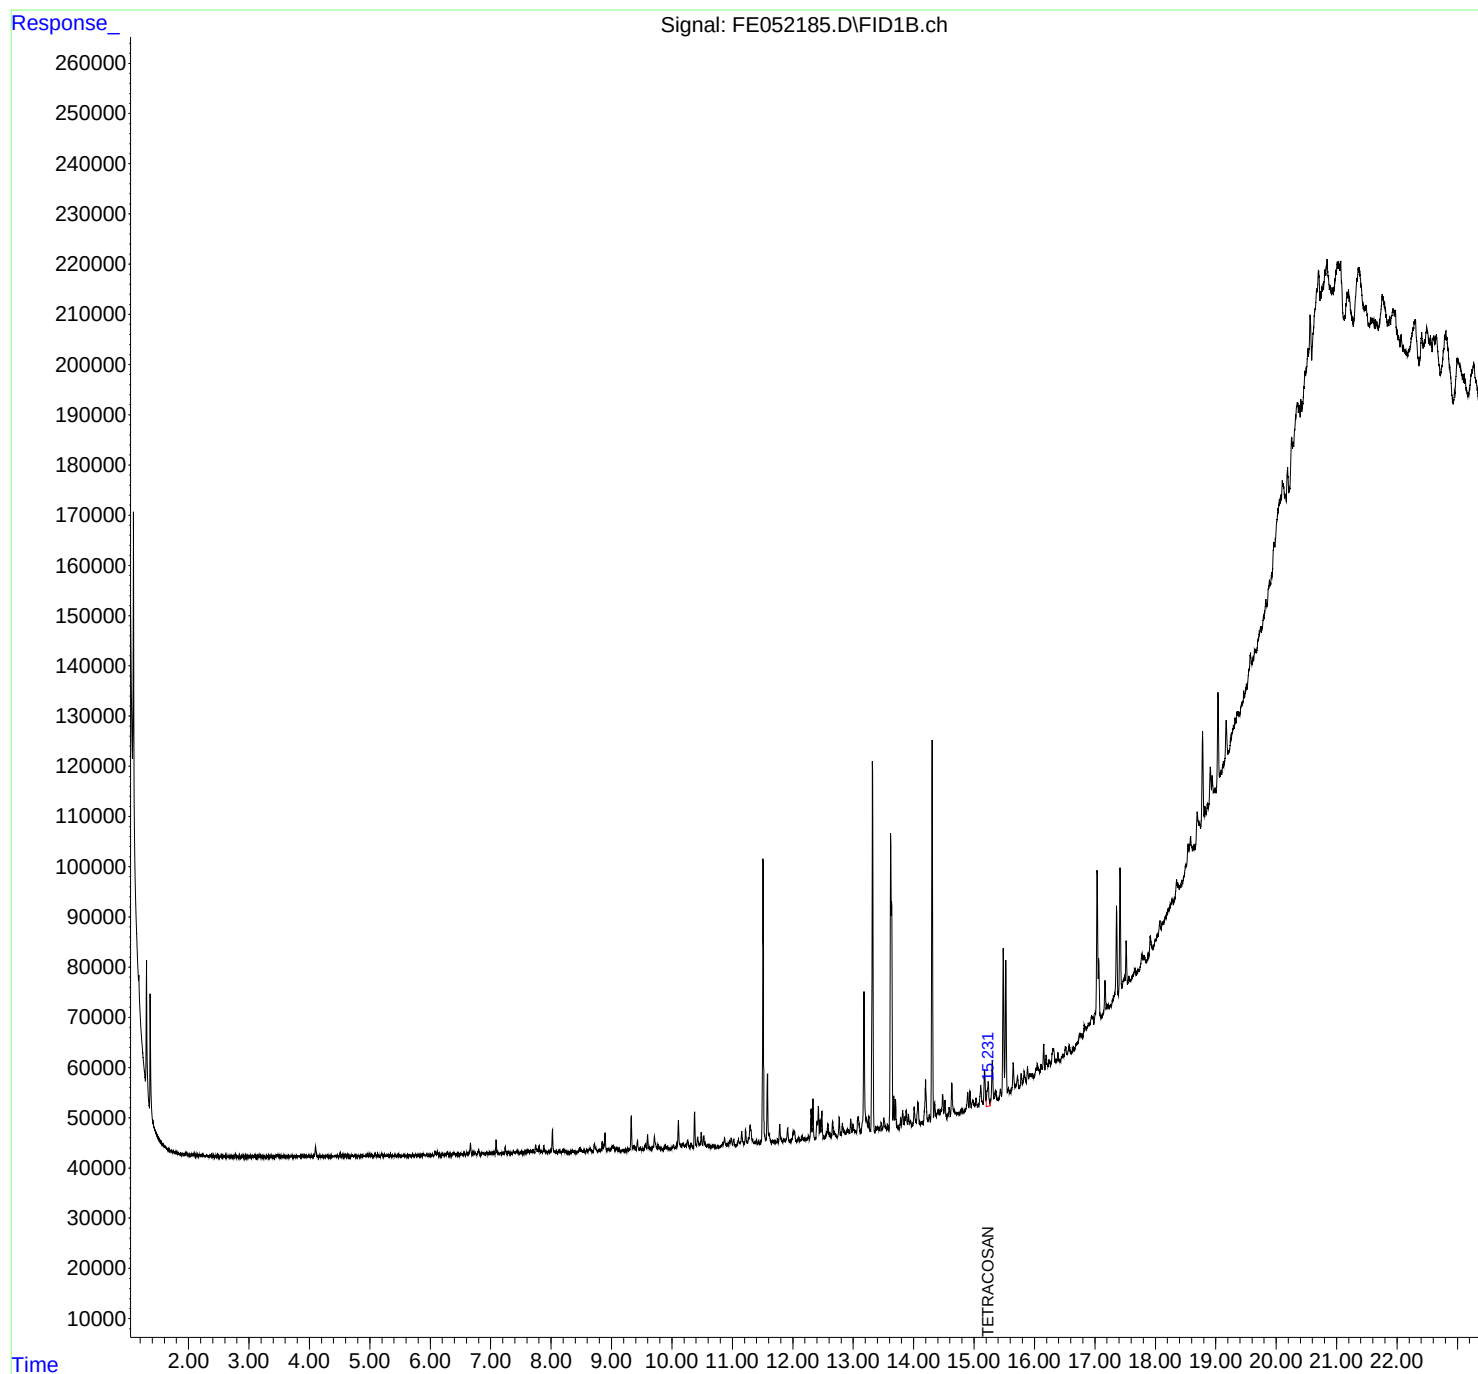

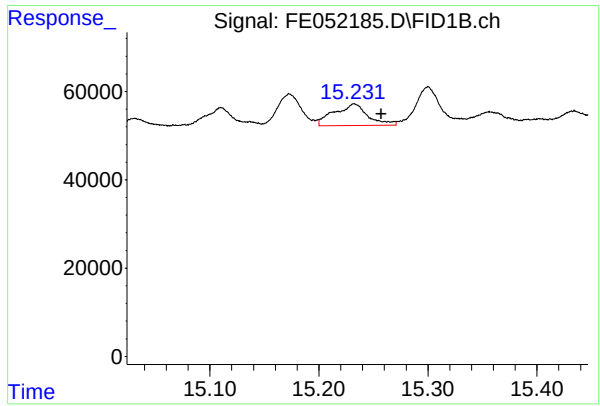

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.231 min  
Delta R.T.: -0.026 min  
Response: 105253  
Conc: 1.06 ug/ml

Instrument :

FID\_E

ClientSampleId :

JPP-5.2-013025

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 02/03/2025

Supervised By :Ankita Jodhani 02/03/2025