

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE020124AL\
 Data File : FE046502.D
 Signal(s) : FID1B.ch
 Acq On : 01 Feb 2024 09:57
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 01 11:47:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 012524.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 25 14:56:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

16) T	n-Octacosane (C28)	17.102	35563	0.227 ug/ml
17) T	n-Tricontane (C30)	17.989	55914	0.357 ug/ml
18) T	n-Dotriacontane (C32)	18.826	99080	0.655 ug/ml
19) T	n-Tetratriacontane (C34)	19.611	99277	0.700 ug/ml
20) T	n-Hexatriacontane (C36)	20.352	44419	0.322 ug/ml
21) T	n-Octatriacontane (C38)	21.092	102637	0.801 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE020124AL\
Data File : FE046502.D
Signal(s) : FID1B.ch
Acq On : 01 Feb 2024 09:57
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 01 11:47:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 012524.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 14:56:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

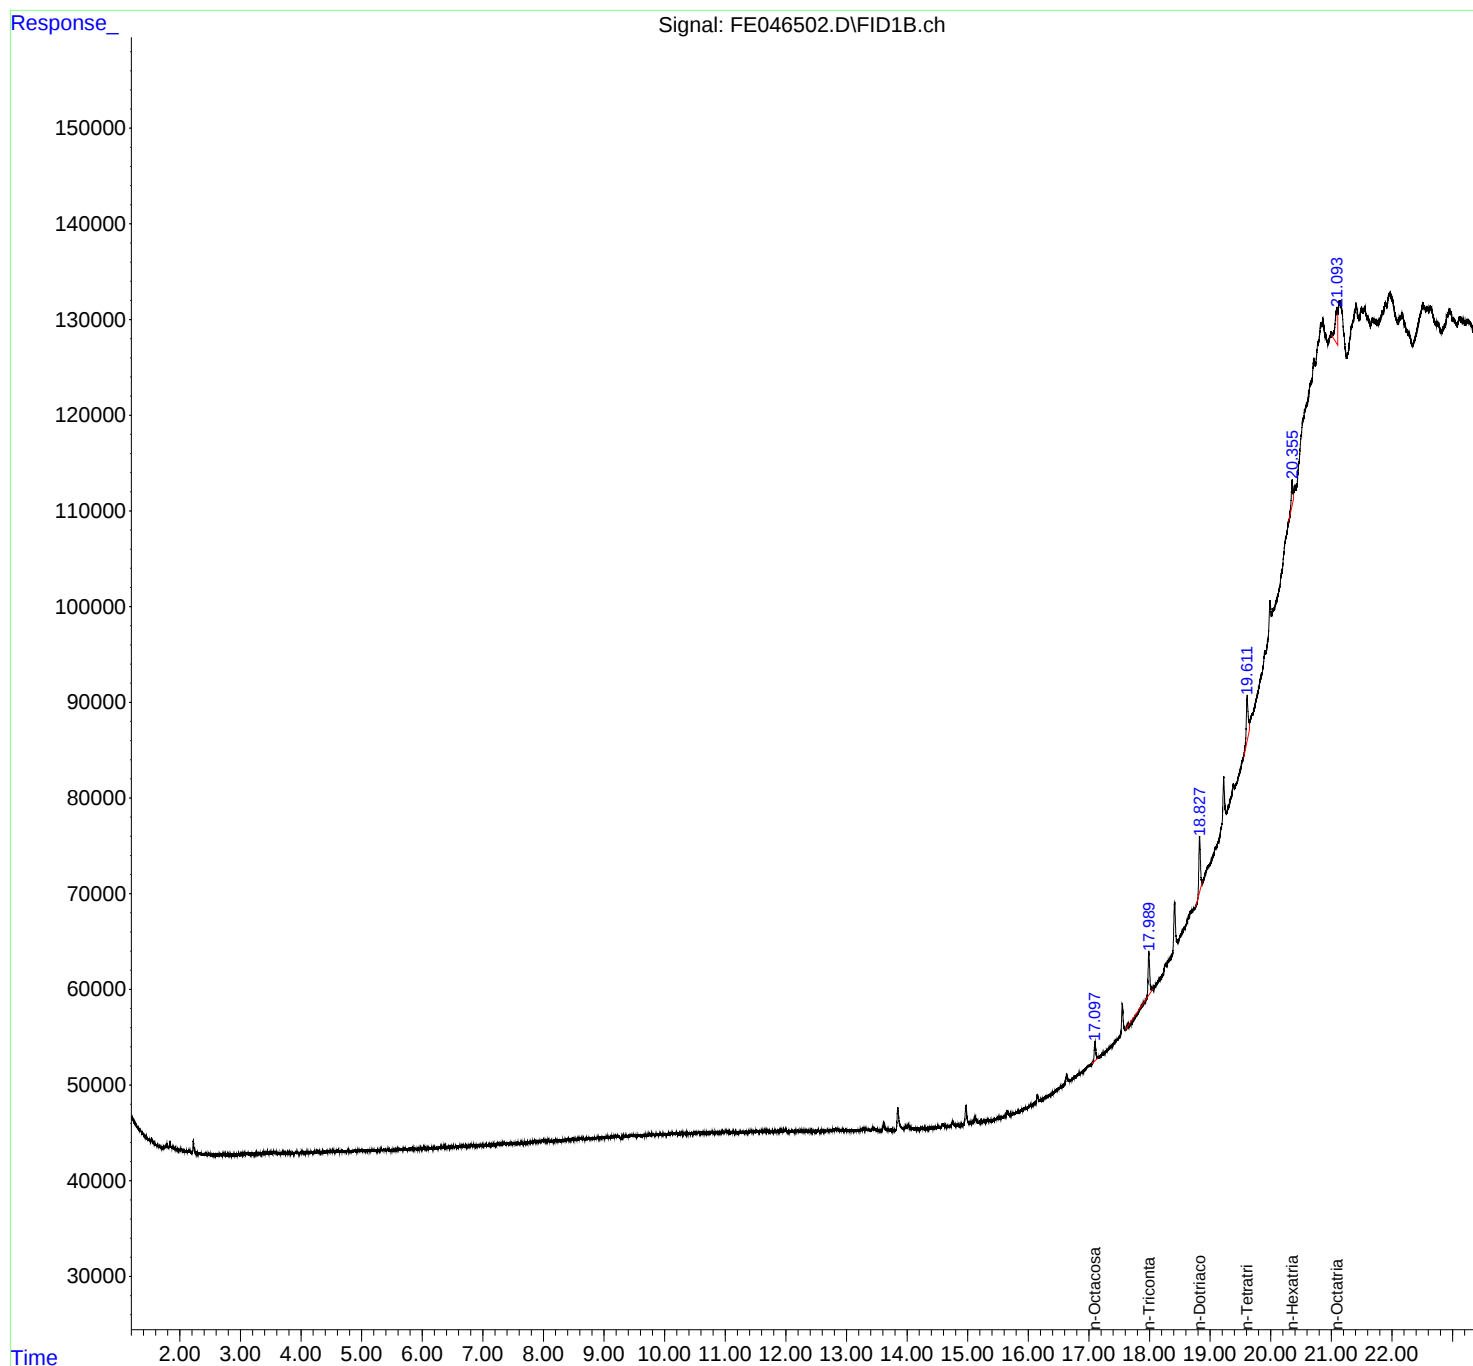


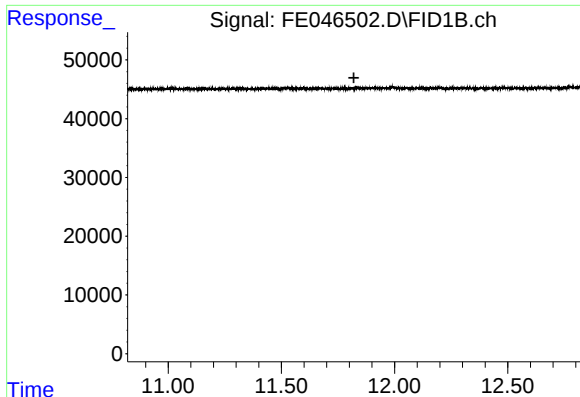

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.820 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

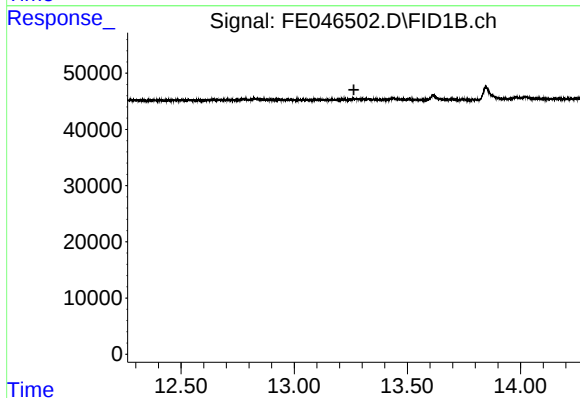


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.264 min
Response: 0
Conc: N.D.

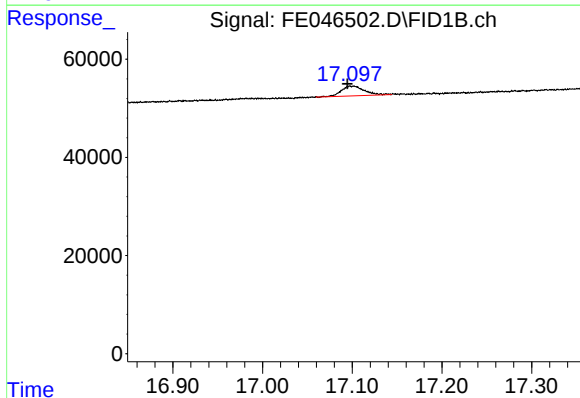


#16 n-Octacosane (C28)

R.T.: 17.102 min
Delta R.T.: 0.007 min
Response: 35563
Conc: 0.23 ug/ml

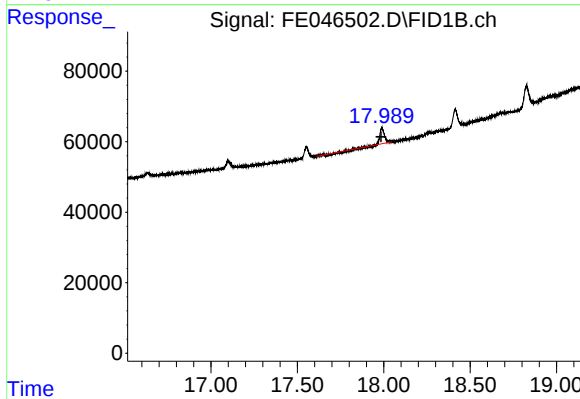

#17 n-Tricontane (C30)


R.T.: 17.989 min
Delta R.T.: 0.005 min
Response: 55914
Conc: 0.36 ug/ml

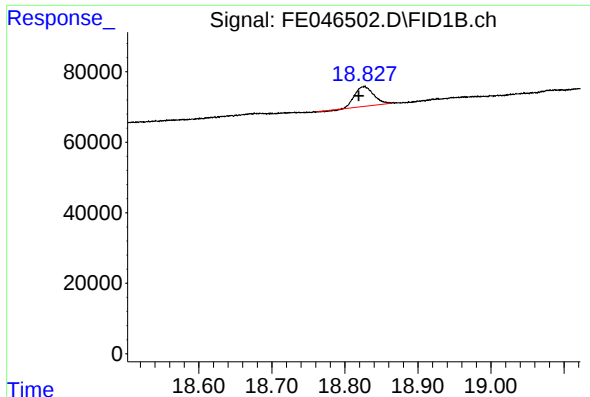

#18 n-Dotriacontane (C32)


R.T.: 18.826 min
Delta R.T.: 0.008 min
Response: 99080
Conc: 0.66 ug/ml

Instrument :
FID_E
ClientSampleId :

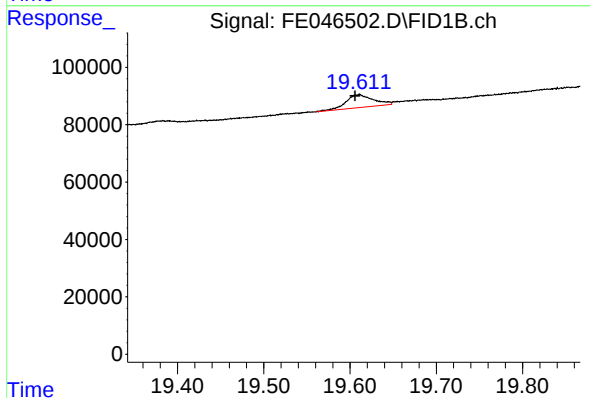


#19 n-Tetratriacontane (C34)

R.T.: 19.611 min
Delta R.T.: 0.005 min
Response: 99277
Conc: 0.70 ug/ml

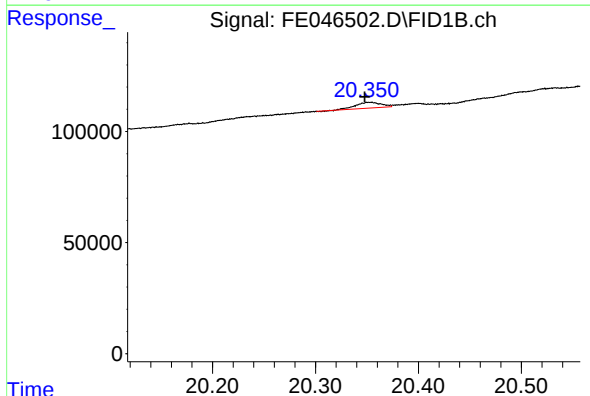

#20 n-Hexatriacontane (C36)

R.T.: 20.352 min
Delta R.T.: 0.004 min
Response: 44419
Conc: 0.32 ug/ml

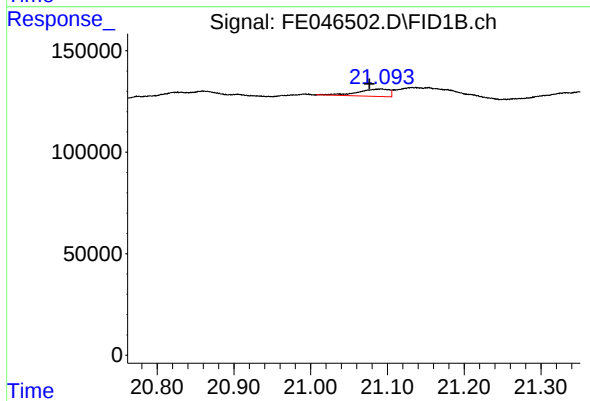

#21 n-Octatriacontane (C38)

R.T.: 21.092 min
Delta R.T.: 0.016 min
Response: 102637
Conc: 0.80 ug/ml