

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0020224\
 Data File : P0101576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Feb 2024 10:09
 Operator : YP/AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 11:44:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0012424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 24 04:51:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.330	3.629	185.9E6	124.3E6	48.421	48.093
2)	SA Decachlor...	10.056	8.673	115.6E6	91935887	49.617	48.515
Target Compounds							
3)	L1 AR-1016-1	5.496	4.720	1794048	1337060	18.353	18.086
4)	L1 AR-1016-2	5.523	4.738	2398474	1072708	17.436	10.884 #
5)	L1 AR-1016-3	5.581	4.918	1519099	1176934	16.934	21.453 #
6)	L1 AR-1016-4	5.679	4.958	1589166	27889103	22.235	548.800 #
7)	L1 AR-1016-5	5.975	5.174	21922463	16612414	277.339	254.457
8)	L2 AR-1221-1	4.537	3.856	1140071	248876	27.229	8.690 #
9)	L2 AR-1221-2	4.635	3.930	3190491	2255047	100.560	100.829
10)	L2 AR-1221-3	4.701	4.005	1239856	513255	14.002	8.075 #
11)	L3 AR-1232-1	4.701	4.005	1239856	513255	16.398	9.407 #
12)	L3 AR-1232-2	5.228	4.738	1112474	1072708	24.481	22.308
13)	L3 AR-1232-3	5.523	4.918	2398474	1176934	35.831	44.886 #
14)	L3 AR-1232-4	5.679	4.999	1589166	9262571	44.392	332.617 #
15)	L3 AR-1232-5	5.771	5.174	38189137	16612414	1119.369	543.255 #
16)	L4 AR-1242-1	5.496	4.720	1794048	1337060	23.186	22.726
17)	L4 AR-1242-2	5.523	4.738	2398474	1072708	22.147	13.833 #
18)	L4 AR-1242-3	5.581	4.918	1519099	1176934	21.372	27.150 #
19)	L4 AR-1242-4	5.679	4.999	1589166	9262571	27.902	186.090 #
20)	L4 AR-1242-5	6.422	5.529	19323604	63699576	360.086	1202.493 #
21)	L5 AR-1248-1	5.496	4.720	1794048	1337060	30.952	29.882
22)	L5 AR-1248-2	5.771	4.958	38189137	27889103	379.206	396.646
23)	L5 AR-1248-3	5.975	4.999	21922463	9262571	211.580	127.346 #
24)	L5 AR-1248-4	6.379	5.174	26855622	16612414	295.733	195.415 #
25)	L5 AR-1248-5	6.422	5.570	19323604	8911383	216.642	130.149 #
26)	L6 AR-1254-1	6.354	5.529	57118299	63699576	480.068	512.006
27)	L6 AR-1254-2	6.573	5.676	85001469	56932617	499.069	508.612
28)	L6 AR-1254-3	6.940	6.084	87511073	86152766	532.881	517.766
29)	L6 AR-1254-4	7.227	6.314	57147459	48571395	571.746	569.441
30)	L6 AR-1254-5	7.648	6.734	62921771	70563552	535.366	520.772
31)	L7 AR-1260-1	7.105	6.214	36847836	44915249	258.377	363.998 #
32)	L7 AR-1260-2	7.363	6.403	39077335	36819131	266.770	269.281
33)	L7 AR-1260-3	7.708	6.557	9190084	33218359	78.705	258.943 #
34)	L7 AR-1260-4	7.937	7.032	23185746	3614419	196.943	34.973 #
35)	L7 AR-1260-5	8.267	7.274	8875300	8169842	40.473	38.921
36)	L8 AR-1262-1	7.648	6.734	62921771	70563552	563.040	870.424 #
37)	L8 AR-1262-2	8.267	7.032	8875300	3614419	32.624	24.291 #
38)	L8 AR-1262-3	8.590	7.560	7325270	279234	37.659	2.718 #
39)	L8 AR-1262-4	8.638	7.624	2486796	7448751	16.016	38.145 #
40)	L8 AR-1262-5	9.320	8.124	459522	559124	4.892	6.672 #
41)	L9 AR-1268-1	8.590	7.560	7325270	279234	23.099	0.999 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020224\
 Data File : P0101576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Feb 2024 10:09
 Operator : YP/AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 11:44:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 24 04:51:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.638	7.624	2486796	7448751	8.611	29.125 #
43) L9	AR-1268-3	8.895	7.830	192989	349964	0.749	1.505 #
44) L9	AR-1268-4	9.320	8.124	459522	559124	5.001	6.579 #
45) L9	AR-1268-5	9.719	8.416	920830	781485	1.149	1.188



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO020224\
Data File : PO101576.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Feb 2024 10:09
Operator : YP/AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 11:44:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO012424.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 24 04:51:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

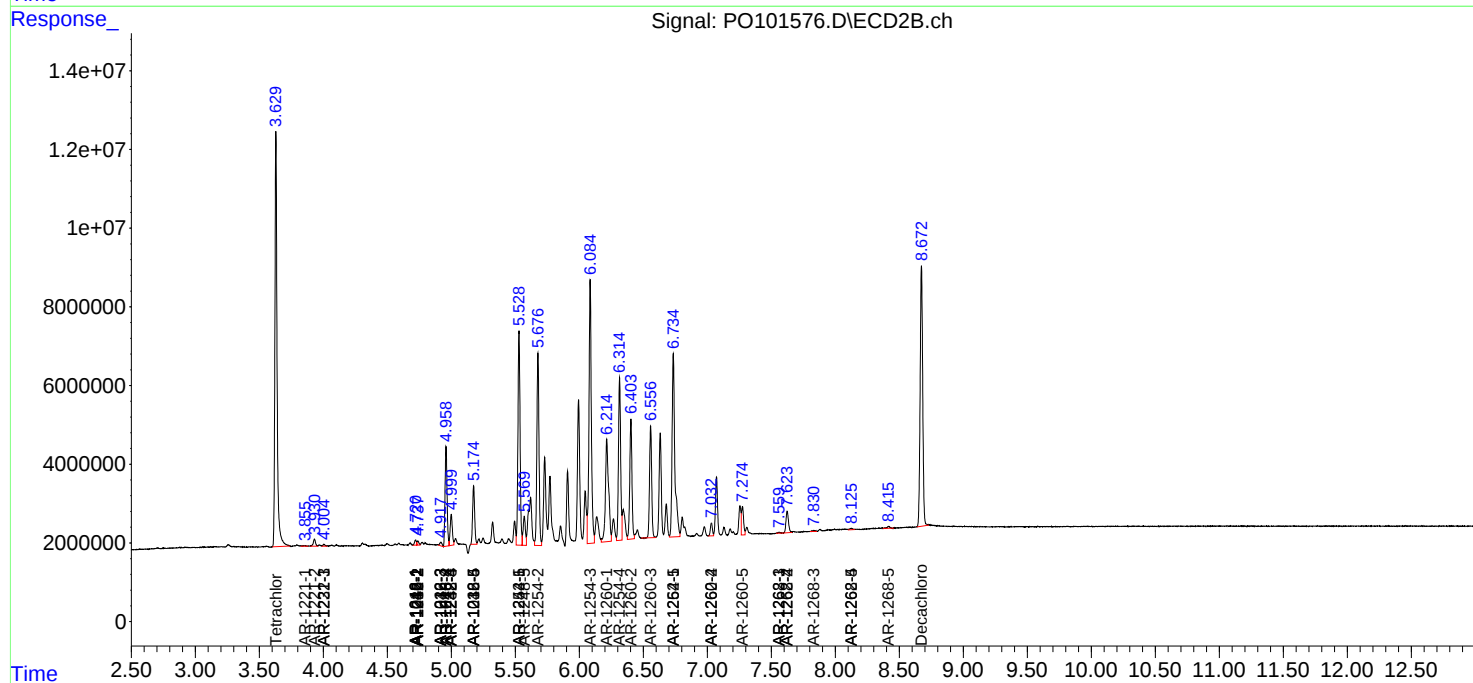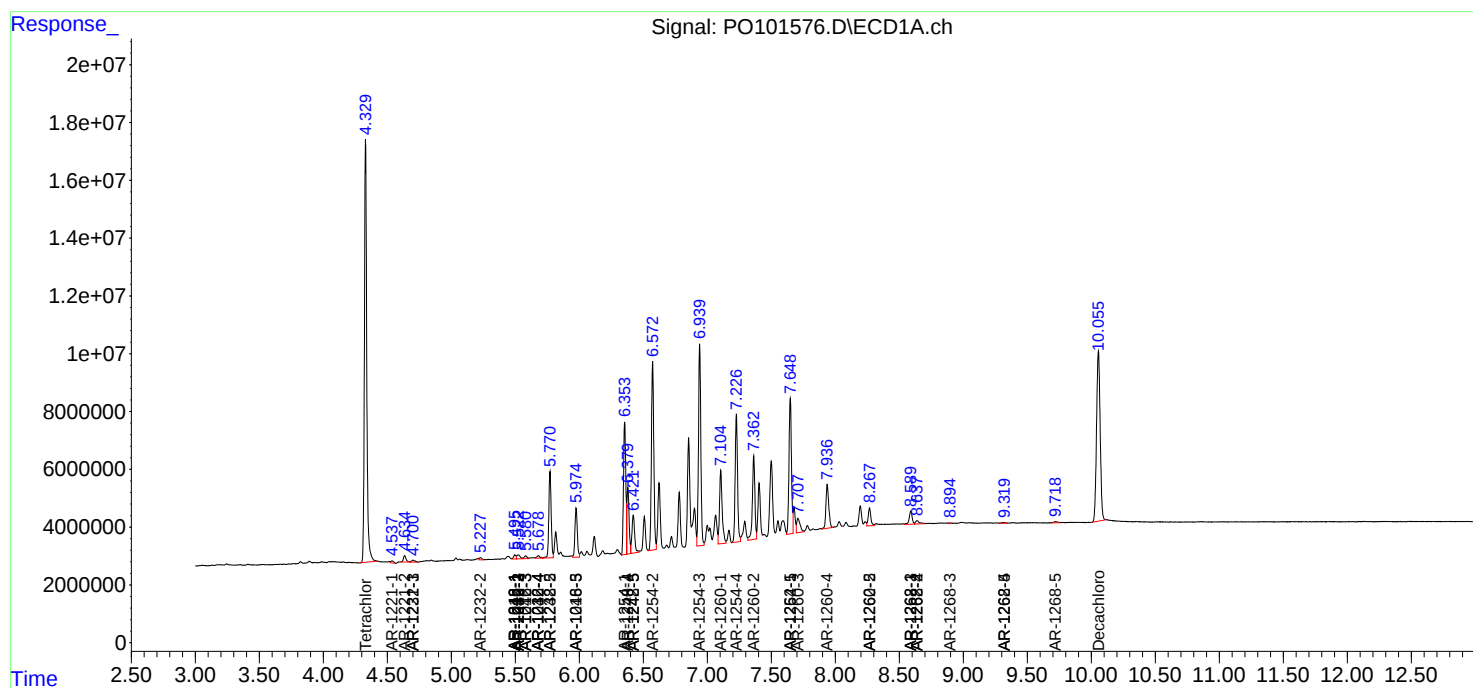


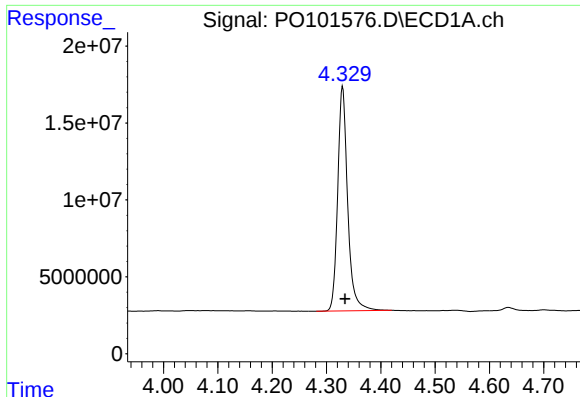

#1 Tetrachloro-m-xylene


R.T.: 4.330 min
Delta R.T.: -0.004 min
Response: 185866153
Conc: 48.42 ng/ml

Instrument :
FID_E
ClientSampleId :

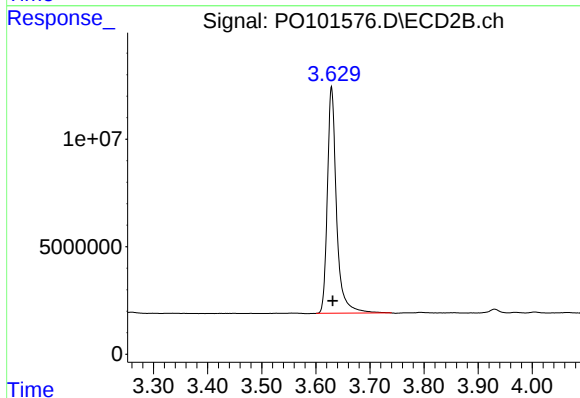


#1 Tetrachloro-m-xylene

R.T.: 3.629 min
Delta R.T.: -0.002 min
Response: 124288408
Conc: 48.09 ng/ml

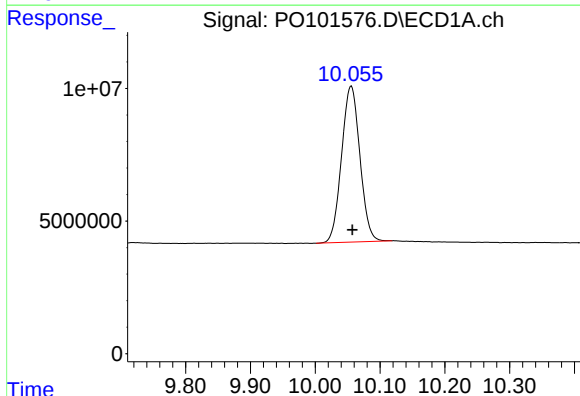


#2 Decachlorobiphenyl

R.T.: 10.056 min
Delta R.T.: -0.002 min
Response: 115613999
Conc: 49.62 ng/ml

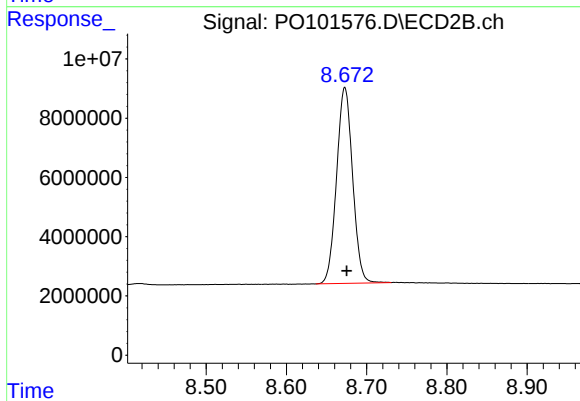

#2 Decachlorobiphenyl


R.T.: 8.673 min
Delta R.T.: -0.002 min
Response: 91935887
Conc: 48.52 ng/ml

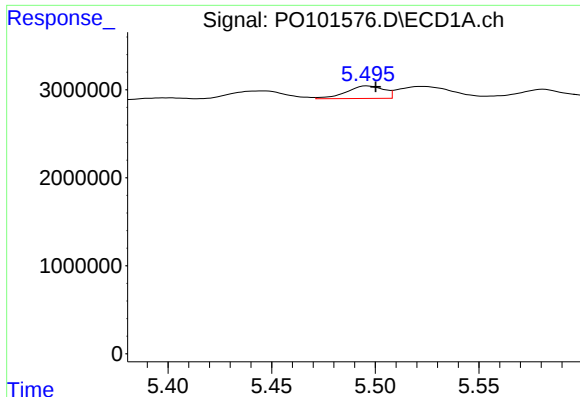

#3 AR-1016-1


R.T.: 5.496 min
Delta R.T.: -0.004 min
Response: 1794048
Conc: 18.35 ng/ml

Instrument :
FID_E
ClientSampleId :

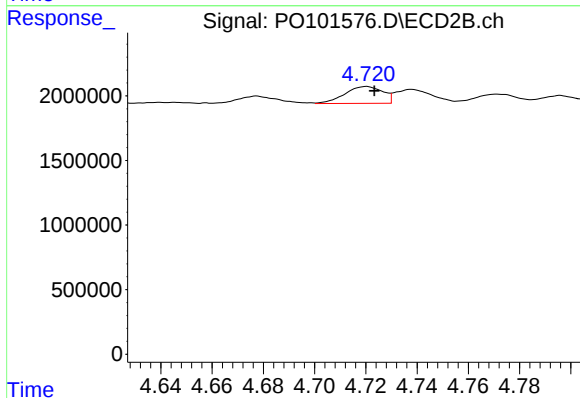


#3 AR-1016-1

R.T.: 4.720 min
Delta R.T.: -0.003 min
Response: 1337060
Conc: 18.09 ng/ml

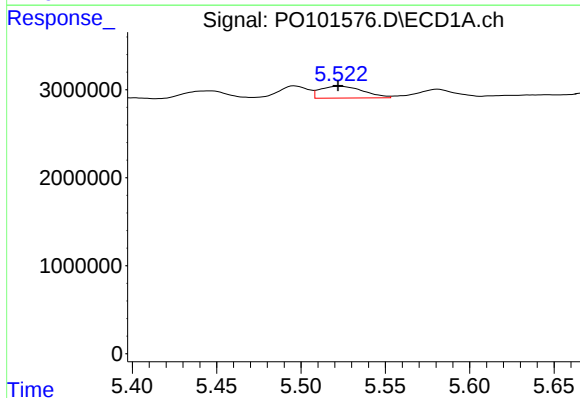


#4 AR-1016-2

R.T.: 5.523 min
Delta R.T.: 0.000 min
Response: 2398474
Conc: 17.44 ng/ml

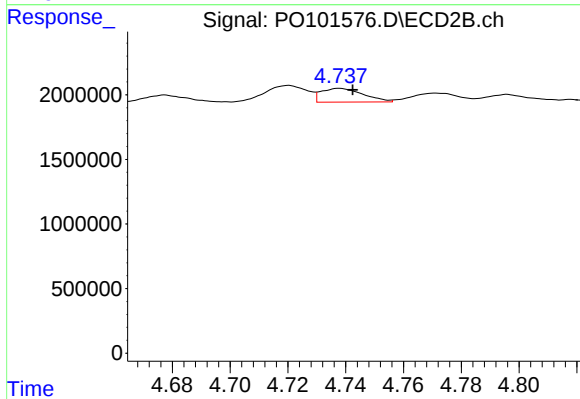

#4 AR-1016-2


R.T.: 4.738 min
Delta R.T.: -0.004 min
Response: 1072708
Conc: 10.88 ng/ml

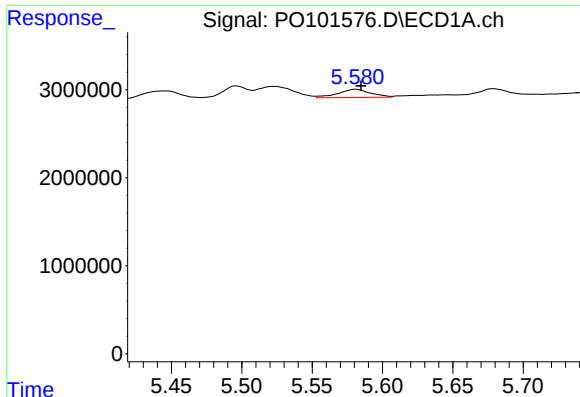

#5 AR-1016-3


R.T.: 5.581 min
Delta R.T.: -0.004 min
Response: 1519099
Conc: 16.93 ng/ml

Instrument :
FID_E
ClientSampleId :

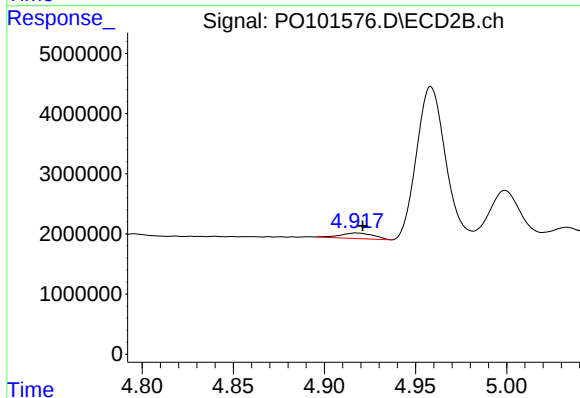


#5 AR-1016-3

R.T.: 4.918 min
Delta R.T.: -0.003 min
Response: 1176934
Conc: 21.45 ng/ml

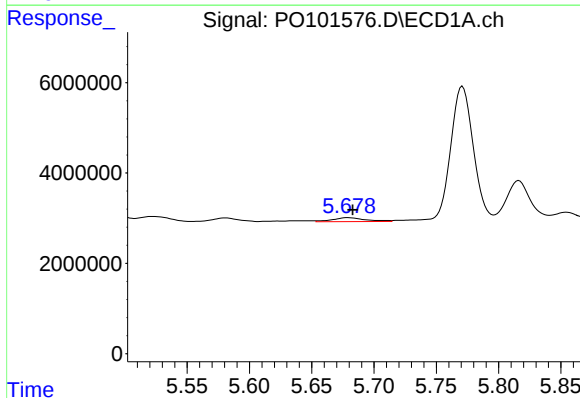


#6 AR-1016-4

R.T.: 5.679 min
Delta R.T.: -0.004 min
Response: 1589166
Conc: 22.23 ng/ml

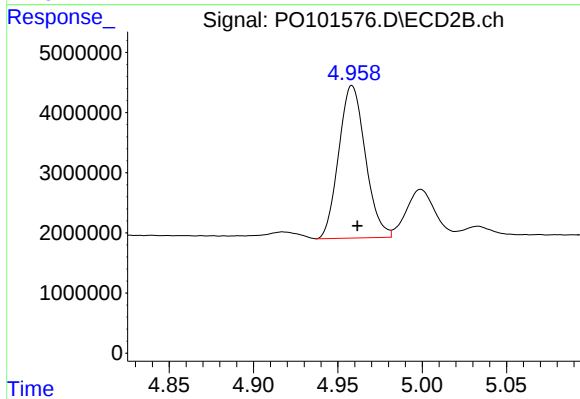

#6 AR-1016-4


R.T.: 4.958 min
Delta R.T.: -0.003 min
Response: 27889103
Conc: 548.80 ng/ml

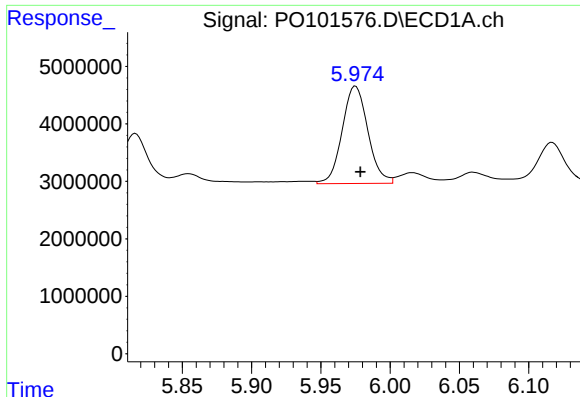

#7 AR-1016-5


R.T.: 5.975 min
Delta R.T.: -0.003 min
Response: 21922463
Conc: 277.34 ng/ml

Instrument :
FID_E
ClientSampleId :

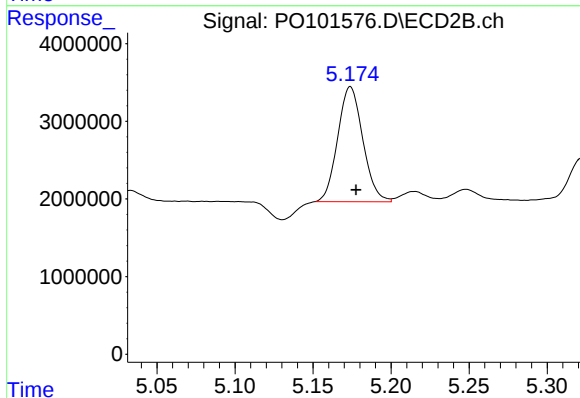


#7 AR-1016-5

R.T.: 5.174 min
Delta R.T.: -0.004 min
Response: 16612414
Conc: 254.46 ng/ml

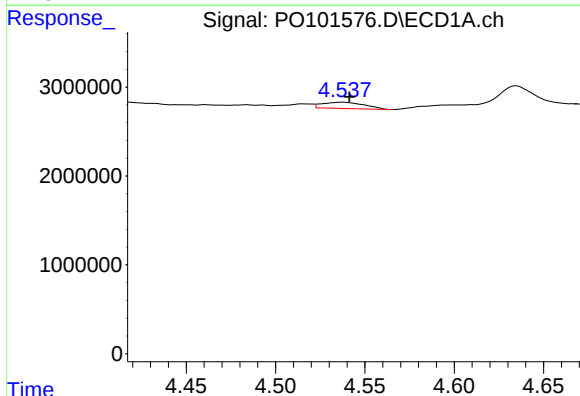


#8 AR-1221-1

R.T.: 4.537 min
Delta R.T.: -0.004 min
Response: 1140071
Conc: 27.23 ng/ml

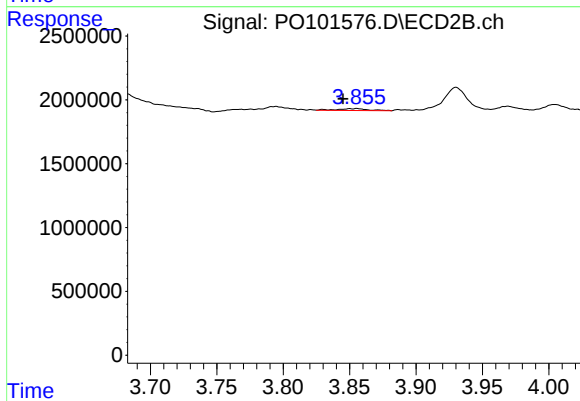

#8 AR-1221-1


R.T.: 3.856 min
Delta R.T.: 0.010 min
Response: 248876
Conc: 8.69 ng/ml

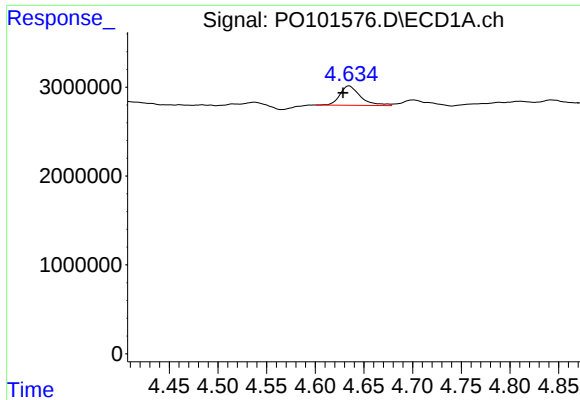

#9 AR-1221-2


R.T.: 4.635 min
Delta R.T.: 0.006 min
Response: 3190491
Conc: 100.56 ng/ml

Instrument :
FID_E
ClientSampleId :

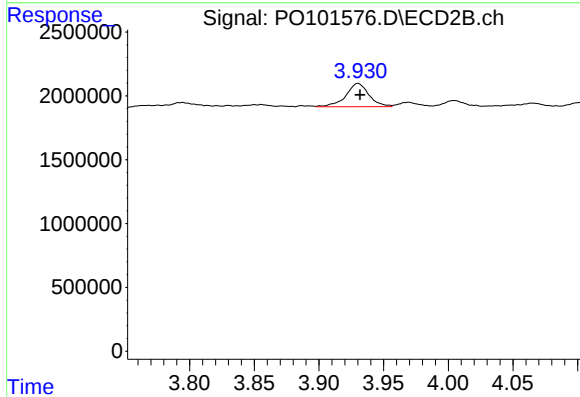


#9 AR-1221-2

R.T.: 3.930 min
Delta R.T.: -0.002 min
Response: 2255047
Conc: 100.83 ng/ml

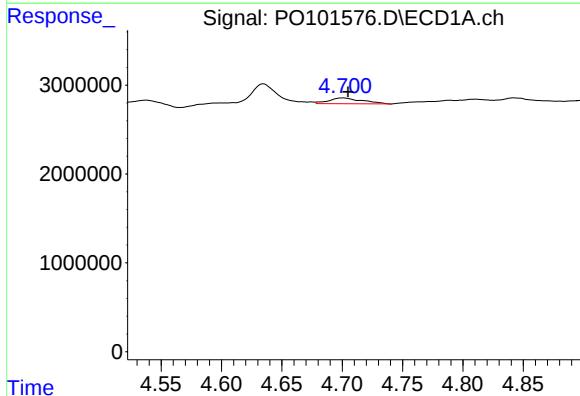


#10 AR-1221-3

R.T.: 4.701 min
Delta R.T.: -0.004 min
Response: 1239856
Conc: 14.00 ng/ml

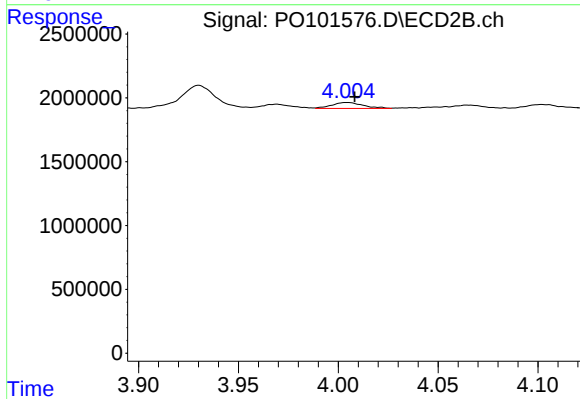

#10 AR-1221-3


R.T.: 4.005 min
Delta R.T.: -0.004 min
Response: 513255
Conc: 8.07 ng/ml

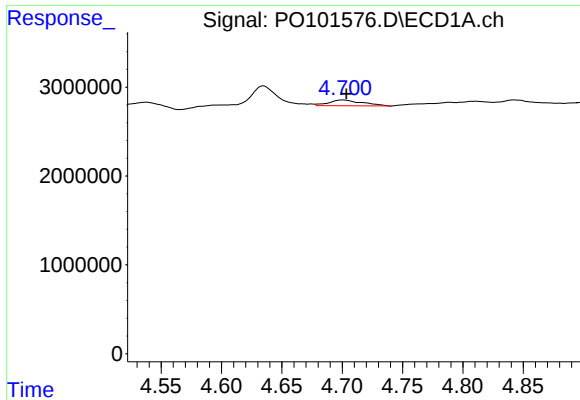

#11 AR-1232-1


R.T.: 4.701 min
Delta R.T.: -0.003 min
Response: 1239856
Conc: 16.40 ng/ml

Instrument :
FID_E
ClientSampleId :

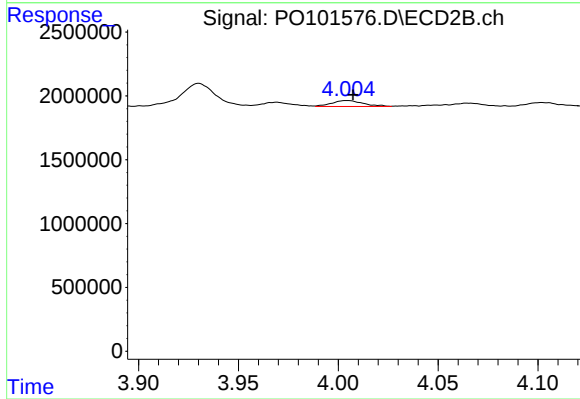


#11 AR-1232-1

R.T.: 4.005 min
Delta R.T.: -0.003 min
Response: 513255
Conc: 9.41 ng/ml

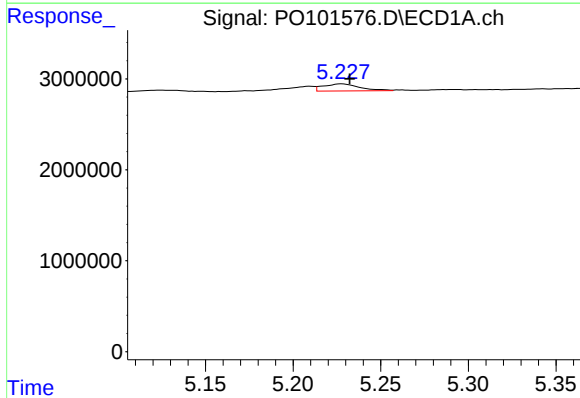


#12 AR-1232-2

R.T.: 5.228 min
Delta R.T.: -0.005 min
Response: 1112474
Conc: 24.48 ng/ml

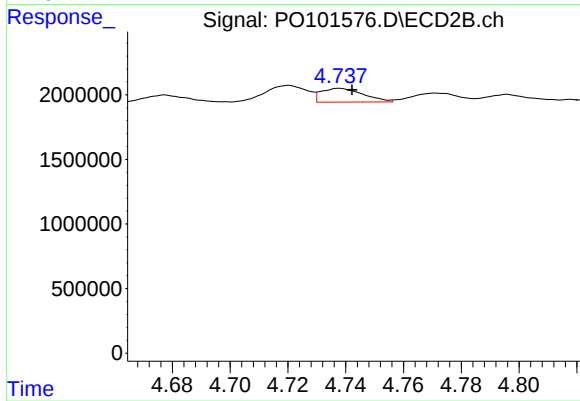

#12 AR-1232-2


R.T.: 4.738 min
Delta R.T.: -0.004 min
Response: 1072708
Conc: 22.31 ng/ml

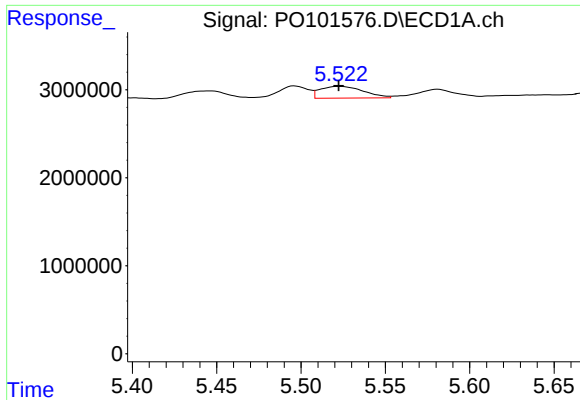

#13 AR-1232-3


R.T.: 5.523 min
Delta R.T.: 0.000 min
Response: 2398474
Conc: 35.83 ng/ml

Instrument :
FID_E
ClientSampleId :

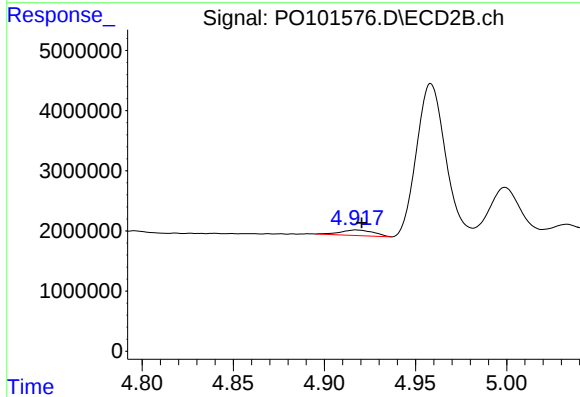


#13 AR-1232-3

R.T.: 4.918 min
Delta R.T.: -0.003 min
Response: 1176934
Conc: 44.89 ng/ml

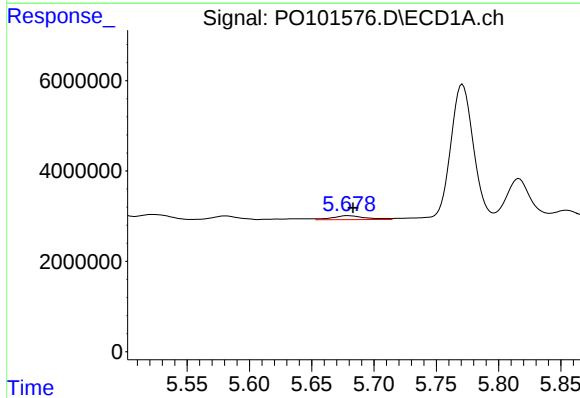


#14 AR-1232-4

R.T.: 5.679 min
Delta R.T.: -0.004 min
Response: 1589166
Conc: 44.39 ng/ml

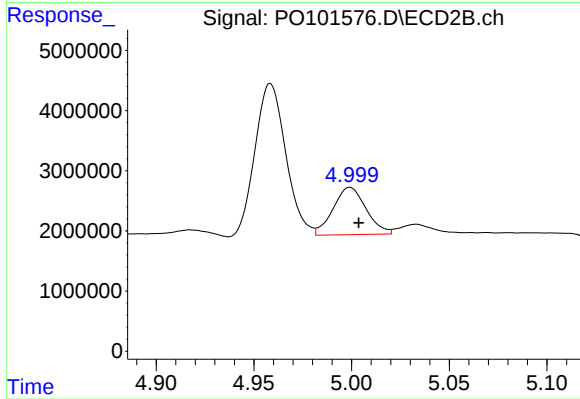

#14 AR-1232-4


R.T.: 4.999 min
Delta R.T.: -0.004 min
Response: 9262571
Conc: 332.62 ng/ml

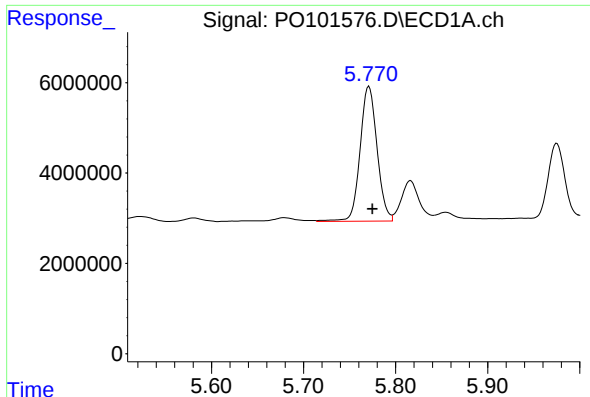

#15 AR-1232-5


R.T.: 5.771 min
Delta R.T.: -0.004 min
Response: 38189137
Conc: 1119.37 ng/ml

Instrument :
FID_E
ClientSampleId :

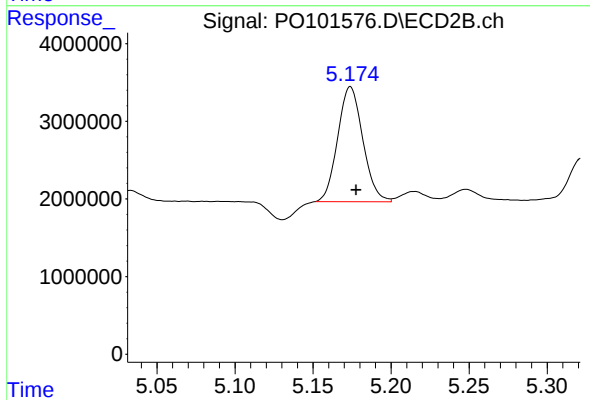


#15 AR-1232-5

R.T.: 5.174 min
Delta R.T.: -0.004 min
Response: 16612414
Conc: 543.26 ng/ml

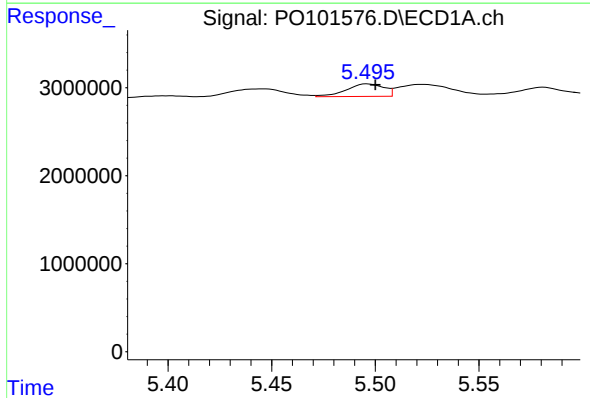


#16 AR-1242-1

R.T.: 5.496 min
Delta R.T.: -0.004 min
Response: 1794048
Conc: 23.19 ng/ml

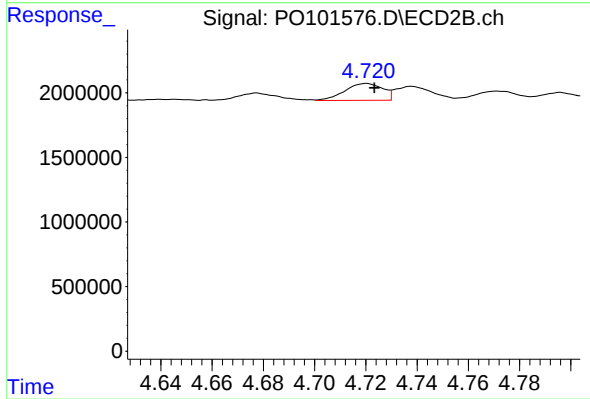

#16 AR-1242-1


R.T.: 4.720 min
Delta R.T.: -0.003 min
Response: 1337060
Conc: 22.73 ng/ml

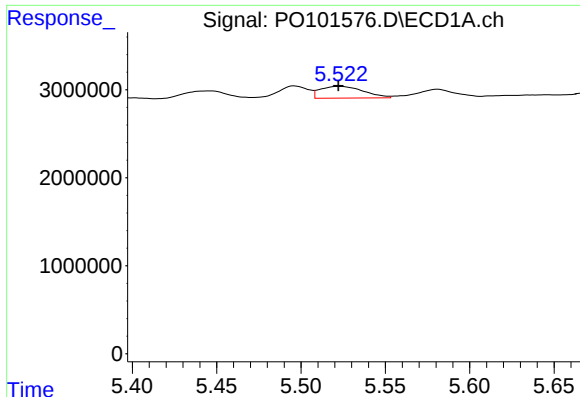

#17 AR-1242-2


R.T.: 5.523 min
Delta R.T.: 0.000 min
Response: 2398474
Conc: 22.15 ng/ml

Instrument :
FID_E
ClientSampleId :

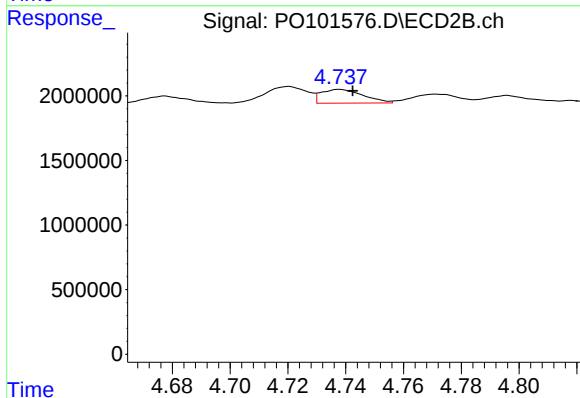


#17 AR-1242-2

R.T.: 4.738 min
Delta R.T.: -0.005 min
Response: 1072708
Conc: 13.83 ng/ml

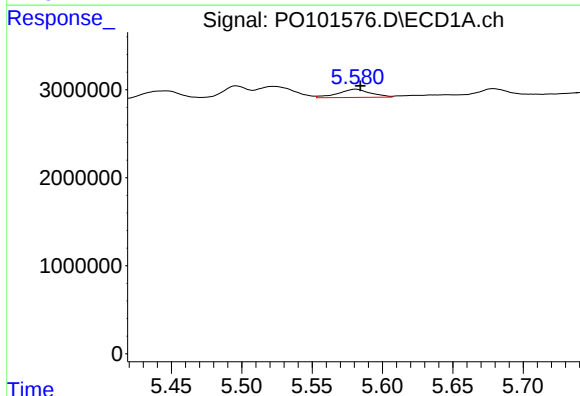


#18 AR-1242-3

R.T.: 5.581 min
Delta R.T.: -0.003 min
Response: 1519099
Conc: 21.37 ng/ml

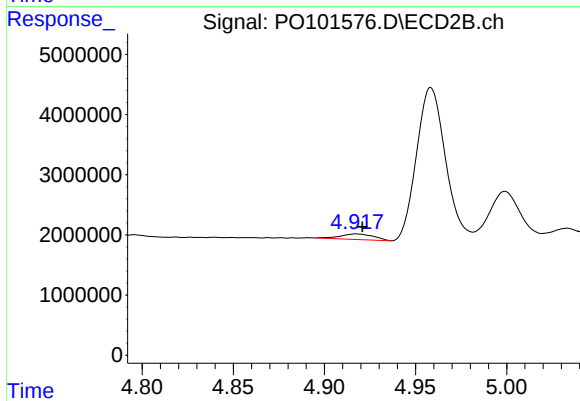

#18 AR-1242-3


R.T.: 4.918 min
Delta R.T.: -0.003 min
Response: 1176934
Conc: 27.15 ng/ml

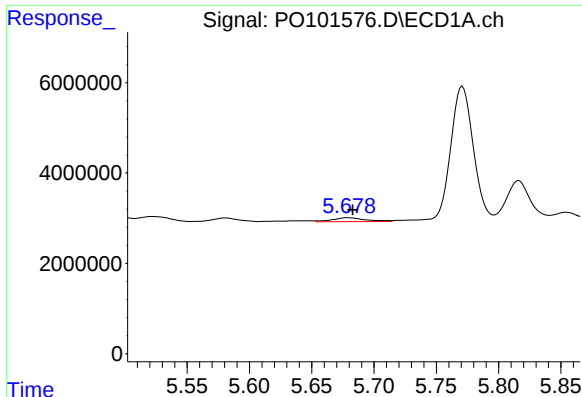

#19 AR-1242-4


R.T.: 5.679 min
Delta R.T.: -0.004 min
Response: 1589166
Conc: 27.90 ng/ml

Instrument :
FID_E
ClientSampleId :

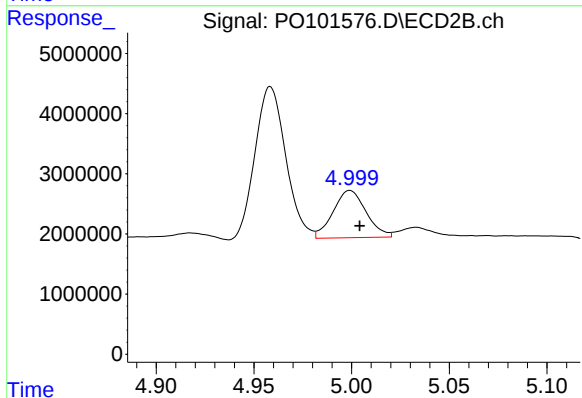


#19 AR-1242-4

R.T.: 4.999 min
Delta R.T.: -0.005 min
Response: 9262571
Conc: 186.09 ng/ml

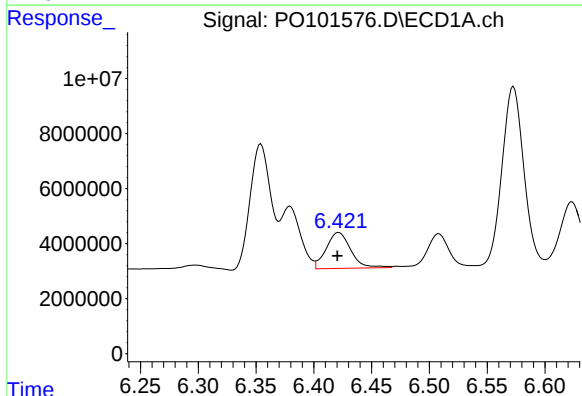


#20 AR-1242-5

R.T.: 6.422 min
Delta R.T.: 0.001 min
Response: 19323604
Conc: 360.09 ng/ml

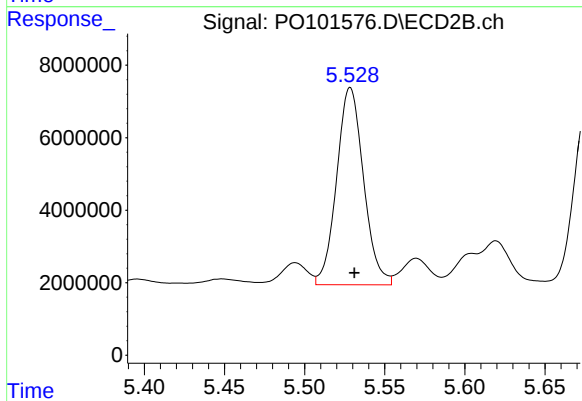

#20 AR-1242-5


R.T.: 5.529 min
Delta R.T.: -0.003 min
Response: 63699576
Conc: 1202.49 ng/ml

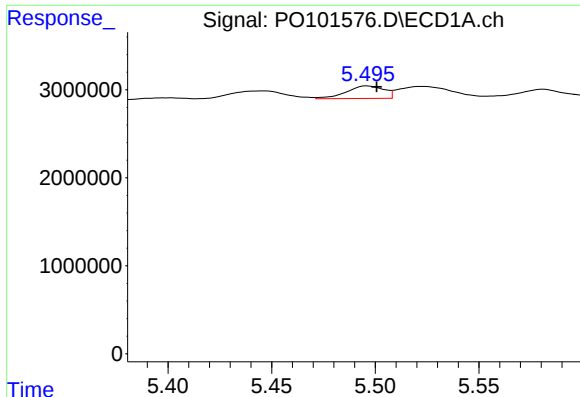

#21 AR-1248-1


R.T.: 5.496 min
Delta R.T.: -0.005 min
Response: 1794048
Conc: 30.95 ng/ml

Instrument :
FID_E
ClientSampleId :

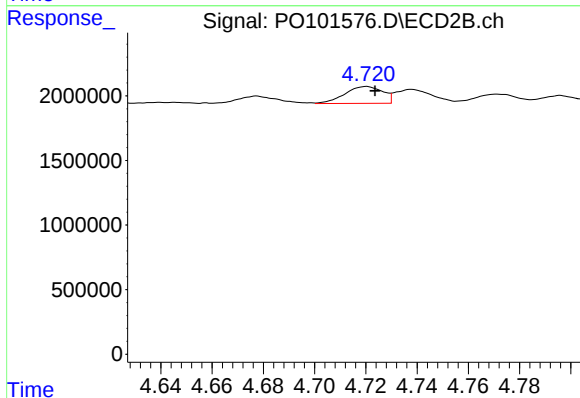


#21 AR-1248-1

R.T.: 4.720 min
Delta R.T.: -0.003 min
Response: 1337060
Conc: 29.88 ng/ml

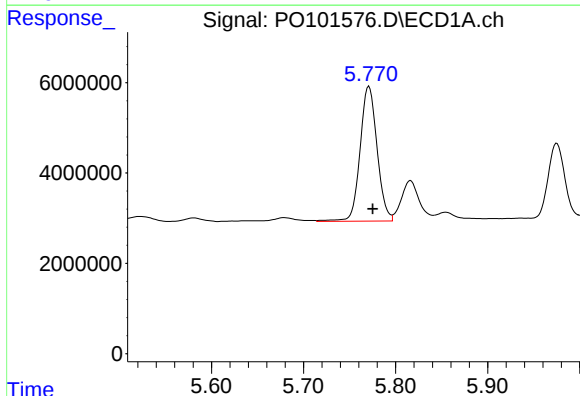


#22 AR-1248-2

R.T.: 5.771 min
Delta R.T.: -0.004 min
Response: 38189137
Conc: 379.21 ng/ml

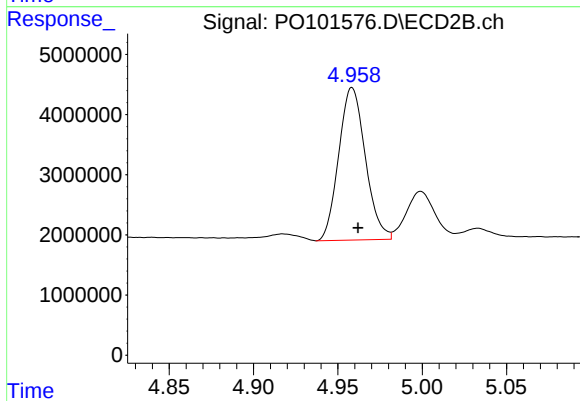

#22 AR-1248-2


R.T.: 4.958 min
Delta R.T.: -0.004 min
Response: 27889103
Conc: 396.65 ng/ml

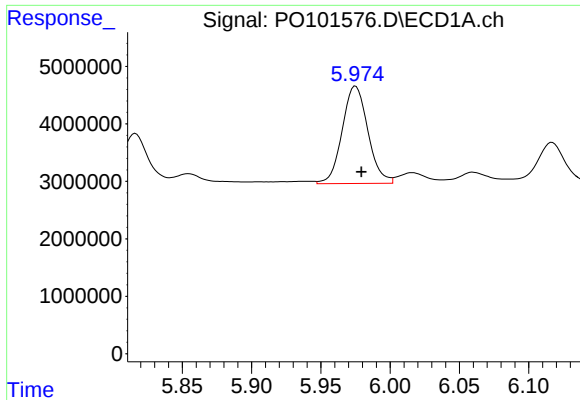

#23 AR-1248-3


R.T.: 5.975 min
Delta R.T.: -0.004 min
Response: 21922463
Conc: 211.58 ng/ml

Instrument :
FID_E
ClientSampleId :

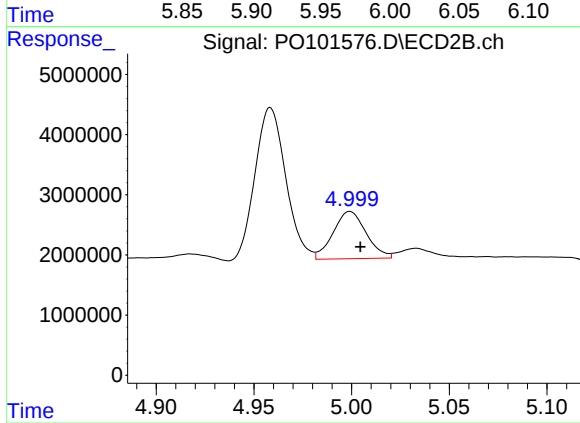


#23 AR-1248-3

R.T.: 4.999 min
Delta R.T.: -0.005 min
Response: 9262571
Conc: 127.35 ng/ml

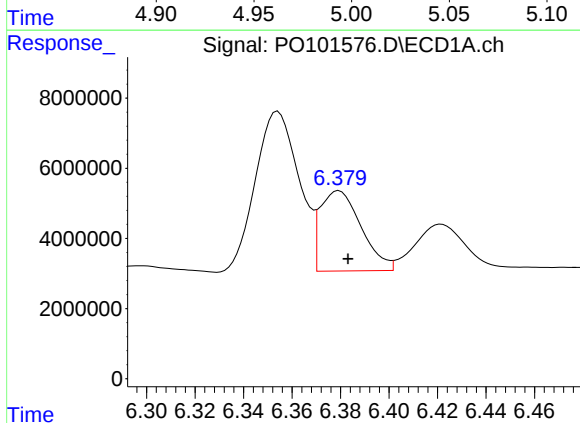


#24 AR-1248-4

R.T.: 6.379 min
Delta R.T.: -0.004 min
Response: 26855622
Conc: 295.73 ng/ml

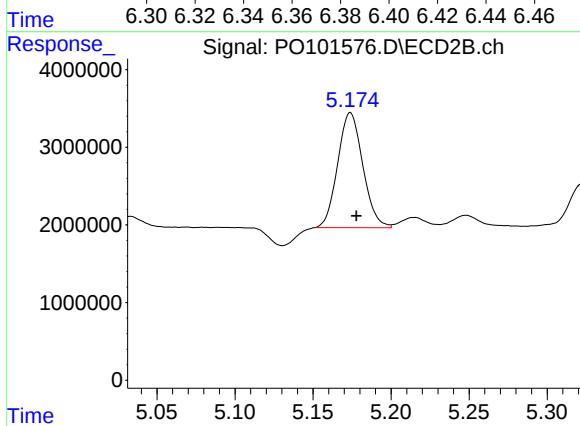

#24 AR-1248-4


R.T.: 5.174 min
Delta R.T.: -0.004 min
Response: 16612414
Conc: 195.41 ng/ml

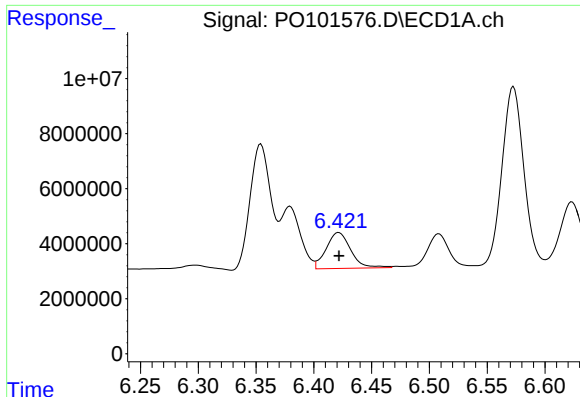

#25 AR-1248-5


R.T.: 6.422 min
Delta R.T.: 0.000 min
Response: 19323604
Conc: 216.64 ng/ml

Instrument :
FID_E
ClientSampleId :

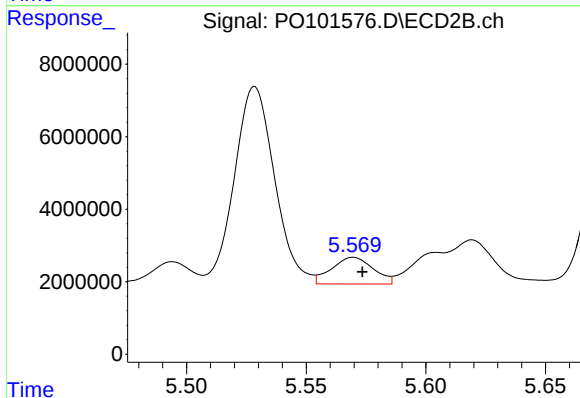


#25 AR-1248-5

R.T.: 5.570 min
Delta R.T.: -0.004 min
Response: 8911383
Conc: 130.15 ng/ml

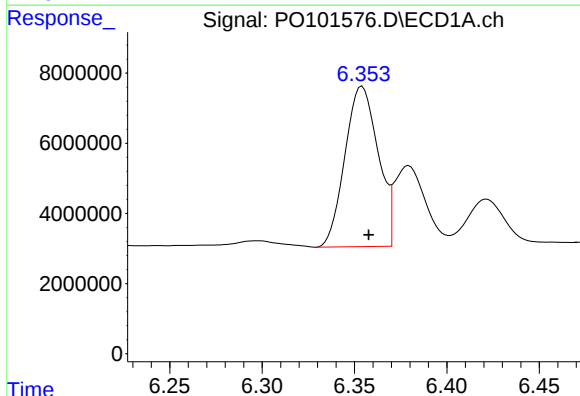


#26 AR-1254-1

R.T.: 6.354 min
Delta R.T.: -0.004 min
Response: 57118299
Conc: 480.07 ng/ml

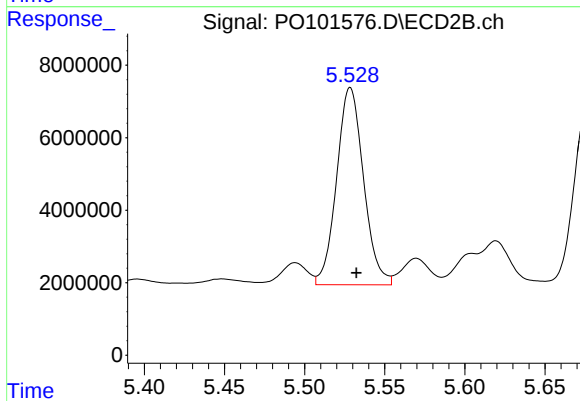

#26 AR-1254-1


R.T.: 5.529 min
Delta R.T.: -0.004 min
Response: 63699576
Conc: 512.01 ng/ml

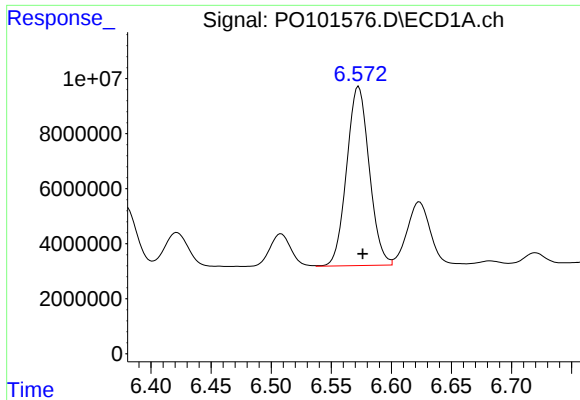

#27 AR-1254-2


R.T.: 6.573 min
Delta R.T.: -0.003 min
Response: 85001469
Conc: 499.07 ng/ml

Instrument :
FID_E
ClientSampleId :

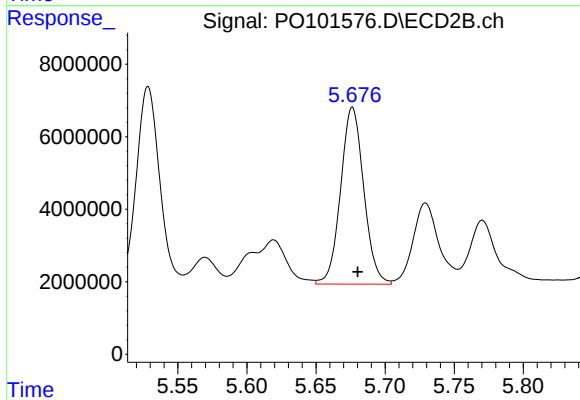


#27 AR-1254-2

R.T.: 5.676 min
Delta R.T.: -0.004 min
Response: 56932617
Conc: 508.61 ng/ml

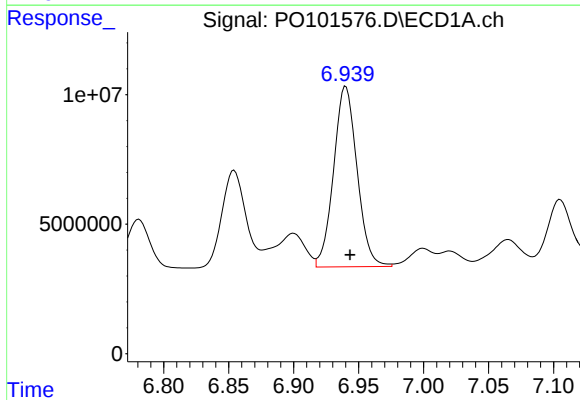


#28 AR-1254-3

R.T.: 6.940 min
Delta R.T.: -0.003 min
Response: 87511073
Conc: 532.88 ng/ml

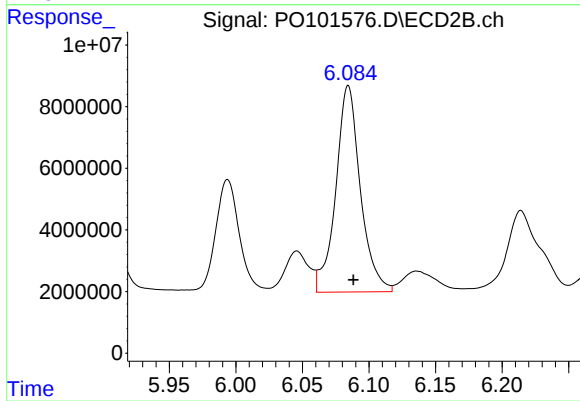

#28 AR-1254-3


R.T.: 6.084 min
Delta R.T.: -0.004 min
Response: 86152766
Conc: 517.77 ng/ml

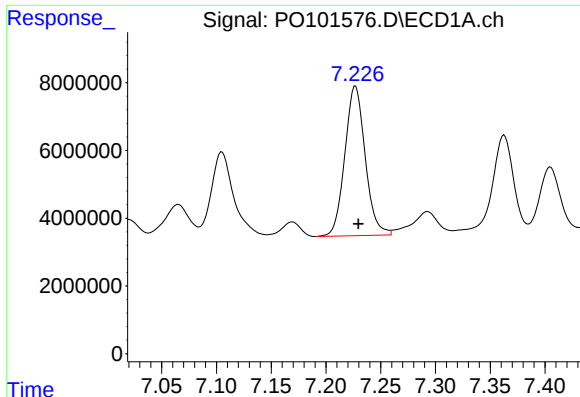

#29 AR-1254-4


R.T.: 7.227 min
Delta R.T.: -0.003 min
Response: 57147459
Conc: 571.75 ng/ml

Instrument :
FID_E
ClientSampleId :

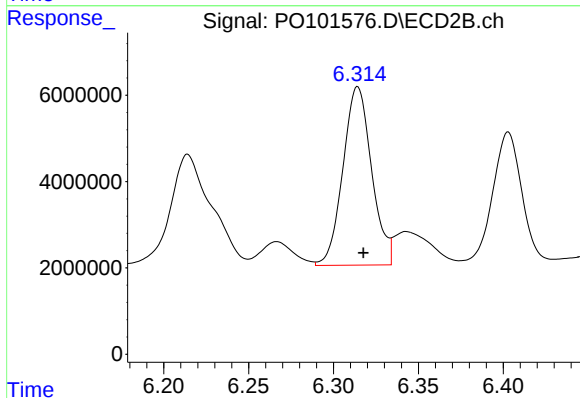


#29 AR-1254-4

R.T.: 6.314 min
Delta R.T.: -0.003 min
Response: 48571395
Conc: 569.44 ng/ml

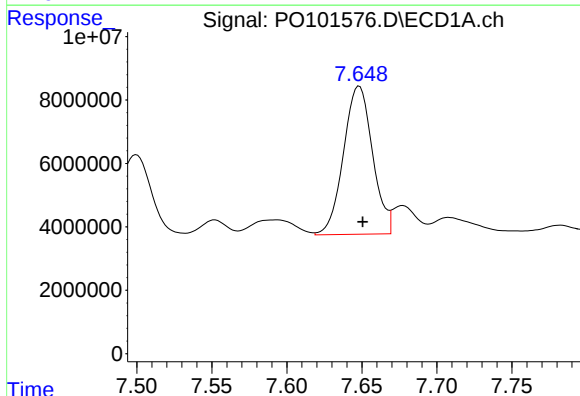


#30 AR-1254-5

R.T.: 7.648 min
Delta R.T.: -0.002 min
Response: 62921771
Conc: 535.37 ng/ml

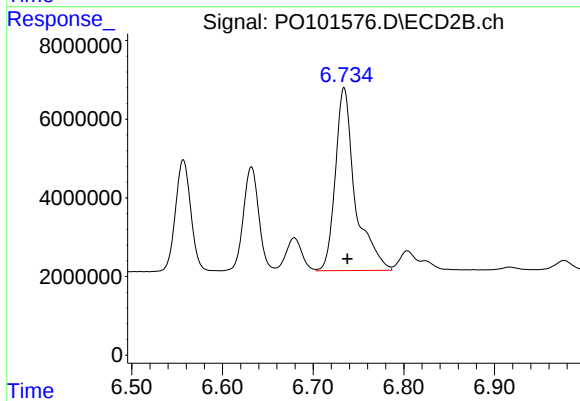

#30 AR-1254-5


R.T.: 6.734 min
Delta R.T.: -0.004 min
Response: 70563552
Conc: 520.77 ng/ml

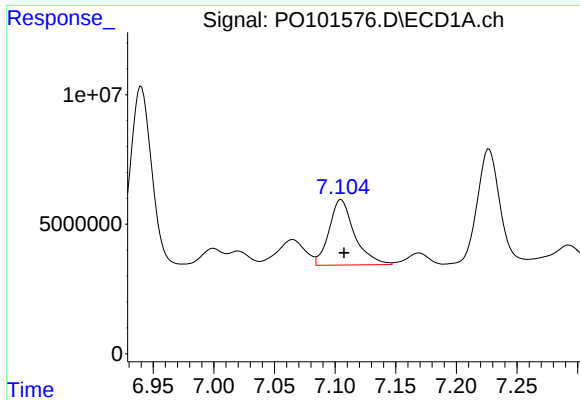

#31 AR-1260-1


R.T.: 7.105 min
Delta R.T.: -0.002 min
Response: 36847836
Conc: 258.38 ng/ml

Instrument :
FID_E
ClientSampleId :

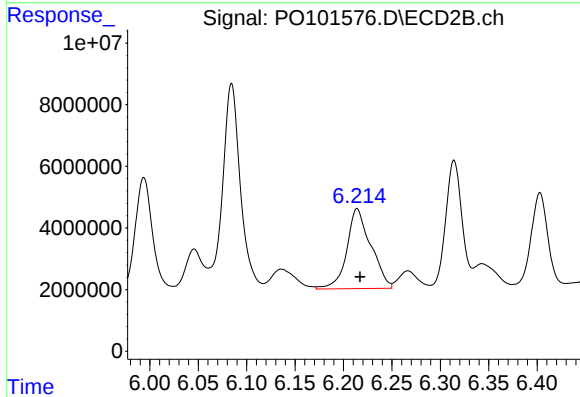


#31 AR-1260-1

R.T.: 6.214 min
Delta R.T.: -0.003 min
Response: 44915249
Conc: 364.00 ng/ml

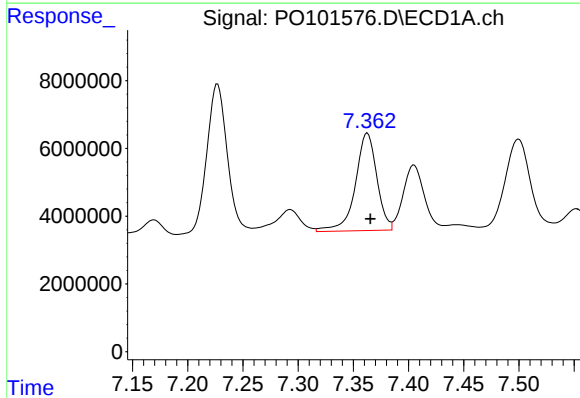


#32 AR-1260-2

R.T.: 7.363 min
Delta R.T.: -0.003 min
Response: 39077335
Conc: 266.77 ng/ml

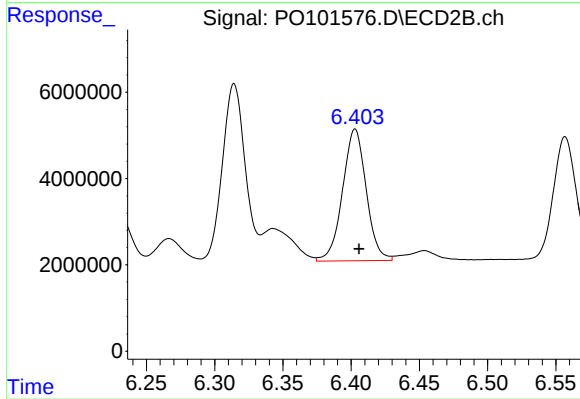

#32 AR-1260-2


R.T.: 6.403 min
Delta R.T.: -0.003 min
Response: 36819131
Conc: 269.28 ng/ml

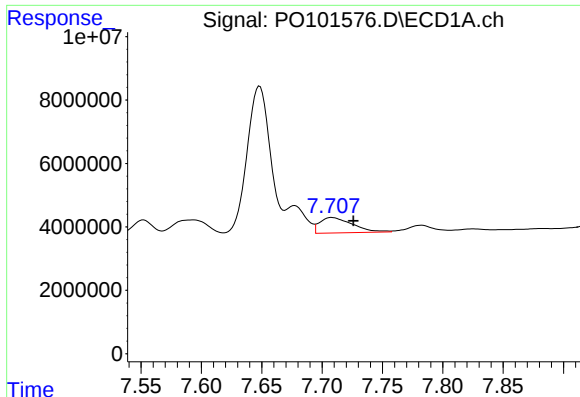

#33 AR-1260-3


R.T.: 7.708 min
Delta R.T.: -0.018 min
Response: 9190084
Conc: 78.70 ng/ml

Instrument :
FID_E
ClientSampleId :

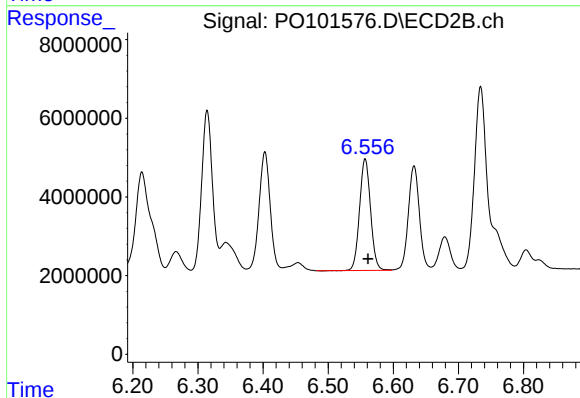


#33 AR-1260-3

R.T.: 6.557 min
Delta R.T.: -0.005 min
Response: 33218359
Conc: 258.94 ng/ml

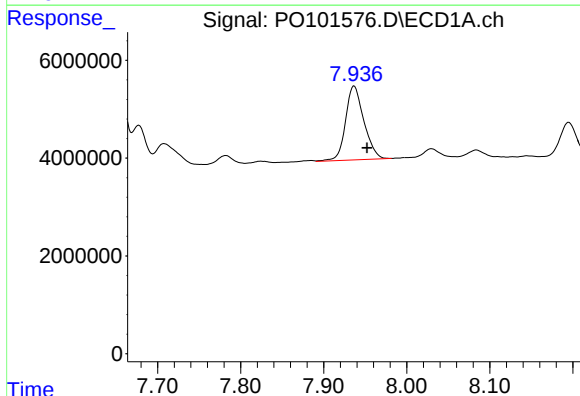


#34 AR-1260-4

R.T.: 7.937 min
Delta R.T.: -0.016 min
Response: 23185746
Conc: 196.94 ng/ml

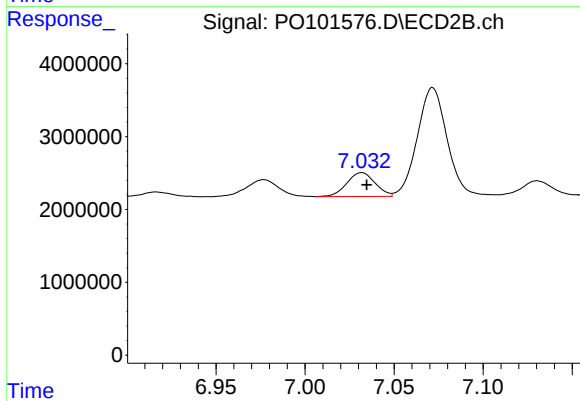

#34 AR-1260-4


R.T.: 7.032 min
Delta R.T.: -0.003 min
Response: 3614419
Conc: 34.97 ng/ml

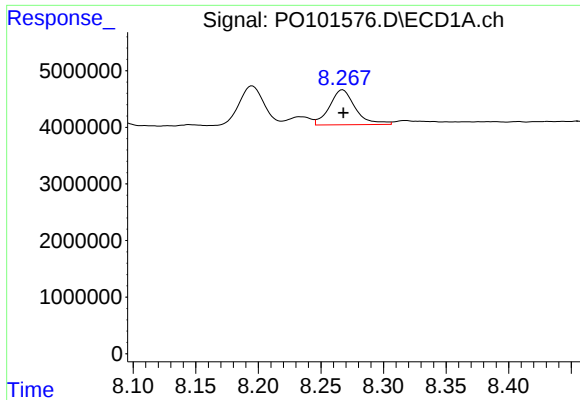

#35 AR-1260-5


R.T.: 8.267 min
Delta R.T.: 0.000 min
Response: 8875300
Conc: 40.47 ng/ml

Instrument :
FID_E
ClientSampleId :

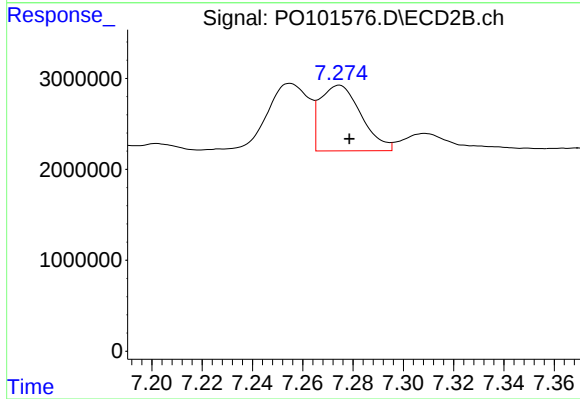


#35 AR-1260-5

R.T.: 7.274 min
Delta R.T.: -0.004 min
Response: 8169842
Conc: 38.92 ng/ml

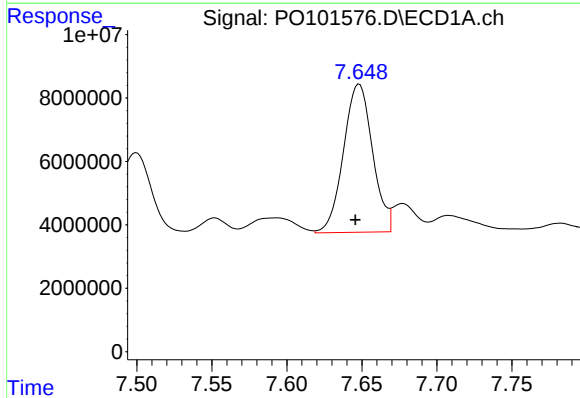


#36 AR-1262-1

R.T.: 7.648 min
Delta R.T.: 0.003 min
Response: 62921771
Conc: 563.04 ng/ml

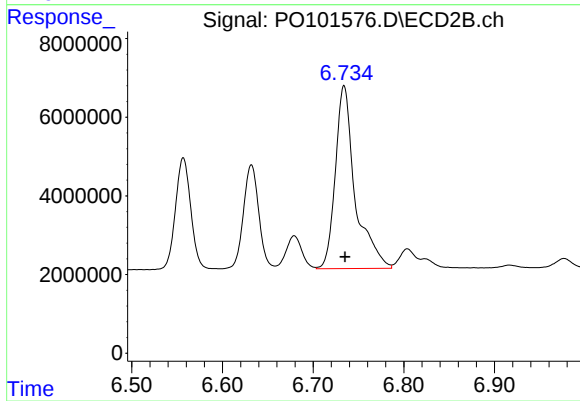

#36 AR-1262-1


R.T.: 6.734 min
Delta R.T.: -0.001 min
Response: 70563552
Conc: 870.42 ng/ml

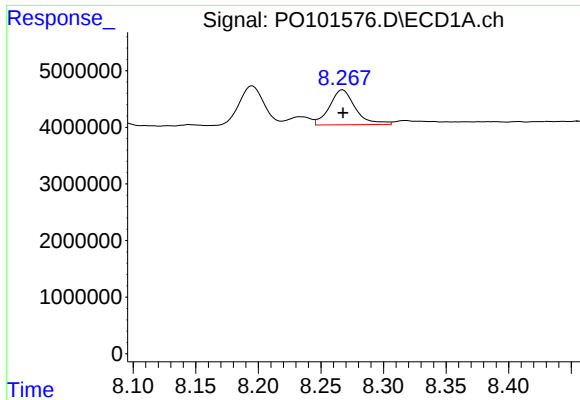

#37 AR-1262-2


R.T.: 8.267 min
Delta R.T.: 0.000 min
Response: 8875300
Conc: 32.62 ng/ml

Instrument :
FID_E
ClientSampleId :

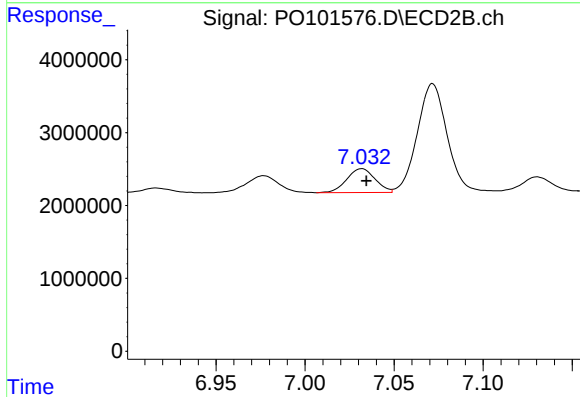


#37 AR-1262-2

R.T.: 7.032 min
Delta R.T.: -0.003 min
Response: 3614419
Conc: 24.29 ng/ml

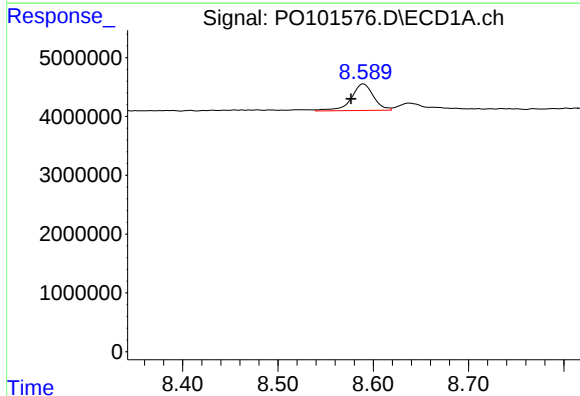


#38 AR-1262-3

R.T.: 8.590 min
Delta R.T.: 0.013 min
Response: 7325270
Conc: 37.66 ng/ml

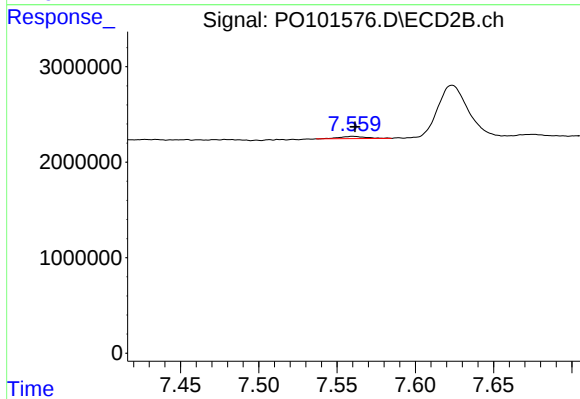

#38 AR-1262-3


R.T.: 7.560 min
Delta R.T.: -0.001 min
Response: 279234
Conc: 2.72 ng/ml

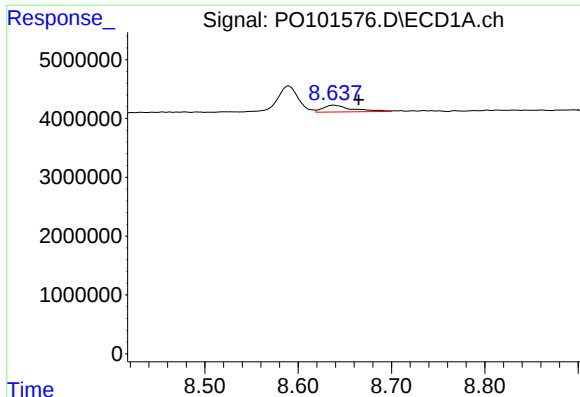

#39 AR-1262-4


R.T.: 8.638 min
Delta R.T.: -0.027 min
Response: 2486796
Conc: 16.02 ng/ml

Instrument :
FID_E
ClientSampleId :

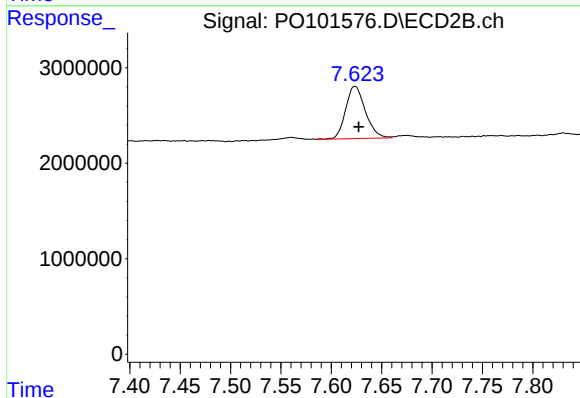


#39 AR-1262-4

R.T.: 7.624 min
Delta R.T.: -0.004 min
Response: 7448751
Conc: 38.15 ng/ml

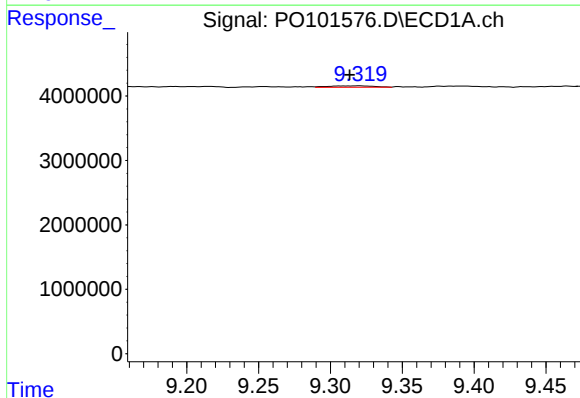


#40 AR-1262-5

R.T.: 9.320 min
Delta R.T.: 0.006 min
Response: 459522
Conc: 4.89 ng/ml

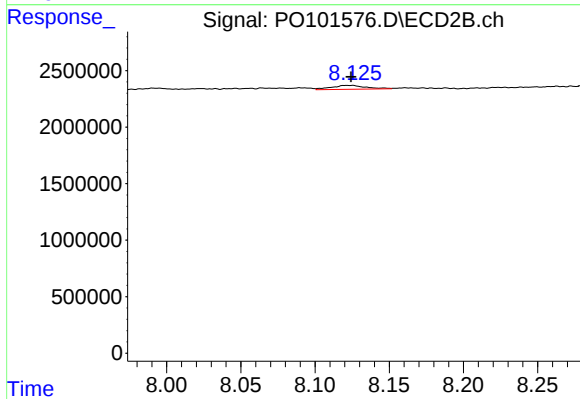

#40 AR-1262-5


R.T.: 8.124 min
Delta R.T.: 0.000 min
Response: 559124
Conc: 6.67 ng/ml

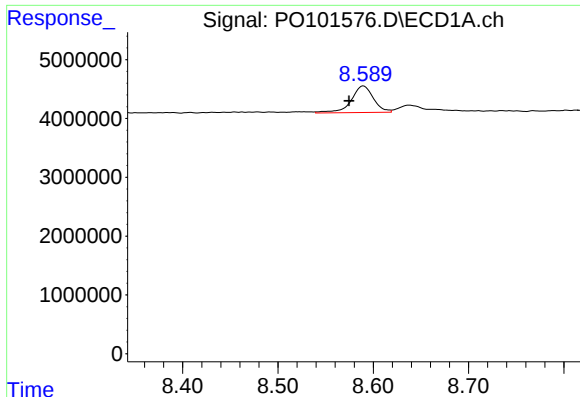

#41 AR-1268-1


R.T.: 8.590 min
Delta R.T.: 0.015 min
Response: 7325270
Conc: 23.10 ng/ml

Instrument :
FID_E
ClientSampleId :

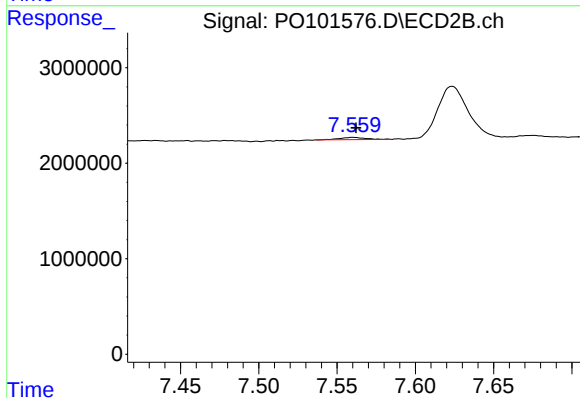


#41 AR-1268-1

R.T.: 7.560 min
Delta R.T.: -0.002 min
Response: 279234
Conc: 1.00 ng/ml

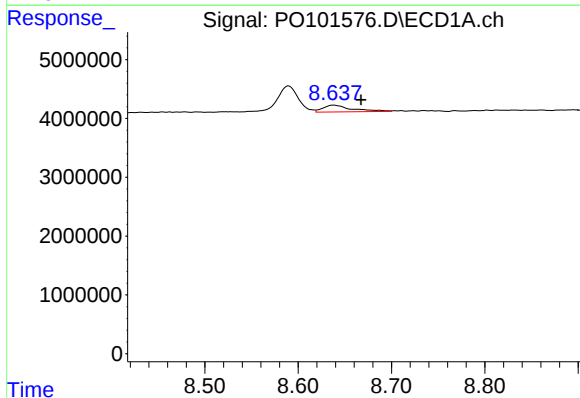


#42 AR-1268-2

R.T.: 8.638 min
Delta R.T.: -0.030 min
Response: 2486796
Conc: 8.61 ng/ml

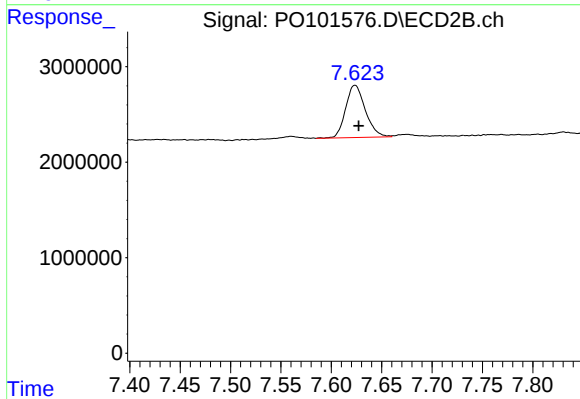

#42 AR-1268-2


R.T.: 7.624 min
Delta R.T.: -0.004 min
Response: 7448751
Conc: 29.13 ng/ml

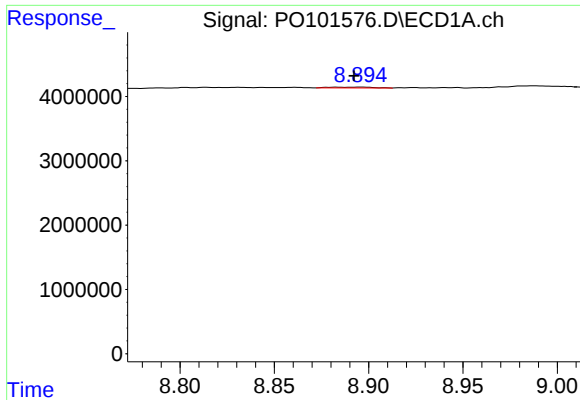

#43 AR-1268-3


R.T.: 8.895 min
Delta R.T.: 0.003 min
Response: 192989
Conc: 0.75 ng/ml

Instrument :
FID_E
ClientSampleId :

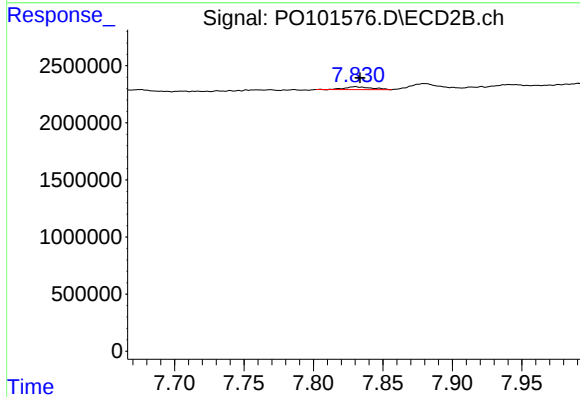


#43 AR-1268-3

R.T.: 7.830 min
Delta R.T.: -0.003 min
Response: 349964
Conc: 1.50 ng/ml

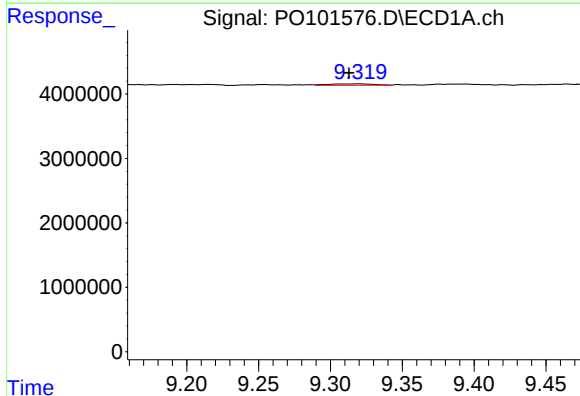


#44 AR-1268-4

R.T.: 9.320 min
Delta R.T.: 0.007 min
Response: 459522
Conc: 5.00 ng/ml

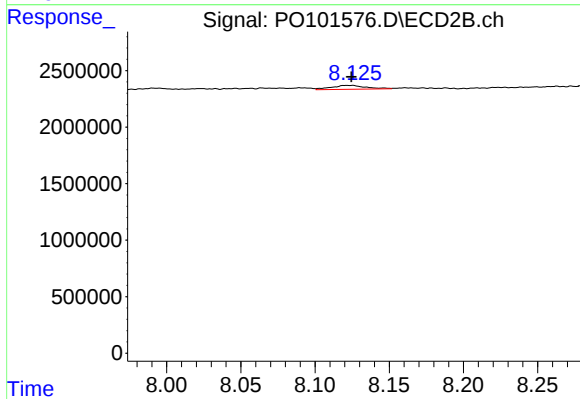

#44 AR-1268-4


R.T.: 8.124 min
Delta R.T.: 0.000 min
Response: 559124
Conc: 6.58 ng/ml

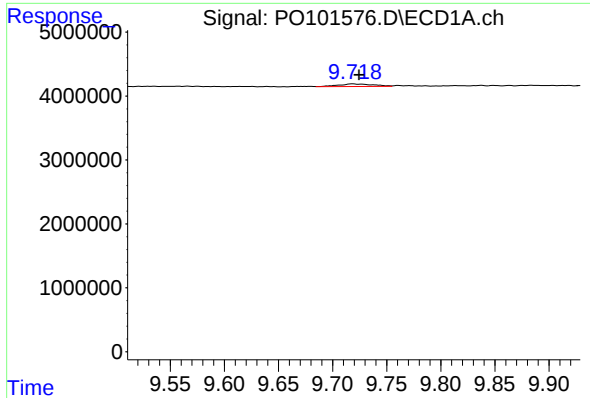

#45 AR-1268-5

R.T.: 9.719 min
Delta R.T.: -0.006 min
Response: 920830
Conc: 1.15 ng/ml

Instrument :
FID_E
ClientSampleId :

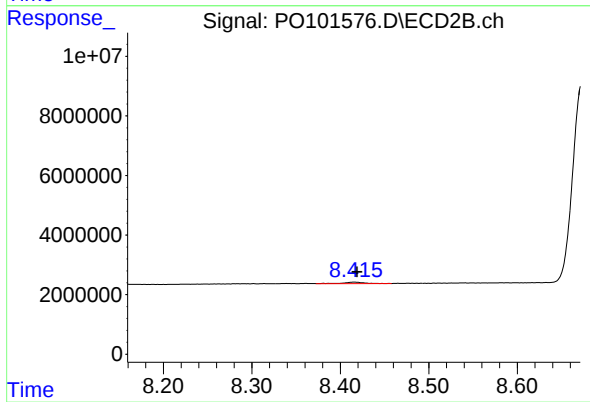

#45 AR-1268-5

R.T.: 8.416 min
Delta R.T.: -0.003 min
Response: 781485
Conc: 1.19 ng/ml