

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0020224\
 Data File : P0101577.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Feb 2024 10:30
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 11:44:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0012424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 24 04:51:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.337	3.630	77254450	51110922	20.126	19.777
2)	SA Decachlor...	10.067	8.677	48520955	40105151	20.823	21.164
Target Compounds							
3)	L1 AR-1016-1	5.500	4.729	1215231	1127706	12.432	15.254
4)	L1 AR-1016-2	5.519	4.729	414850	1127706	3.016	11.442 #
5)	L1 AR-1016-3	5.580	4.922	3892274	874372	43.388	15.938 #
6)	L1 AR-1016-4	5.689	4.968	902335	2008049	12.625	39.514 #
7)	L1 AR-1016-5	5.964	5.172	856033	445775	10.830	6.828 #
8)	L2 AR-1221-1	4.545	3.855	619034	182827	14.785	6.384 #
9)	L2 AR-1221-2	4.644	3.933	1754337	1005825	55.294	44.973
10)	L2 AR-1221-3	4.703	4.004	248014	87988	2.801	1.384 #
11)	L3 AR-1232-1	4.703	4.004	248014	87988	3.280	1.613 #
12)	L3 AR-1232-2	5.229	4.729	159097	1127706	3.501	23.452 #
13)	L3 AR-1232-3	5.519	4.922	414850	874372	6.197	33.347 #
14)	L3 AR-1232-4	5.689	4.997	902335	804964	25.206	28.906
15)	L3 AR-1232-5	5.780	5.172	3853176	445775	112.941	14.578 #
16)	L4 AR-1242-1	5.500	4.729	1215231	1127706	15.706	19.167
17)	L4 AR-1242-2	5.519	4.729	414850	1127706	3.831	14.543 #
18)	L4 AR-1242-3	5.580	4.922	3892274	874372	54.759	20.170 #
19)	L4 AR-1242-4	5.689	4.997	902335	804964	15.843	16.172
20)	L4 AR-1242-5	6.431	5.556	3382568	5787339	63.033	109.251 #
21)	L5 AR-1248-1	5.500	4.729	1215231	1127706	20.966	25.203
22)	L5 AR-1248-2	5.780	4.968	3853176	2008049	38.261	28.559 #
23)	L5 AR-1248-3	5.964	4.997	856033	804964	8.262	11.067 #
24)	L5 AR-1248-4	6.393	5.172	1575623	445775	17.351	5.244 #
25)	L5 AR-1248-5	6.431	5.588	3382568	2033062	37.923	29.693
26)	L6 AR-1254-1	6.365	5.556	3922395	5787339	32.967	46.518 #
27)	L6 AR-1254-2	6.583	5.680	881871	3221374	5.178	28.778 #
28)	L6 AR-1254-3	6.953	6.064	4518412	1846142	27.514	11.095 #
29)	L6 AR-1254-4	7.262	6.321	4927358	1186382	49.297	13.909 #
30)	L6 AR-1254-5	7.651	6.740	180017	195901	1.532	1.446
31)	L7 AR-1260-1	7.125	6.220	5773623	2262753	40.485	18.338 #
32)	L7 AR-1260-2	7.393	6.397	3585208	2781512	24.475	20.343
33)	L7 AR-1260-3	7.721	6.541	469943	626873	4.025	4.887
34)	L7 AR-1260-4	7.915f	7.031	1267186	111386	10.764	1.078 #
35)	L7 AR-1260-5	8.243	7.283	73211	747736	0.334	3.562 #
36)	L8 AR-1262-1	7.651	6.740	180017	195901	1.611	2.416 #
37)	L8 AR-1262-2	8.243	7.031	73211	111386	0.269	0.749 #
38)	L8 AR-1262-3	8.580	7.555	358997	168390	1.846	1.639
39)	L8 AR-1262-4	8.671	7.637	125180	126369	0.806	0.647
40)	L8 AR-1262-5	9.311	8.126	50808	340897	0.541	4.068 #
41)	L9 AR-1268-1	8.580	7.555	358997	168390	1.132	0.602 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020224\
 Data File : P0101577.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Feb 2024 10:30
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 11:44:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 24 04:51:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.671	7.637	125180	126369	0.433	0.494
43) L9	AR-1268-3	8.902	7.830	246657	161452	0.957	0.694 #
44) L9	AR-1268-4	9.311	8.126	50808	340897	0.553	4.011 #
45) L9	AR-1268-5	9.723	8.420	191759	626595	0.239	0.952 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO020224\
Data File : PO101577.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Feb 2024 10:30
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 11:44:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO012424.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 24 04:51:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

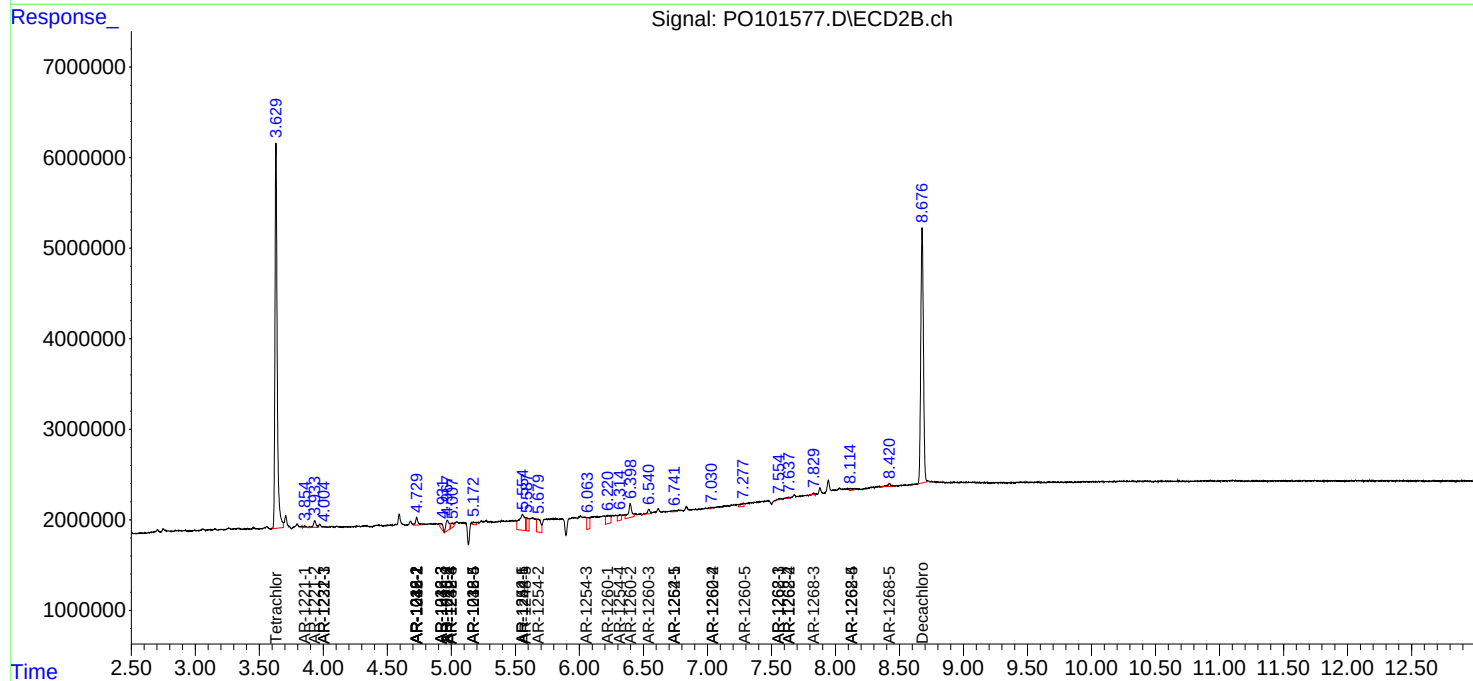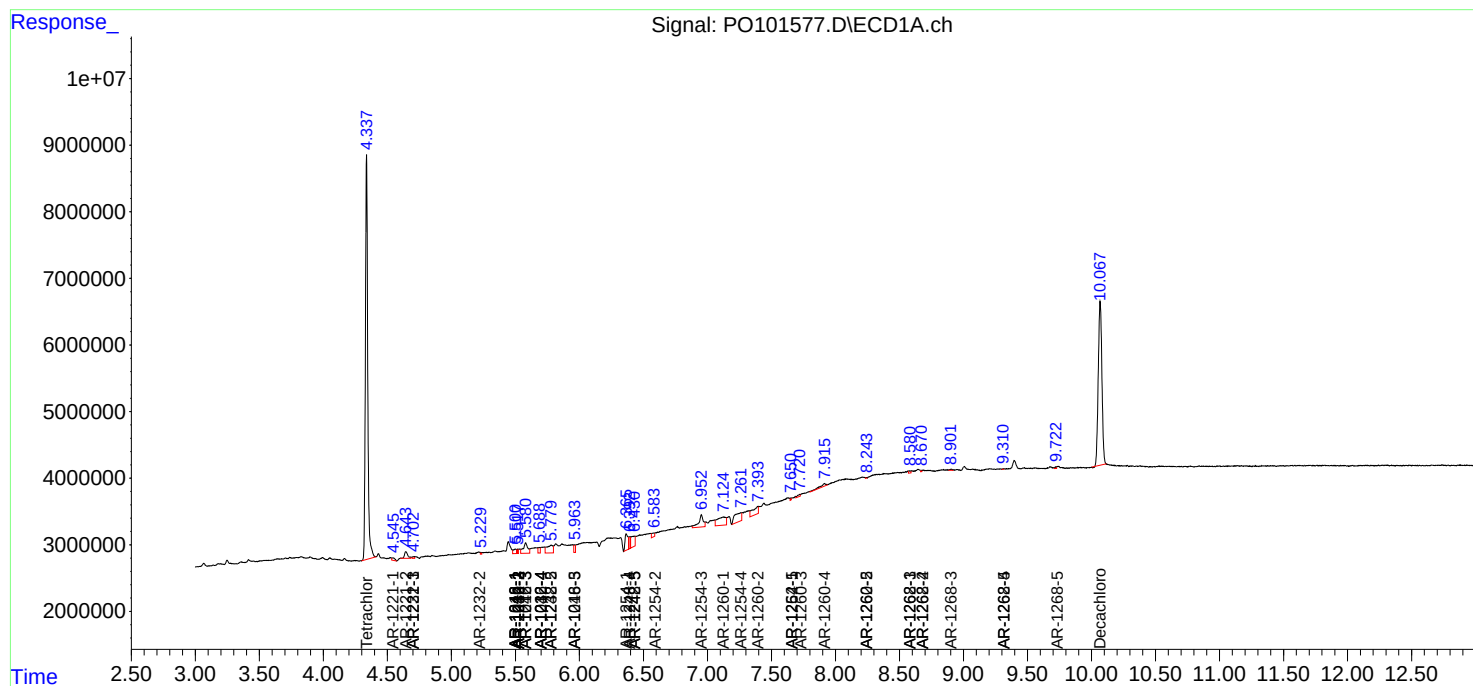


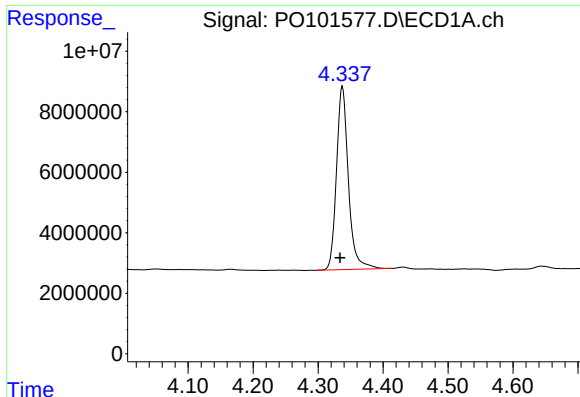

#1 Tetrachloro-m-xylene


R.T.: 4.337 min
Delta R.T.: 0.003 min
Response: 77254450
Conc: 20.13 ng/ml

Instrument :
FID_E
ClientSampleId :

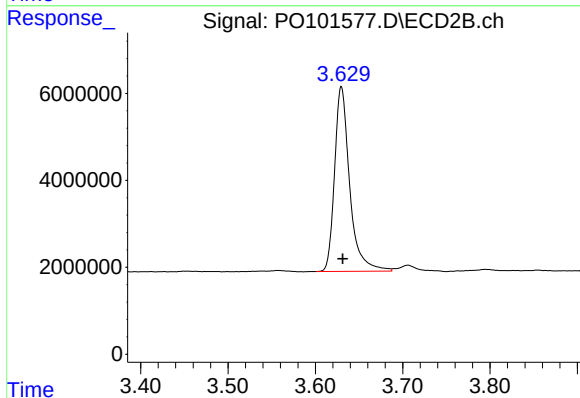


#1 Tetrachloro-m-xylene

R.T.: 3.630 min
Delta R.T.: -0.001 min
Response: 51110922
Conc: 19.78 ng/ml

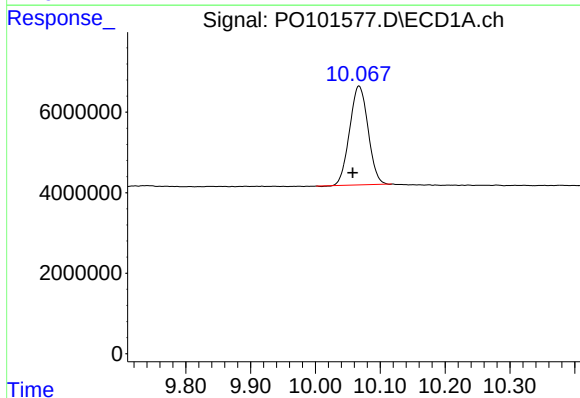


#2 Decachlorobiphenyl

R.T.: 10.067 min
Delta R.T.: 0.010 min
Response: 48520955
Conc: 20.82 ng/ml

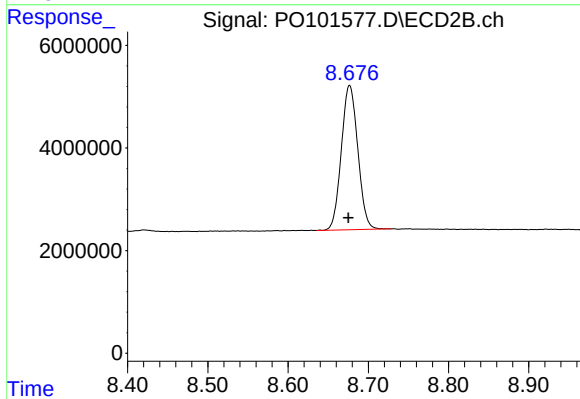

#2 Decachlorobiphenyl


R.T.: 8.677 min
Delta R.T.: 0.002 min
Response: 40105151
Conc: 21.16 ng/ml

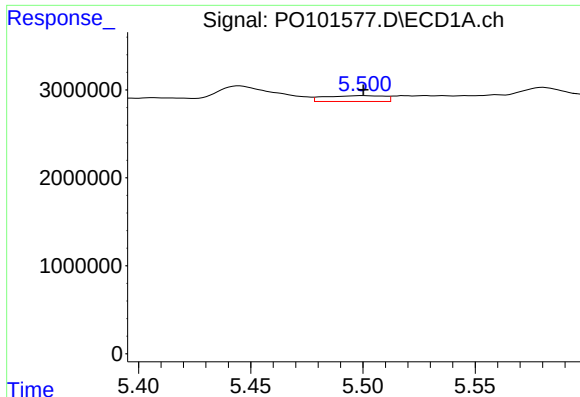

#3 AR-1016-1


R.T.: 5.500 min
Delta R.T.: 0.000 min
Response: 1215231
Conc: 12.43 ng/ml

Instrument :
FID_E
ClientSampleId :

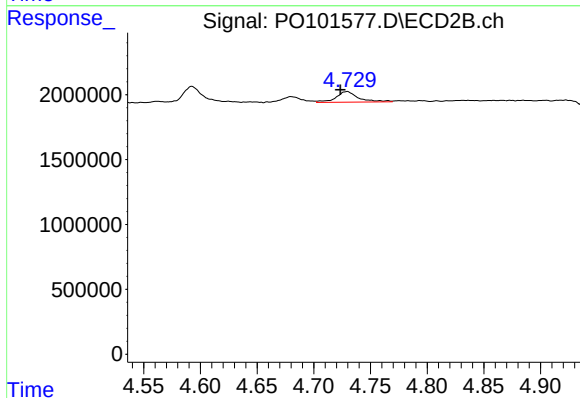


#3 AR-1016-1

R.T.: 4.729 min
Delta R.T.: 0.006 min
Response: 1127706
Conc: 15.25 ng/ml

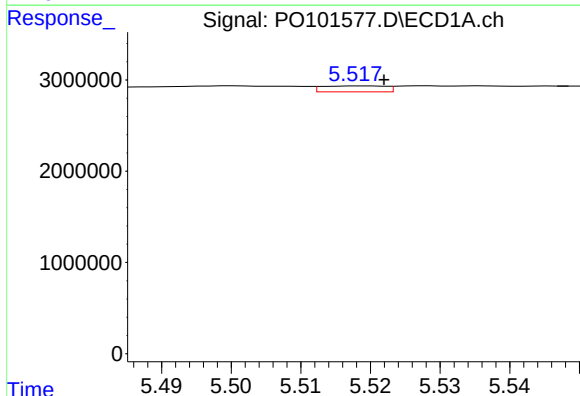


#4 AR-1016-2

R.T.: 5.519 min
Delta R.T.: -0.003 min
Response: 414850
Conc: 3.02 ng/ml

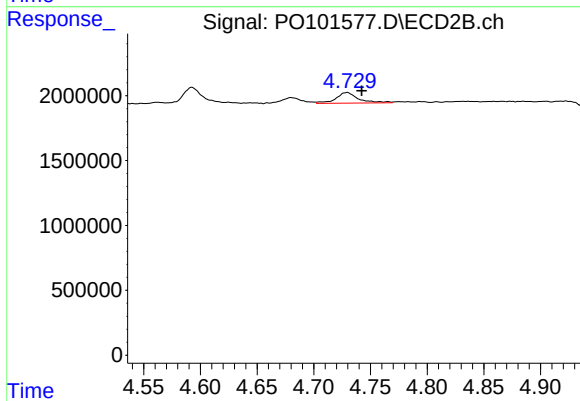

#4 AR-1016-2


R.T.: 4.729 min
Delta R.T.: -0.013 min
Response: 1127706
Conc: 11.44 ng/ml

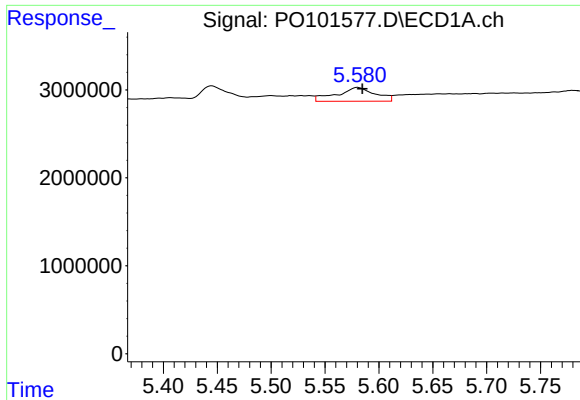

#5 AR-1016-3


R.T.: 5.580 min
Delta R.T.: -0.004 min
Response: 3892274
Conc: 43.39 ng/ml

Instrument :
FID_E
ClientSampleId :

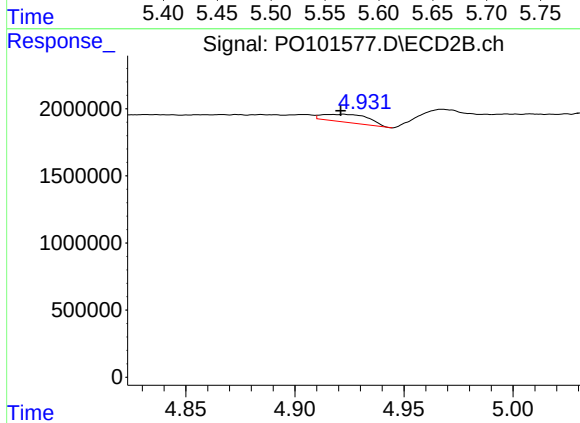


#5 AR-1016-3

R.T.: 4.922 min
Delta R.T.: 0.001 min
Response: 874372
Conc: 15.94 ng/ml

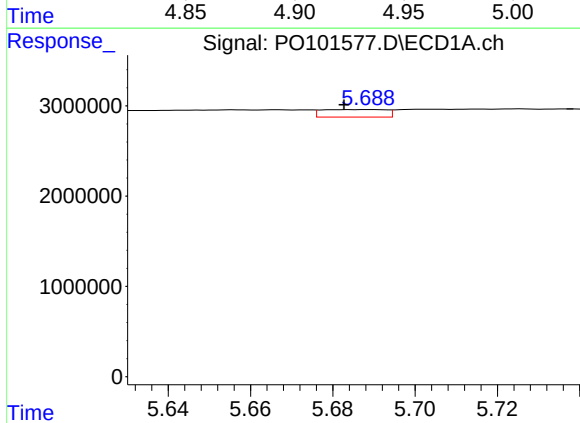


#6 AR-1016-4

R.T.: 5.689 min
Delta R.T.: 0.006 min
Response: 902335
Conc: 12.62 ng/ml

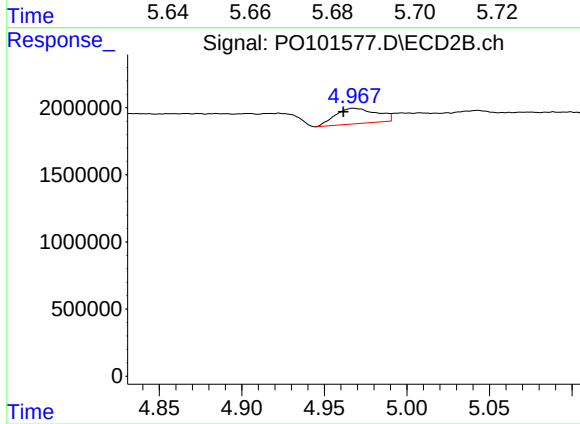

#6 AR-1016-4


R.T.: 4.968 min
Delta R.T.: 0.006 min
Response: 2008049
Conc: 39.51 ng/ml

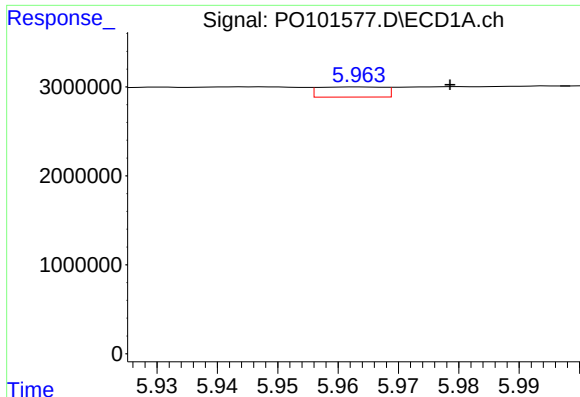

#7 AR-1016-5


R.T.: 5.964 min
Delta R.T.: -0.015 min
Response: 856033
Conc: 10.83 ng/ml

Instrument :
FID_E
ClientSampleId :

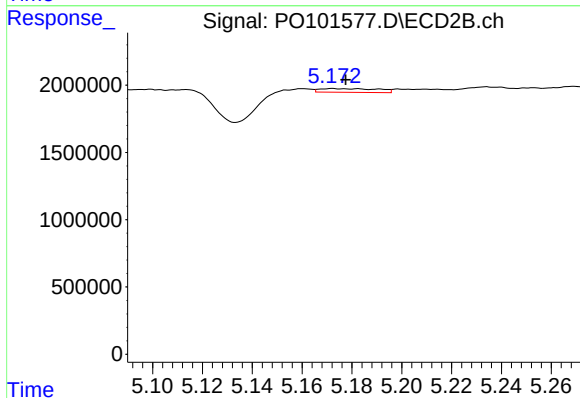


#7 AR-1016-5

R.T.: 5.172 min
Delta R.T.: -0.005 min
Response: 445775
Conc: 6.83 ng/ml

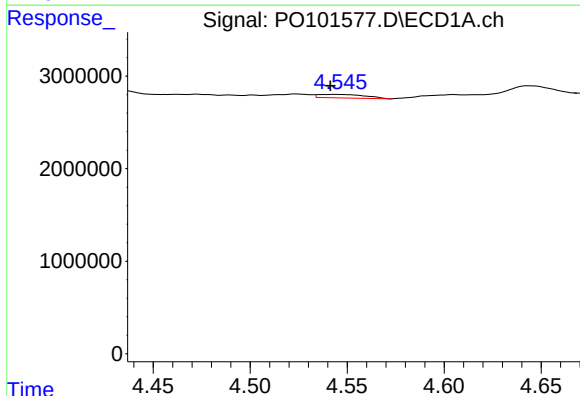


#8 AR-1221-1

R.T.: 4.545 min
Delta R.T.: 0.003 min
Response: 619034
Conc: 14.78 ng/ml

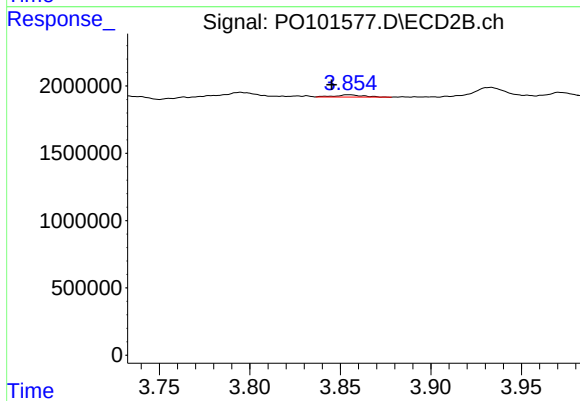

#8 AR-1221-1


R.T.: 3.855 min
Delta R.T.: 0.010 min
Response: 182827
Conc: 6.38 ng/ml

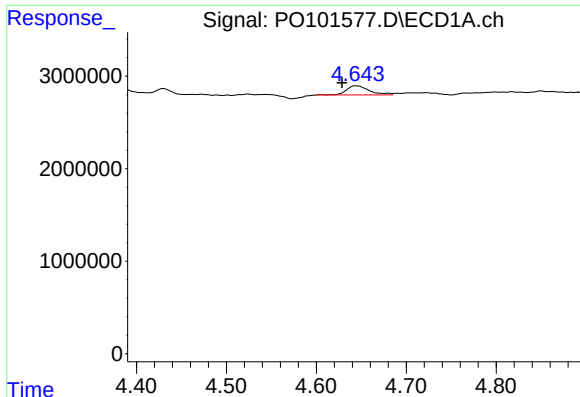

#9 AR-1221-2


R.T.: 4.644 min
Delta R.T.: 0.015 min
Response: 1754337
Conc: 55.29 ng/ml

Instrument :
FID_E
ClientSampleId :

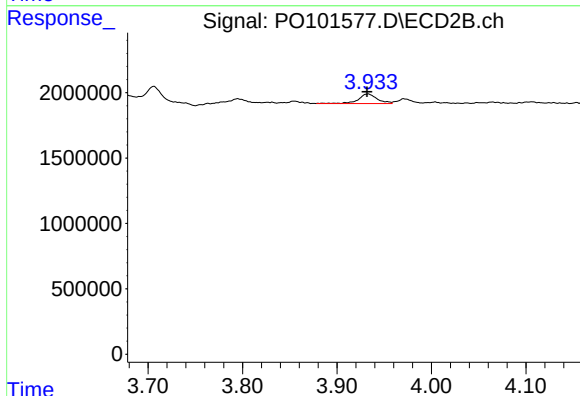


#9 AR-1221-2

R.T.: 3.933 min
Delta R.T.: 0.001 min
Response: 1005825
Conc: 44.97 ng/ml

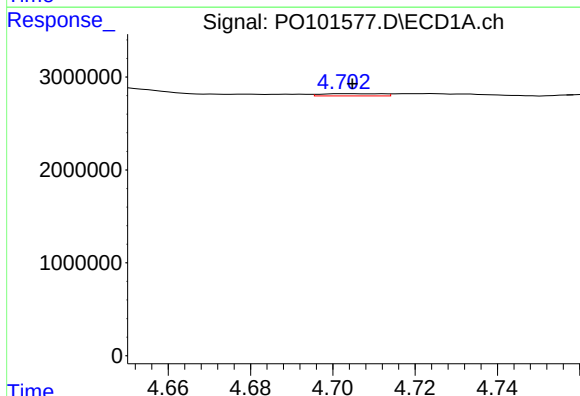


#10 AR-1221-3

R.T.: 4.703 min
Delta R.T.: -0.002 min
Response: 248014
Conc: 2.80 ng/ml

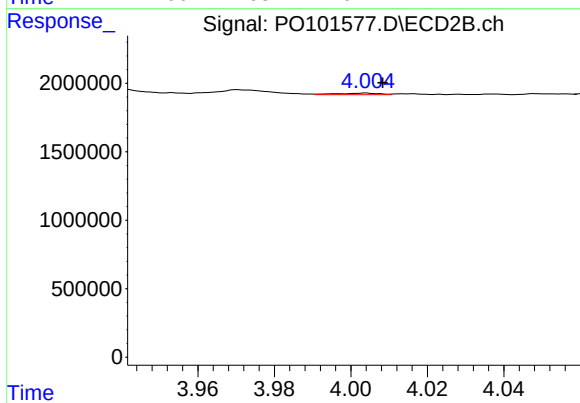

#10 AR-1221-3


R.T.: 4.004 min
Delta R.T.: -0.005 min
Response: 87988
Conc: 1.38 ng/ml

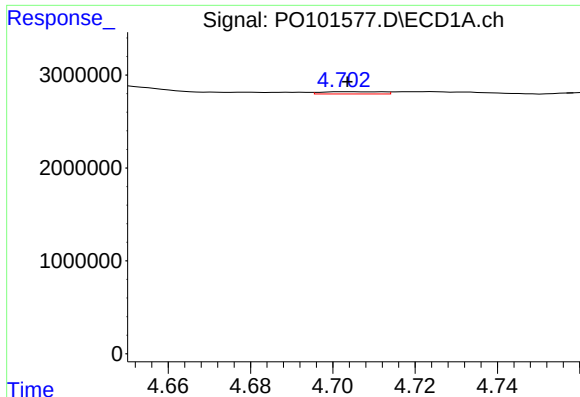

#11 AR-1232-1


R.T.: 4.703 min
Delta R.T.: 0.000 min
Response: 248014
Conc: 3.28 ng/ml

Instrument :
FID_E
ClientSampleId :

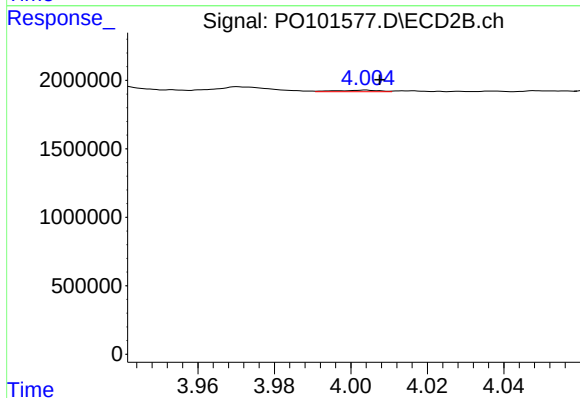


#11 AR-1232-1

R.T.: 4.004 min
Delta R.T.: -0.004 min
Response: 87988
Conc: 1.61 ng/ml

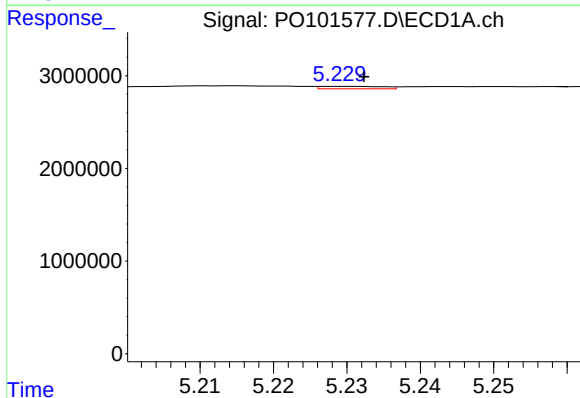


#12 AR-1232-2

R.T.: 5.229 min
Delta R.T.: -0.003 min
Response: 159097
Conc: 3.50 ng/ml

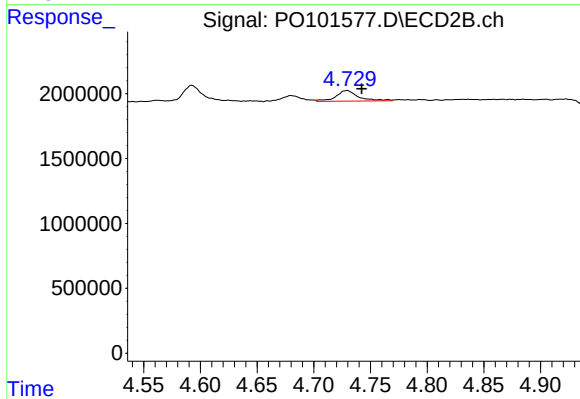

#12 AR-1232-2


R.T.: 4.729 min
Delta R.T.: -0.013 min
Response: 1127706
Conc: 23.45 ng/ml

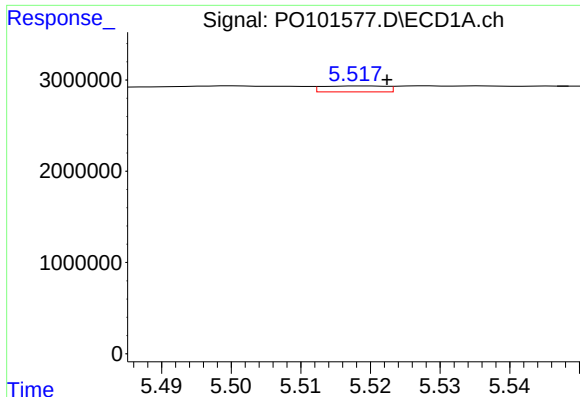

#13 AR-1232-3


R.T.: 5.519 min
Delta R.T.: -0.003 min
Response: 414850
Conc: 6.20 ng/ml

Instrument :
FID_E
ClientSampleId :

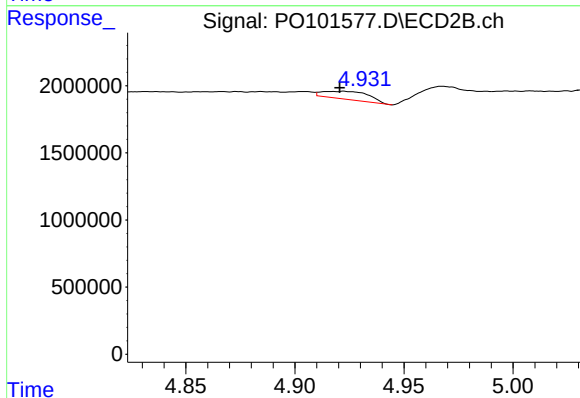


#13 AR-1232-3

R.T.: 4.922 min
Delta R.T.: 0.002 min
Response: 874372
Conc: 33.35 ng/ml

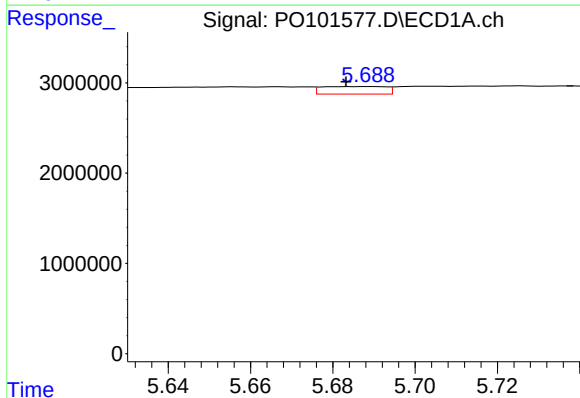


#14 AR-1232-4

R.T.: 5.689 min
Delta R.T.: 0.006 min
Response: 902335
Conc: 25.21 ng/ml

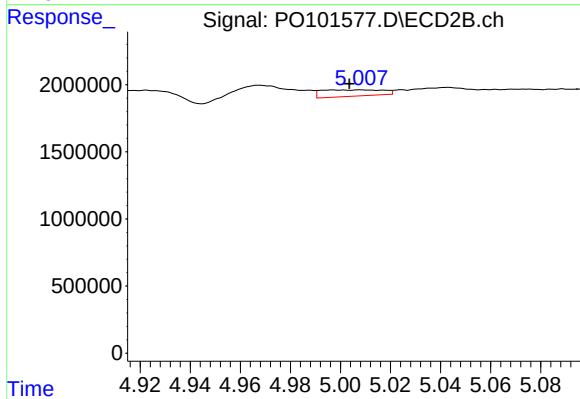

#14 AR-1232-4


R.T.: 4.997 min
Delta R.T.: -0.007 min
Response: 804964
Conc: 28.91 ng/ml

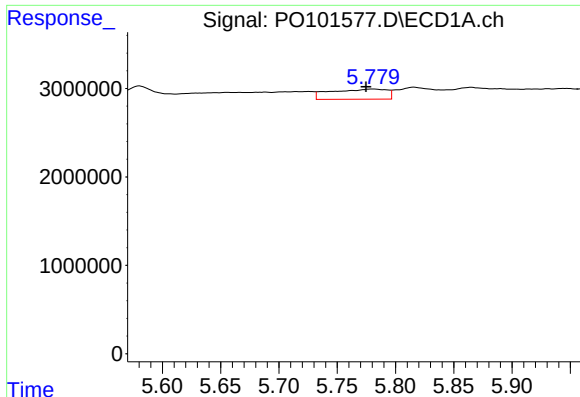

#15 AR-1232-5


R.T.: 5.780 min
Delta R.T.: 0.005 min
Response: 3853176
Conc: 112.94 ng/ml

Instrument :
FID_E
ClientSampleId :

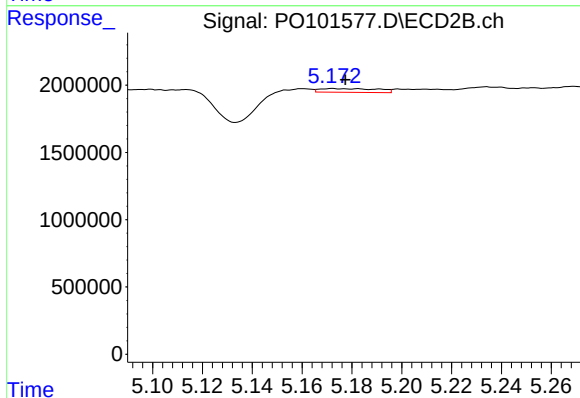


#15 AR-1232-5

R.T.: 5.172 min
Delta R.T.: -0.005 min
Response: 445775
Conc: 14.58 ng/ml

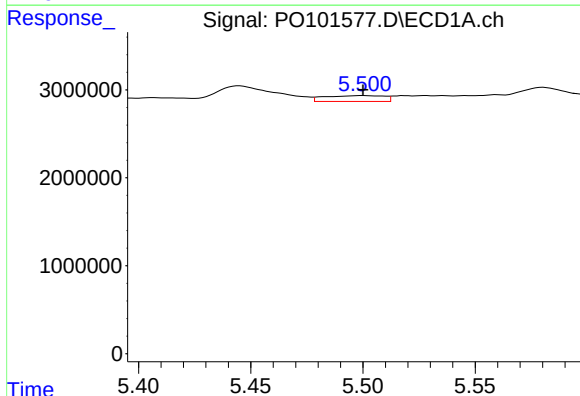


#16 AR-1242-1

R.T.: 5.500 min
Delta R.T.: 0.000 min
Response: 1215231
Conc: 15.71 ng/ml

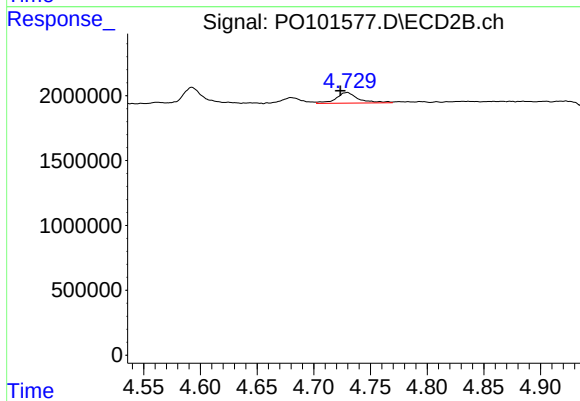

#16 AR-1242-1


R.T.: 4.729 min
Delta R.T.: 0.006 min
Response: 1127706
Conc: 19.17 ng/ml

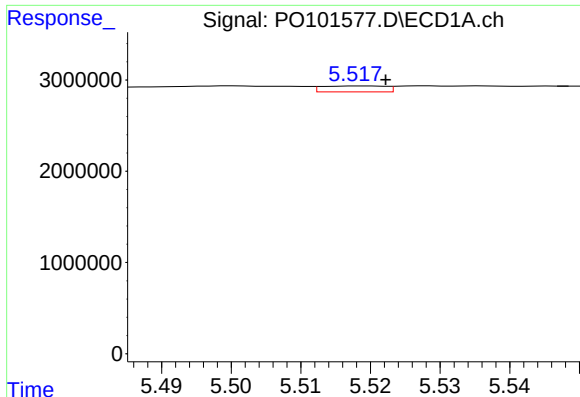

#17 AR-1242-2


R.T.: 5.519 min
Delta R.T.: -0.003 min
Response: 414850
Conc: 3.83 ng/ml

Instrument :
FID_E
ClientSampleId :

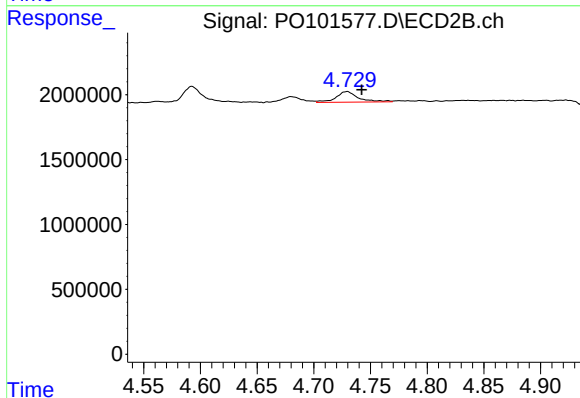


#17 AR-1242-2

R.T.: 4.729 min
Delta R.T.: -0.013 min
Response: 1127706
Conc: 14.54 ng/ml

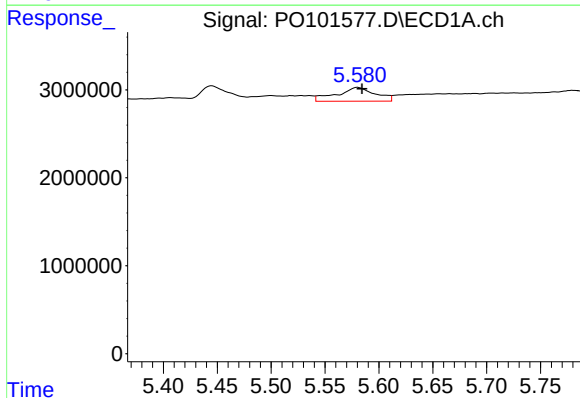


#18 AR-1242-3

R.T.: 5.580 min
Delta R.T.: -0.004 min
Response: 3892274
Conc: 54.76 ng/ml

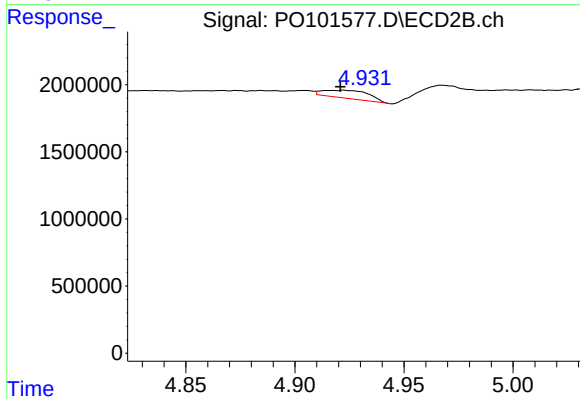

#18 AR-1242-3


R.T.: 4.922 min
Delta R.T.: 0.002 min
Response: 874372
Conc: 20.17 ng/ml

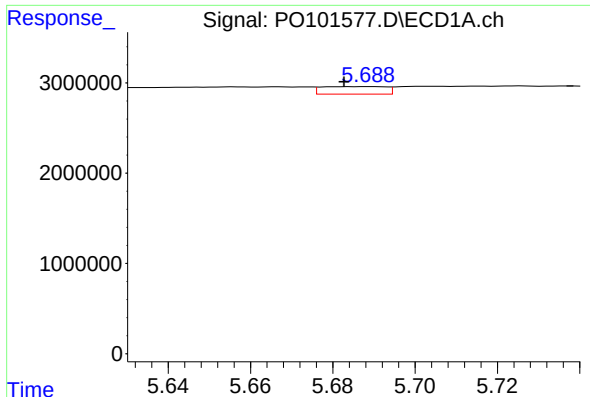

#19 AR-1242-4


R.T.: 5.689 min
Delta R.T.: 0.006 min
Response: 902335
Conc: 15.84 ng/ml

Instrument :
FID_E
ClientSampleId :

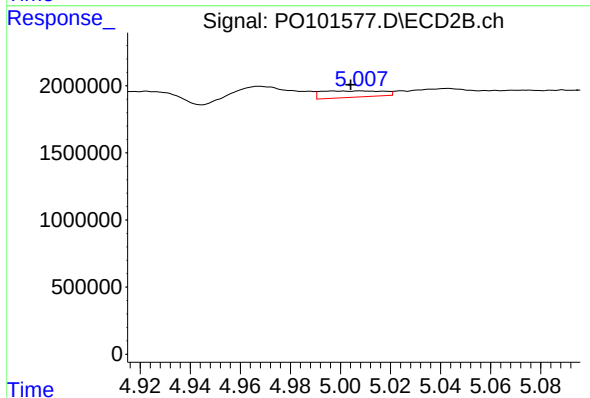


#19 AR-1242-4

R.T.: 4.997 min
Delta R.T.: -0.007 min
Response: 804964
Conc: 16.17 ng/ml

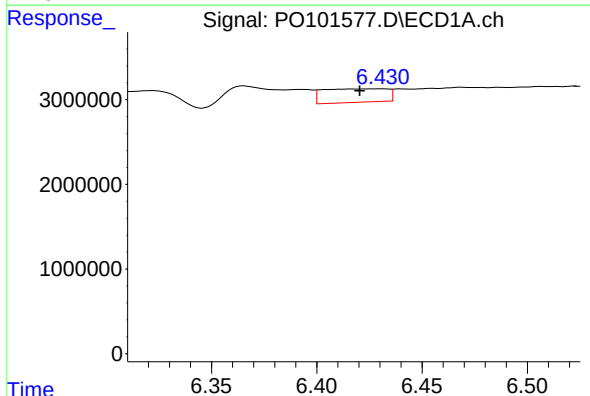


#20 AR-1242-5

R.T.: 6.431 min
Delta R.T.: 0.010 min
Response: 3382568
Conc: 63.03 ng/ml

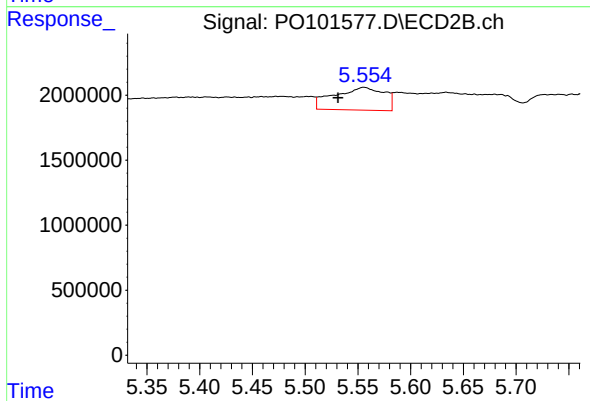

#20 AR-1242-5


R.T.: 5.556 min
Delta R.T.: 0.025 min
Response: 5787339
Conc: 109.25 ng/ml

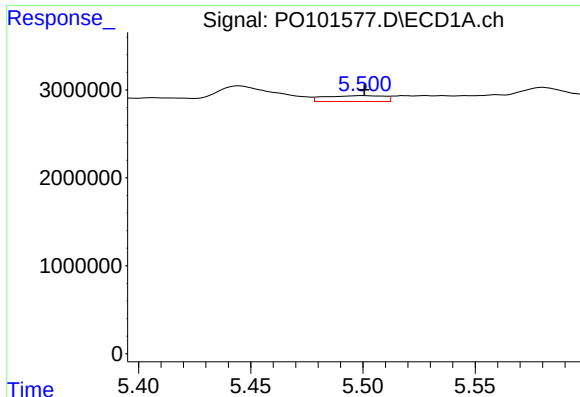

#21 AR-1248-1


R.T.: 5.500 min
Delta R.T.: 0.000 min
Response: 1215231
Conc: 20.97 ng/ml

Instrument :
FID_E
ClientSampleId :

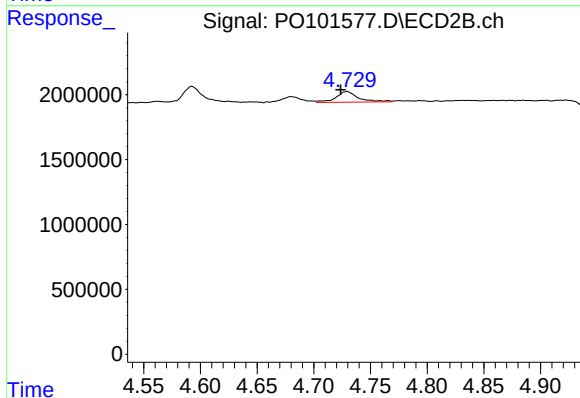


#21 AR-1248-1

R.T.: 4.729 min
Delta R.T.: 0.006 min
Response: 1127706
Conc: 25.20 ng/ml

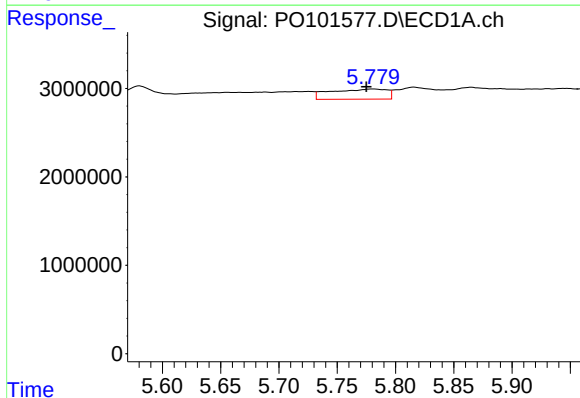


#22 AR-1248-2

R.T.: 5.780 min
Delta R.T.: 0.004 min
Response: 3853176
Conc: 38.26 ng/ml

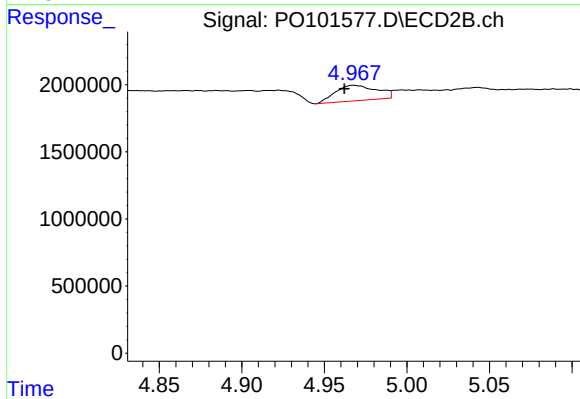

#22 AR-1248-2


R.T.: 4.968 min
Delta R.T.: 0.006 min
Response: 2008049
Conc: 28.56 ng/ml

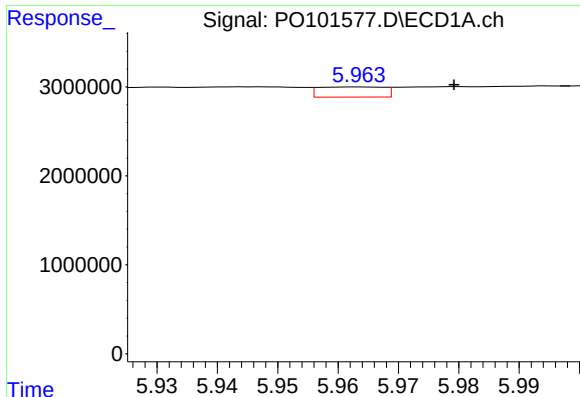

#23 AR-1248-3


R.T.: 5.964 min
Delta R.T.: -0.016 min
Response: 856033
Conc: 8.26 ng/ml

Instrument :
FID_E
ClientSampleId :

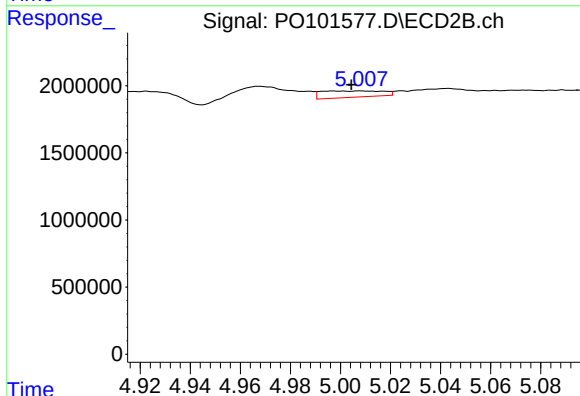


#23 AR-1248-3

R.T.: 4.997 min
Delta R.T.: -0.007 min
Response: 804964
Conc: 11.07 ng/ml

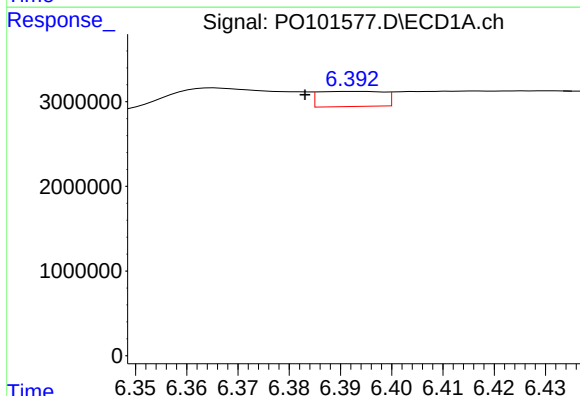


#24 AR-1248-4

R.T.: 6.393 min
Delta R.T.: 0.010 min
Response: 1575623
Conc: 17.35 ng/ml

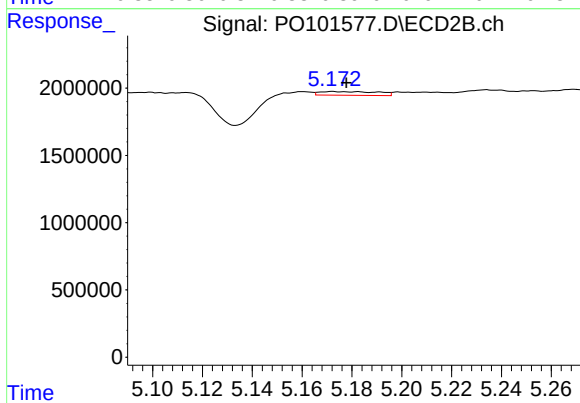

#24 AR-1248-4


R.T.: 5.172 min
Delta R.T.: -0.006 min
Response: 445775
Conc: 5.24 ng/ml

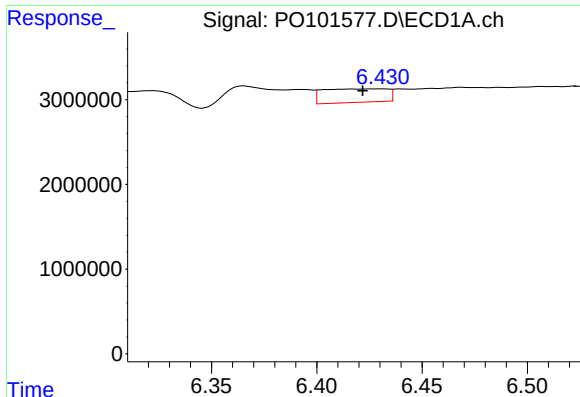

#25 AR-1248-5


R.T.: 6.431 min
Delta R.T.: 0.009 min
Response: 3382568
Conc: 37.92 ng/ml

Instrument :
FID_E
ClientSampleId :

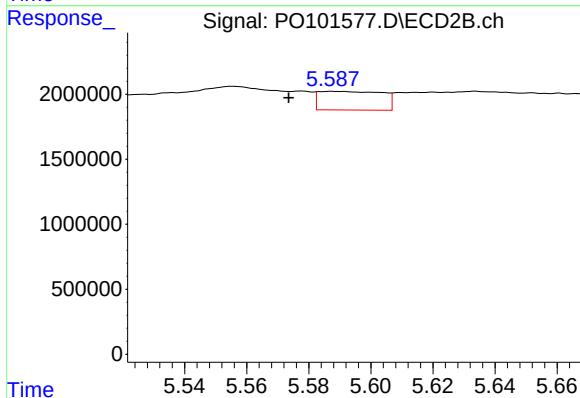


#25 AR-1248-5

R.T.: 5.588 min
Delta R.T.: 0.014 min
Response: 2033062
Conc: 29.69 ng/ml

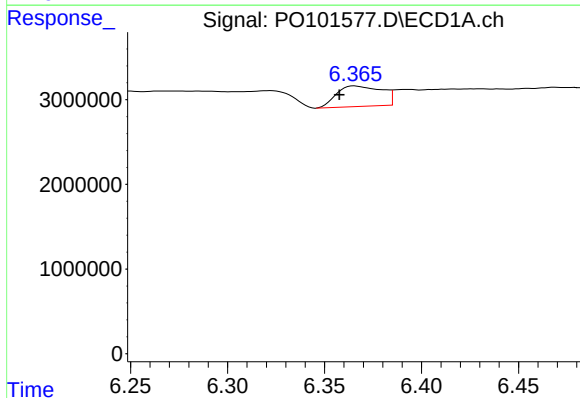


#26 AR-1254-1

R.T.: 6.365 min
Delta R.T.: 0.008 min
Response: 3922395
Conc: 32.97 ng/ml

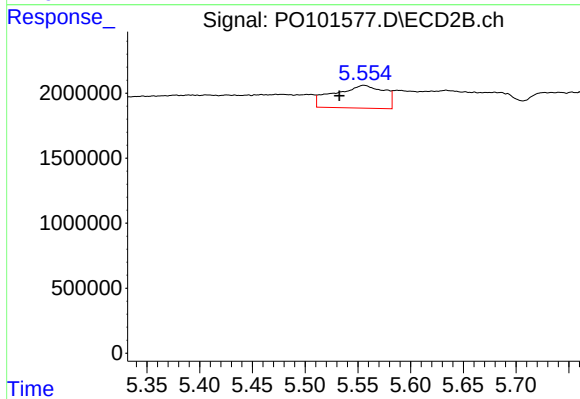

#26 AR-1254-1


R.T.: 5.556 min
Delta R.T.: 0.023 min
Response: 5787339
Conc: 46.52 ng/ml

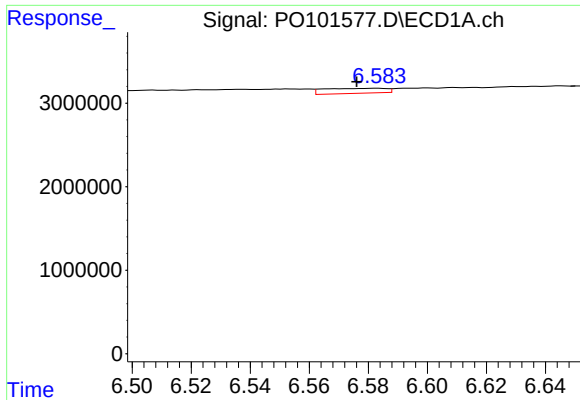

#27 AR-1254-2


R.T.: 6.583 min
Delta R.T.: 0.007 min
Response: 881871
Conc: 5.18 ng/ml

Instrument :
FID_E
ClientSampleId :

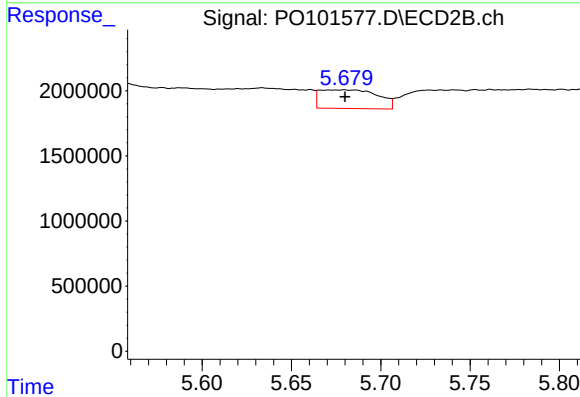


#27 AR-1254-2

R.T.: 5.680 min
Delta R.T.: 0.000 min
Response: 3221374
Conc: 28.78 ng/ml

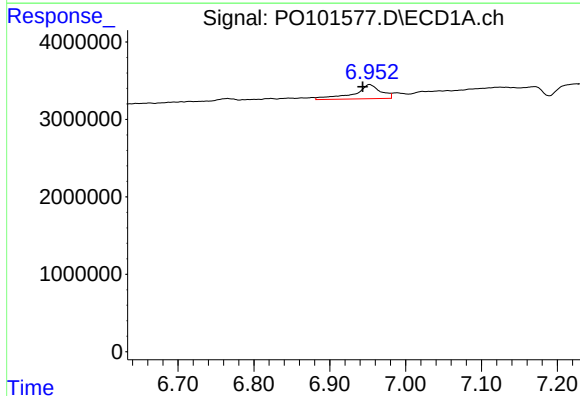


#28 AR-1254-3

R.T.: 6.953 min
Delta R.T.: 0.009 min
Response: 4518412
Conc: 27.51 ng/ml

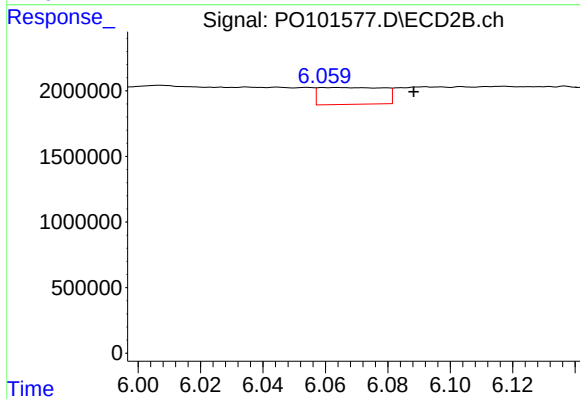

#28 AR-1254-3


R.T.: 6.064 min
Delta R.T.: -0.025 min
Response: 1846142
Conc: 11.10 ng/ml

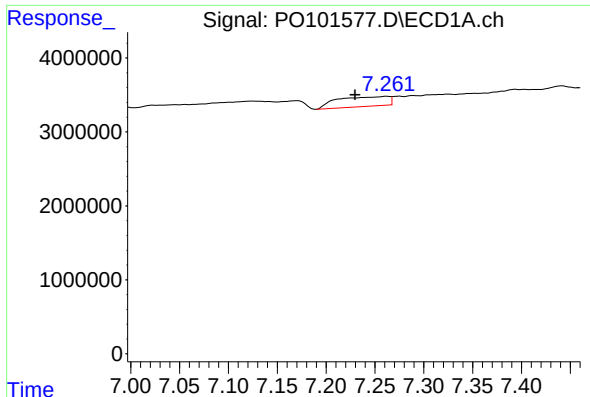

#29 AR-1254-4


R.T.: 7.262 min
Delta R.T.: 0.032 min
Response: 4927358
Conc: 49.30 ng/ml

Instrument :
FID_E
ClientSampleId :

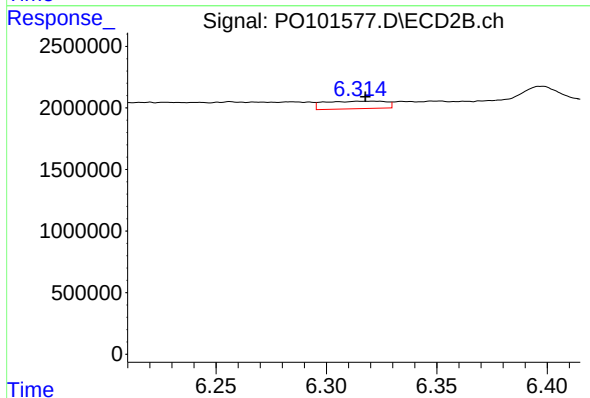


#29 AR-1254-4

R.T.: 6.321 min
Delta R.T.: 0.004 min
Response: 1186382
Conc: 13.91 ng/ml

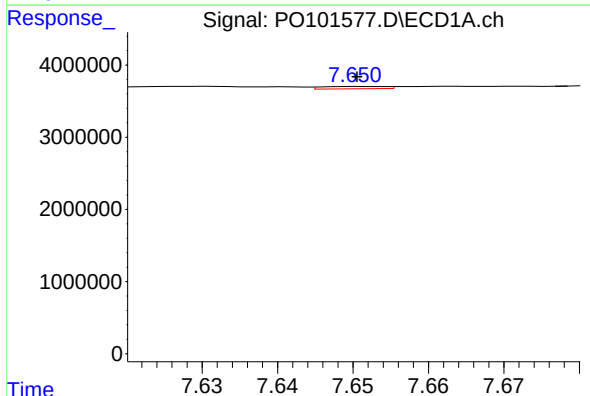


#30 AR-1254-5

R.T.: 7.651 min
Delta R.T.: 0.000 min
Response: 180017
Conc: 1.53 ng/ml

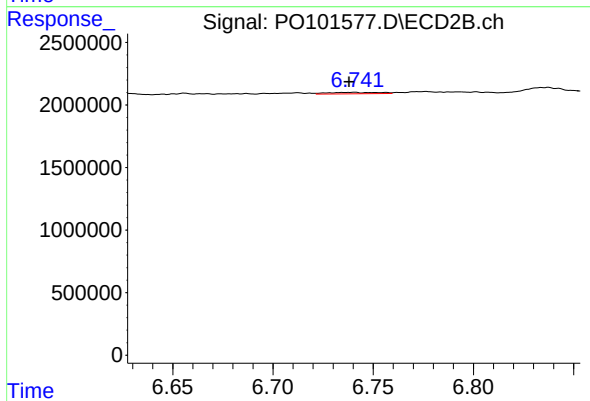

#30 AR-1254-5


R.T.: 6.740 min
Delta R.T.: 0.002 min
Response: 195901
Conc: 1.45 ng/ml

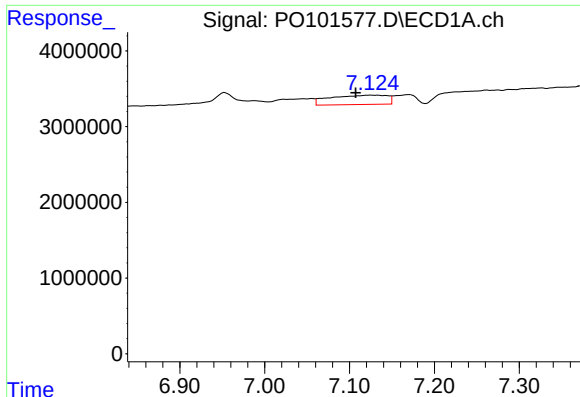

#31 AR-1260-1


R.T.: 7.125 min
Delta R.T.: 0.017 min
Response: 5773623
Conc: 40.48 ng/ml

Instrument :
FID_E
ClientSampleId :

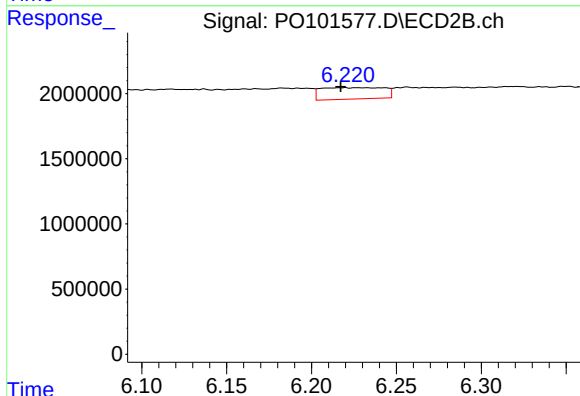


#31 AR-1260-1

R.T.: 6.220 min
Delta R.T.: 0.002 min
Response: 2262753
Conc: 18.34 ng/ml

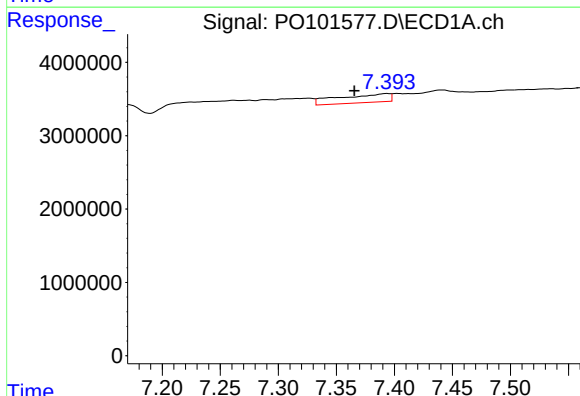


#32 AR-1260-2

R.T.: 7.393 min
Delta R.T.: 0.028 min
Response: 3585208
Conc: 24.48 ng/ml

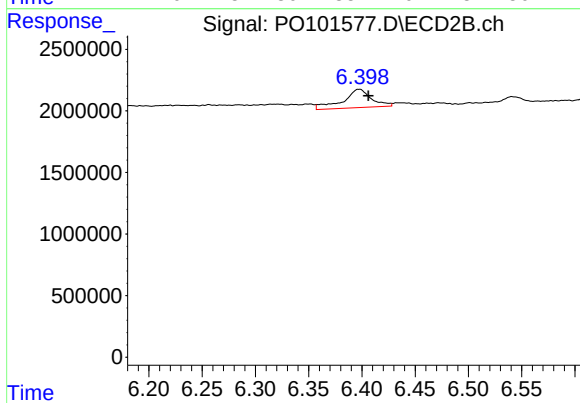

#32 AR-1260-2


R.T.: 6.397 min
Delta R.T.: -0.008 min
Response: 2781512
Conc: 20.34 ng/ml

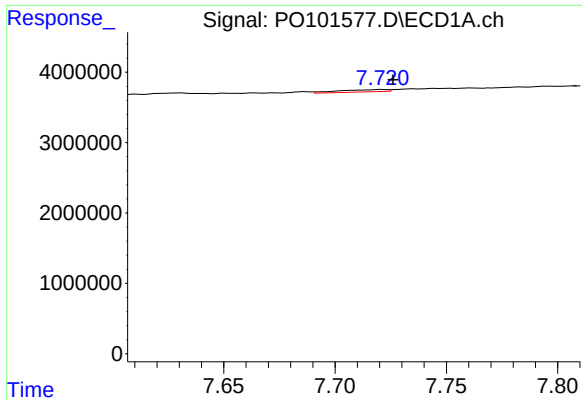

#33 AR-1260-3


R.T.: 7.721 min
Delta R.T.: -0.005 min
Response: 469943
Conc: 4.02 ng/ml

Instrument :
FID_E
ClientSampleId :

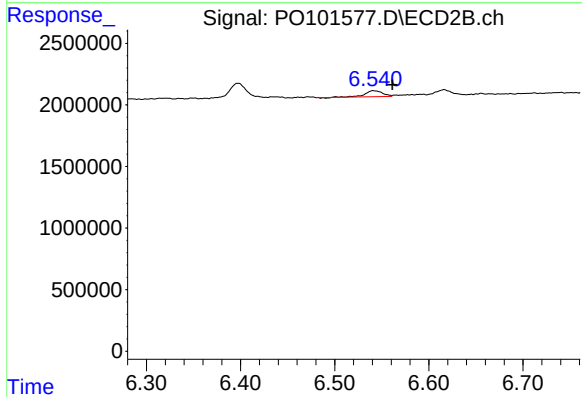


#33 AR-1260-3

R.T.: 6.541 min
Delta R.T.: -0.020 min
Response: 626873
Conc: 4.89 ng/ml

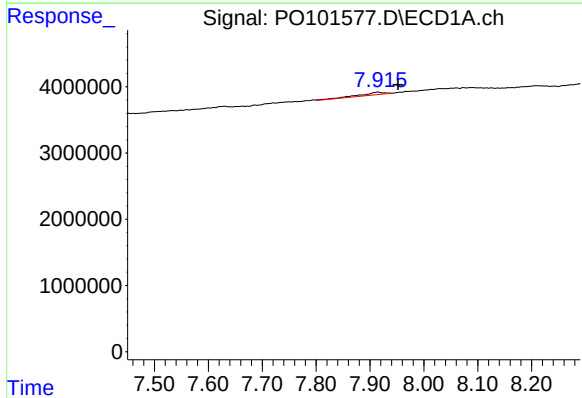


#34 AR-1260-4

R.T.: 7.915 min
Delta R.T.: -0.037 min
Response: 1267186
Conc: 10.76 ng/ml

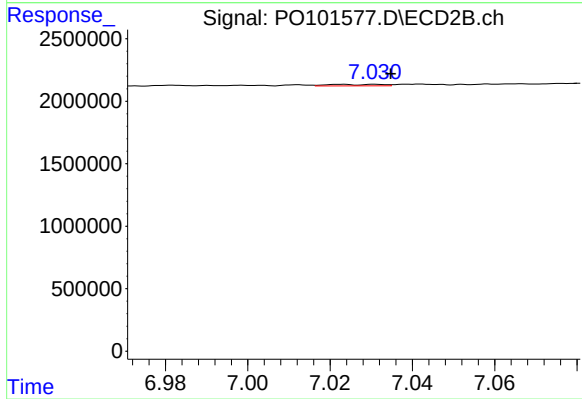

#34 AR-1260-4


R.T.: 7.031 min
Delta R.T.: -0.004 min
Response: 111386
Conc: 1.08 ng/ml

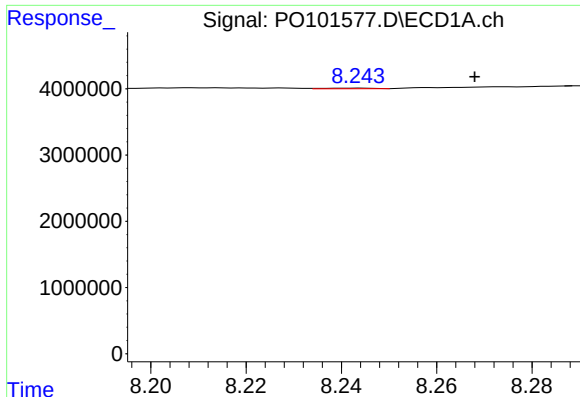

#35 AR-1260-5


R.T.: 8.243 min
Delta R.T.: -0.025 min
Response: 73211
Conc: 0.33 ng/ml

Instrument :
FID_E
ClientSampleId :

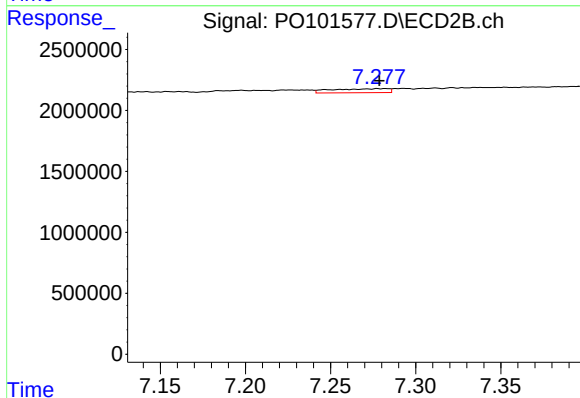


#35 AR-1260-5

R.T.: 7.283 min
Delta R.T.: 0.004 min
Response: 747736
Conc: 3.56 ng/ml

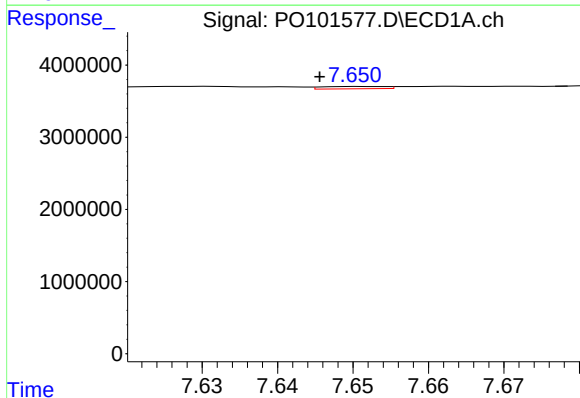


#36 AR-1262-1

R.T.: 7.651 min
Delta R.T.: 0.005 min
Response: 180017
Conc: 1.61 ng/ml

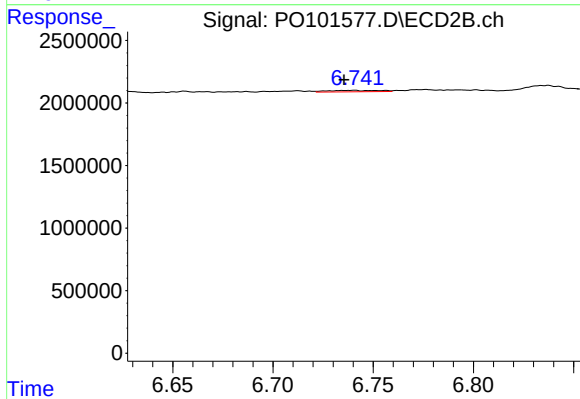

#36 AR-1262-1


R.T.: 6.740 min
Delta R.T.: 0.005 min
Response: 195901
Conc: 2.42 ng/ml

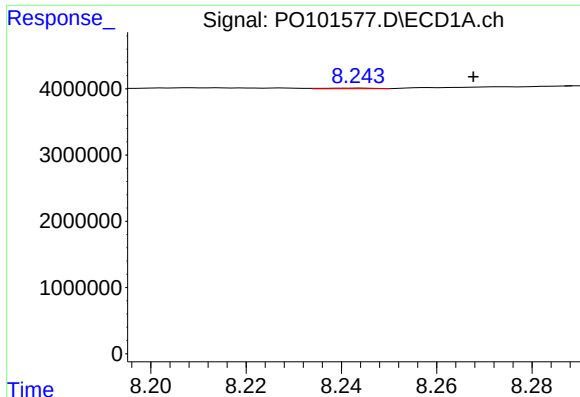

#37 AR-1262-2


R.T.: 8.243 min
Delta R.T.: -0.025 min
Response: 73211
Conc: 0.27 ng/ml

Instrument :
FID_E
ClientSampleId :

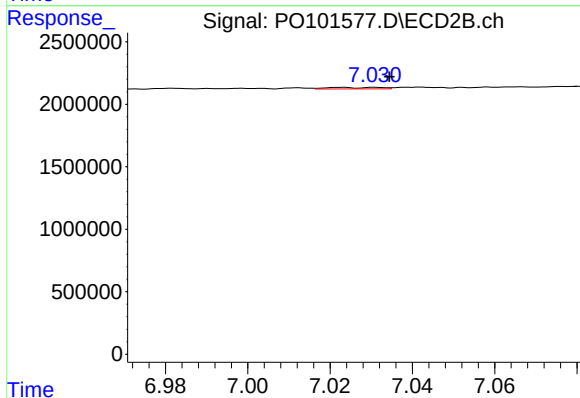


#37 AR-1262-2

R.T.: 7.031 min
Delta R.T.: -0.003 min
Response: 111386
Conc: 0.75 ng/ml

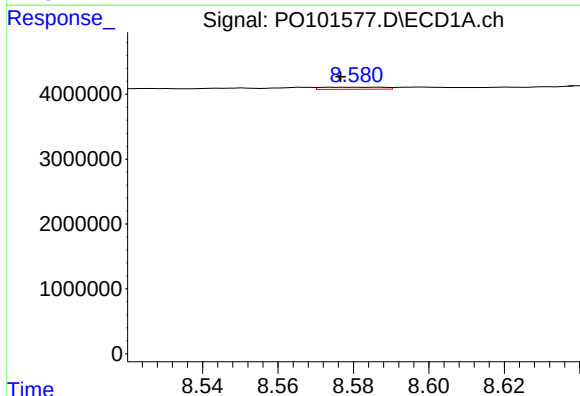


#38 AR-1262-3

R.T.: 8.580 min
Delta R.T.: 0.004 min
Response: 358997
Conc: 1.85 ng/ml

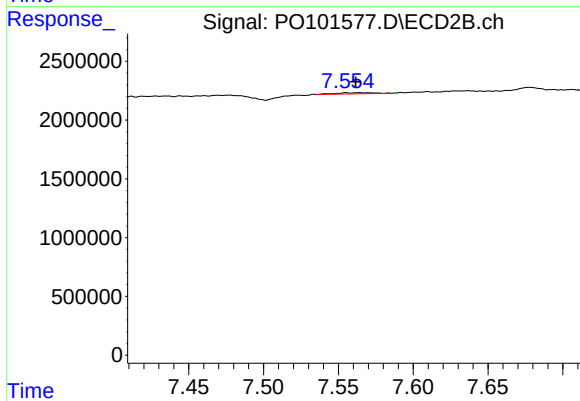

#38 AR-1262-3


R.T.: 7.555 min
Delta R.T.: -0.006 min
Response: 168390
Conc: 1.64 ng/ml

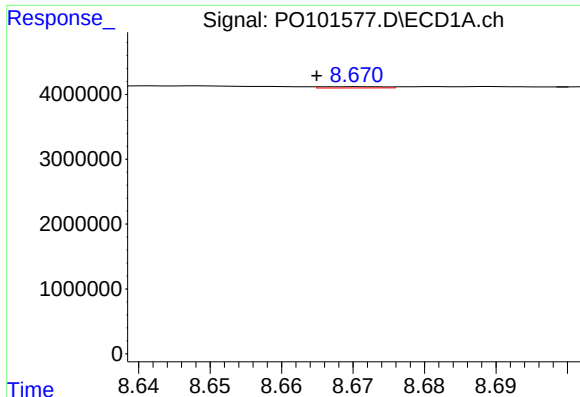

#39 AR-1262-4


R.T.: 8.671 min
Delta R.T.: 0.006 min
Response: 125180
Conc: 0.81 ng/ml

Instrument :
FID_E
ClientSampleId :

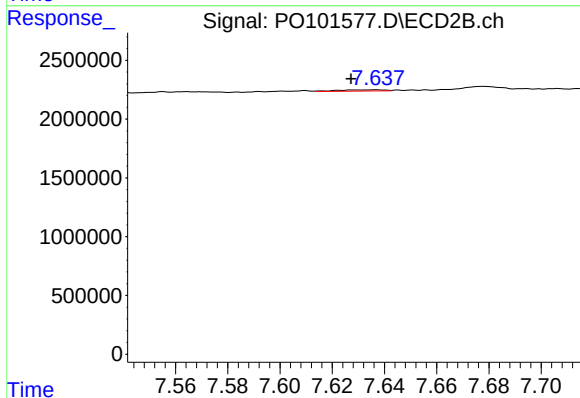


#39 AR-1262-4

R.T.: 7.637 min
Delta R.T.: 0.009 min
Response: 126369
Conc: 0.65 ng/ml

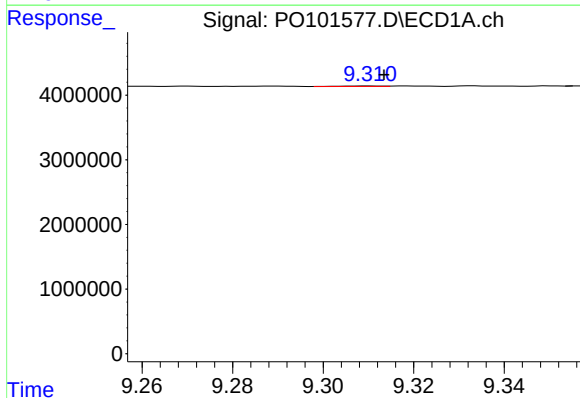


#40 AR-1262-5

R.T.: 9.311 min
Delta R.T.: -0.003 min
Response: 50808
Conc: 0.54 ng/ml

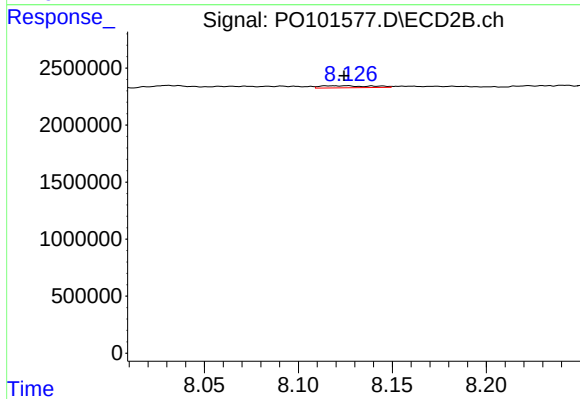

#40 AR-1262-5


R.T.: 8.126 min
Delta R.T.: 0.002 min
Response: 340897
Conc: 4.07 ng/ml

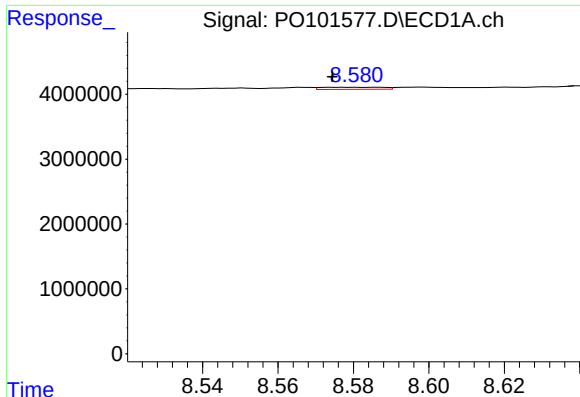

#41 AR-1268-1


R.T.: 8.580 min
Delta R.T.: 0.006 min
Response: 358997
Conc: 1.13 ng/ml

Instrument :
FID_E
ClientSampleId :

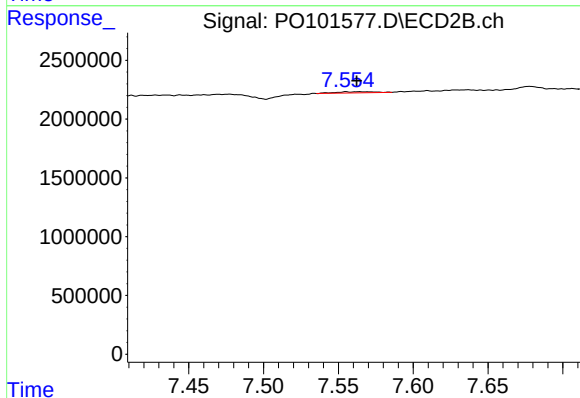


#41 AR-1268-1

R.T.: 7.555 min
Delta R.T.: -0.007 min
Response: 168390
Conc: 0.60 ng/ml

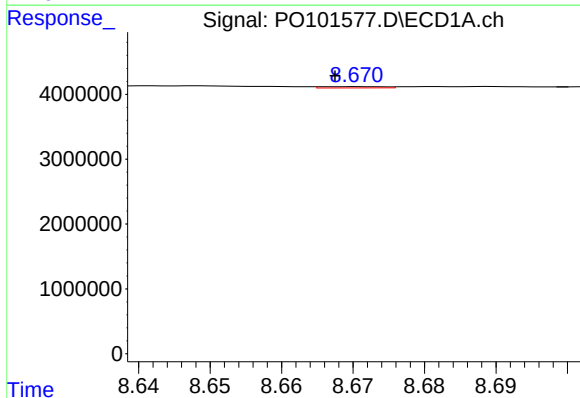


#42 AR-1268-2

R.T.: 8.671 min
Delta R.T.: 0.003 min
Response: 125180
Conc: 0.43 ng/ml

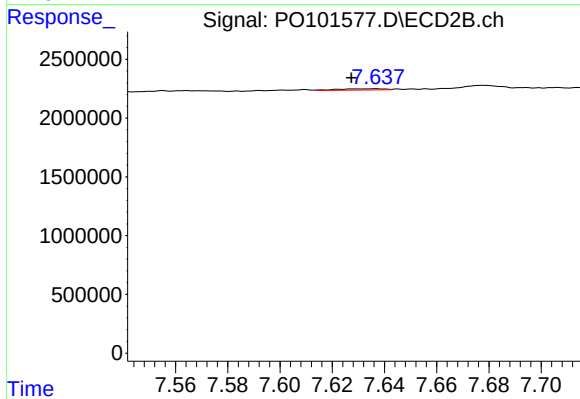

#42 AR-1268-2


R.T.: 7.637 min
Delta R.T.: 0.009 min
Response: 126369
Conc: 0.49 ng/ml

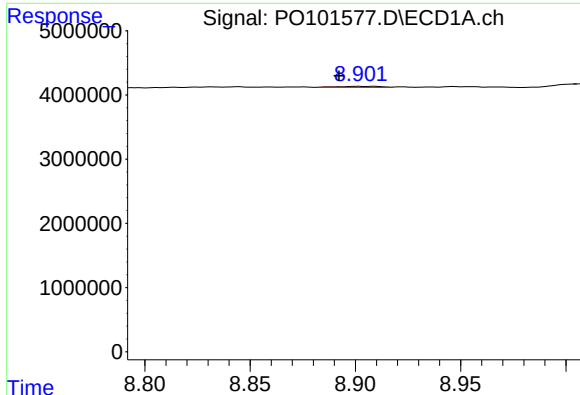

#43 AR-1268-3


R.T.: 8.902 min
Delta R.T.: 0.009 min
Response: 246657
Conc: 0.96 ng/ml

Instrument :
FID_E
ClientSampleId :

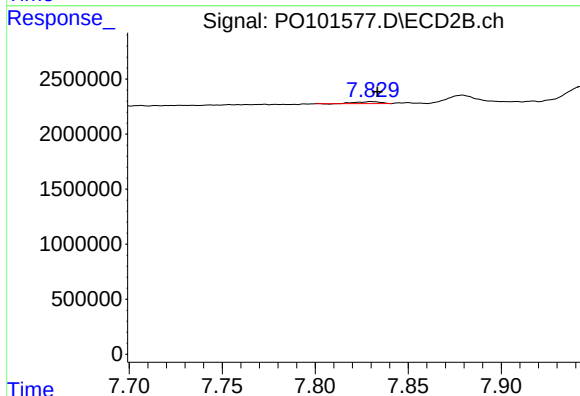


#43 AR-1268-3

R.T.: 7.830 min
Delta R.T.: -0.003 min
Response: 161452
Conc: 0.69 ng/ml

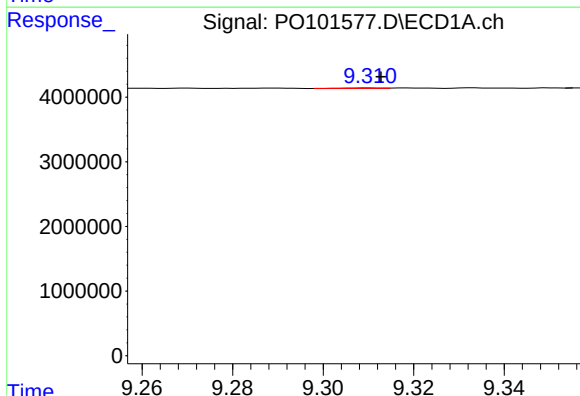


#44 AR-1268-4

R.T.: 9.311 min
Delta R.T.: -0.002 min
Response: 50808
Conc: 0.55 ng/ml

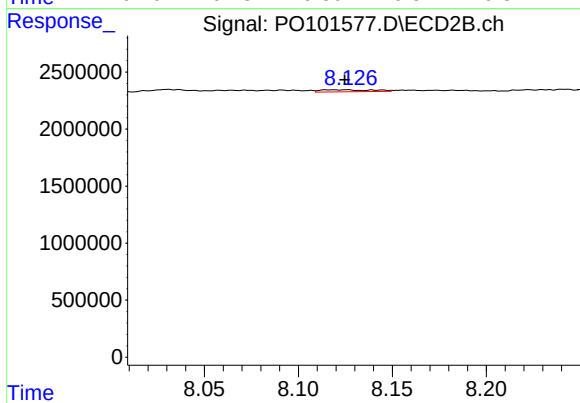

#44 AR-1268-4


R.T.: 8.126 min
Delta R.T.: 0.001 min
Response: 340897
Conc: 4.01 ng/ml

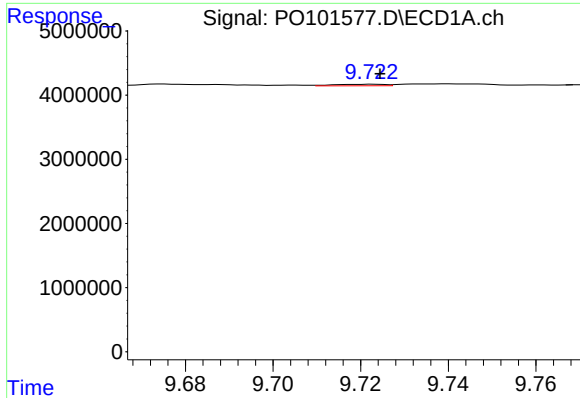

#45 AR-1268-5

R.T.: 9.723 min
Delta R.T.: -0.002 min
Response: 191759
Conc: 0.24 ng/ml

Instrument :
FID_E
ClientSampleId :

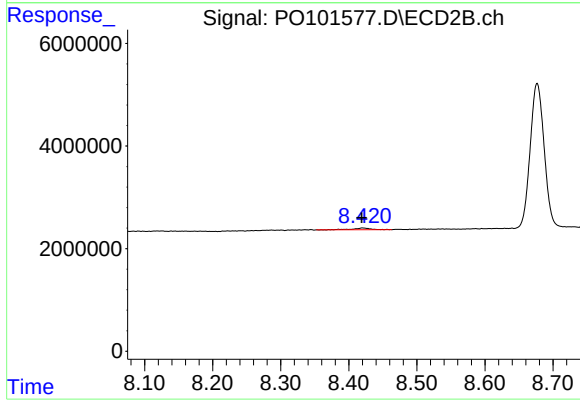

#45 AR-1268-5

R.T.: 8.420 min
Delta R.T.: 0.001 min
Response: 626595
Conc: 0.95 ng/ml