

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE020822AL\
 Data File : FE034912.D
 Signal(s) : FID1B.CH
 Acq On : 09 Feb 2022 10:49
 Operator : YP\AJ
 Sample : N1387-02DL 5X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 10 01:17:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 020822.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 08 22:05:03 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.127	1829694	6.247 ug/ml
Spiked Amount 50.000		Recovery =	12.49%
12) S 1-chlorooctadecane (S...	12.559	1377186	6.160 ug/ml
Spiked Amount 50.000		Recovery =	12.32%
Target Compounds			
10) T n-Eicosane (C20)	12.162	547590	2.097 ug/ml
14) T n-Tetracosane (C24)	14.367	300965	<MDL ug/ml
17) T n-Tricontane (C30)	17.254	116280	<MDL ug/ml
18) T n-Dotriacontane (C32)	18.084	220200	<MDL ug/ml
19) T n-Tetratriacontane (C34)	18.870	116371	<MDL ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE020822AL\
Data File : FE034912.D
Signal(s) : FID1B.CH
Acq On : 09 Feb 2022 10:49
Operator : YP\AJ
Sample : N1387-02DL 5X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 10 01:17:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 020822.M
Quant Title : GC Extractables
QLast Update : Tue Feb 08 22:05:03 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

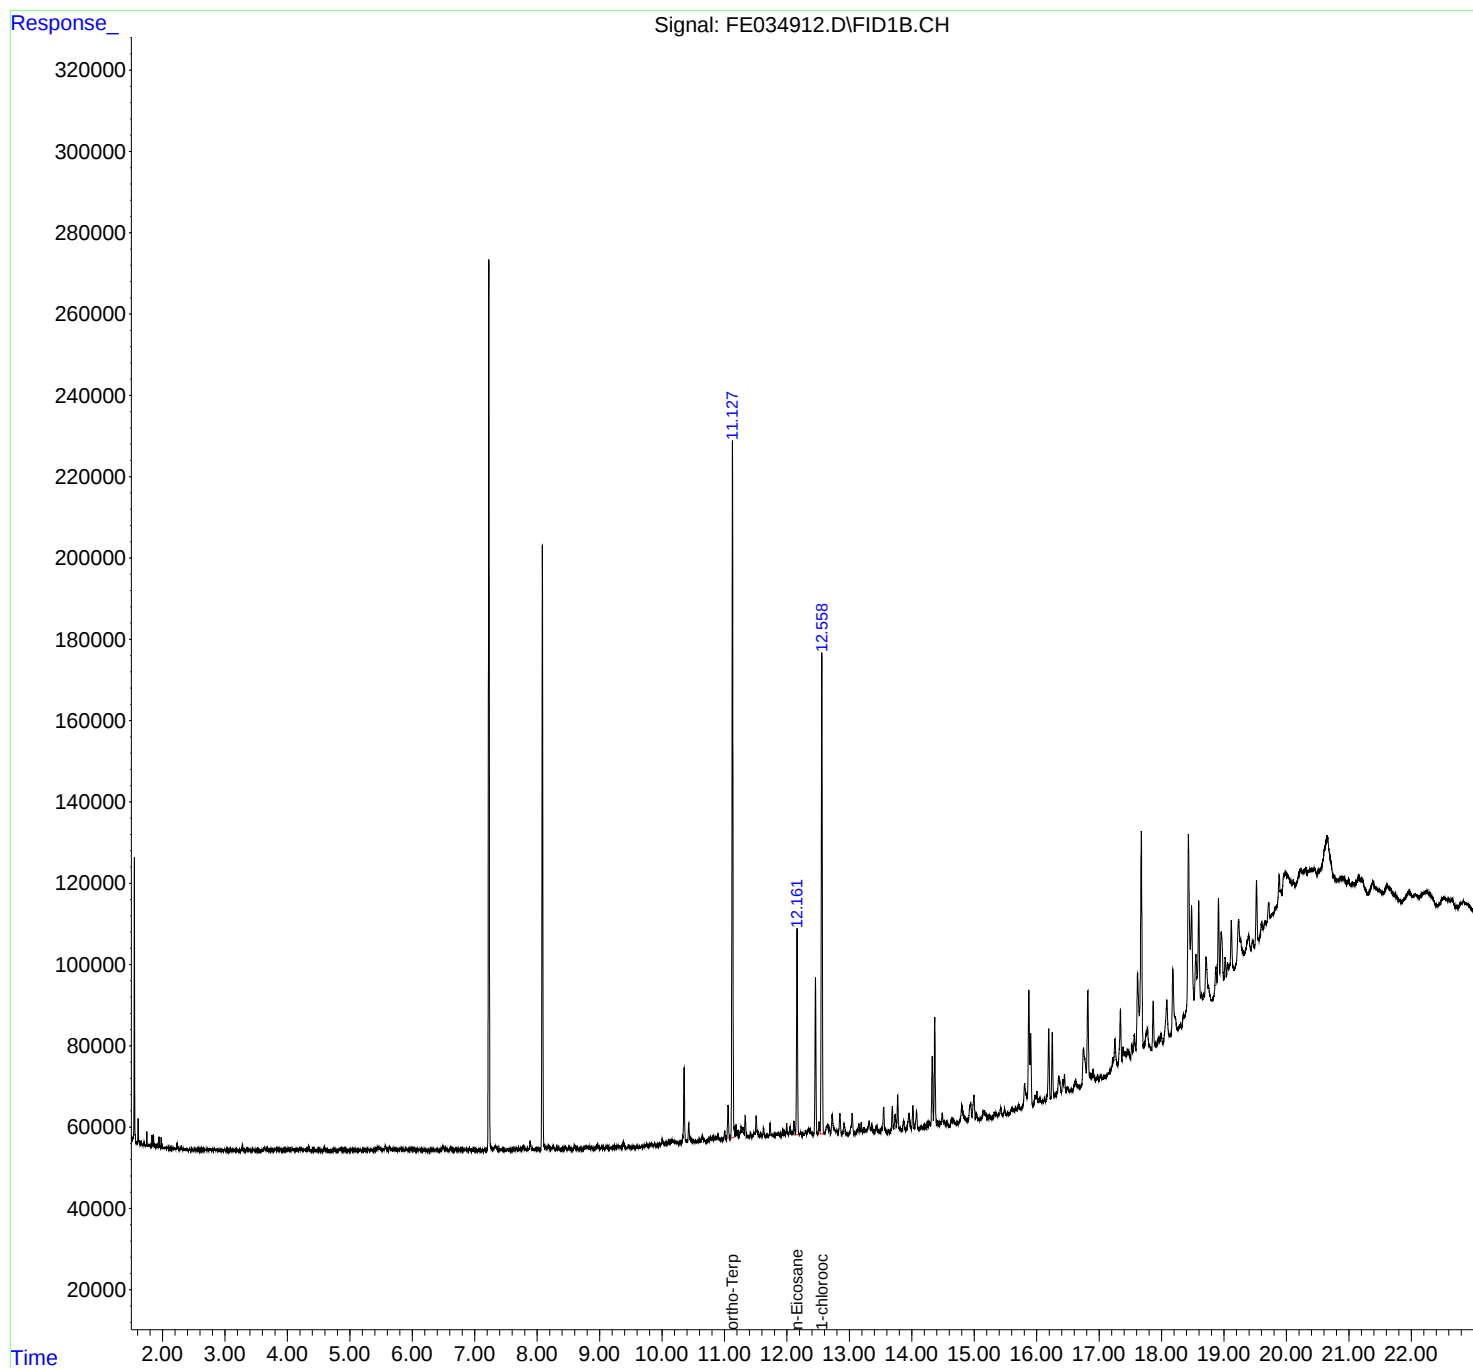


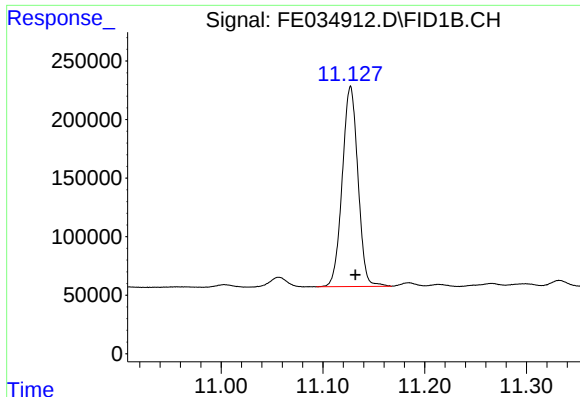

#9 ortho-Terphenyl (SURR)


R.T.: 11.127 min
Delta R.T.: -0.005 min
Response: 1829694
Conc: 6.25 ug/ml

Instrument :
FID_E
ClientSampleId :

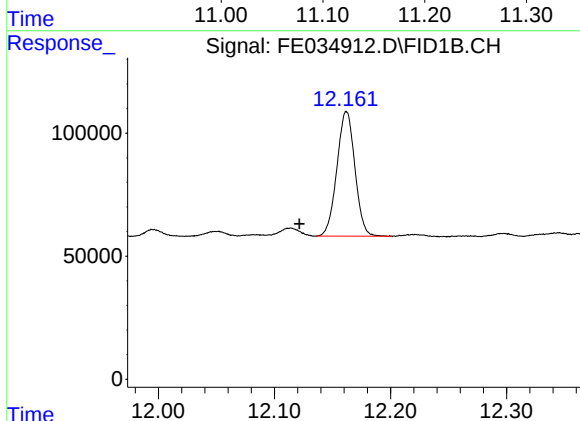

#10 n-Eicosane (C20)

R.T.: 12.162 min
Delta R.T.: 0.041 min
Response: 547590
Conc: 2.10 ug/ml

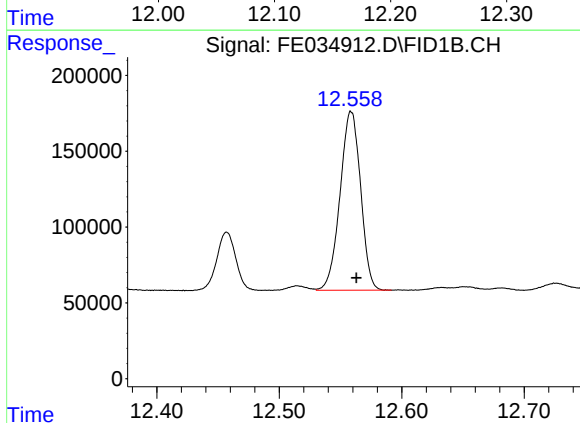

#12 1-chlorooctadecane (SURR)

R.T.: 12.559 min
Delta R.T.: -0.004 min
Response: 1377186
Conc: 6.16 ug/ml