

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE020822AL\
 Data File : FE034939.D
 Signal(s) : FID1B.CH
 Acq On : 10 Feb 2022 00:52
 Operator : YP\AJ
 Sample : N1443-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 10 01:23:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 020822.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 08 22:05:03 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.127	6961380	23.770 ug/ml
Spiked Amount 50.000		Recovery =	47.54%
12) S 1-chlorooctadecane (S...	12.557	5343240	23.899 ug/ml
Spiked Amount 50.000		Recovery =	47.80%
Target Compounds			
3) T A~Naphthalene (C11.7)	5.624f	113380	<MDL ug/ml
6) T n-Tetradecane (C14)	7.749	145545	<MDL ug/ml
7) T n-Hexadecane (C16)	9.387	117728	<MDL ug/ml
10) T n-Eicosane (C20)	12.154	77746	<MDL ug/ml
14) T n-Tetracosane (C24)	14.402	114456	<MDL ug/ml
15) T n-Hexacosane (C26)	15.418	215639	<MDL ug/ml
16) T n-Octacosane (C28)	16.363	175653	<MDL ug/ml
17) T n-Tricontane (C30)	17.246	120486	<MDL ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE020822AL\
Data File : FE034939.D
Signal(s) : FID1B.CH
Acq On : 10 Feb 2022 00:52
Operator : YP\AJ
Sample : N1443-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 10 01:23:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 020822.M
Quant Title : GC Extractables
QLast Update : Tue Feb 08 22:05:03 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

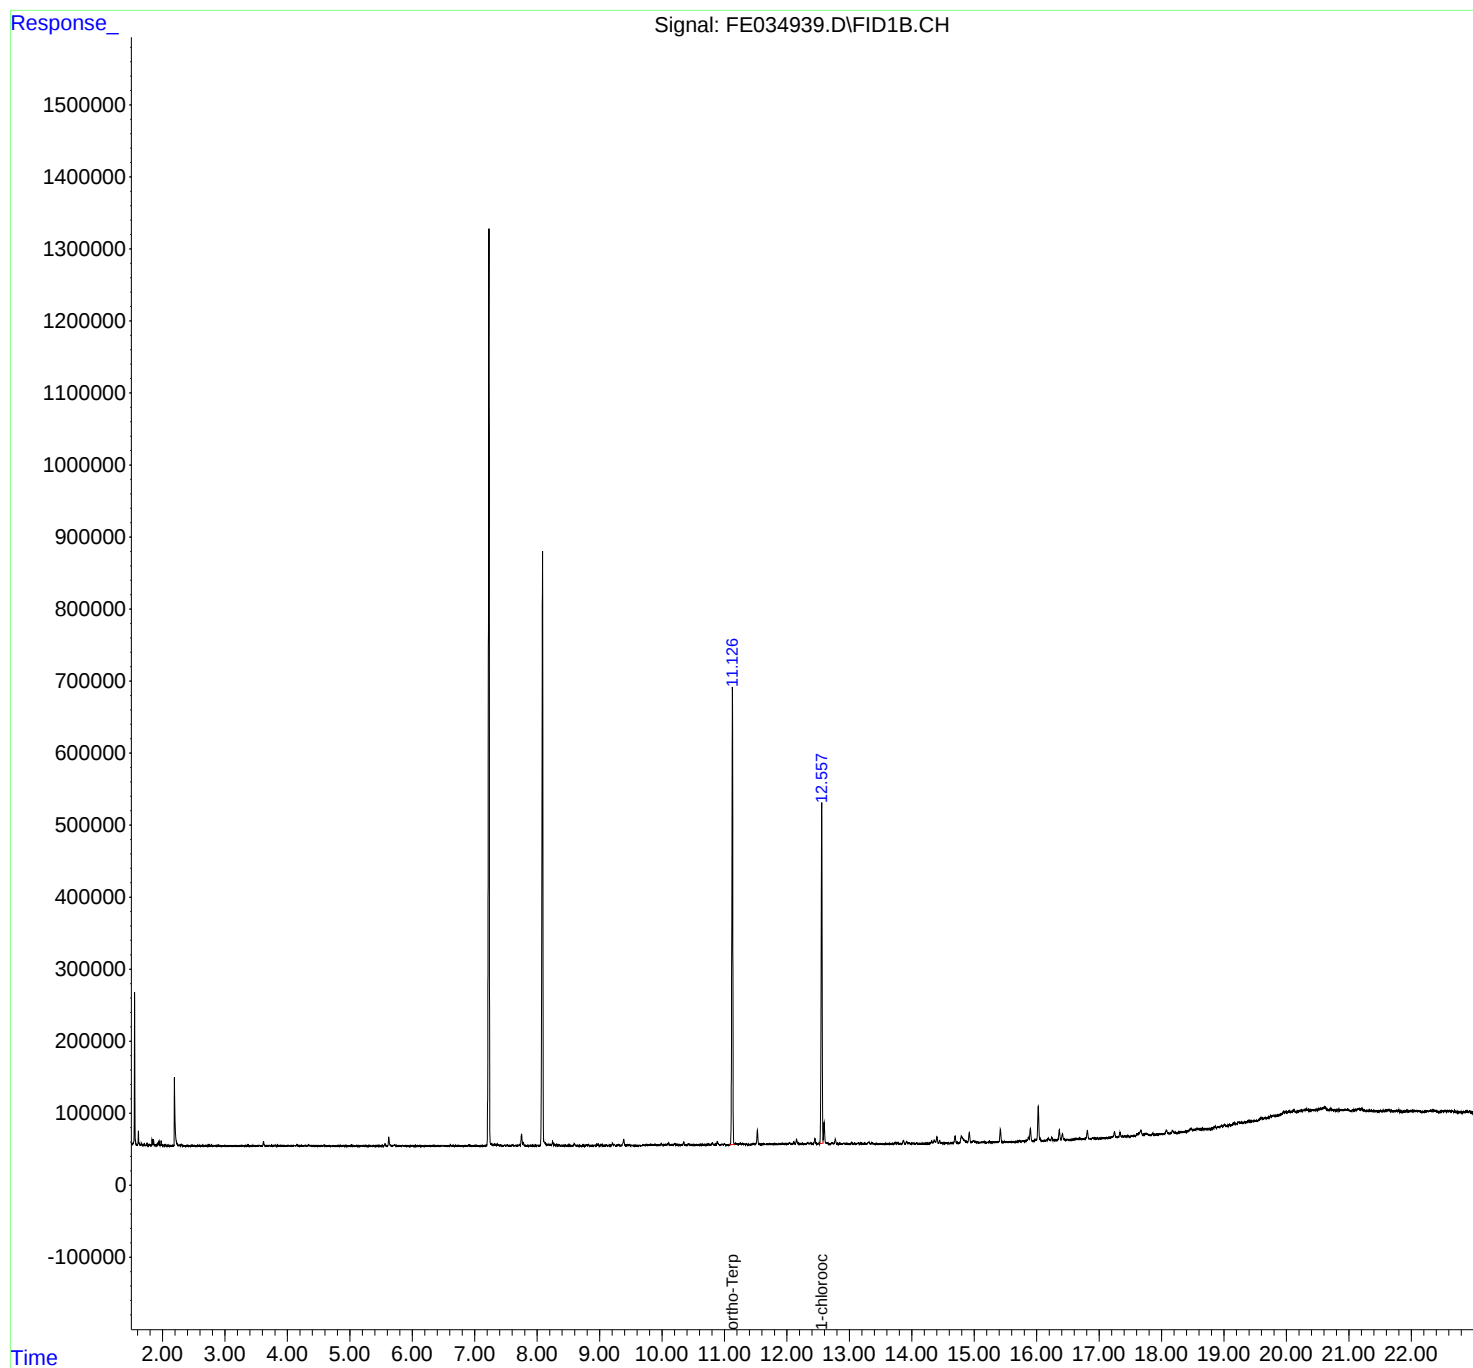


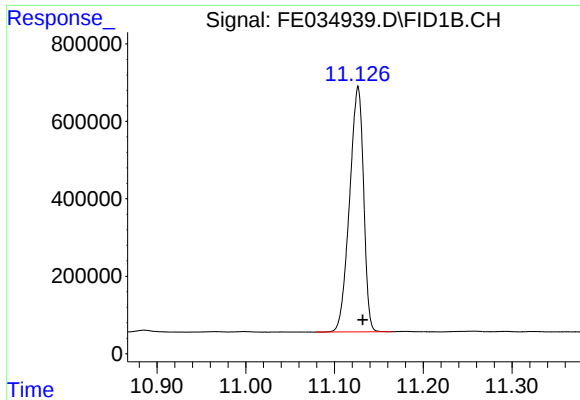

#9 ortho-Terphenyl (SURR)

R.T.: 11.127 min
Delta R.T.: -0.005 min
Response: 6961380
Conc: 23.77 ug/ml

Instrument :
FID_E
ClientSampleId :

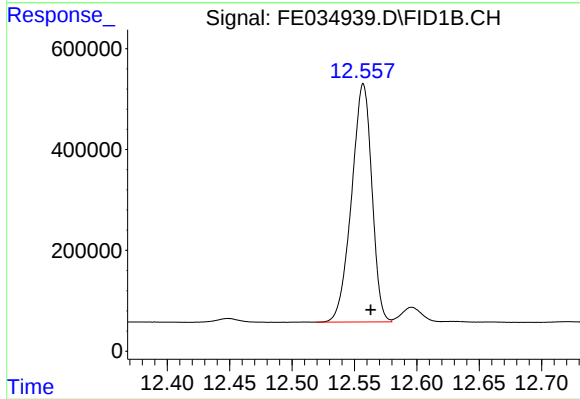

#12 1-chlorooctadecane (SURR)

R.T.: 12.557 min
Delta R.T.: -0.006 min
Response: 5343240
Conc: 23.90 ug/ml