

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE020824AL\  
Data File : FE046659.D  
Signal(s) : FID1B.ch  
Acq On : 09 Feb 2024 01:58  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
I.BLK

Integration File: autoint1.e  
Quant Time: Feb 09 02:44:18 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 012524.M  
Quant Title : GC Extractables  
QLast Update : Thu Jan 25 14:56:03 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

| Compound                    |                          | R.T.   | Response | Conc Units  |
|-----------------------------|--------------------------|--------|----------|-------------|
| -----                       |                          |        |          |             |
| System Monitoring Compounds |                          |        |          |             |
| Target Compounds            |                          |        |          |             |
| 19) T                       | n-Tetratriacontane (C34) | 19.612 | 12937    | 0.091 ug/ml |
| 20) T                       | n-Hexatriacontane (C36)  | 20.320 | 50723    | 0.368 ug/ml |
| 22) T                       | n-Tetracontane (C40)     | 21.967 | 139384   | 1.115 ug/ml |
| -----                       |                          |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE020824AL\  
Data File : FE046659.D  
Signal(s) : FID1B.ch  
Acq On : 09 Feb 2024 01:58  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
I.BLK

Integration File: autoint1.e  
Quant Time: Feb 09 02:44:18 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 012524.M  
Quant Title : GC Extractables  
QLast Update : Thu Jan 25 14:56:03 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

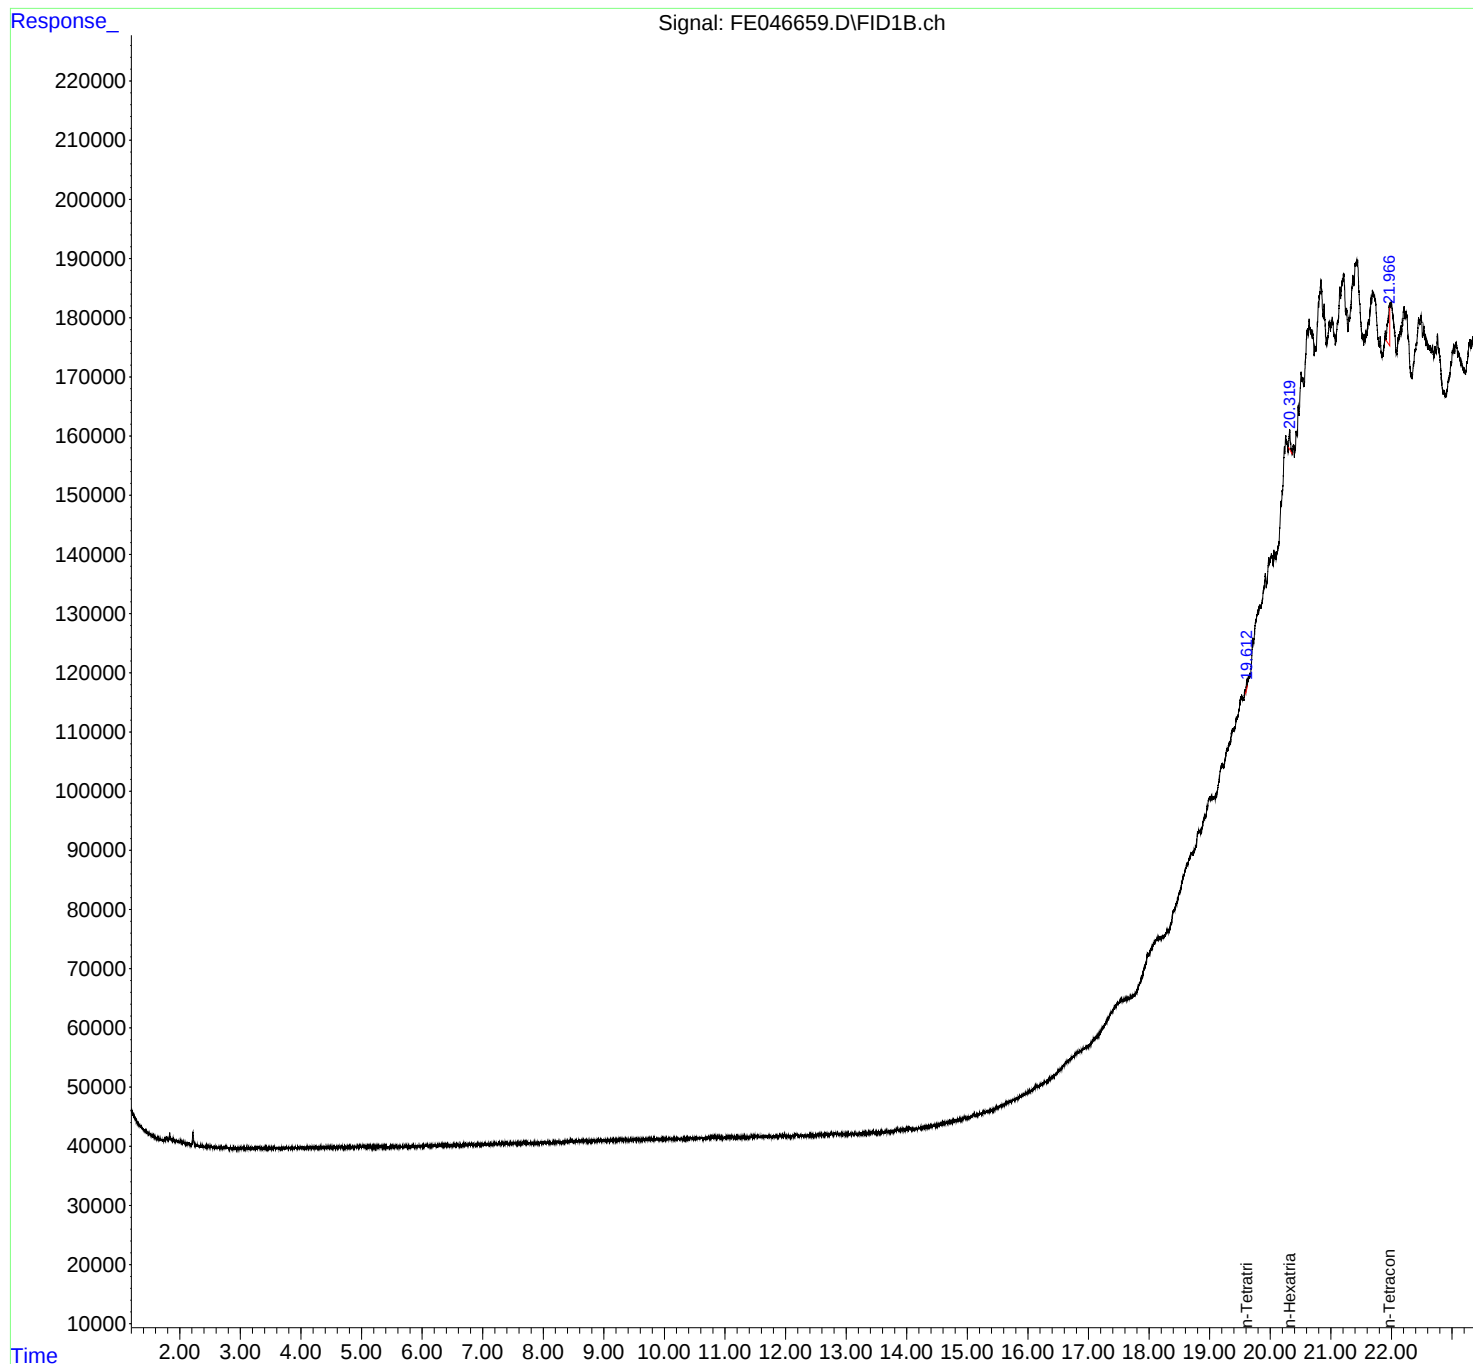


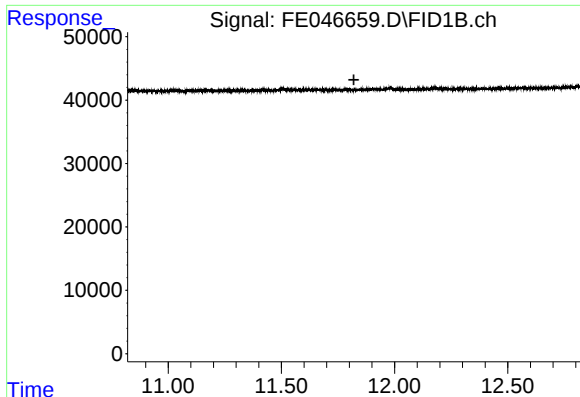

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min  
Exp R.T.: 11.820 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_E  
ClientSampleId :  
I.BLK

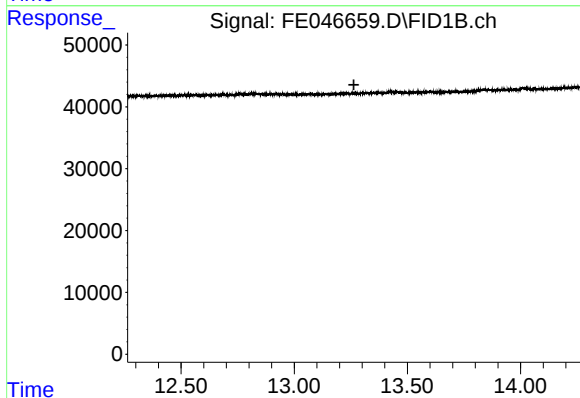


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min  
Exp R.T.: 13.264 min  
Response: 0  
Conc: N.D.

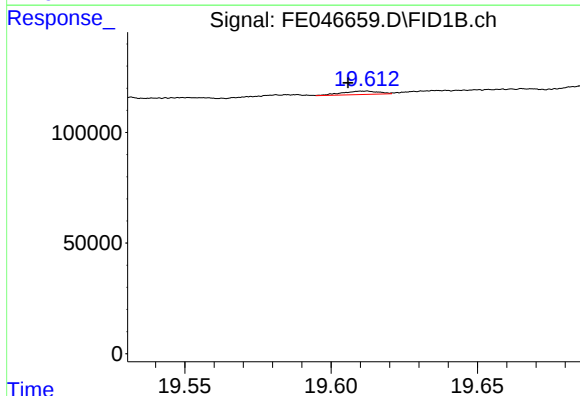


#19 n-Tetratriacontane (C34)

R.T.: 19.612 min  
Delta R.T.: 0.006 min  
Response: 12937  
Conc: 0.09 ug/ml

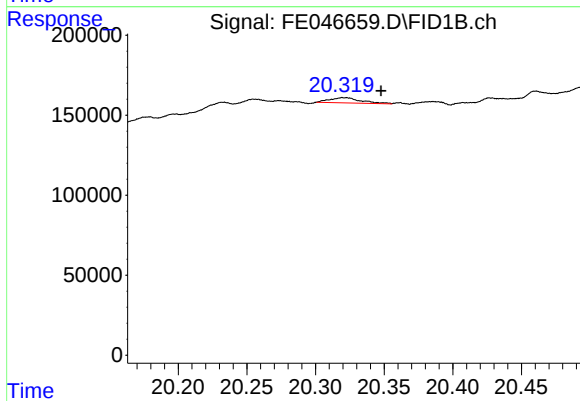

#20 n-Hexatriacontane (C36)

R.T.: 20.320 min  
Delta R.T.: -0.027 min  
Response: 50723  
Conc: 0.37 ug/ml

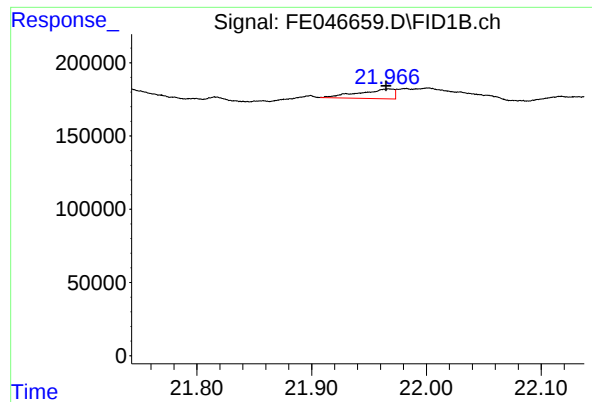

#22 n-Tetracontane (C40)

R.T.: 21.967 min  
Delta R.T.: 0.002 min  
Response: 139384  
Conc: 1.11 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
I.BLK