

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE020824AL\  
 Data File : FE046651.D  
 Signal(s) : FID1B.ch  
 Acq On : 08 Feb 2024 21:57  
 Operator : YP\AJ  
 Sample : P1411-02  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 72-11929-E2

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 02/12/2024  
 Supervised By :Ankita Jodhani 02/12/2024

Integration File: autoint1.e  
 Quant Time: Feb 09 02:41:55 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 012524.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Jan 25 14:56:03 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response | Conc Units    |
|--------------------------------|--------|----------|---------------|
| -----                          |        |          |               |
| System Monitoring Compounds    |        |          |               |
| 9) S ortho-Terphenyl (SURR)    | 11.827 | 6074117  | 32.849 ug/mlm |
| Spiked Amount                  | 50.000 | Recovery | = 65.70%      |
| 12) S 1-chlorooctadecane (S... | 13.257 | 5263310  | 36.994 ug/mlm |
| Spiked Amount                  | 50.000 | Recovery | = 73.99%      |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE020824AL\  
Data File : FE046651.D  
Signal(s) : FID1B.ch  
Acq On : 08 Feb 2024 21:57  
Operator : YP\AJ  
Sample : P1411-02  
Misc :  
ALS Vial : 15 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
72-11929-E2


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 02/12/2024  
Supervised By :Ankita Jodhani 02/12/2024

Integration File: autoint1.e  
Quant Time: Feb 09 02:41:55 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 012524.M  
Quant Title : GC Extractables  
QLast Update : Thu Jan 25 14:56:03 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

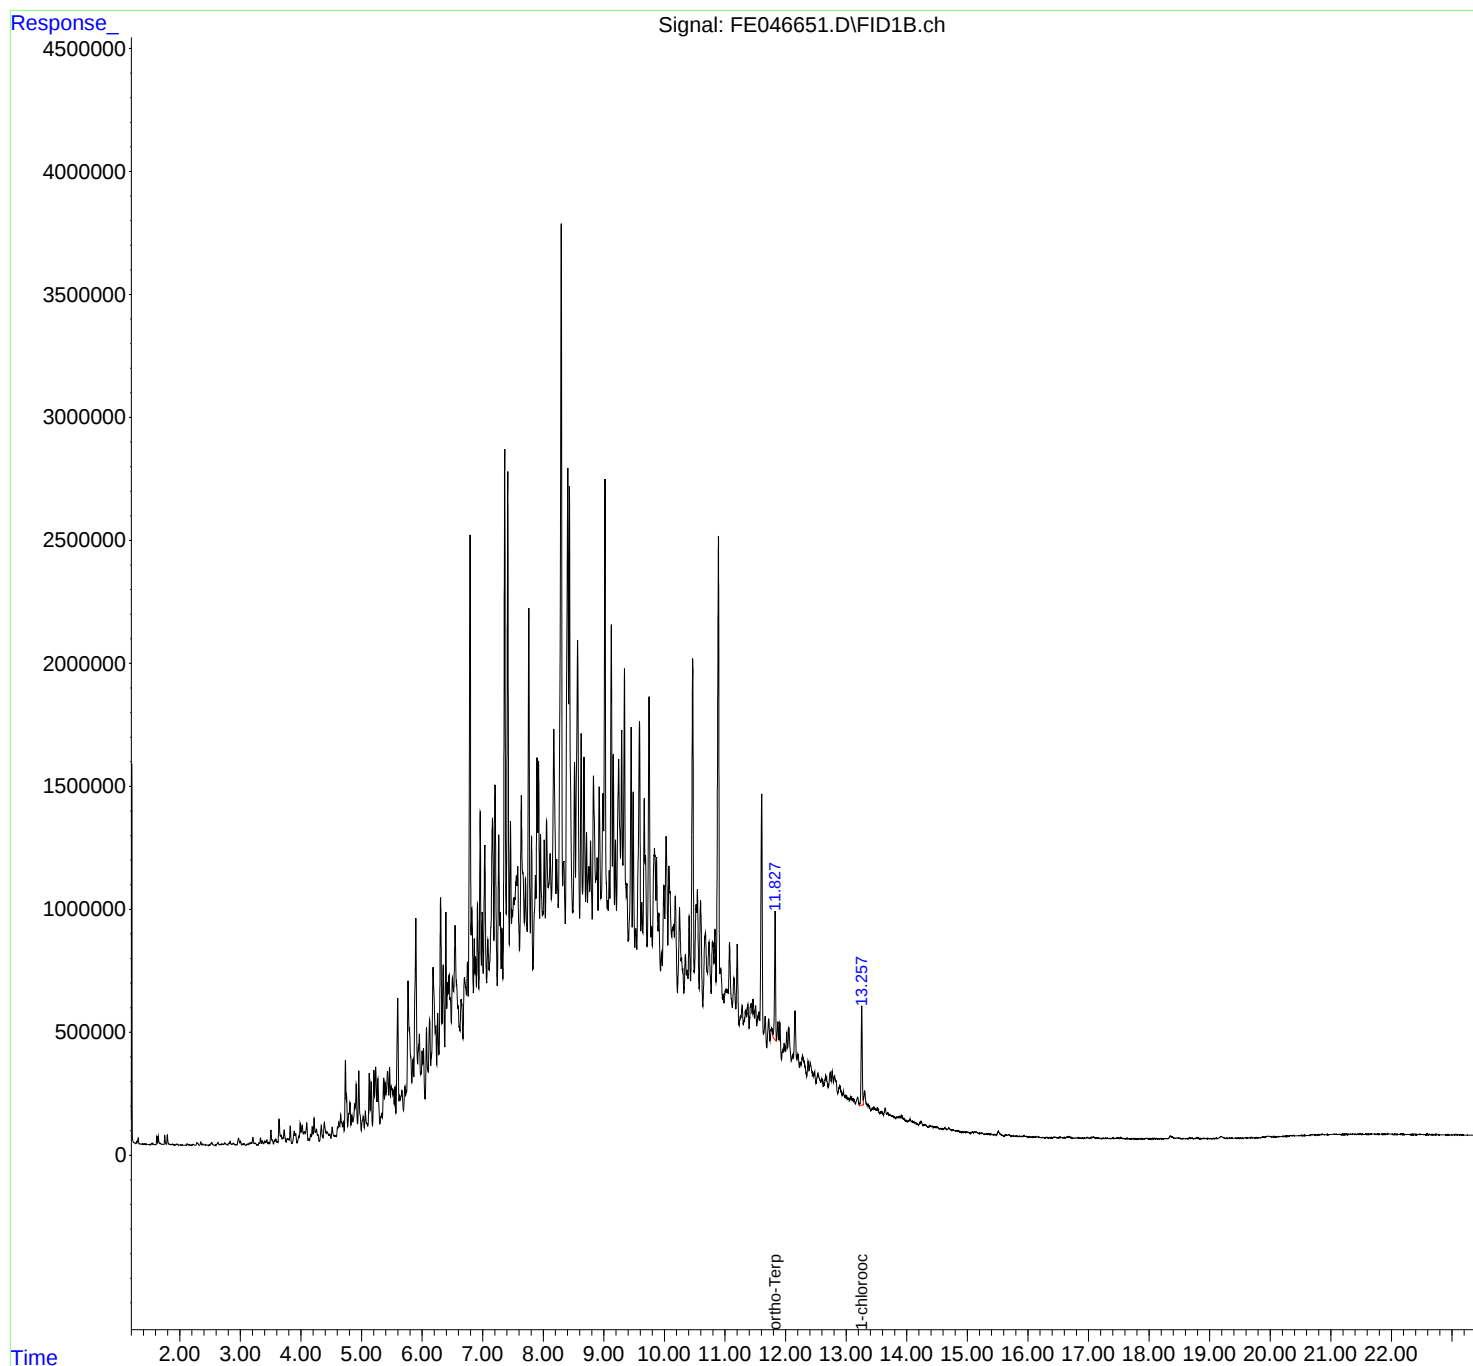

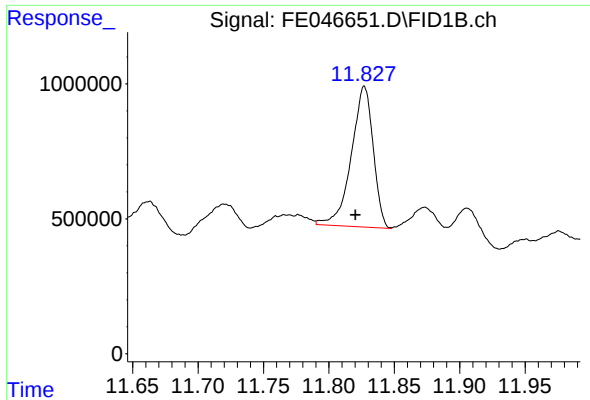


#9 ortho-Terphenyl (SURR)

R.T.: 11.827 min  
Delta R.T.: 0.006 min  
Response: 6074117  
Conc: 32.85 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
72-11929-E2

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 02/12/2024  
Supervised By :Ankita Jodhani 02/12/2024

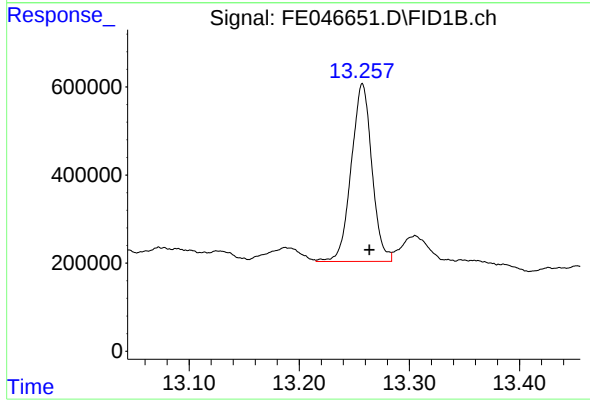

#12 1-chlorooctadecane (SURR)

R.T.: 13.257 min  
Delta R.T.: -0.007 min  
Response: 5263310  
Conc: 36.99 ug/ml m