

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE020923AL\
 Data File : FE040276.D
 Signal(s) : FID1B.ch
 Acq On : 09 Feb 2023 08:42
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 09 23:45:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 020223.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 02 04:52:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.872	153479	1.044 ug/ml
11) T n-Heneicosane (C21)	13.492	122737	0.832 ug/ml
13) T n-Docosane (C22)	14.081	136605	0.922 ug/ml
14) T n-Tetracosane (C24)	15.177	373636	2.461 ug/ml
15) T n-Hexacosane (C26)	16.211	93474	0.631 ug/ml
16) T n-Octacosane (C28)	17.162	115979	0.774 ug/ml
17) T n-Tricontane (C30)	18.050	138755	0.940 ug/ml
18) T n-Dotriacontane (C32)	18.882	221414	1.512 ug/ml
19) T n-Tetratriacontane (C34)	19.667	121370	0.882 ug/ml
20) T n-Hexatriacontane (C36)	20.410	136610	1.030 ug/ml
21) T n-Octatriacontane (C38)	21.142	132012	1.018 ug/ml
22) T n-Tetracontane (C40)	22.039	219171	1.651 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE020923AL\
Data File : FE040276.D
Signal(s) : FID1B.ch
Acq On : 09 Feb 2023 08:42
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 09 23:45:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 020223.M
Quant Title : GC Extractables
QLast Update : Thu Feb 02 04:52:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

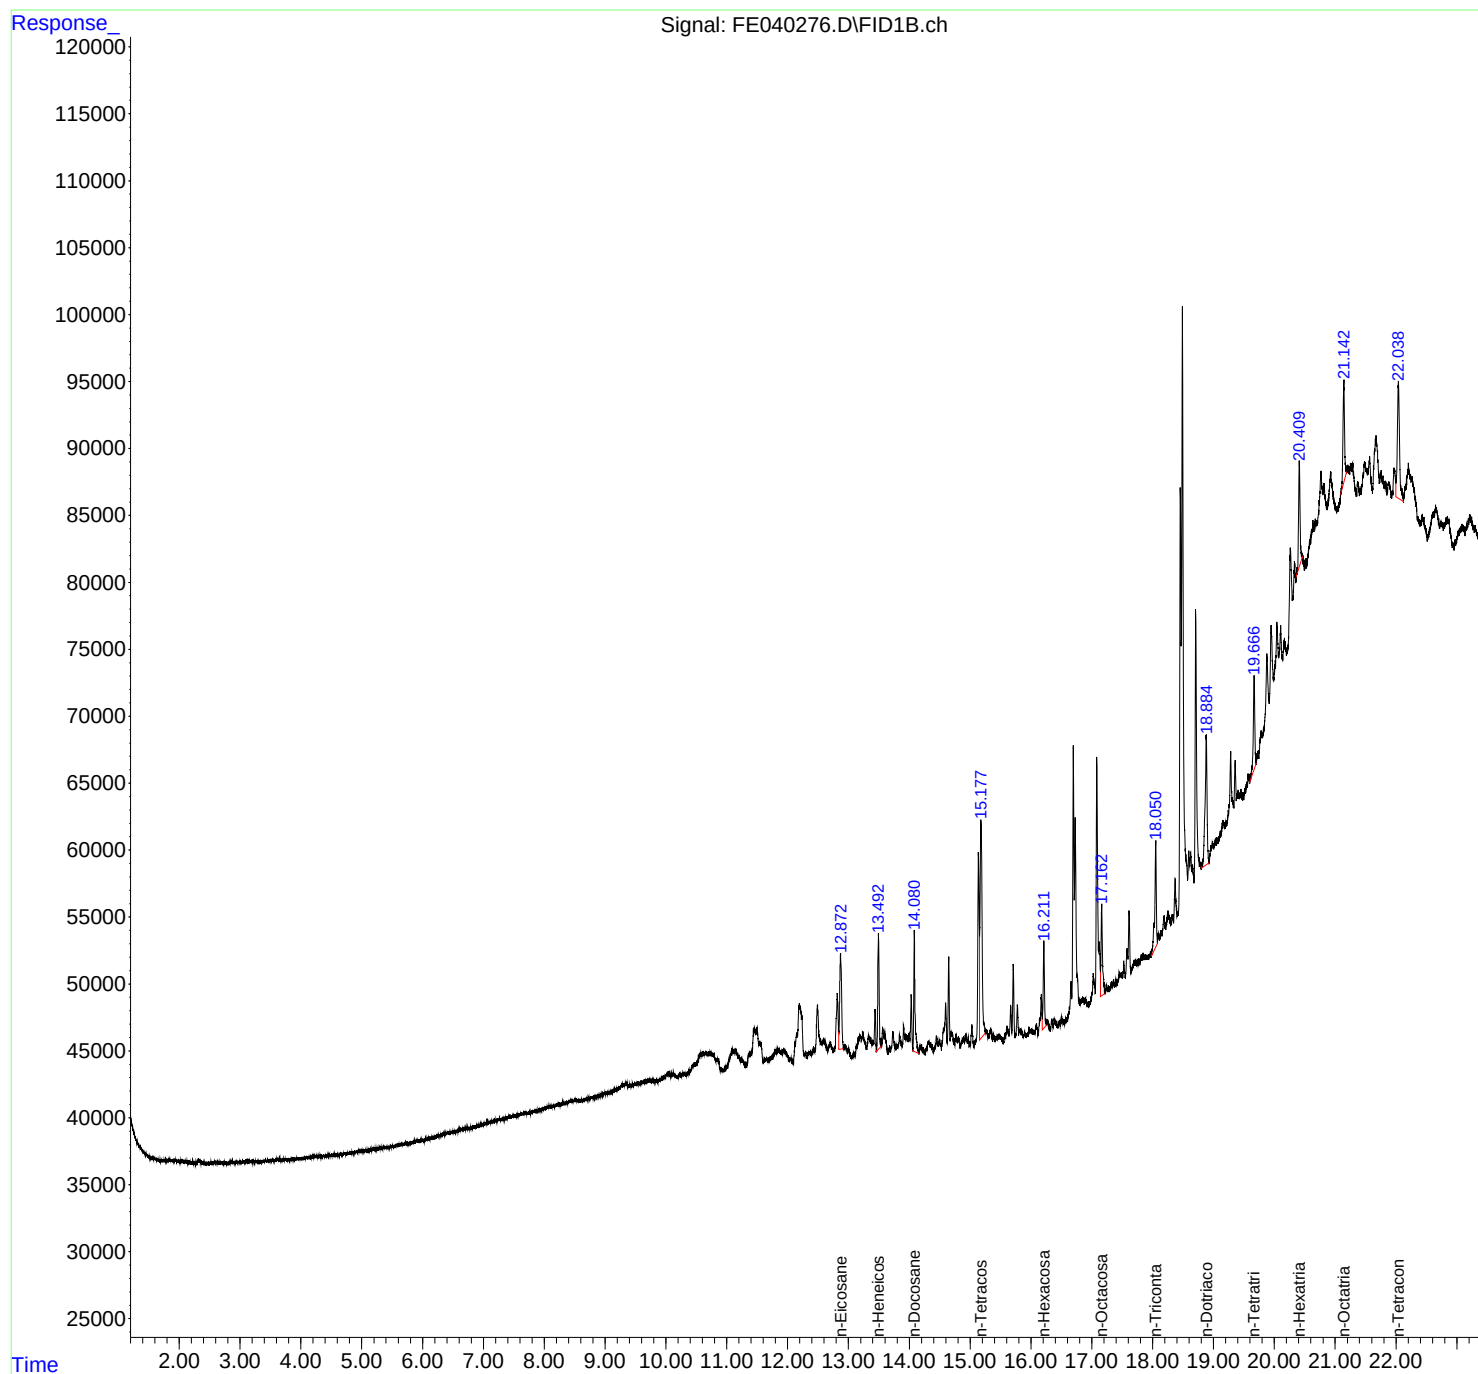


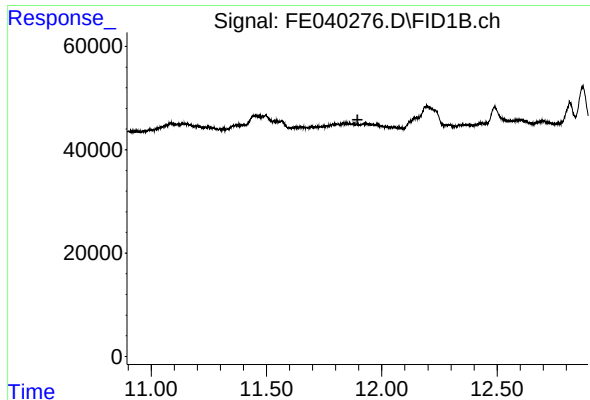

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.895 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

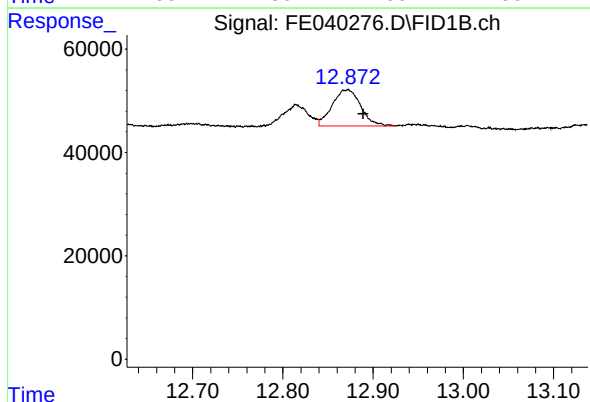


#10 n-Eicosane (C20)

R.T.: 12.872 min
Delta R.T.: -0.017 min
Response: 153479
Conc: 1.04 ug/ml

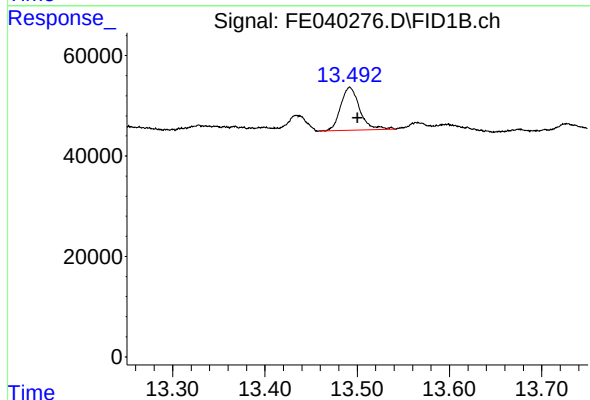


#11 n-Heneicosane (C21)

R.T.: 13.492 min
Delta R.T.: -0.009 min
Response: 122737
Conc: 0.83 ug/ml

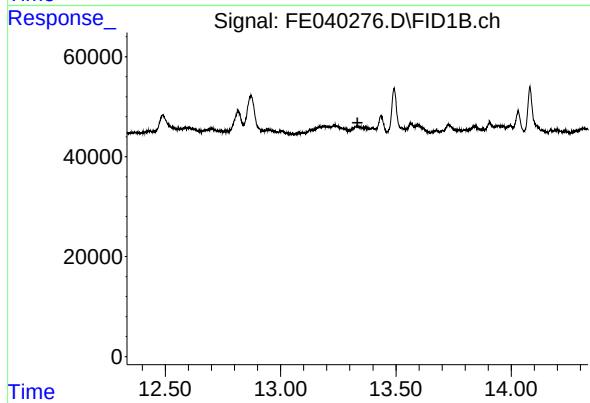

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.333 min
Response: 0
Conc: N.D.

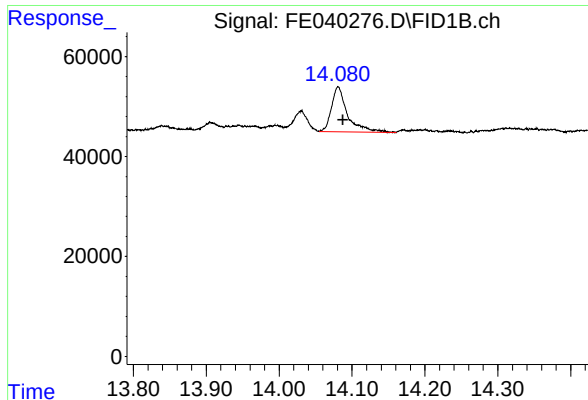

#13 n-Docosane (C22)


R.T.: 14.081 min
Delta R.T.: -0.007 min
Response: 136605
Conc: 0.92 ug/ml

Instrument :
FID_E
ClientSampleId :

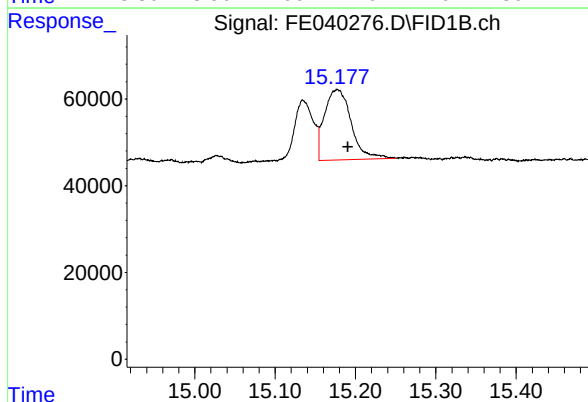


#14 n-Tetracosane (C24)

R.T.: 15.177 min
Delta R.T.: -0.013 min
Response: 373636
Conc: 2.46 ug/ml

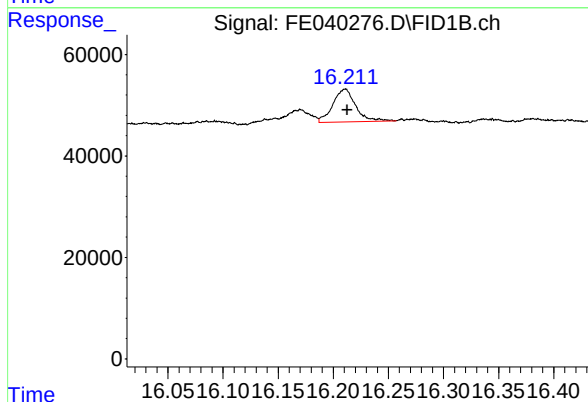


#15 n-Hexacosane (C26)

R.T.: 16.211 min
Delta R.T.: -0.002 min
Response: 93474
Conc: 0.63 ug/ml

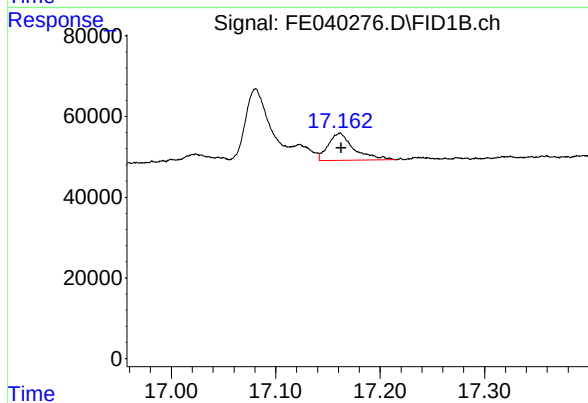

#16 n-Octacosane (C28)


R.T.: 17.162 min
Delta R.T.: -0.001 min
Response: 115979
Conc: 0.77 ug/ml

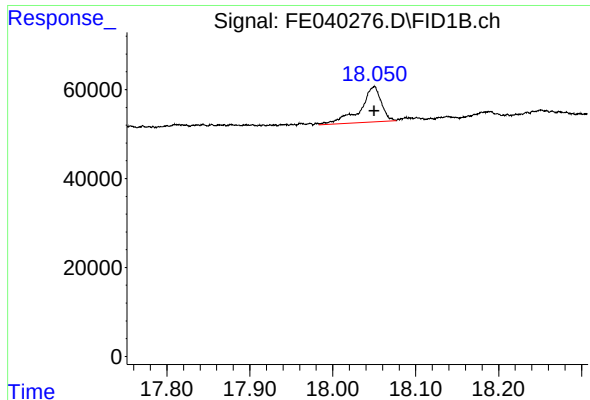

#17 n-Tricontane (C30)


R.T.: 18.050 min
Delta R.T.: 0.000 min
Response: 138755
Conc: 0.94 ug/ml

Instrument :
FID_E
ClientSampleId :

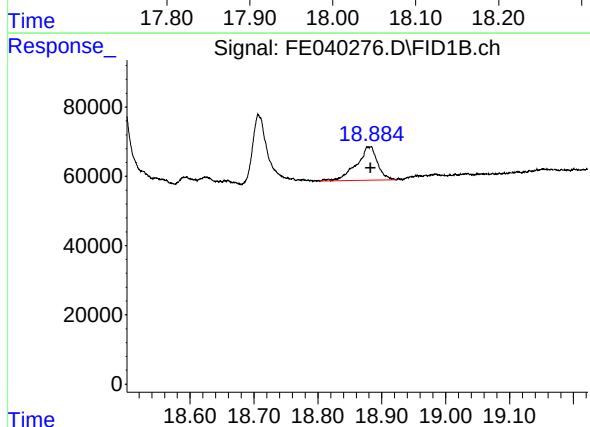


#18 n-Dotriacontane (C32)

R.T.: 18.882 min
Delta R.T.: 0.000 min
Response: 221414
Conc: 1.51 ug/ml

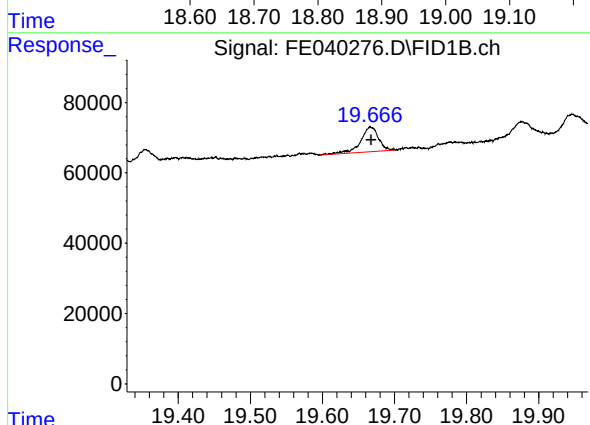


#19 n-Tetratriacontane (C34)

R.T.: 19.667 min
Delta R.T.: 0.000 min
Response: 121370
Conc: 0.88 ug/ml

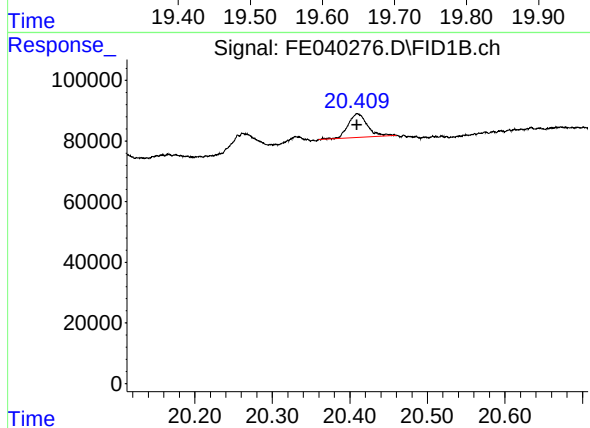

#20 n-Hexatriacontane (C36)


R.T.: 20.410 min
Delta R.T.: 0.000 min
Response: 136610
Conc: 1.03 ug/ml

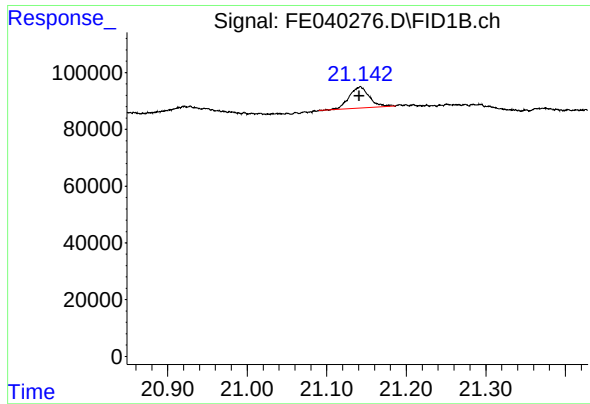

#21 n-Octatriacontane (C38)

R.T.: 21.142 min
Delta R.T.: 0.001 min
Response: 132012
Conc: 1.02 ug/ml

Instrument :
FID_E
ClientSampleId :

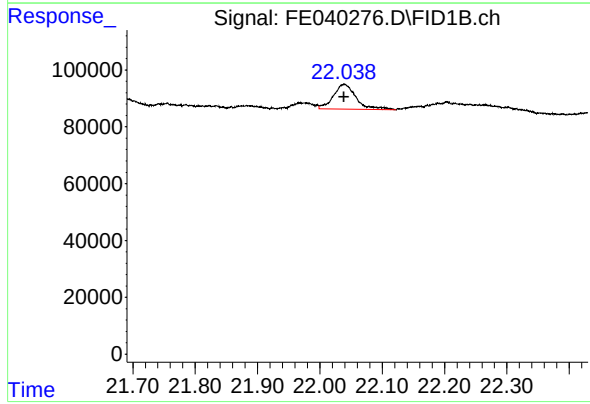

#22 n-Tetracontane (C40)

R.T.: 22.039 min
Delta R.T.: 0.000 min
Response: 219171
Conc: 1.65 ug/ml