

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE020923AL\
 Data File : FE040282.D
 Signal(s) : FID1B.ch
 Acq On : 09 Feb 2023 13:52
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 09 23:46:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 020223.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 02 04:52:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
17) T n-Tricontane (C30)	18.052	45528	0.309 ug/ml
18) T n-Dotriacontane (C32)	18.885	74092	0.506 ug/ml
19) T n-Tetratriacontane (C34)	19.669	67303	0.489 ug/ml
20) T n-Hexatriacontane (C36)	20.412	123954	0.935 ug/ml
21) T n-Octatriacontane (C38)	21.142	75354	0.581 ug/ml
22) T n-Tetracontane (C40)	22.040	91209	0.687 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE020923AL\
Data File : FE040282.D
Signal(s) : FID1B.ch
Acq On : 09 Feb 2023 13:52
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 09 23:46:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 020223.M
Quant Title : GC Extractables
QLast Update : Thu Feb 02 04:52:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

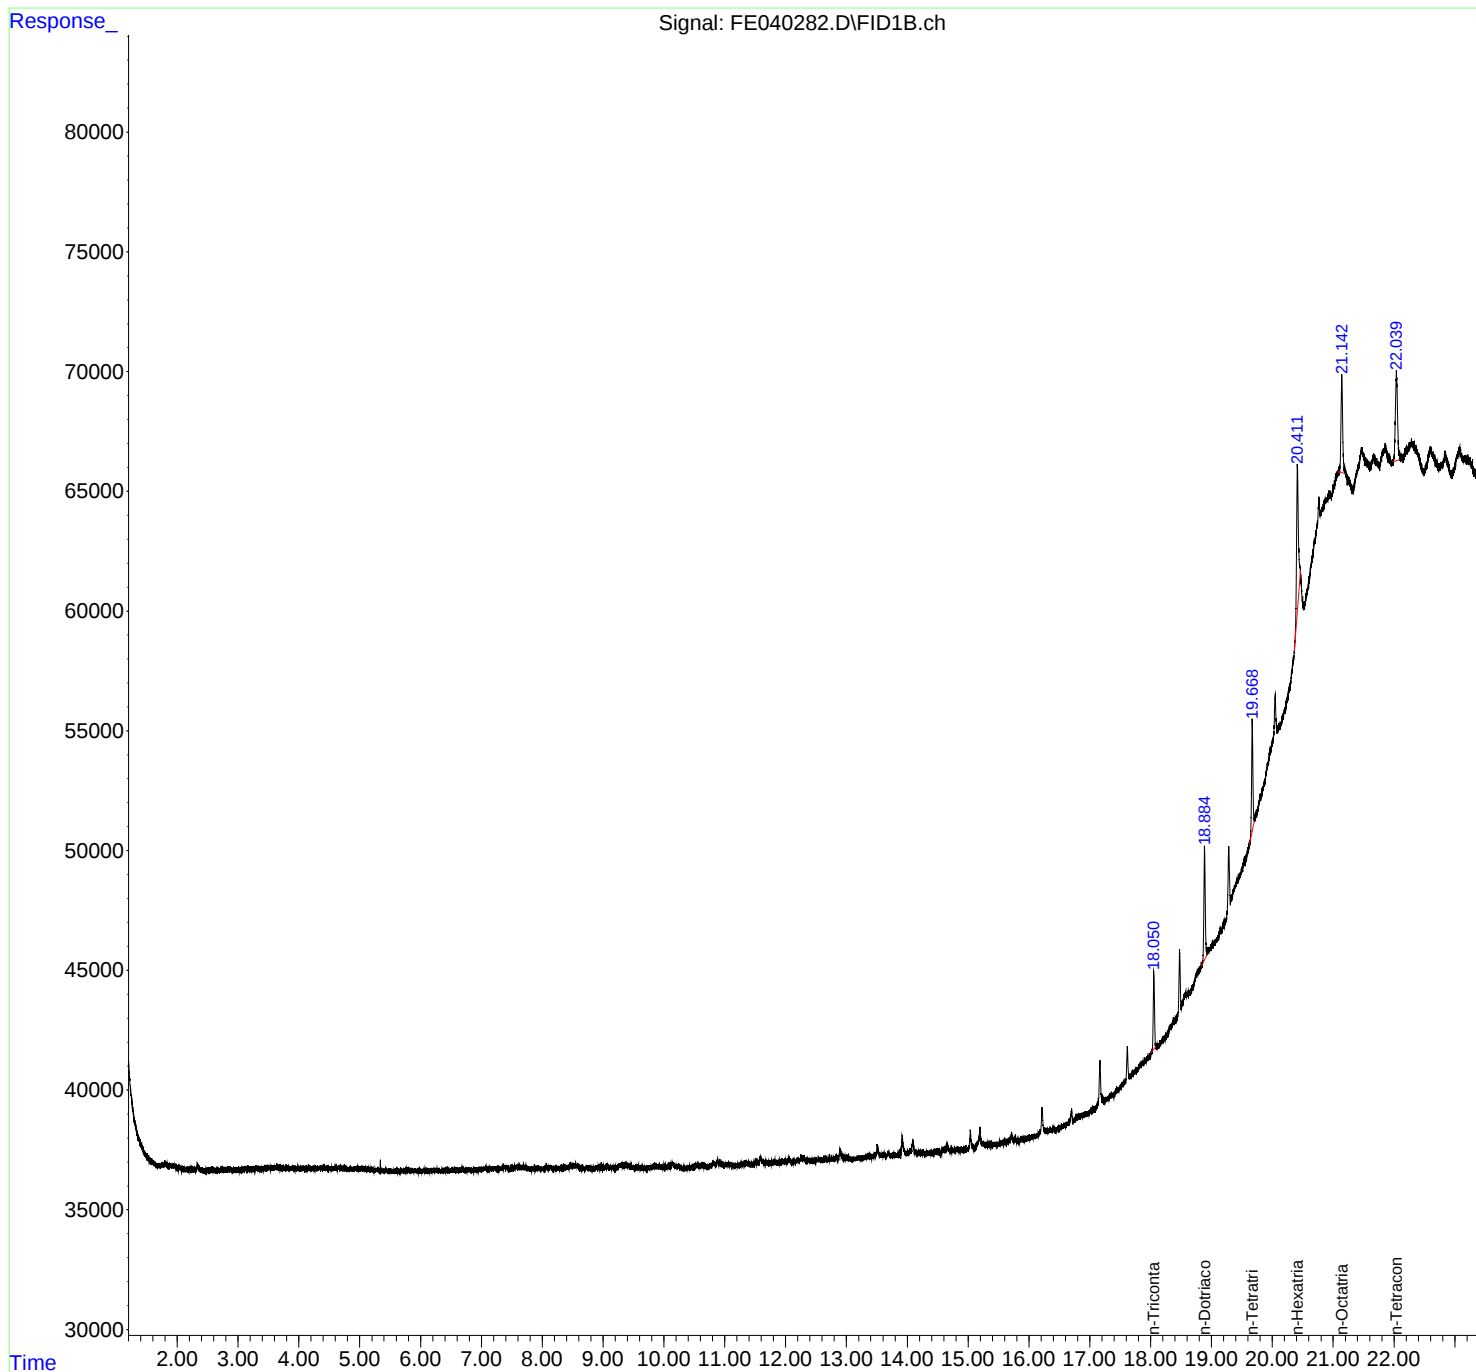


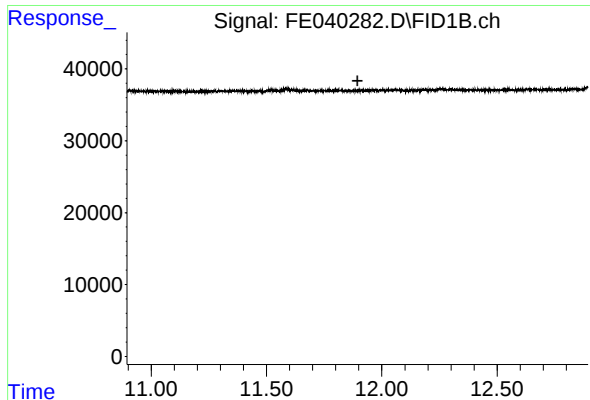

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.895 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

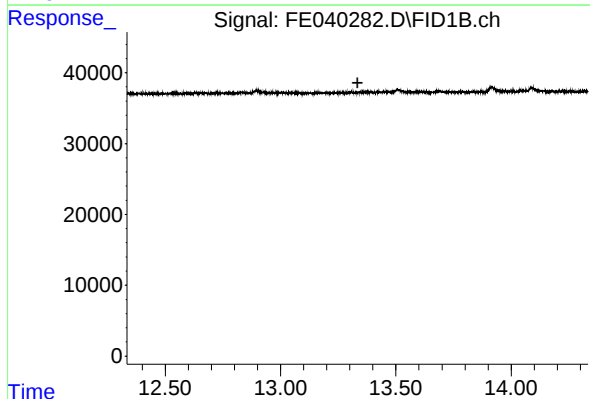


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.333 min
Response: 0
Conc: N.D.

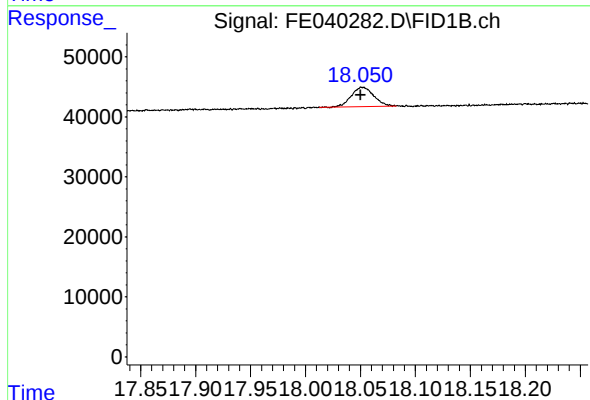


#17 n-Tricontane (C30)

R.T.: 18.052 min
Delta R.T.: 0.001 min
Response: 45528
Conc: 0.31 ug/ml

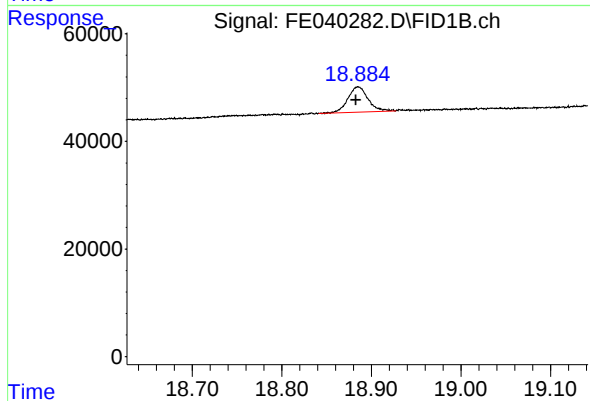

#18 n-Dotriacontane (C32)

R.T.: 18.885 min
Delta R.T.: 0.002 min
Response: 74092
Conc: 0.51 ug/ml

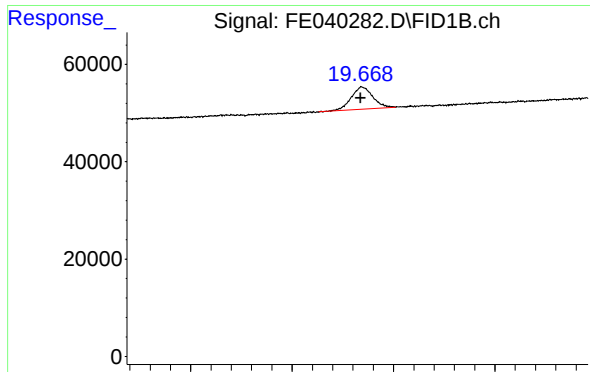


#19 n-Tetratriacontane (C34)

R.T.: 19.669 min
Delta R.T.: 0.001 min
Response: 67303
Conc: 0.49 ug/ml

Instrument :


FID_E

ClientSampleId :

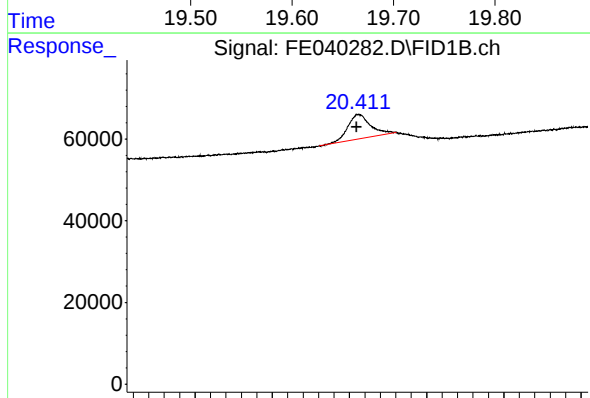


#20 n-Hexatriacontane (C36)

R.T.: 20.412 min
Delta R.T.: 0.003 min
Response: 123954
Conc: 0.93 ug/ml

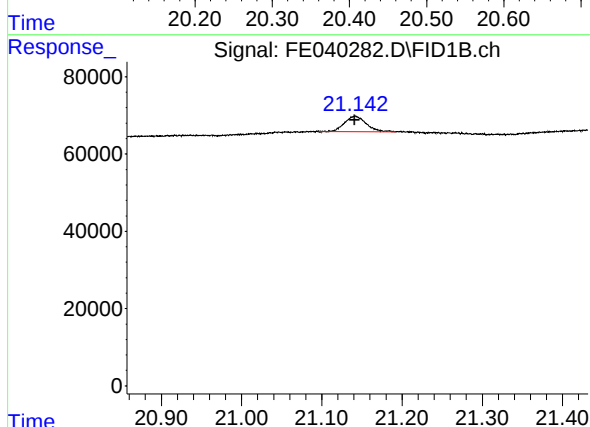

#21 n-Octatriacontane (C38)

R.T.: 21.142 min
Delta R.T.: 0.001 min
Response: 75354
Conc: 0.58 ug/ml

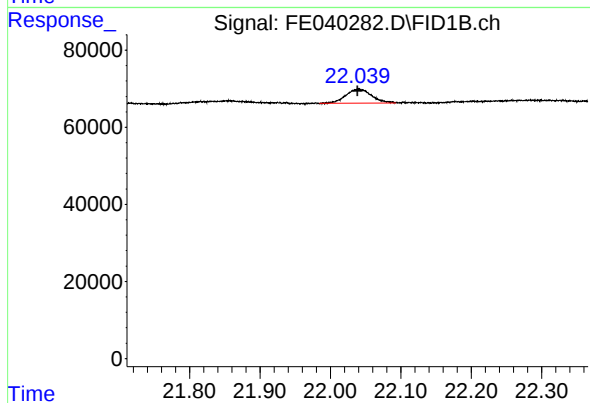

#22 n-Tetracontane (C40)

R.T.: 22.040 min
Delta R.T.: 0.001 min
Response: 91209
Conc: 0.69 ug/ml