

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE020924AL\  
 Data File : FE046664.D  
 Signal(s) : FID1B.ch  
 Acq On : 09 Feb 2024 09:30  
 Operator : YP\AJ  
 Sample : P1411-01DL 5X  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :

Manual Integrations  
 APPROVED

Reviewed By :Ankita Jodhani 02/12/2024  
 Supervised By :Sohil Jodhani 02/12/2024

Integration File: autoint1.e  
 Quant Time: Feb 10 03:52:44 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 012524.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Jan 25 14:56:03 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.813 | 1154476    | 6.243 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 12.49%       |
| 12) S 1-chlorooctadecane (S... | 13.254 | 959108     | 6.741 ug/ml  |
| Spiked Amount 50.000           |        | Recovery = | 13.48%       |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE020924AL\  
Data File : FE046664.D  
Signal(s) : FID1B.ch  
Acq On : 09 Feb 2024 09:30  
Operator : YP\AJ  
Sample : P1411-01DL 5X  
Misc :  
ALS Vial : 3 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :


Manual Integrations  
APPROVED

Reviewed By :Ankita Jodhani 02/12/2024  
Supervised By :Sohil Jodhani 02/12/2024

Integration File: autoint1.e  
Quant Time: Feb 10 03:52:44 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 012524.M  
Quant Title : GC Extractables  
QLast Update : Thu Jan 25 14:56:03 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 u1  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

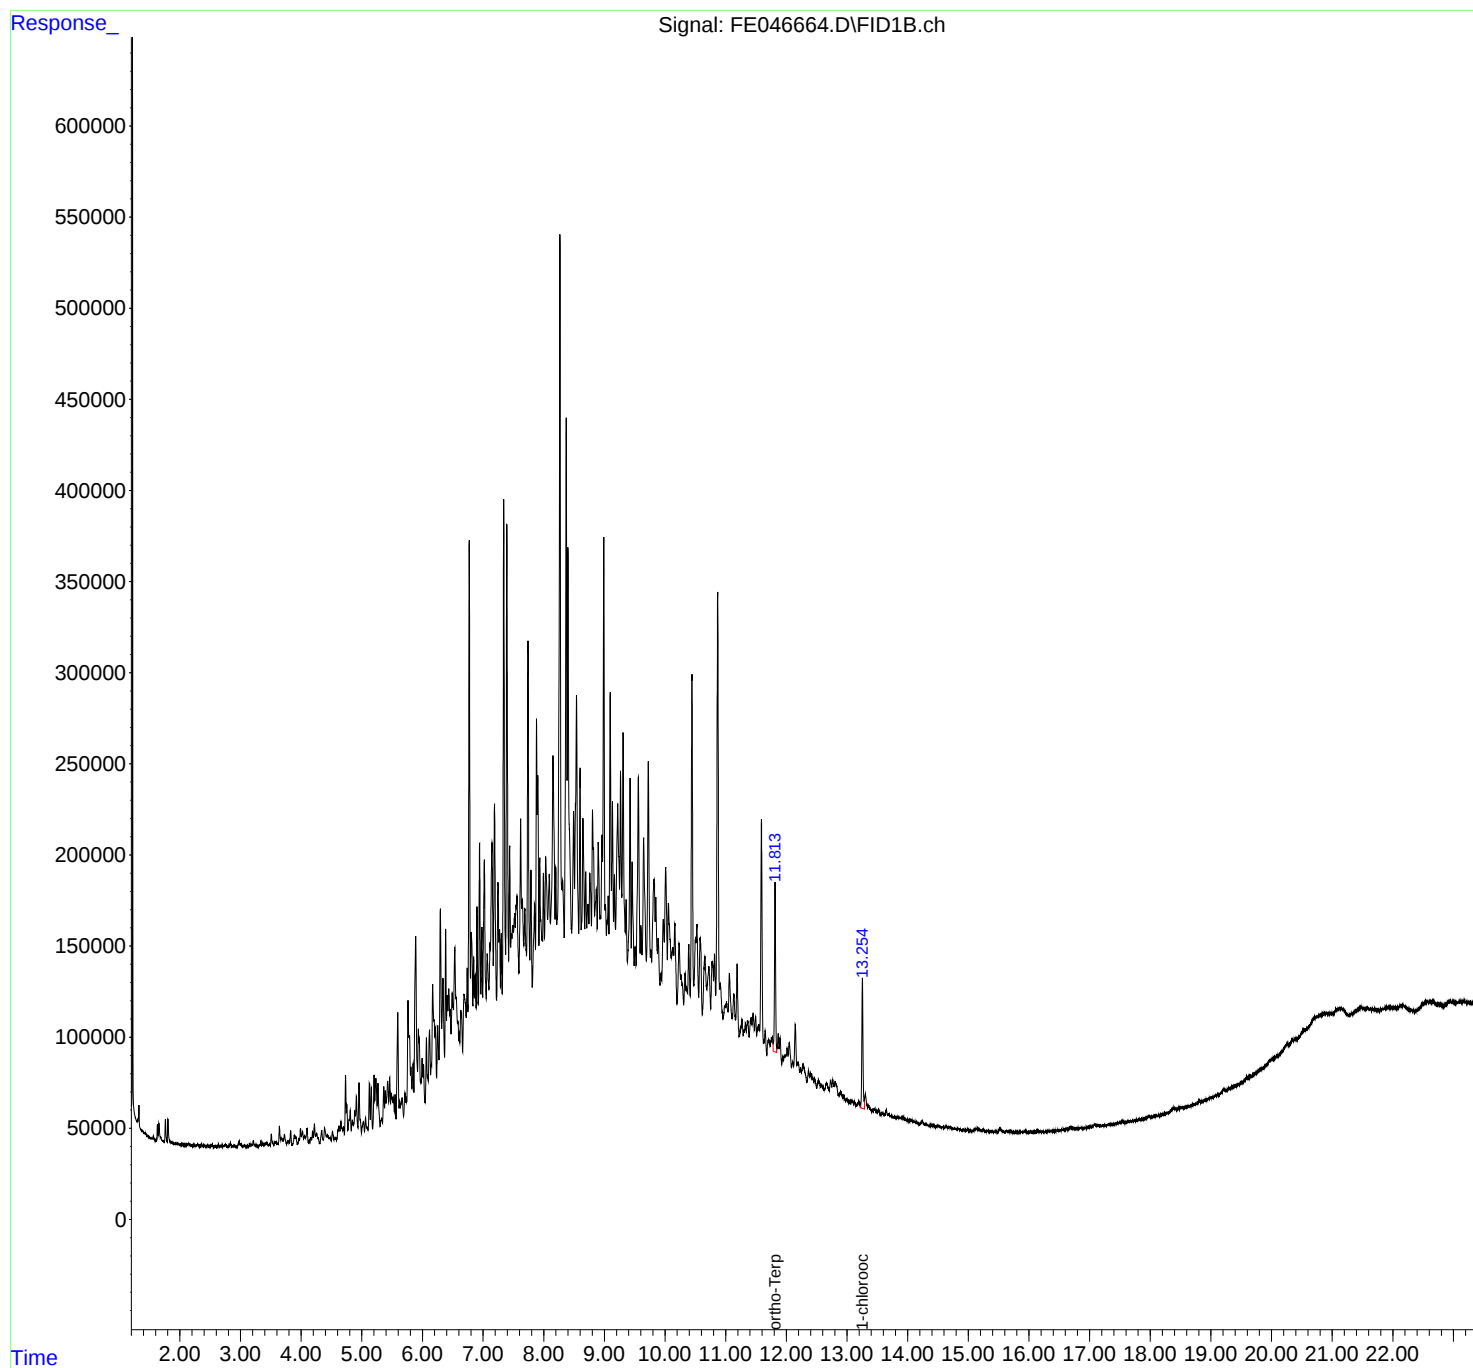

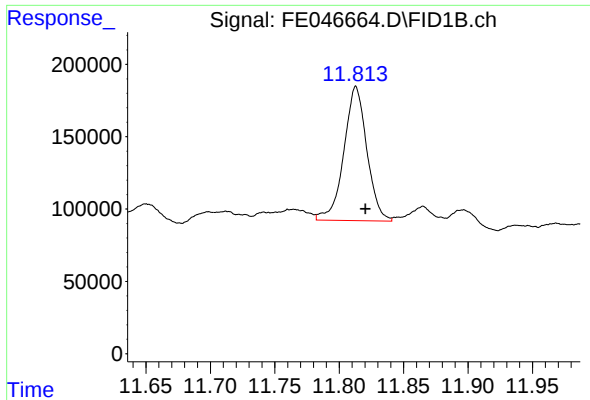


#9 ortho-Terphenyl (SURR)

R.T.: 11.813 min  
Delta R.T.: -0.008 min  
Response: 1154476  
Conc: 6.24 ug/ml

Instrument :  
FID\_E  
ClientSampleId :

Manual Integrations  
APPROVED

Reviewed By :Ankita Jodhani 02/12/2024  
Supervised By :Sohil Jodhani 02/12/2024

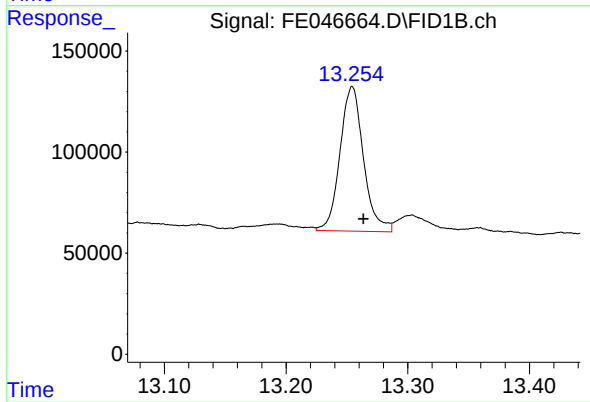

#12 1-chlorooctadecane (SURR)

R.T.: 13.254 min  
Delta R.T.: -0.009 min  
Response: 959108  
Conc: 6.74 ug/ml