

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE021122AL\
 Data File : FE035002.D
 Signal(s) : FID1B.CH
 Acq On : 11 Feb 2022 11:25
 Operator : YP\AJ
 Sample : N1465-06DL 25X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 A5-6-8.5DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/14/2022
 Supervised By :Ankita Jodhani 02/14/2022

Integration File: sample.E
 Quant Time: Feb 11 13:39:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 020822.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 08 22:05:03 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.114	685058	2.339 ug/mlm
Spiked Amount 50.000		Recovery =	4.68%
12) S 1-chlorooctadecane (S...	12.546	414362	1.853 ug/mlm
Spiked Amount 50.000		Recovery =	3.71%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE021122AL\
Data File : FE035002.D
Signal(s) : FID1B.CH
Acq On : 11 Feb 2022 11:25
Operator : YP\AJ
Sample : N1465-06DL 25X
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
A5-6-8.5DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/14/2022
Supervised By :Ankita Jodhani 02/14/2022

Integration File: sample.E
Quant Time: Feb 11 13:39:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 020822.M
Quant Title : GC Extractables
QLast Update : Tue Feb 08 22:05:03 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

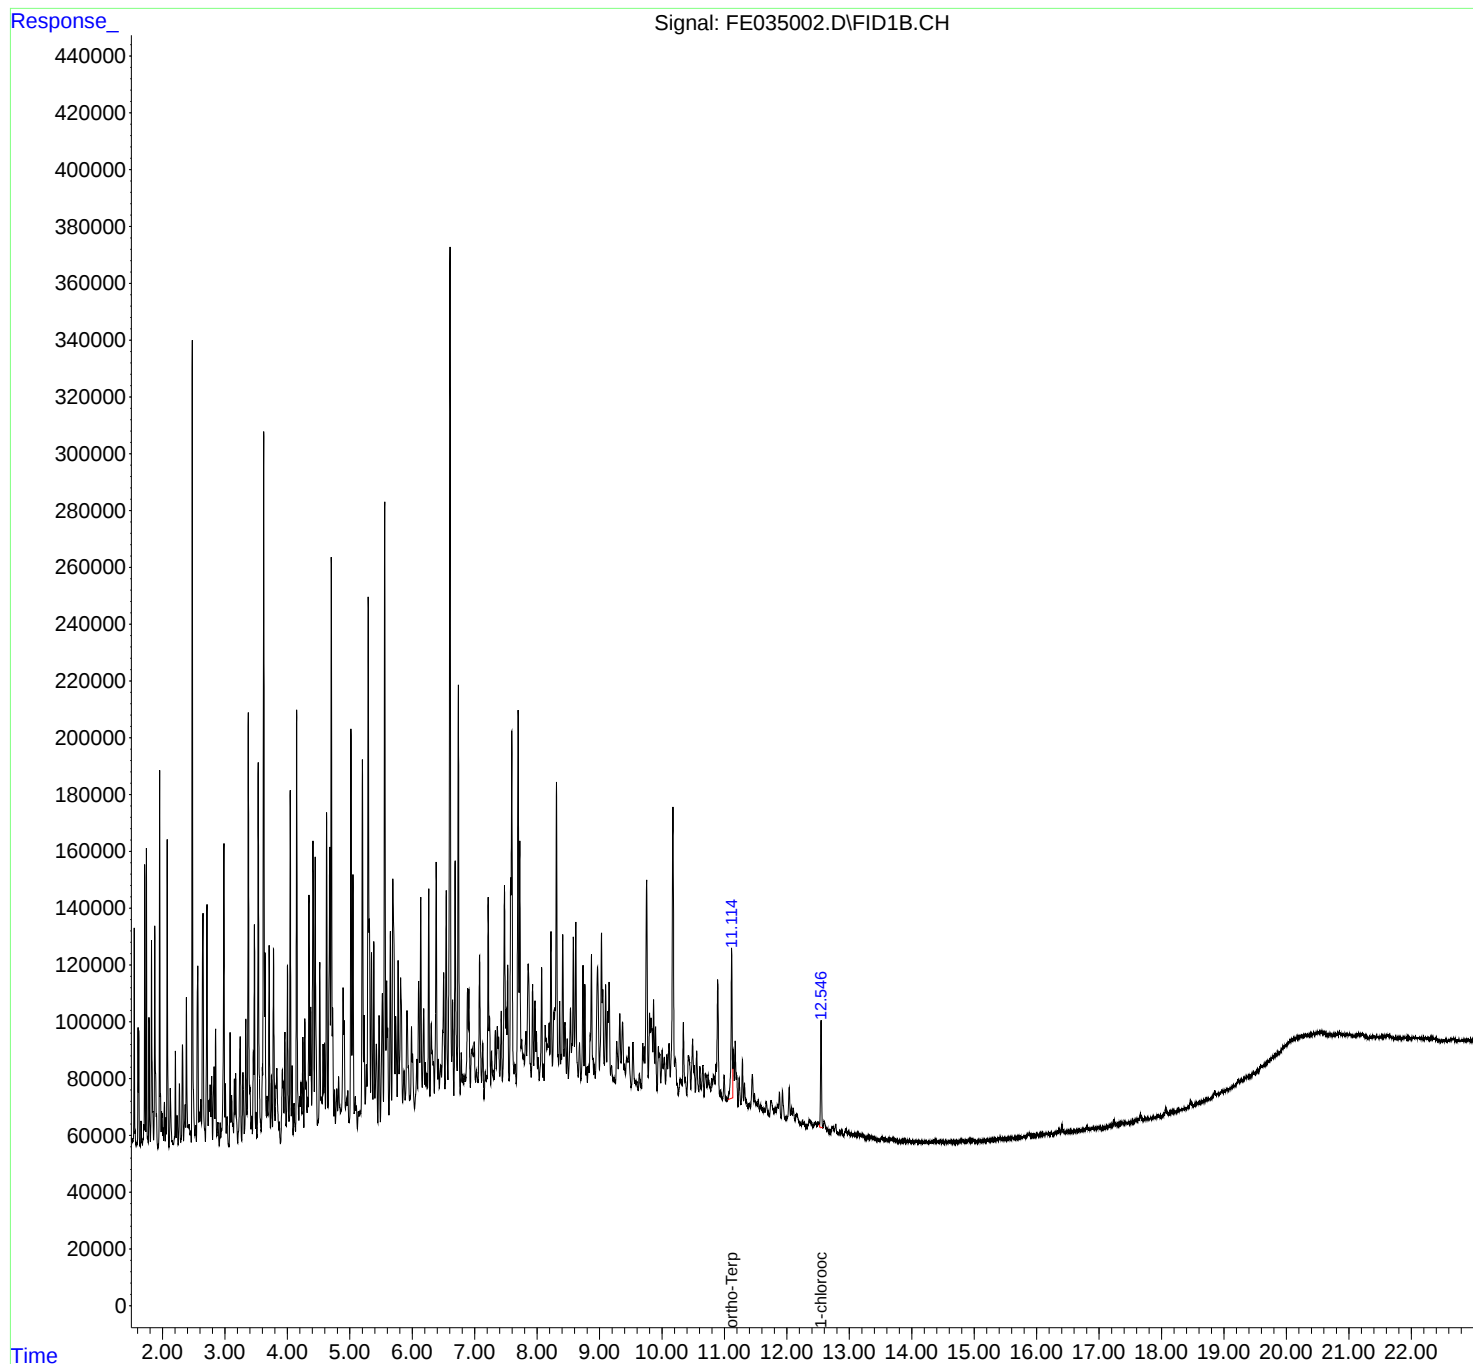

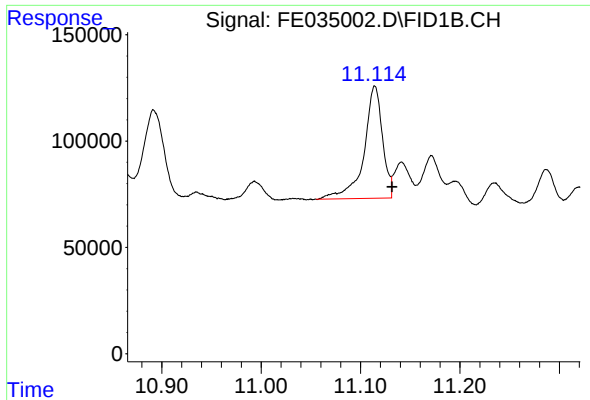


#9 ortho-Terphenyl (SURR)

R.T.: 11.114 min
Delta R.T.: -0.018 min
Response: 685058
Conc: 2.34 ug/ml

Instrument :
FID_E
ClientSampleId :
A5-6-8.5DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/14/2022
Supervised By :Ankita Jodhani 02/14/2022

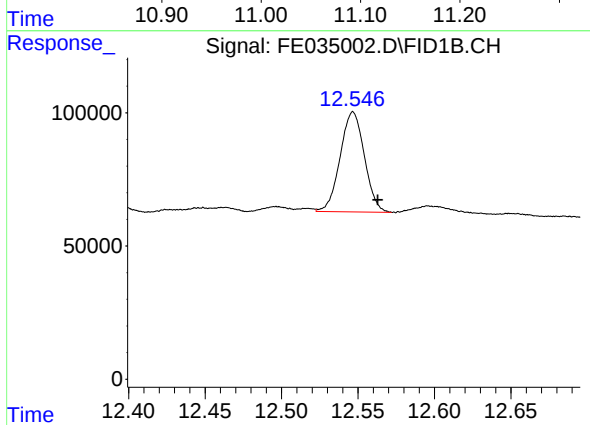

#12 1-chlorooctadecane (SURR)

R.T.: 12.546 min
Delta R.T.: -0.017 min
Response: 414362
Conc: 1.85 ug/ml m