

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE021324AL\
Data File : FE046748.D
Signal(s) : FID1B.ch
Acq On : 13 Feb 2024 14:50
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 13 23:10:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 012524.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 14:56:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.812	22415	0.148 ug/ml
21) T	n-Octatriacontane (C38)	21.077	121205	0.945 ug/ml
22) T	n-Tetracontane (C40)	21.983	115721	0.925 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE021324AL\
Data File : FE046748.D
Signal(s) : FID1B.ch
Acq On : 13 Feb 2024 14:50
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 13 23:10:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 012524.M
Quant Title : GC Extractables
QLast Update : Thu Jan 25 14:56:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

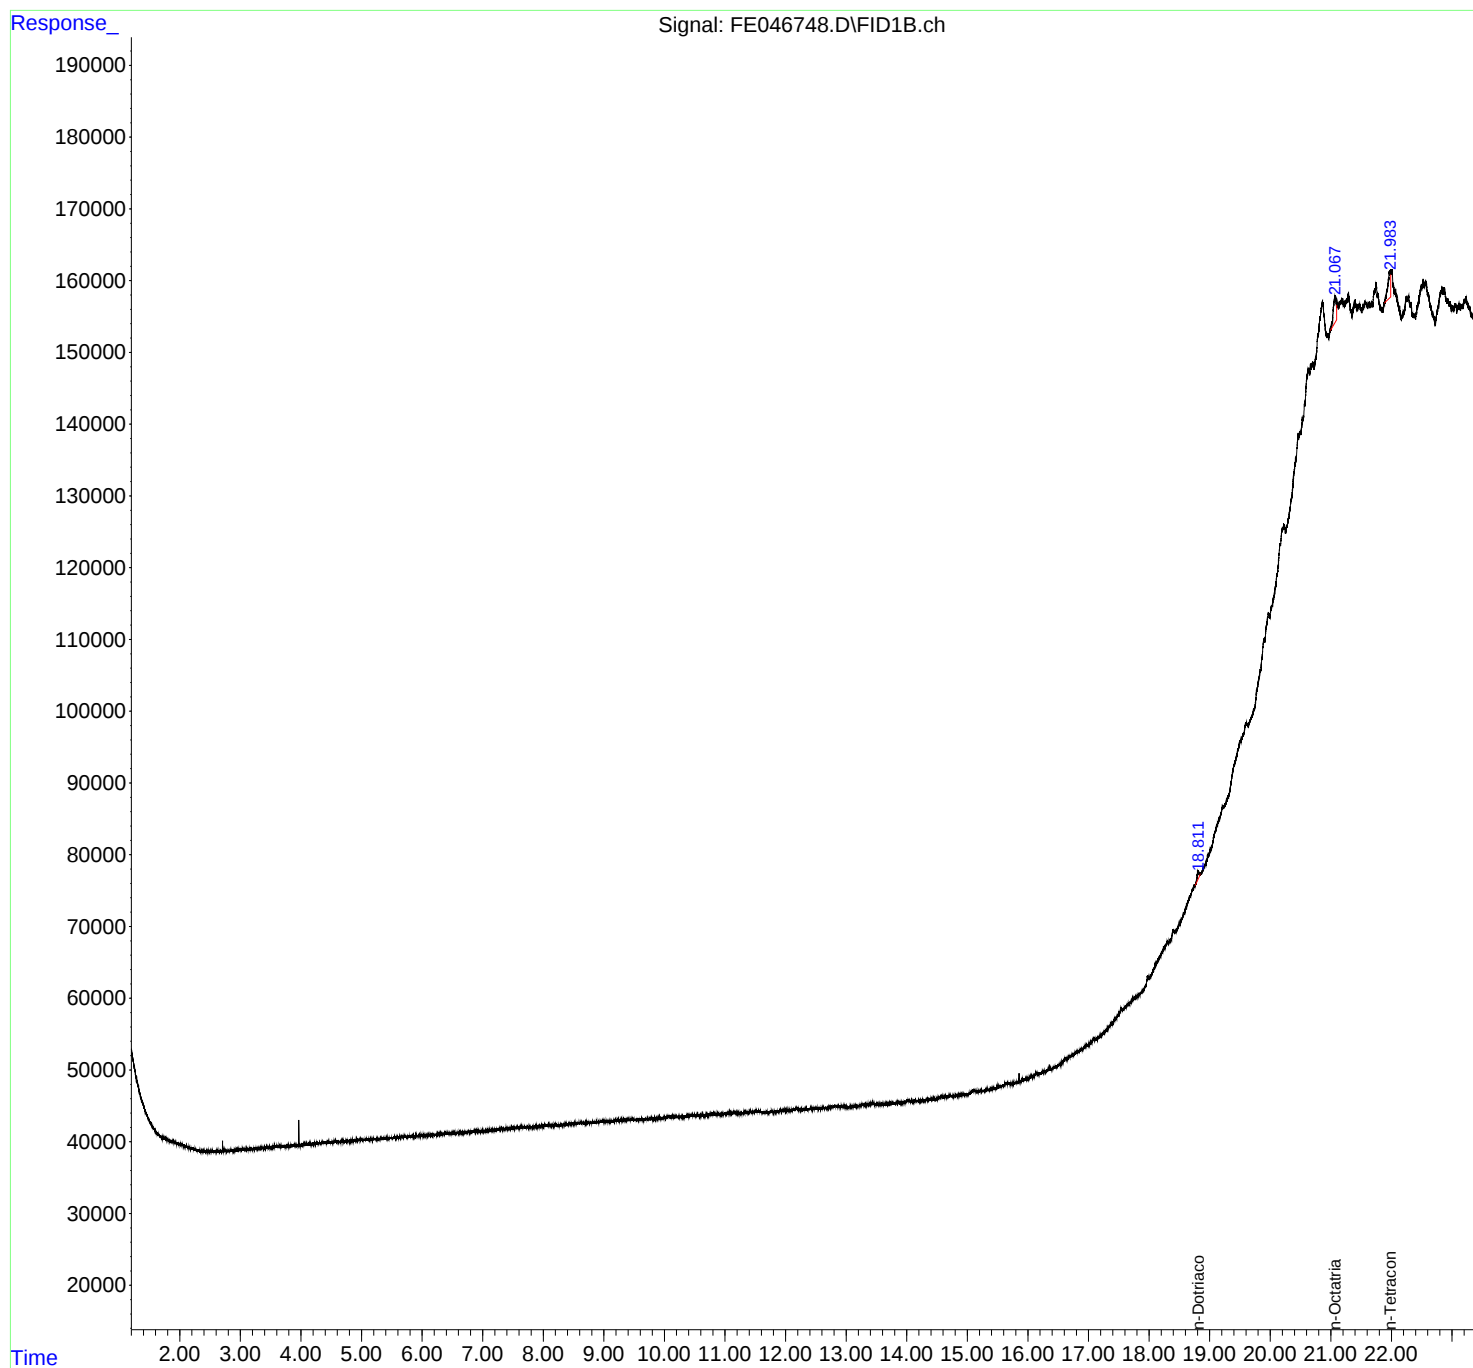


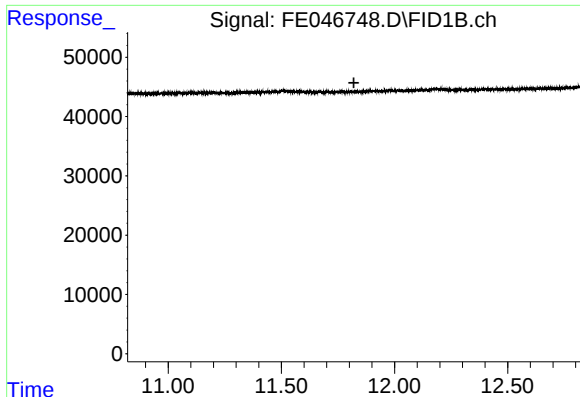

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.820 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

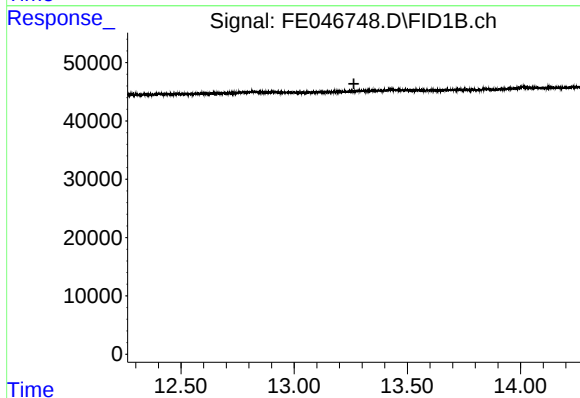


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.264 min
Response: 0
Conc: N.D.

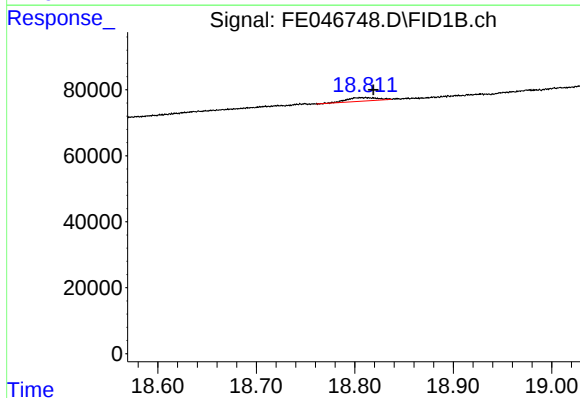


#18 n-Dotriacontane (C32)

R.T.: 18.812 min
Delta R.T.: -0.007 min
Response: 22415
Conc: 0.15 ug/ml

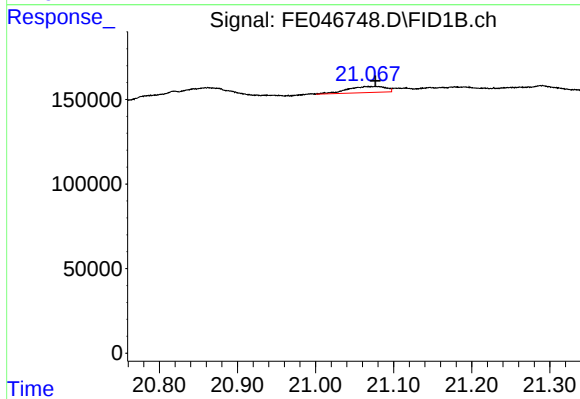

#21 n-Octatriacontane (C38)

R.T.: 21.077 min
Delta R.T.: 0.000 min
Response: 121205
Conc: 0.95 ug/ml

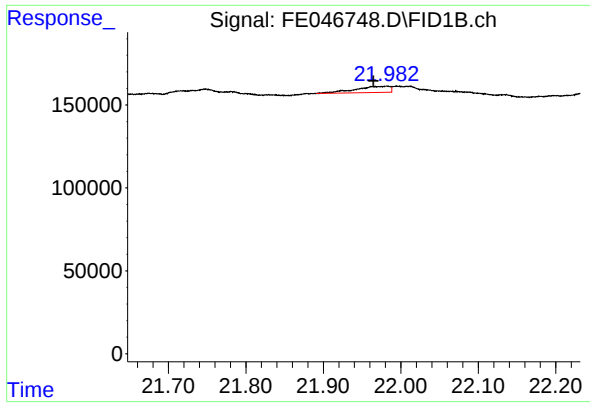

#22 n-Tetracontane (C40)

R.T.: 21.983 min
Delta R.T.: 0.018 min
Response: 115721
Conc: 0.93 ug/ml

Instrument :
FID_E
ClientSampleId :