

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE022023AL\  
 Data File : FE040435.D  
 Signal(s) : FID1B.ch  
 Acq On : 20 Feb 2023 09:32  
 Operator : YP\AJ  
 Sample : 01587-01DL 2X  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 OK-02-02162023DL

Integration File: autoint1.e  
 Quant Time: Feb 21 02:07:37 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 020223.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Feb 02 04:52:48 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.890 | 2538030    | 15.680 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 31.36%       |
| 12) S 1-chlorooctadecane (S... | 13.328 | 3167805    | 25.542 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 51.08%       |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE022023AL\  
Data File : FE040435.D  
Signal(s) : FID1B.ch  
Acq On : 20 Feb 2023 09:32  
Operator : YP\AJ  
Sample : 01587-01DL 2X  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
OK-02-02162023DL

Integration File: autoint1.e  
Quant Time: Feb 21 02:07:37 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 020223.M  
Quant Title : GC Extractables  
QLast Update : Thu Feb 02 04:52:48 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

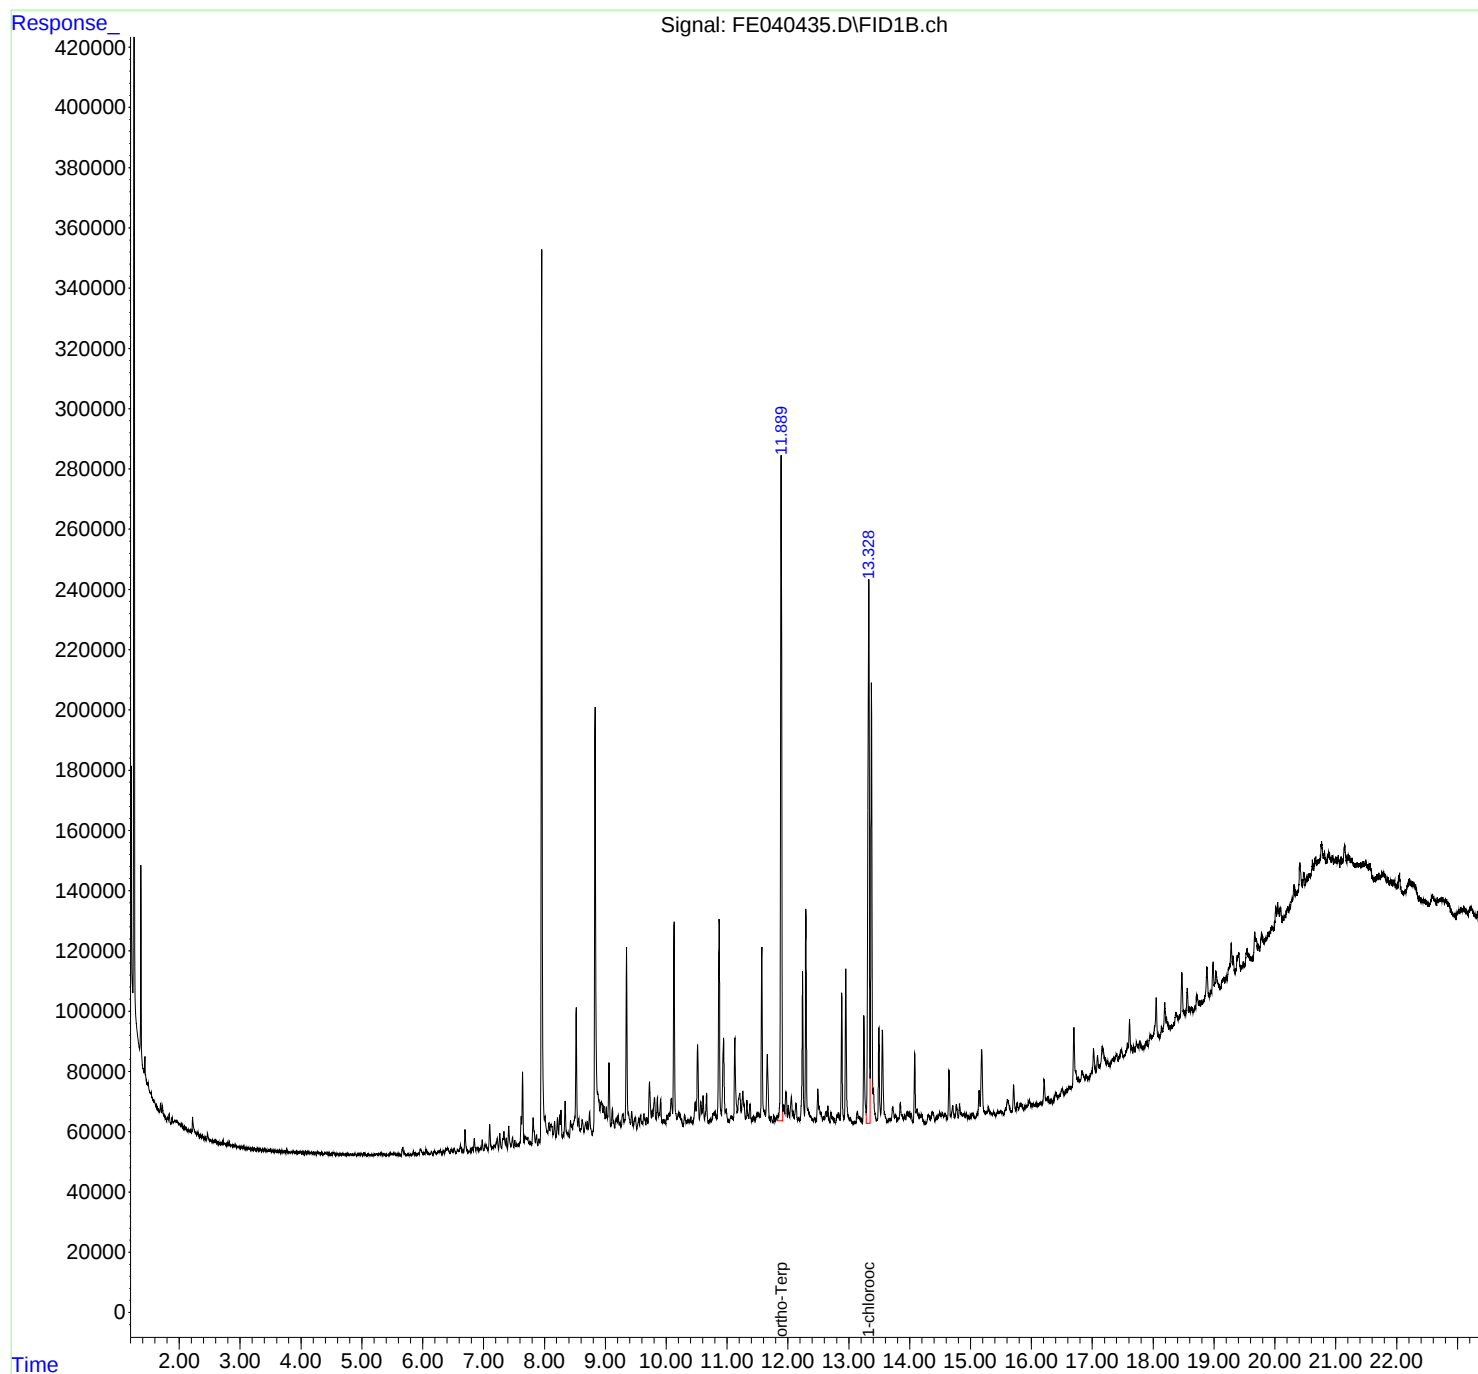


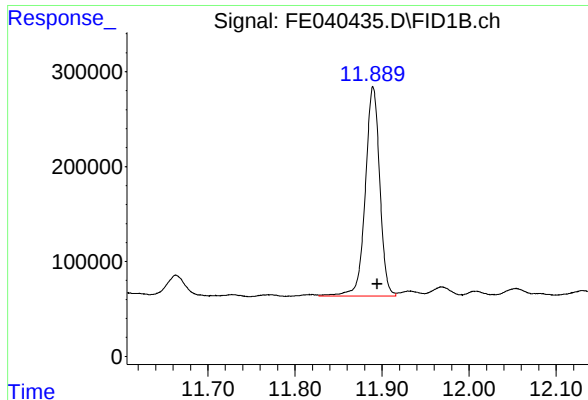

#9 ortho-Terphenyl (SURR)

R.T.: 11.890 min  
Delta R.T.: -0.005 min  
Response: 2538030  
Conc: 15.68 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
OK-02-02162023DL

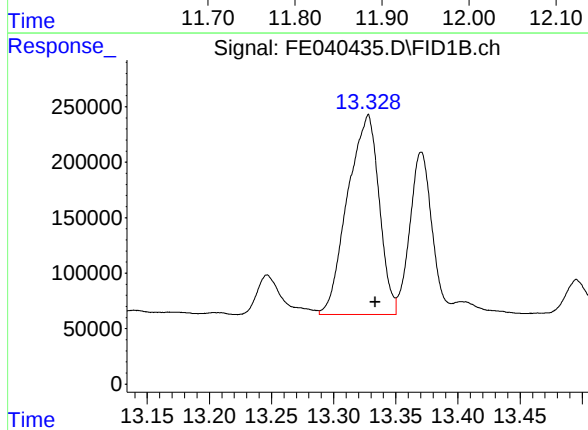

#12 1-chlorooctadecane (SURR)

R.T.: 13.328 min  
Delta R.T.: -0.006 min  
Response: 3167805  
Conc: 25.54 ug/ml