

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022120\
 Data File : FE031335.D
 Signal(s) : FID1B.CH
 Acq On : 21 Feb 2020 14:10
 Operator : DD\AJ
 Sample : L1606-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 21 22:27:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE021120.M
 Quant Title :
 QLast Update : Tue Feb 11 12:55:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.607	4727960	15.212 ug/ml
Target Compounds			
4) N-TETRADECANE	8.202f	196335	0.581 ug/ml
7) N-EICOSANE	12.560f	976346	2.803 ug/ml
10) N-TETRACOSANE	14.792	825277	2.314 ug/ml
11) N-HEXACOSANE	15.831	750202	2.105 ug/ml
12) N-OCTACOSANE	16.785	2018174	5.570 ug/ml
13) N-TRIACONTANE	17.673	1644910	4.478 ug/ml
14) N-DOTRIACONTANE	18.506	1261264	3.575 ug/ml
15) N-TETRATRIACONTANE	19.293	217671	0.713 ug/ml
16) N-HEXATRIACONTANE	20.018	1330944	5.364 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022120\
Data File : FE031335.D
Signal(s) : FID1B.CH
Acq On : 21 Feb 2020 14:10
Operator : DD\AJ
Sample : L1606-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 21 22:27:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE021120.M
Quant Title :
QLast Update : Tue Feb 11 12:55:11 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

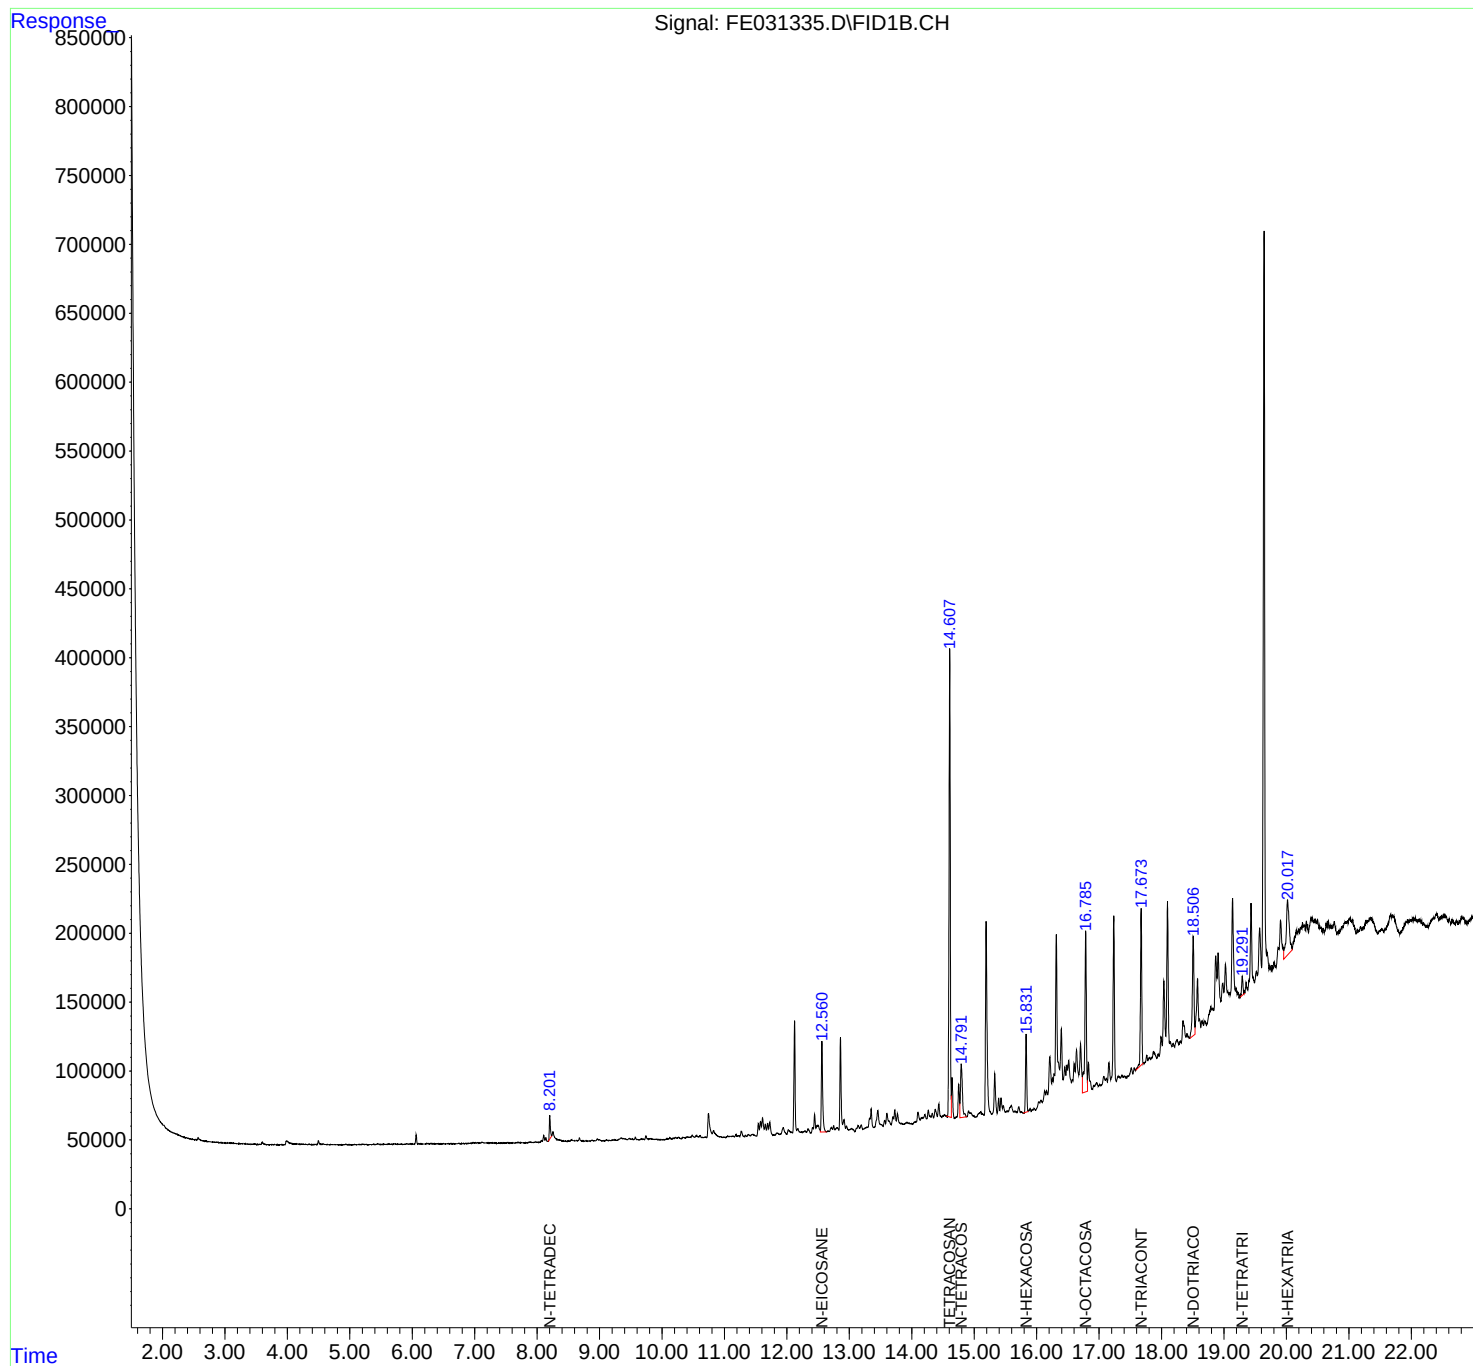

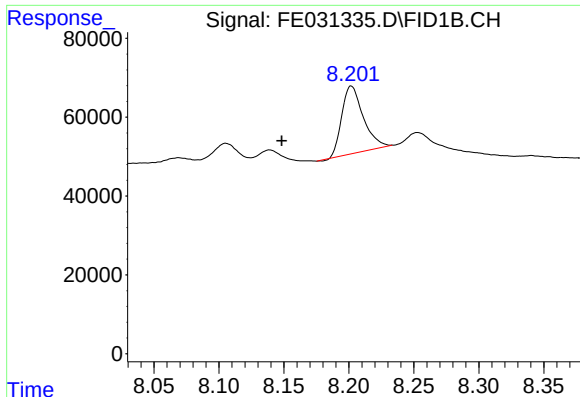


#4 N-TETRADECANE

R.T.: 8.202 min
Delta R.T.: 0.054 min
Response: 196335
Conc: 0.58 ug/ml

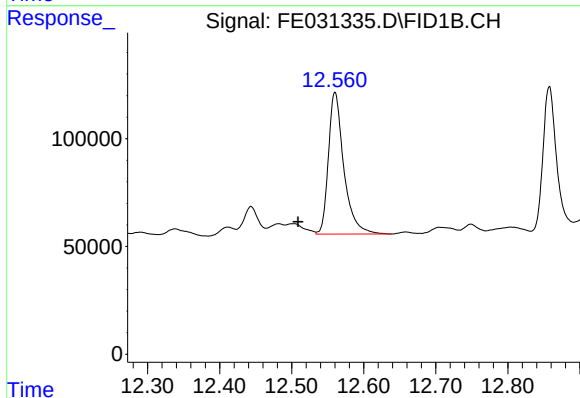


#7 N-EICOSANE

R.T.: 12.560 min
Delta R.T.: 0.052 min
Response: 976346
Conc: 2.80 ug/ml

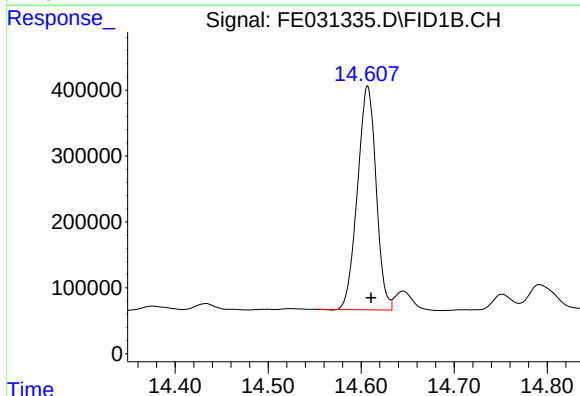


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.607 min
Delta R.T.: -0.004 min
Response: 4727960
Conc: 15.21 ug/ml

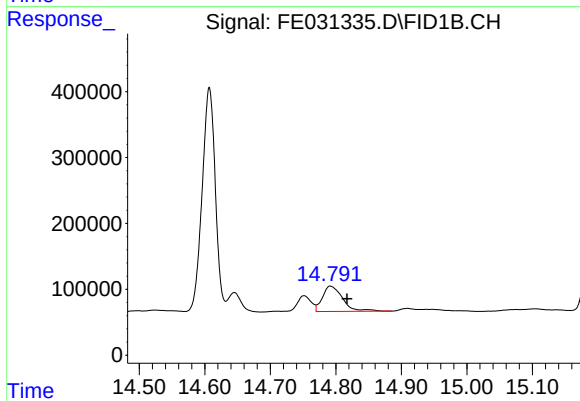


#10 N-TETRACOSANE

R.T.: 14.792 min
Delta R.T.: -0.025 min
Response: 825277
Conc: 2.31 ug/ml

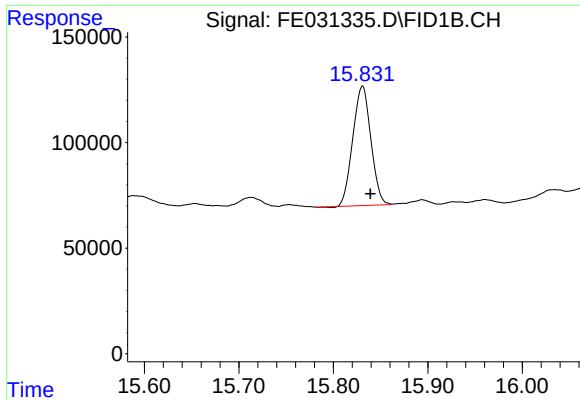


#11 N-HEXACOSANE

R.T.: 15.831 min
Delta R.T.: -0.009 min
Response: 750202
Conc: 2.11 ug/ml

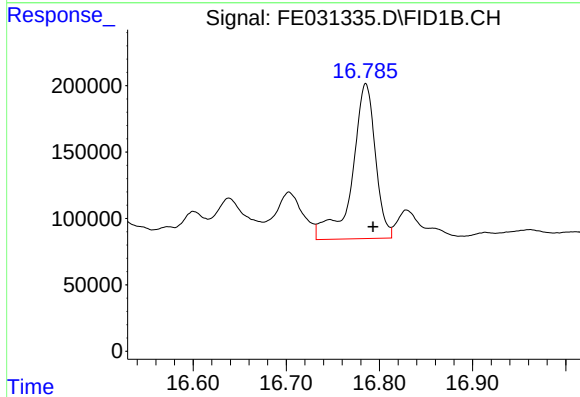


#12 N-OCTACOSANE

R.T.: 16.785 min
Delta R.T.: -0.008 min
Response: 2018174
Conc: 5.57 ug/ml

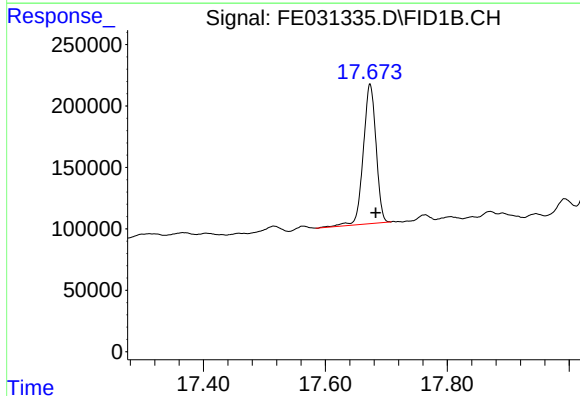


#13 N-TRIACONTANE

R.T.: 17.673 min
Delta R.T.: -0.009 min
Response: 1644910
Conc: 4.48 ug/ml

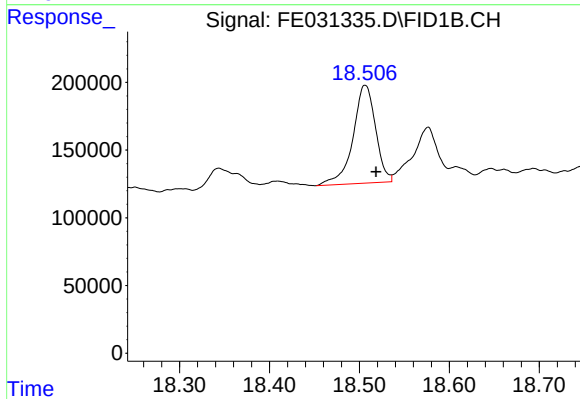

#14 N-DOTRIACONTANE

R.T.: 18.506 min
Delta R.T.: -0.012 min
Response: 1261264
Conc: 3.57 ug/ml

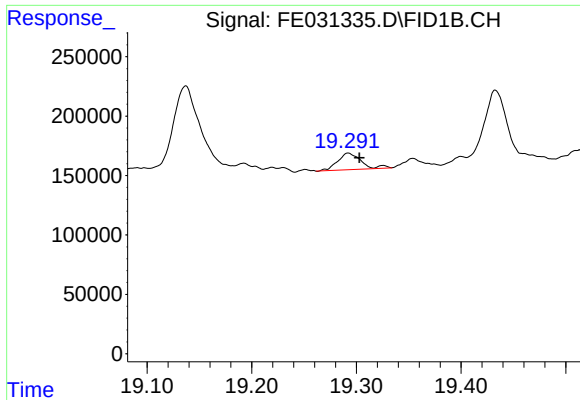


#15 N-TETRATRIACONTANE

R.T.: 19.293 min

Delta R.T.: -0.010 min

Response: 217671

Conc: 0.71 ug/ml

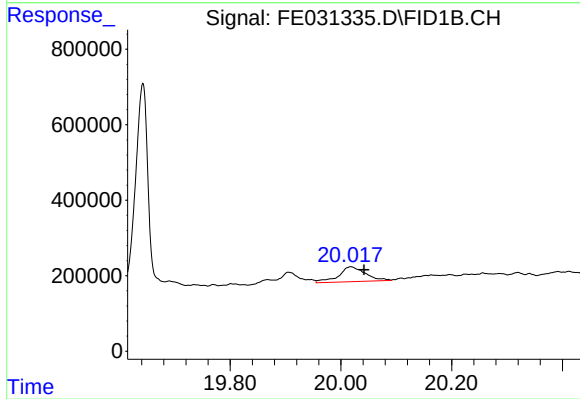

#16 N-HEXATRIACONTANE

R.T.: 20.018 min

Delta R.T.: -0.024 min

Response: 1330944

Conc: 5.36 ug/ml