

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022223\
Data File : FE040494.D
Signal(s) : FID1B.ch
Acq On : 22 Feb 2023 16:35
Operator : YP\AJ
Sample : PB150992BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 23 02:24:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022123.M
Quant Title :
QLast Update : Wed Feb 22 06:24:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.975	2497681	18.915 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.400	49172	0.417 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022223\
Data File : FE040494.D
Signal(s) : FID1B.ch
Acq On : 22 Feb 2023 16:35
Operator : YP\AJ
Sample : PB150992BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 23 02:24:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022123.M
Quant Title :
QLast Update : Wed Feb 22 06:24:20 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

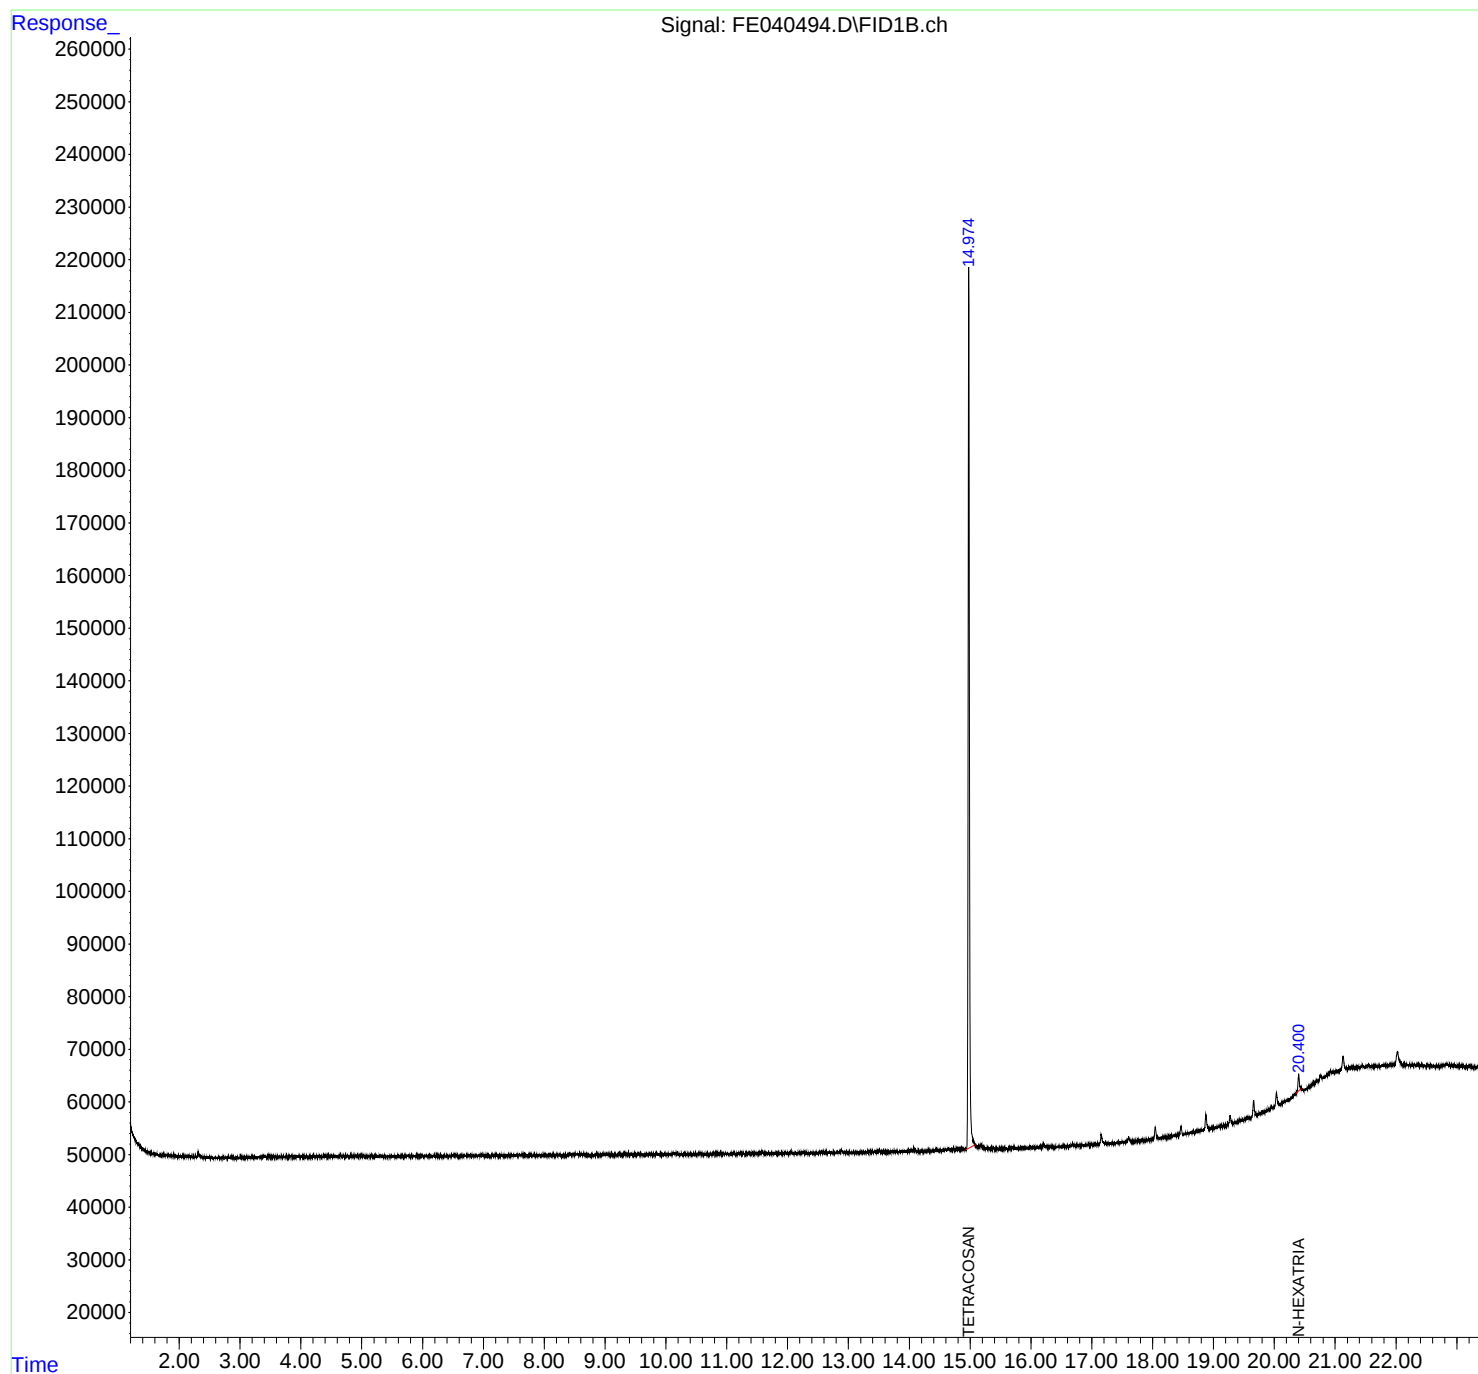

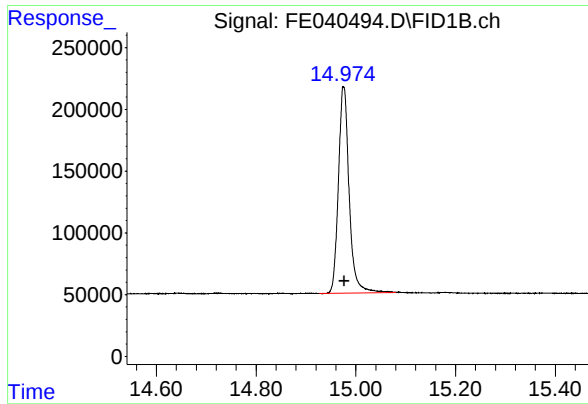

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.975 min
Delta R.T.: -0.001 min
Response: 2497681
Conc: 18.92 ug/ml

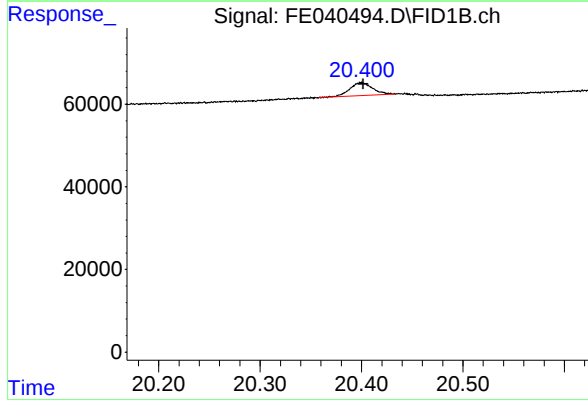

#16 N-HEXATRIACONTANE

R.T.: 20.400 min
Delta R.T.: -0.001 min
Response: 49172
Conc: 0.42 ug/ml