

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022321\
 Data File : FE033271.D
 Signal(s) : FID1B.CH
 Acq On : 23 Feb 2021 7:50
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 24 00:23:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022221.M
 Quant Title :
 QLast Update : Tue Feb 23 10:21:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.473	258855	0.654 ug/ml
16) N-HEXATRIACONTANE	20.037f	851382	2.281 ug/ml
18) N-TETRACONTANE	21.638f	584022	1.619 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022321\
Data File : FE033271.D
Signal(s) : FID1B.CH
Acq On : 23 Feb 2021 7:50
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 24 00:23:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022221.M
Quant Title :
QLast Update : Tue Feb 23 10:21:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

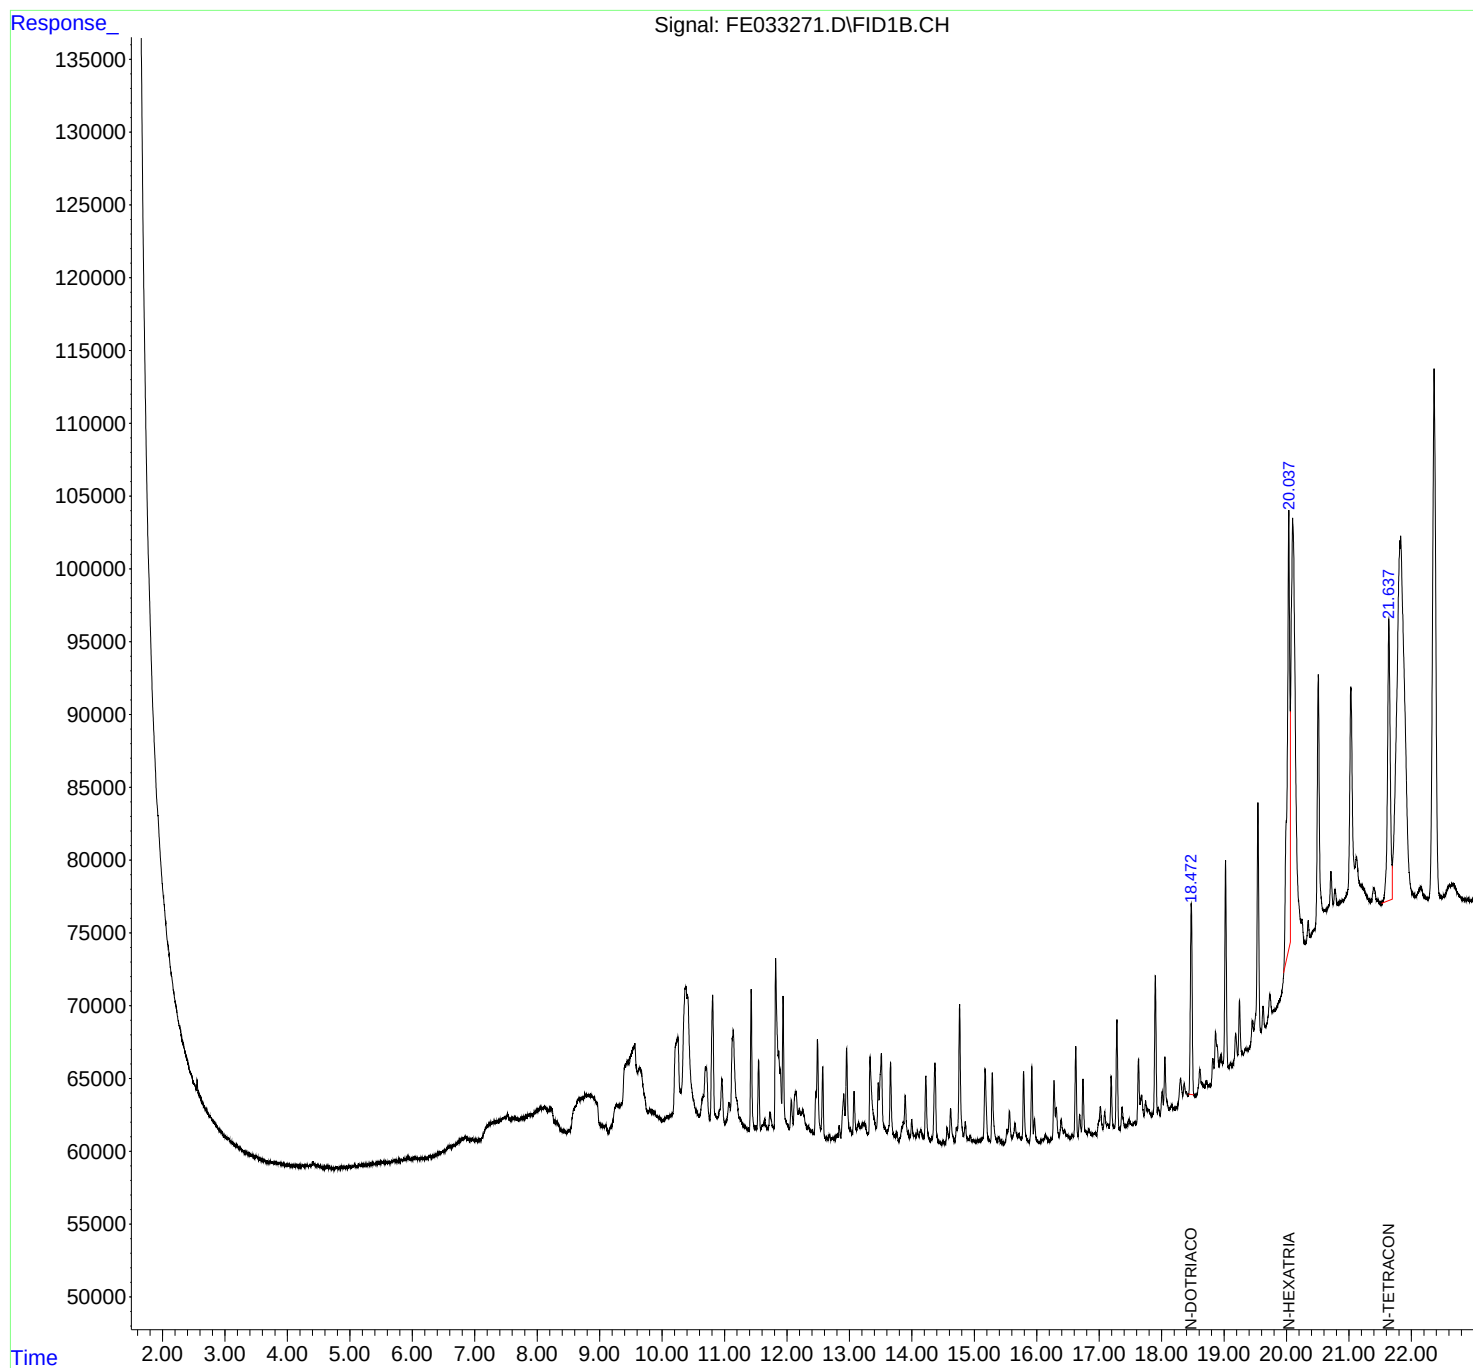


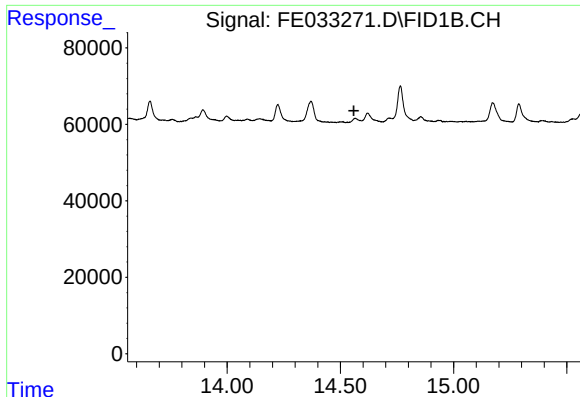

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.560 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

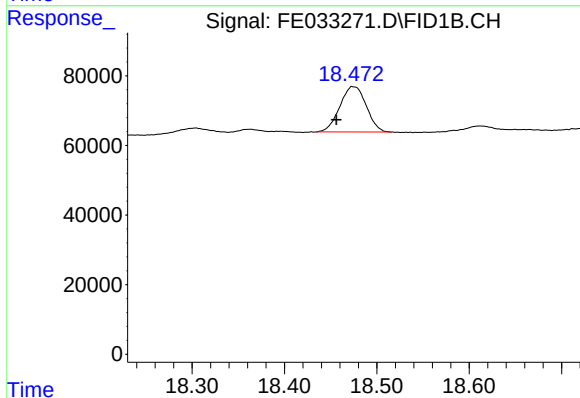


#14 N-DOTRIACONTANE

R.T.: 18.473 min
Delta R.T.: 0.017 min
Response: 258855
Conc: 0.65 ug/ml

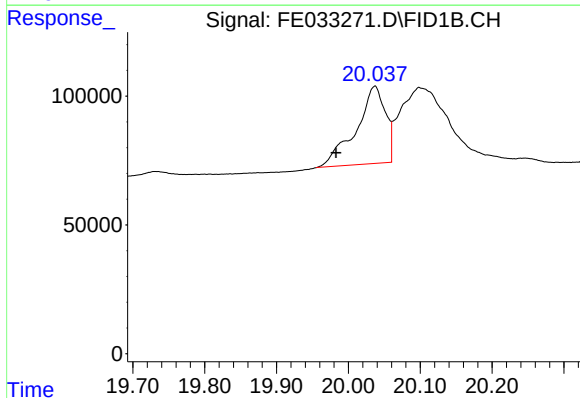

#16 N-HEXATRIACONTANE

R.T.: 20.037 min
Delta R.T.: 0.054 min
Response: 851382
Conc: 2.28 ug/ml

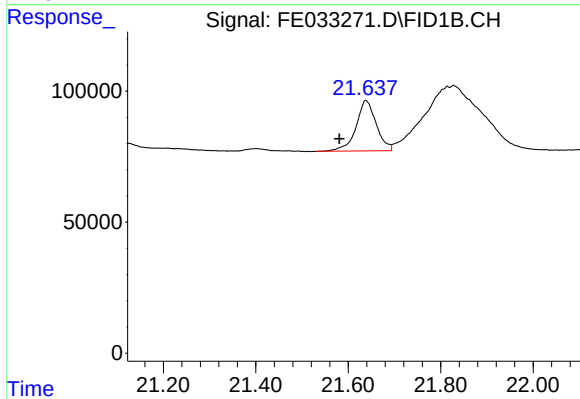

#18 N-TETRACONTANE

R.T.: 21.638 min
Delta R.T.: 0.057 min
Response: 584022
Conc: 1.62 ug/ml