

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022322AL\
 Data File : FE035148.D
 Signal(s) : FID1B.CH
 Acq On : 22 Feb 2022 16:40
 Operator : YP\AJ
 Sample : N1626-02DL 50X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 23 01:02:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022222.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 22 01:24:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.783	197842	<MDL ug/ml
Spiked Amount 50.000		Recovery =	0.00%
12) S 1-chlorooctadecane (S...	13.188	1444237	<MDL ug/ml
Spiked Amount 50.000		Recovery =	0.00%
Target Compounds			
3) T A~Naphthalene (C11.7)	6.135f	125268	<MDL ug/ml
8) T n-Octadecane (C18)	11.477	342667	<MDL ug/ml
10) T n-Eicosane (C20)	12.758	616802	<MDL ug/ml
11) T n-Heneicosane (C21)	13.342	1073474	<MDL ug/ml
13) T n-Docosane (C22)	13.949	1372814	<MDL ug/ml
14) T n-Tetracosane (C24)	15.044	6717657	7.628 ug/ml
15) T n-Hexacosane (C26)	16.051	5851224	6.934 ug/ml
16) T n-Octacosane (C28)	16.993	4510117	5.744 ug/ml
17) T n-Tricontane (C30)	17.905	3794599	5.447 ug/ml
18) T n-Dotriacontane (C32)	18.663	5523245	9.785 ug/ml
19) T n-Tetratriacontane (C34)	19.465	2197712	5.274 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022322AL\
Data File : FE035148.D
Signal(s) : FID1B.CH
Acq On : 22 Feb 2022 16:40
Operator : YP\AJ
Sample : N1626-02DL 50X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 23 01:02:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022222.M
Quant Title : GC Extractables
QLast Update : Tue Feb 22 01:24:23 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

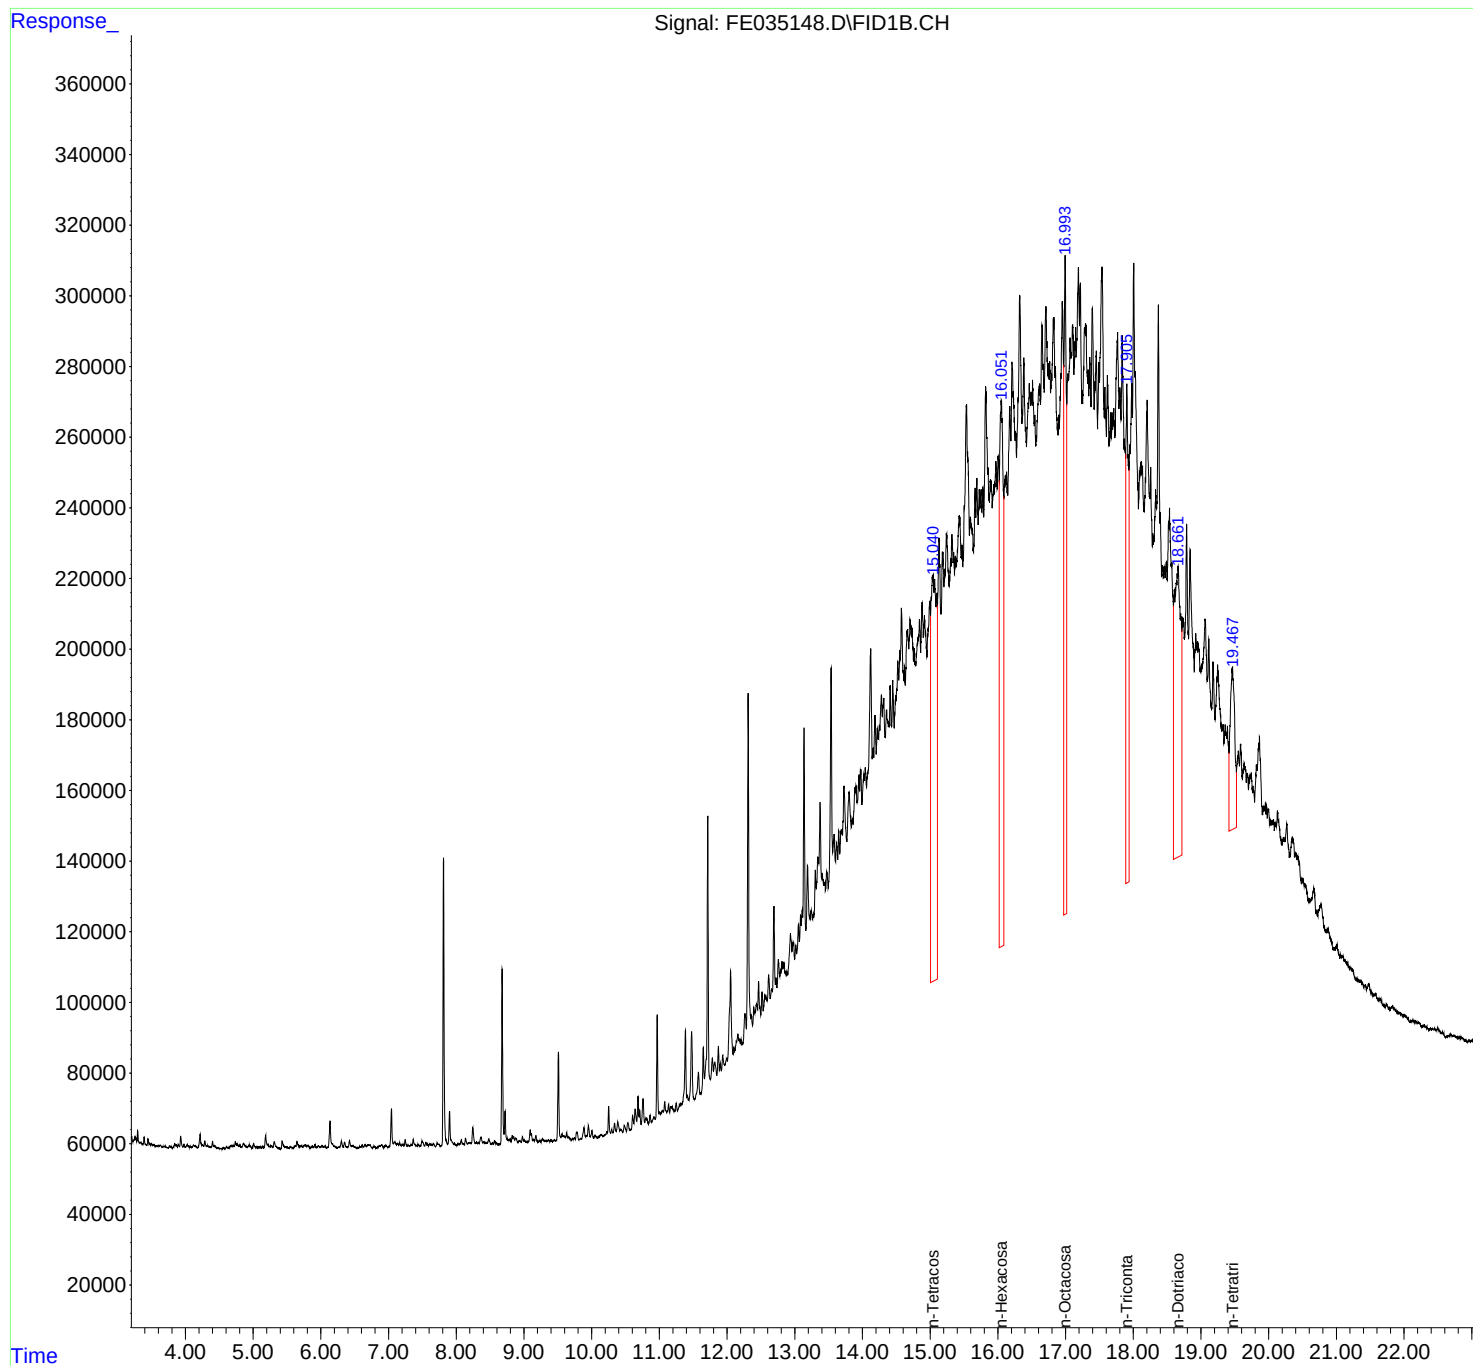


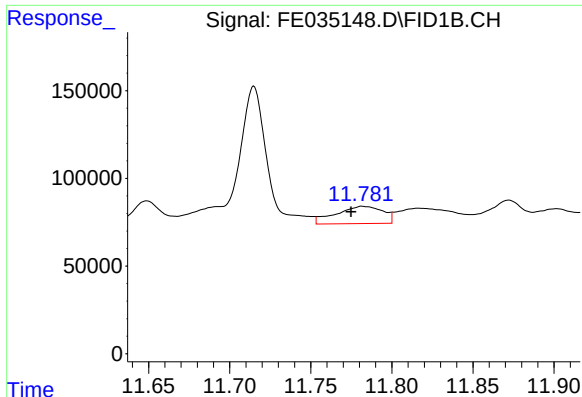

#9 ortho-Terphenyl (SURR)


R.T.: 11.783 min
Delta R.T.: 0.008 min
Response: 197842
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

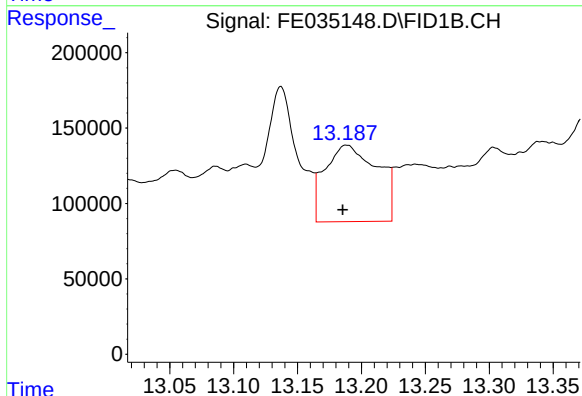


#12 1-chlorooctadecane (SURR)

R.T.: 13.188 min
Delta R.T.: 0.003 min
Response: 1444237
Conc: N.D.

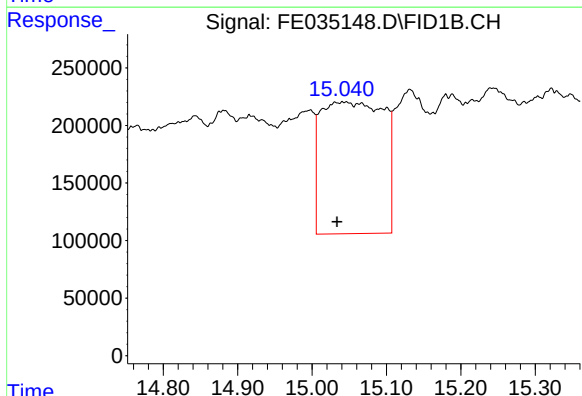


#14 n-Tetracosane (C24)

R.T.: 15.044 min
Delta R.T.: 0.011 min
Response: 6717657
Conc: 7.63 ug/ml

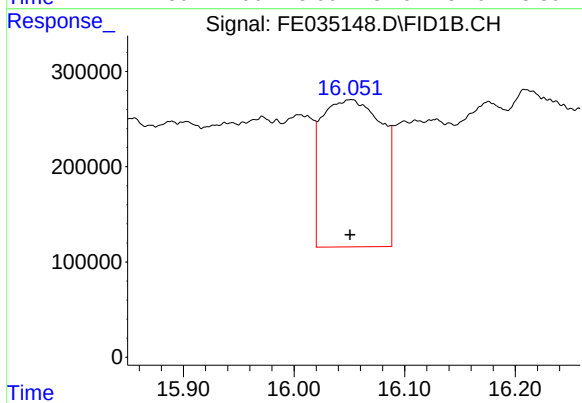

#15 n-Hexacosane (C26)


R.T.: 16.051 min
Delta R.T.: 0.000 min
Response: 5851224
Conc: 6.93 ug/ml

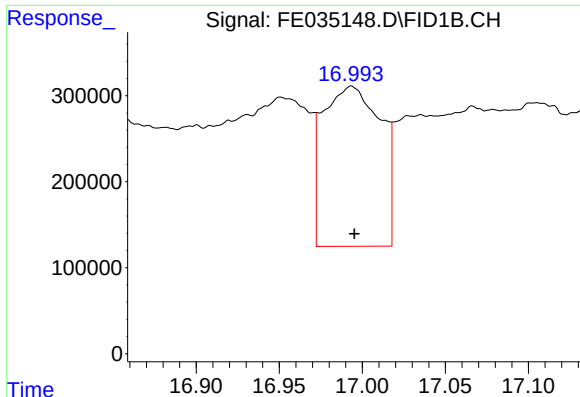

#16 n-Octacosane (C28)


R.T.: 16.993 min
Delta R.T.: -0.002 min
Response: 4510117
Conc: 5.74 ug/ml

Instrument :
FID_E
ClientSampleId :

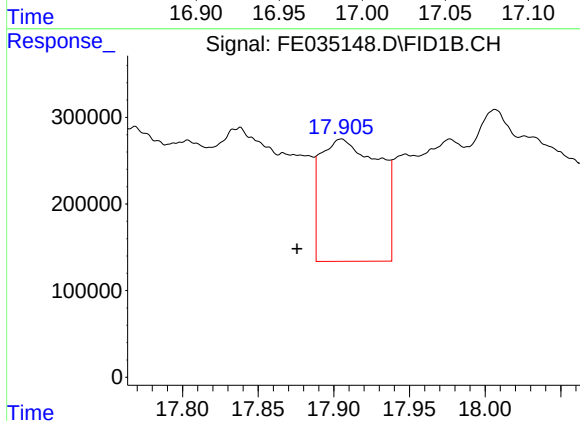


#17 n-Tricontane (C30)

R.T.: 17.905 min
Delta R.T.: 0.029 min
Response: 3794599
Conc: 5.45 ug/ml

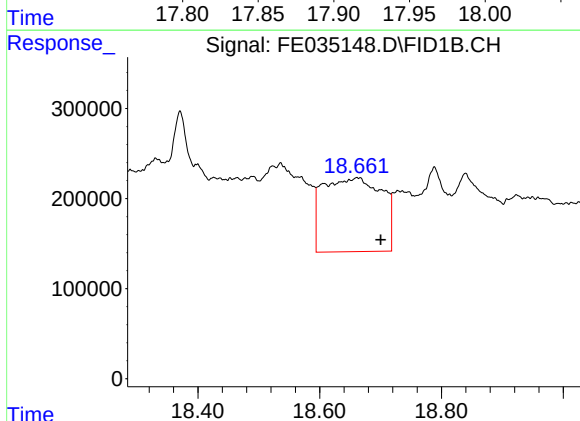

#18 n-Dotriacontane (C32)

R.T.: 18.663 min
Delta R.T.: -0.037 min
Response: 5523245
Conc: 9.79 ug/ml

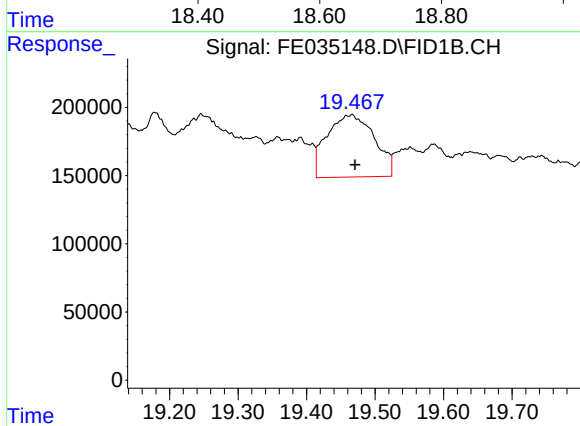

#19 n-Tetratriacontane (C34)

R.T.: 19.465 min
Delta R.T.: -0.006 min
Response: 2197712
Conc: 5.27 ug/ml