

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022322AL\
 Data File : FE035150.D
 Signal(s) : FID1B.CH
 Acq On : 22 Feb 2022 17:46
 Operator : YP\AJ
 Sample : N1626-04DL 50X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 23 01:02:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022222.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 22 01:24:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.715	797691	<MDL ug/ml
Spiked Amount 50.000		Recovery =	0.00%
12) S 1-chlorooctadecane (S...	13.186	858972	<MDL ug/ml
Spiked Amount 50.000		Recovery =	0.00%
Target Compounds			
8) T n-Octadecane (C18)	11.477	132343	<MDL ug/ml
10) T n-Eicosane (C20)	12.755	307278	<MDL ug/ml
11) T n-Heneicosane (C21)	13.339	408122	<MDL ug/ml
13) T n-Docosane (C22)	13.937	990693	<MDL ug/ml
14) T n-Tetracosane (C24)	15.061	3129483	3.554 ug/ml
15) T n-Hexacosane (C26)	16.044	3845562	4.557 ug/ml
16) T n-Octacosane (C28)	16.990	3502519	4.461 ug/ml
17) T n-Tricontane (C30)	17.900	3217237	4.618 ug/ml
18) T n-Dotriacontane (C32)	18.660	4493701	7.961 ug/ml
19) T n-Tetratriacontane (C34)	19.462	4265214	10.236 ug/ml
20) T n-Hexatriacontane (C36)	20.227	1018913	3.634 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022322AL\
Data File : FE035150.D
Signal(s) : FID1B.CH
Acq On : 22 Feb 2022 17:46
Operator : YP\AJ
Sample : N1626-04DL 50X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 23 01:02:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022222.M
Quant Title : GC Extractables
QLast Update : Tue Feb 22 01:24:23 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 uL
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

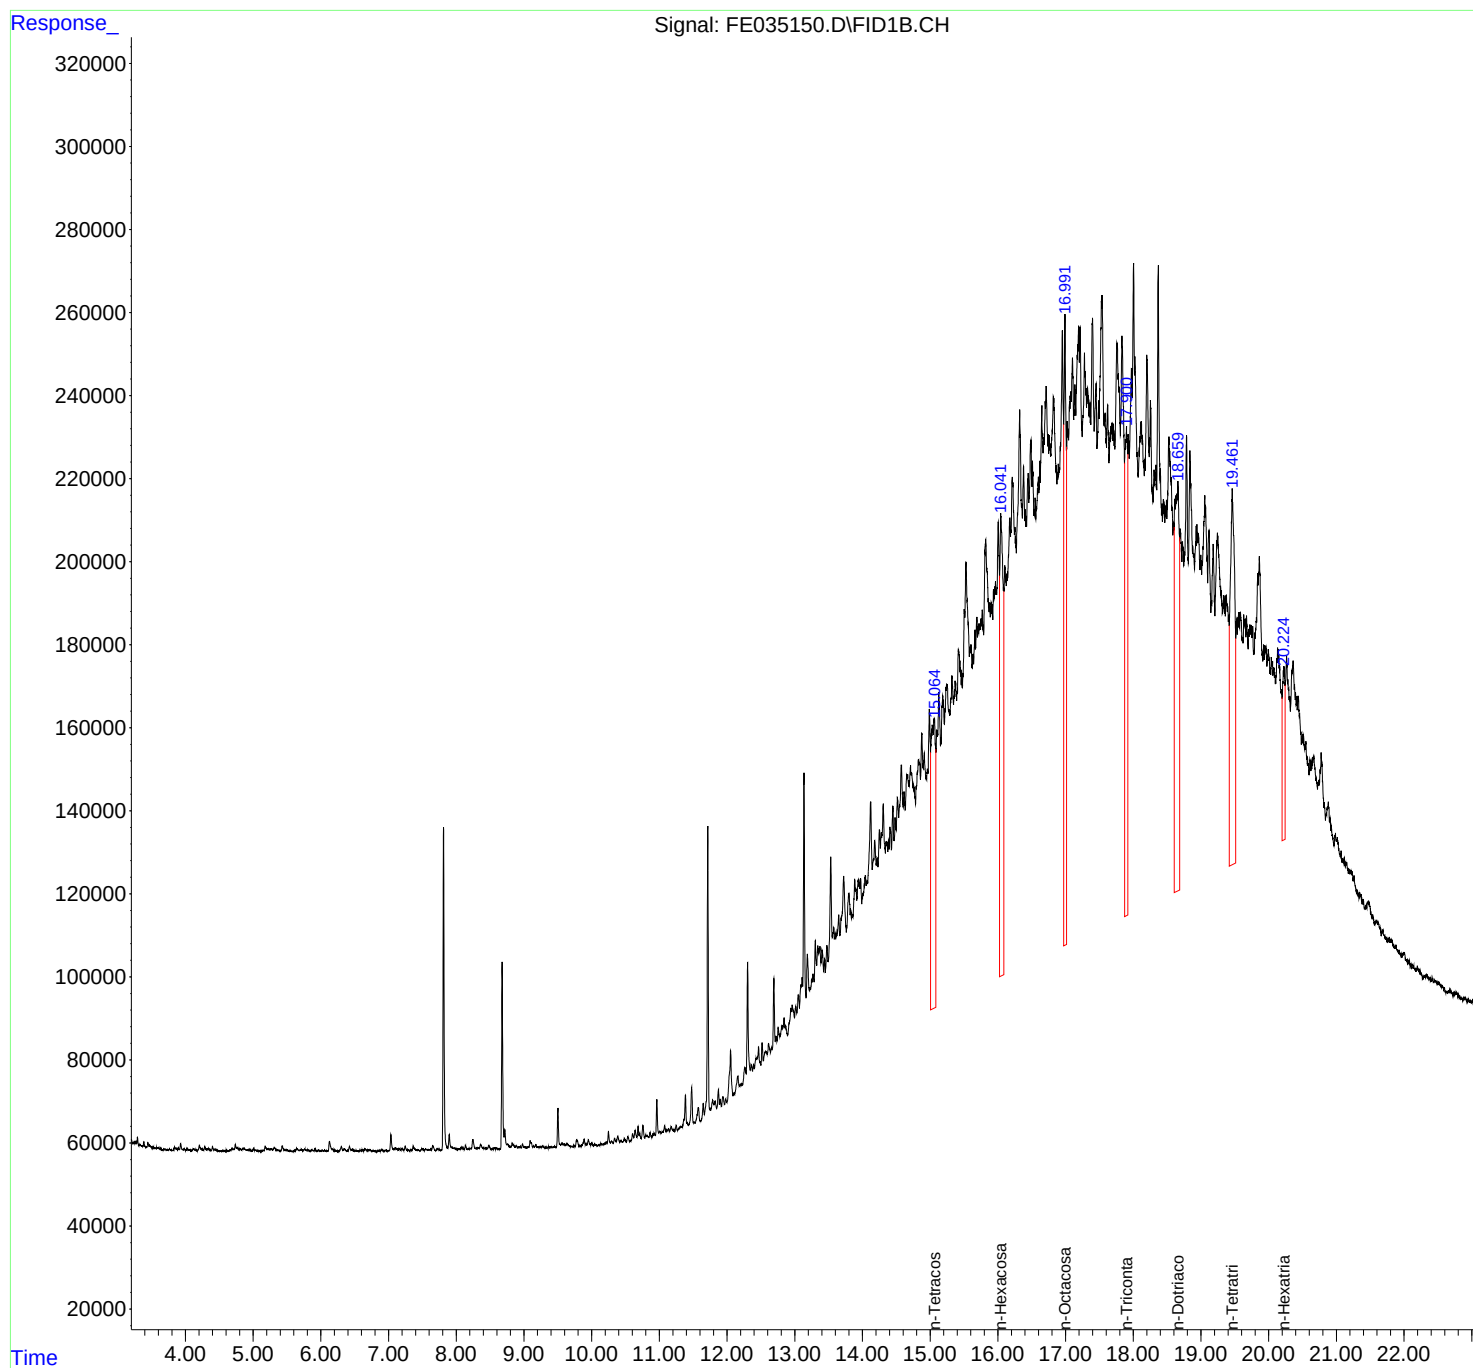


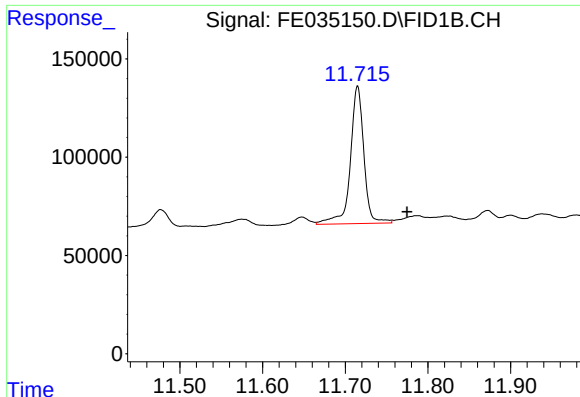

#9 ortho-Terphenyl (SURR)


R.T.: 11.715 min
Delta R.T.: -0.060 min
Response: 797691
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

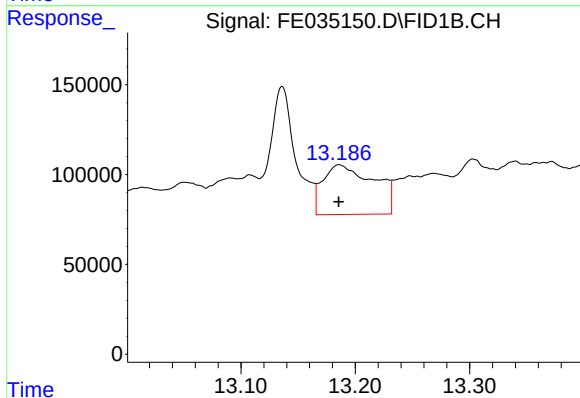


#12 1-chlorooctadecane (SURR)

R.T.: 13.186 min
Delta R.T.: 0.000 min
Response: 858972
Conc: N.D.

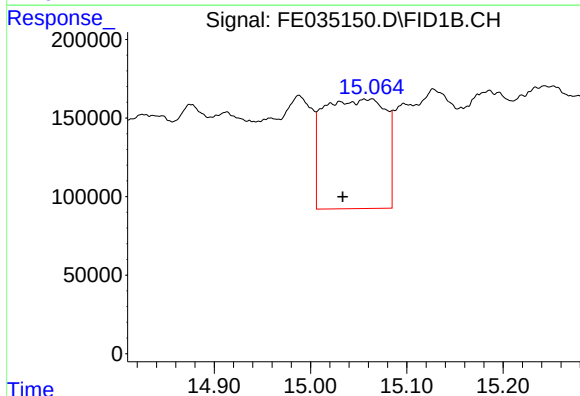


#14 n-Tetracosane (C24)

R.T.: 15.061 min
Delta R.T.: 0.028 min
Response: 3129483
Conc: 3.55 ug/ml

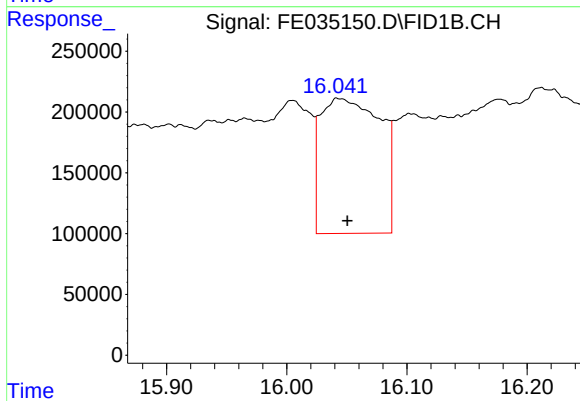

#15 n-Hexacosane (C26)


R.T.: 16.044 min
Delta R.T.: -0.006 min
Response: 3845562
Conc: 4.56 ug/ml

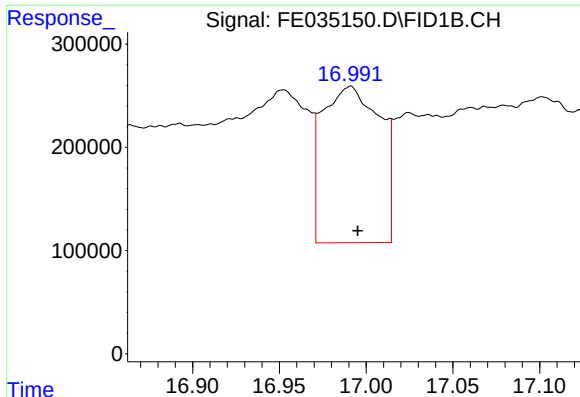

#16 n-Octacosane (C28)


R.T.: 16.990 min
Delta R.T.: -0.005 min
Response: 3502519
Conc: 4.46 ug/ml

Instrument :
FID_E
ClientSampleId :

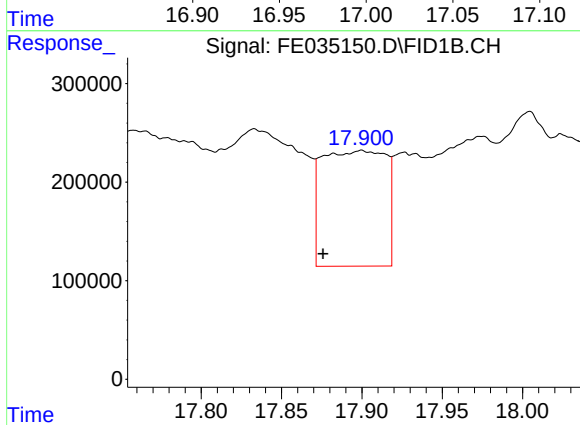


#17 n-Tricontane (C30)

R.T.: 17.900 min
Delta R.T.: 0.024 min
Response: 3217237
Conc: 4.62 ug/ml

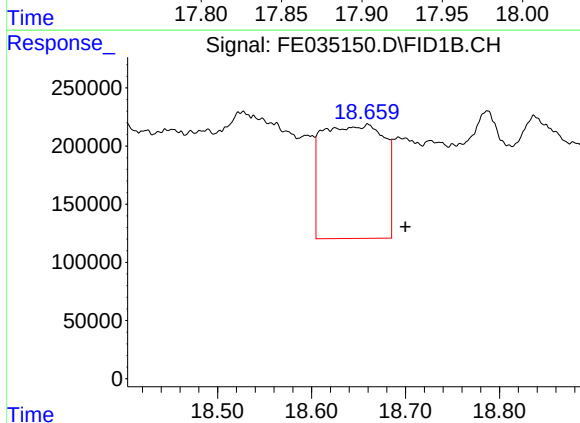


#18 n-Dotriacontane (C32)

R.T.: 18.660 min
Delta R.T.: -0.040 min
Response: 4493701
Conc: 7.96 ug/ml

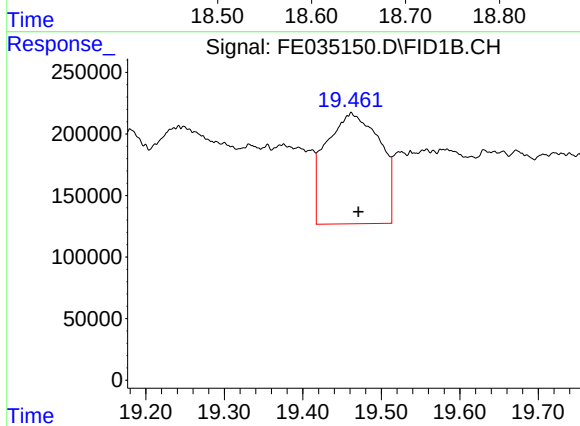

#19 n-Tetratriacontane (C34)

R.T.: 19.462 min
Delta R.T.: -0.009 min
Response: 4265214
Conc: 10.24 ug/ml

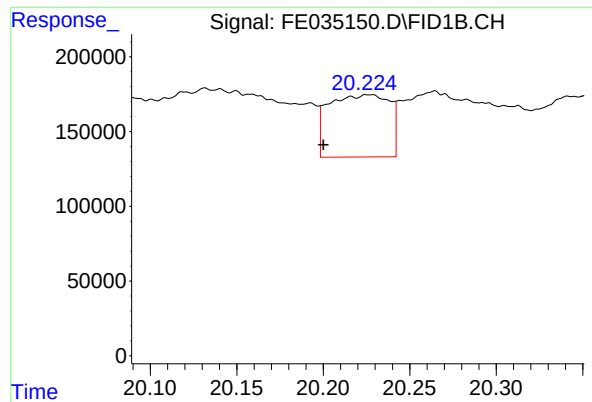

#20 n-Hexatriacontane (C36)

R.T.: 20.227 min
Delta R.T.: 0.026 min
Response: 1018913
Conc: 3.63 ug/ml

Instrument :
FID_E
ClientSampleId :