

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022322AL\
 Data File : FE035152.D
 Signal(s) : FID1B.CH
 Acq On : 22 Feb 2022 18:53
 Operator : YP\AJ
 Sample : N1626-06DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 23 01:02:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022222.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 22 01:24:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.784	957210	<MDL ug/ml
Spiked Amount 50.000		Recovery =	0.00%
12) S 1-chlorooctadecane (S...	13.186	1906102	2.454 ug/ml
Spiked Amount 50.000		Recovery =	4.91%
Target Compounds			
7) T n-Hexadecane (C16)	9.950	94234	<MDL ug/ml
8) T n-Octadecane (C18)	11.478	830626	<MDL ug/ml
10) T n-Eicosane (C20)	12.767	3111182	3.467 ug/ml
11) T n-Heneicosane (C21)	13.353	1396329	<MDL ug/ml
13) T n-Docosane (C22)	13.949	2325669	2.597 ug/ml
14) T n-Tetracosane (C24)	15.070	7019664	7.971 ug/ml
15) T n-Hexacosane (C26)	16.048	7128125	8.447 ug/ml
16) T n-Octacosane (C28)	16.993	4528564	5.768 ug/ml
17) T n-Tricontane (C30)	17.834	8533380	12.250 ug/ml
18) T n-Dotriacontane (C32)	18.658	2309131	4.091 ug/ml
19) T n-Tetratriacontane (C34)	19.437	286434	<MDL ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022322AL\
Data File : FE035152.D
Signal(s) : FID1B.CH
Acq On : 22 Feb 2022 18:53
Operator : YP\AJ
Sample : N1626-06DL 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 23 01:02:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022222.M
Quant Title : GC Extractables
QLast Update : Tue Feb 22 01:24:23 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

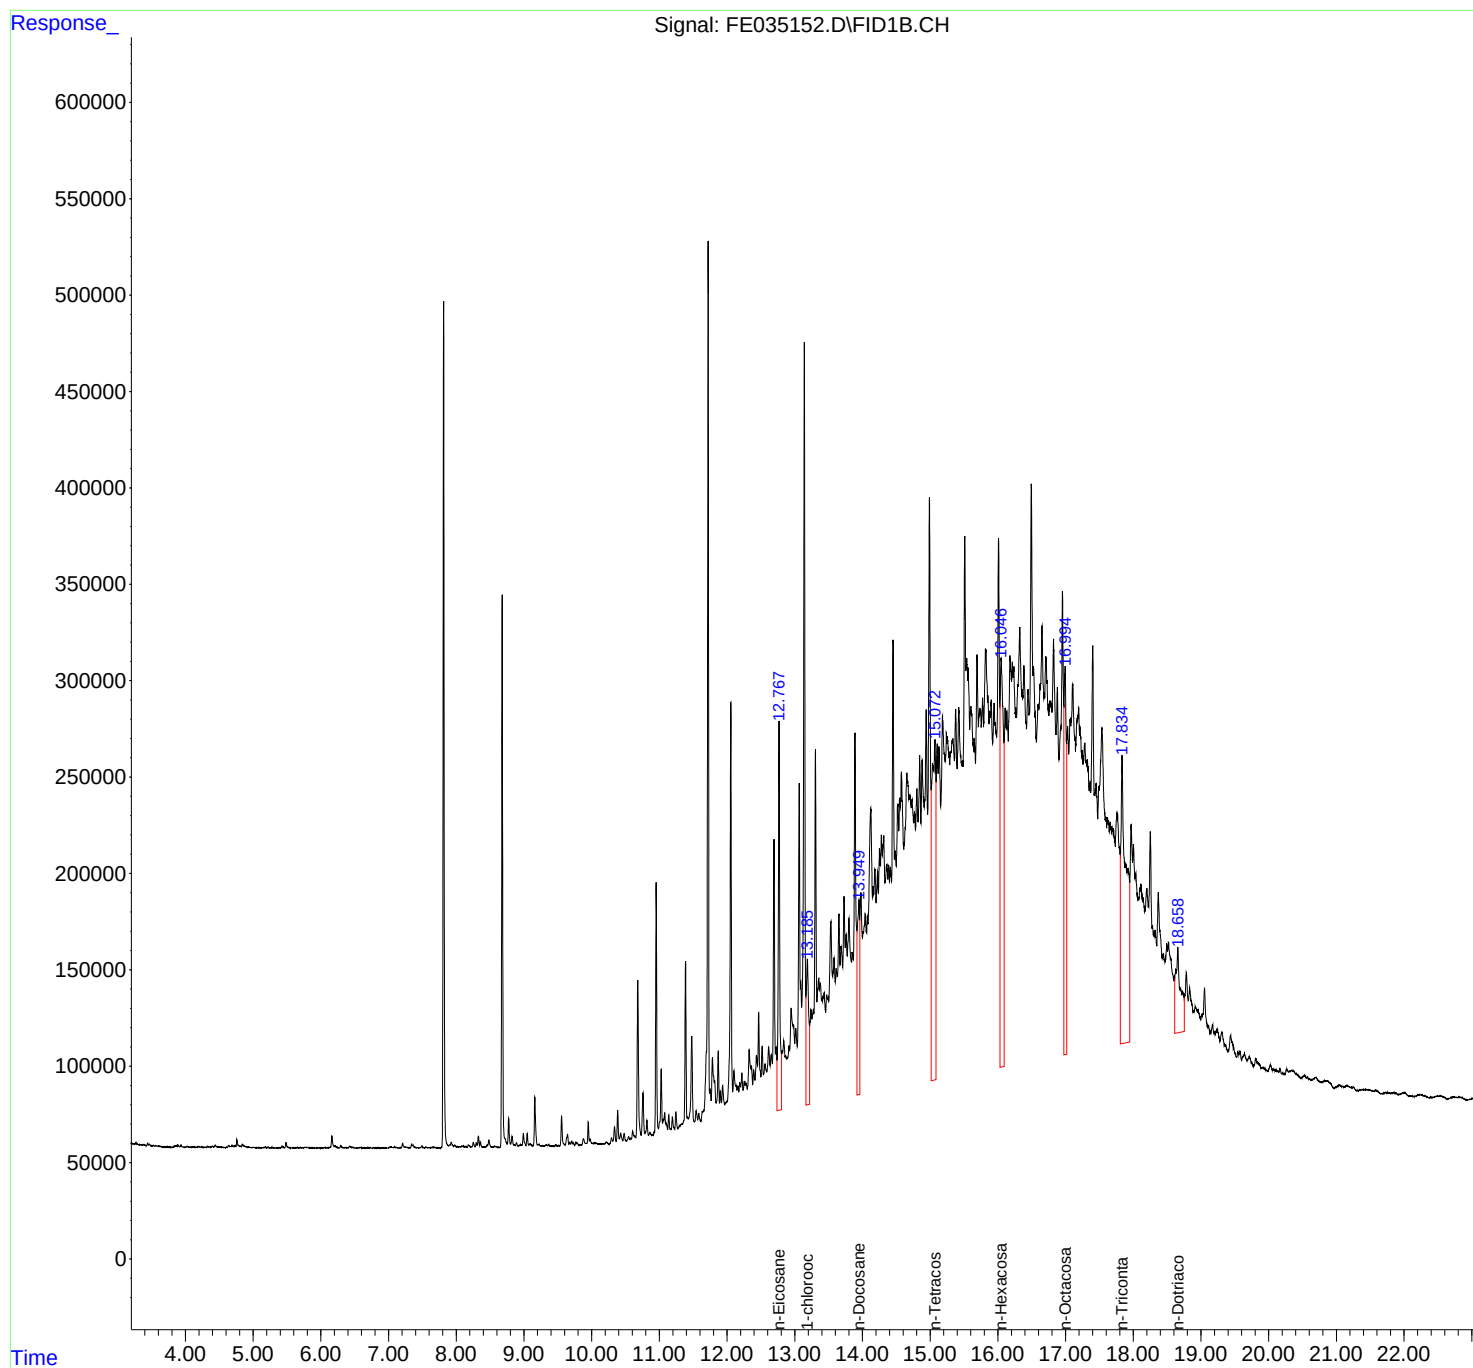


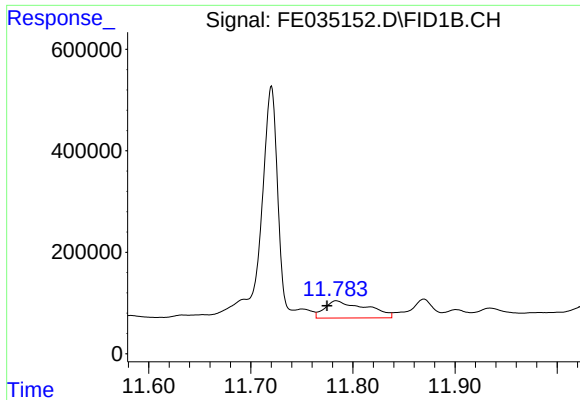

#9 ortho-Terphenyl (SURR)


R.T.: 11.784 min
Delta R.T.: 0.009 min
Response: 957210
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

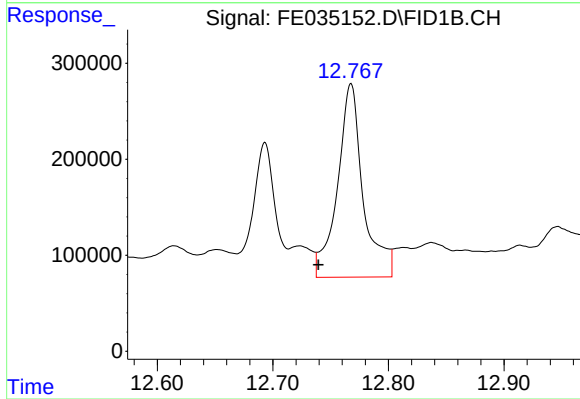


#10 n-Eicosane (C20)

R.T.: 12.767 min
Delta R.T.: 0.028 min
Response: 311182
Conc: 3.47 ug/ml

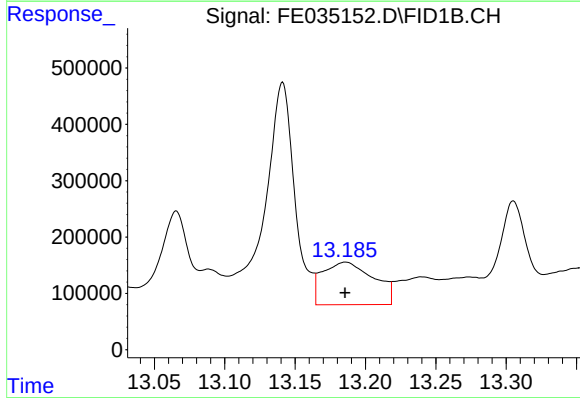


#12 1-chlorooctadecane (SURR)

R.T.: 13.186 min
Delta R.T.: 0.000 min
Response: 1906102
Conc: 2.45 ug/ml

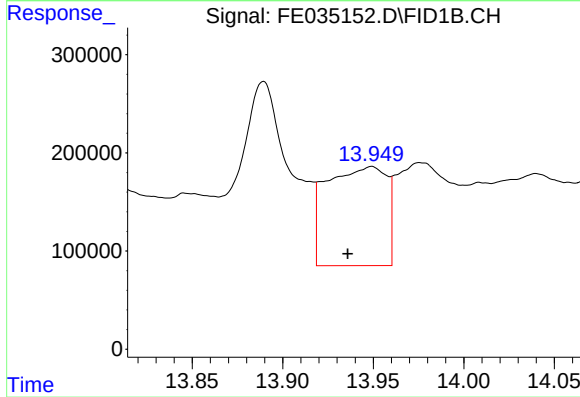

#13 n-Docosane (C22)


R.T.: 13.949 min
Delta R.T.: 0.013 min
Response: 2325669
Conc: 2.60 ug/ml

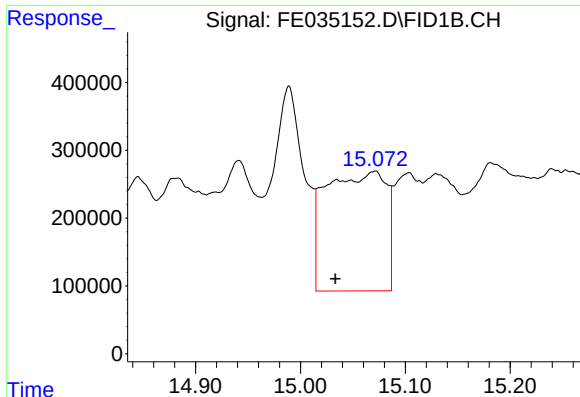

#14 n-Tetracosane (C24)


R.T.: 15.070 min
Delta R.T.: 0.037 min
Response: 7019664
Conc: 7.97 ug/ml

Instrument :
FID_E
ClientSampleId :

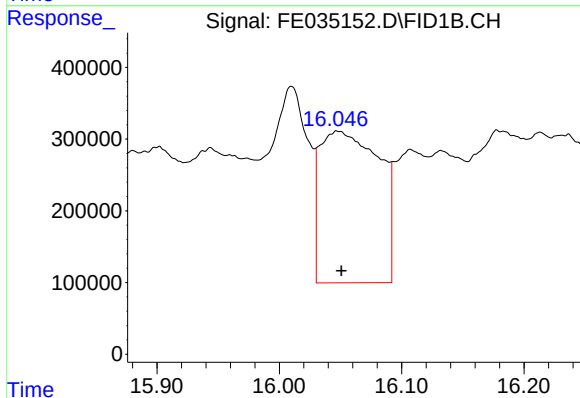


#15 n-Hexacosane (C26)

R.T.: 16.048 min
Delta R.T.: -0.002 min
Response: 7128125
Conc: 8.45 ug/ml

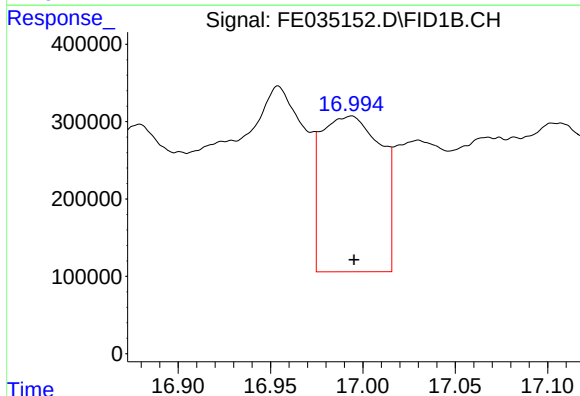


#16 n-Octacosane (C28)

R.T.: 16.993 min
Delta R.T.: -0.002 min
Response: 4528564
Conc: 5.77 ug/ml

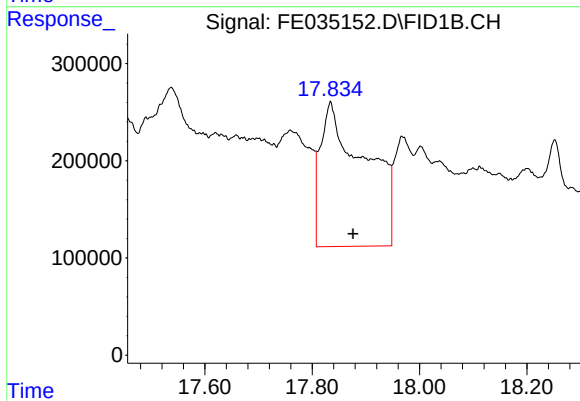

#17 n-Tricontane (C30)

R.T.: 17.834 min
Delta R.T.: -0.042 min
Response: 8533380
Conc: 12.25 ug/ml

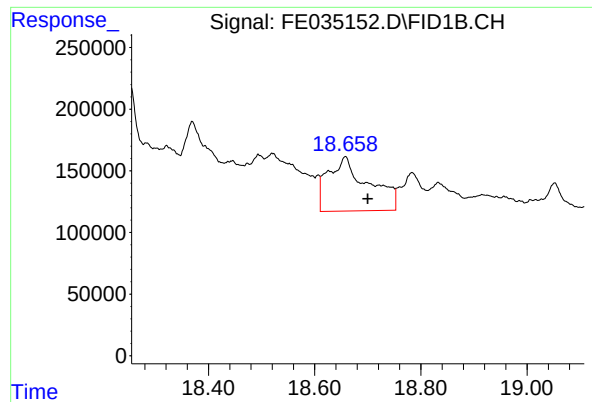

#18 n-Dotriacontane (C32)

R.T.: 18.658 min
Delta R.T.: -0.042 min
Response: 2309131
Conc: 4.09 ug/ml

Instrument :

FID_E

ClientSampleId :