

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022322AL\
 Data File : FE035153.D
 Signal(s) : FID1B.CH
 Acq On : 22 Feb 2022 19:26
 Operator : YP\AJ
 Sample : N1626-07DL 20X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 23 01:03:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022222.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 22 01:24:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.784	1252543	<MDL ug/ml
Spiked Amount 50.000		Recovery =	0.00%
12) S 1-chlorooctadecane (S...	13.190	3512326	4.523 ug/ml
Spiked Amount 50.000		Recovery =	9.05%
Target Compounds			
7) T n-Hexadecane (C16)	9.950	310167	<MDL ug/ml
8) T n-Octadecane (C18)	11.434	225503	<MDL ug/ml
10) T n-Eicosane (C20)	12.727	1068844	<MDL ug/ml
11) T n-Heneicosane (C21)	13.370	3439043	3.823 ug/ml
13) T n-Docosane (C22)	13.948	2457586	2.744 ug/ml
14) T n-Tetracosane (C24)	15.056	5137555	5.834 ug/ml
15) T n-Hexacosane (C26)	16.046	5052669	5.987 ug/ml
16) T n-Octacosane (C28)	16.991	3996029	5.090 ug/ml
17) T n-Tricontane (C30)	17.831	2791951	4.008 ug/ml
18) T n-Dotriacontane (C32)	18.657	900886	<MDL ug/ml
19) T n-Tetratriacontane (C34)	19.443	433855	<MDL ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022322AL\
Data File : FE035153.D
Signal(s) : FID1B.CH
Acq On : 22 Feb 2022 19:26
Operator : YP\AJ
Sample : N1626-07DL 20X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 23 01:03:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022222.M
Quant Title : GC Extractables
QLast Update : Tue Feb 22 01:24:23 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

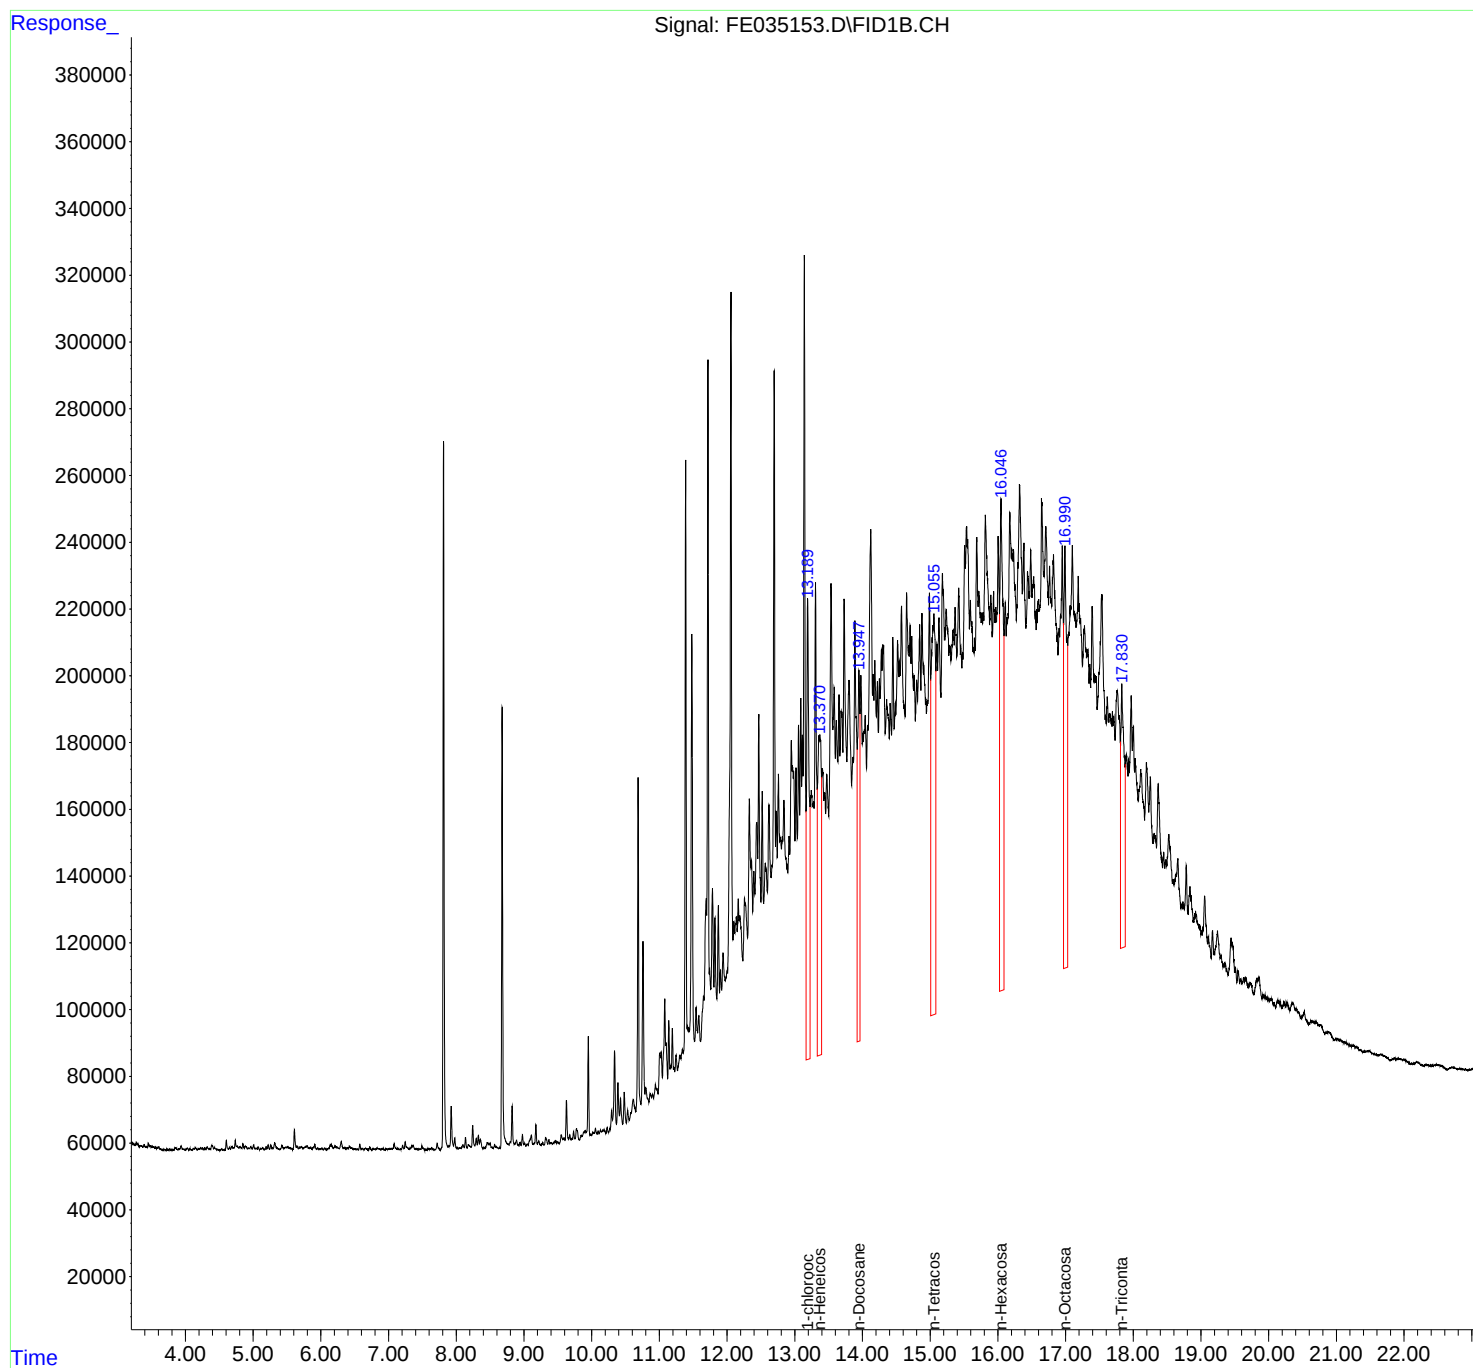


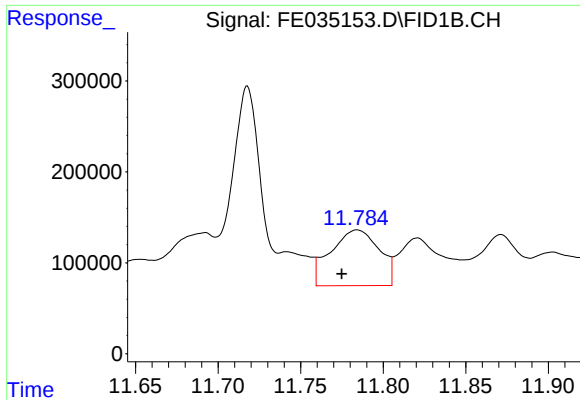

#9 ortho-Terphenyl (SURR)


R.T.: 11.784 min
Delta R.T.: 0.009 min
Response: 1252543
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

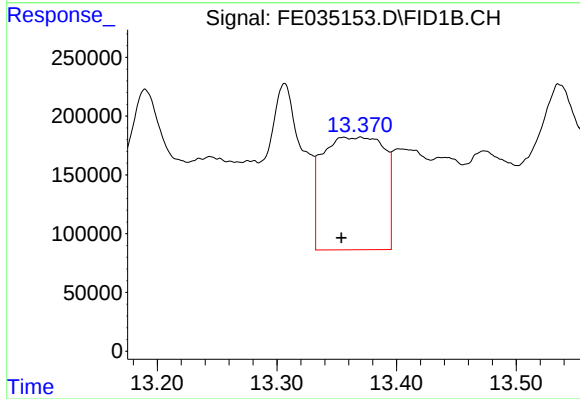


#11 n-Heneicosane (C21)

R.T.: 13.370 min
Delta R.T.: 0.016 min
Response: 3439043
Conc: 3.82 ug/ml

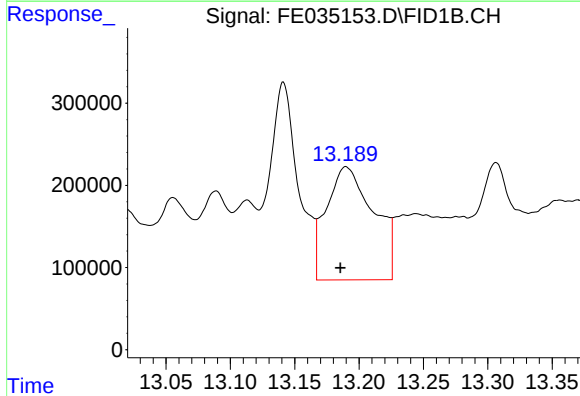


#12 1-chlorooctadecane (SURR)

R.T.: 13.190 min
Delta R.T.: 0.005 min
Response: 3512326
Conc: 4.52 ug/ml

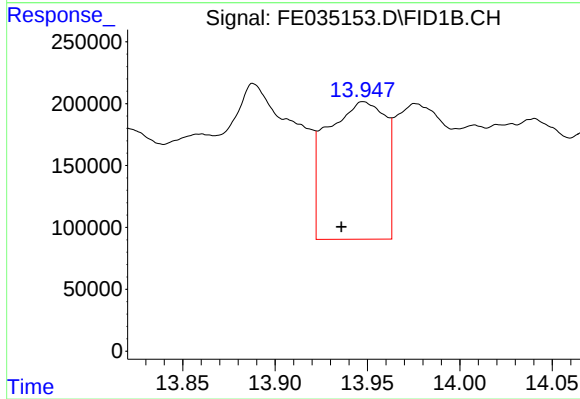

#13 n-Docosane (C22)


R.T.: 13.948 min
Delta R.T.: 0.013 min
Response: 2457586
Conc: 2.74 ug/ml

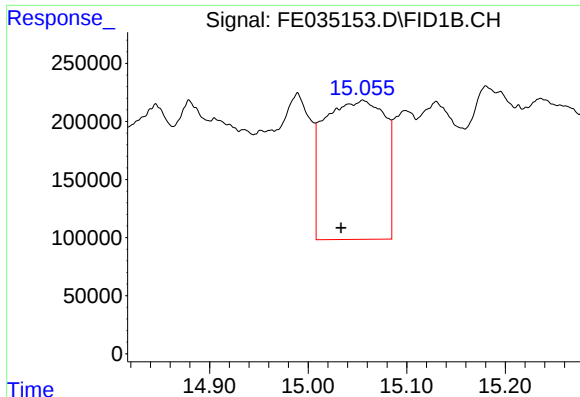

#14 n-Tetracosane (C24)


R.T.: 15.056 min
Delta R.T.: 0.022 min
Response: 5137555
Conc: 5.83 ug/ml

Instrument :
FID_E
ClientSampleId :

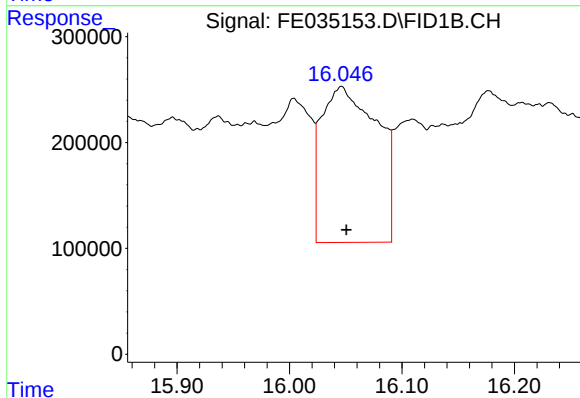


#15 n-Hexacosane (C26)

R.T.: 16.046 min
Delta R.T.: -0.005 min
Response: 5052669
Conc: 5.99 ug/ml

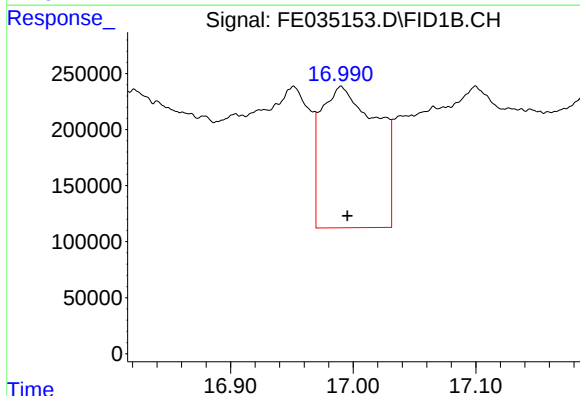

#16 n-Octacosane (C28)

R.T.: 16.991 min
Delta R.T.: -0.005 min
Response: 3996029
Conc: 5.09 ug/ml

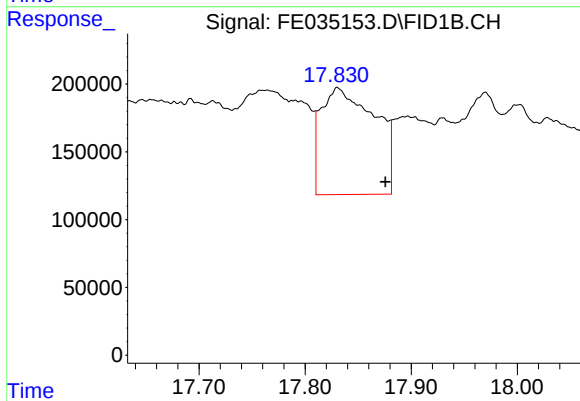

#17 n-Tricontane (C30)

R.T.: 17.831 min
Delta R.T.: -0.045 min
Response: 2791951
Conc: 4.01 ug/ml