

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022322AL\
 Data File : FE035161.D
 Signal(s) : FID1B.CH
 Acq On : 22 Feb 2022 23:47
 Operator : YP\AJ
 Sample : N1626-14DL 50X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 23 01:04:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022222.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 22 01:24:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.784	97882	<MDL ug/ml
Spiked Amount 50.000		Recovery =	0.00%
12) S 1-chlorooctadecane (S...	13.187	1109135	<MDL ug/ml
Spiked Amount 50.000		Recovery =	0.00%
Target Compounds			
7) T n-Hexadecane (C16)	9.949	74312	<MDL ug/ml
8) T n-Octadecane (C18)	11.477	280058	<MDL ug/ml
10) T n-Eicosane (C20)	12.755	311459	<MDL ug/ml
11) T n-Heneicosane (C21)	13.352	1493703	<MDL ug/ml
13) T n-Docosane (C22)	13.948	1873941	2.093 ug/ml
14) T n-Tetracosane (C24)	15.045	5016649	5.697 ug/ml
15) T n-Hexacosane (C26)	16.049	14499955	17.183 ug/ml
16) T n-Octacosane (C28)	16.996	7381192	9.401 ug/ml
17) T n-Tricontane (C30)	17.905	5999111	8.612 ug/ml
18) T n-Dotriacontane (C32)	18.663	5280593	9.355 ug/ml
19) T n-Tetratriacontane (C34)	19.461	3440503	8.257 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022322AL\
Data File : FE035161.D
Signal(s) : FID1B.CH
Acq On : 22 Feb 2022 23:47
Operator : YP\AJ
Sample : N1626-14DL 50X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 23 01:04:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022222.M
Quant Title : GC Extractables
QLast Update : Tue Feb 22 01:24:23 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

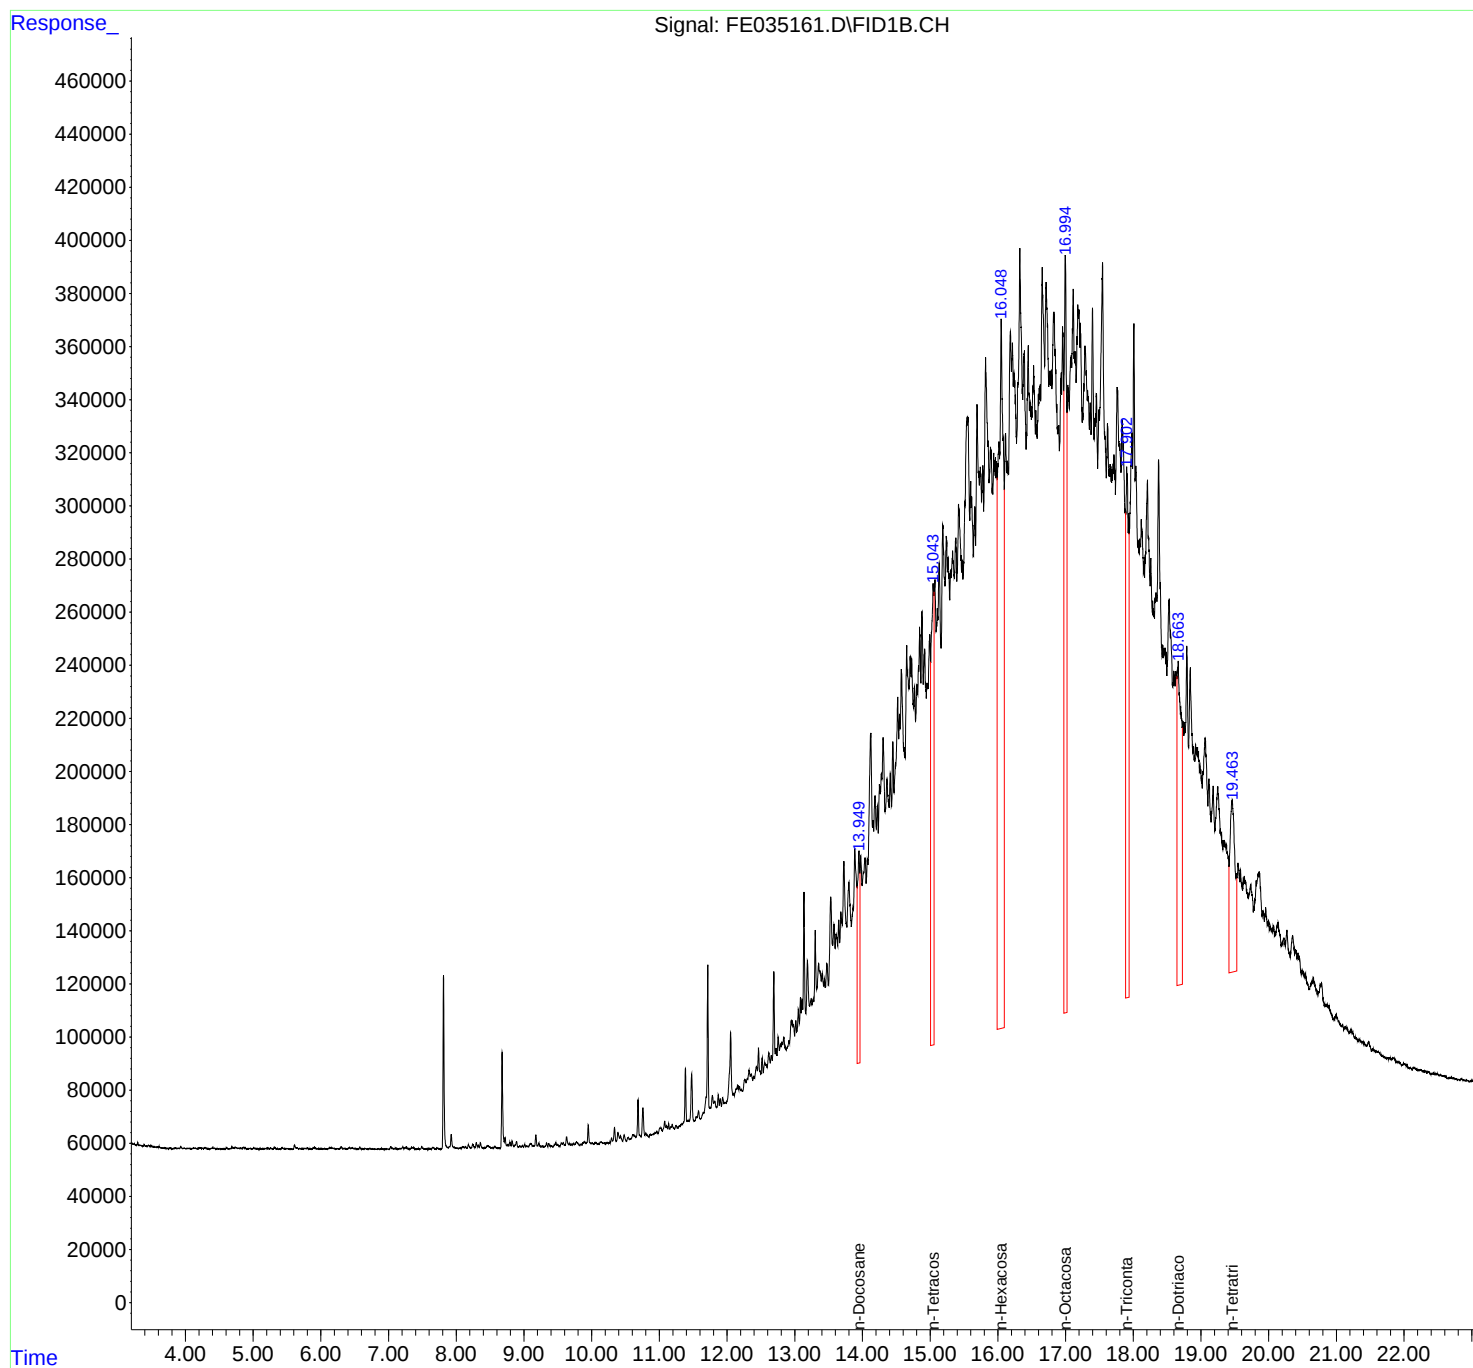


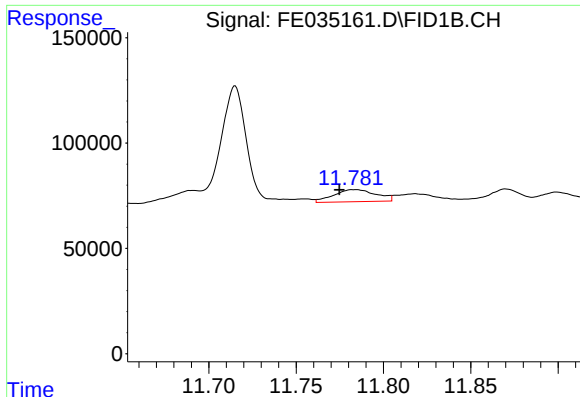

#9 ortho-Terphenyl (SURR)


R.T.: 11.784 min
Delta R.T.: 0.009 min
Response: 97882
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

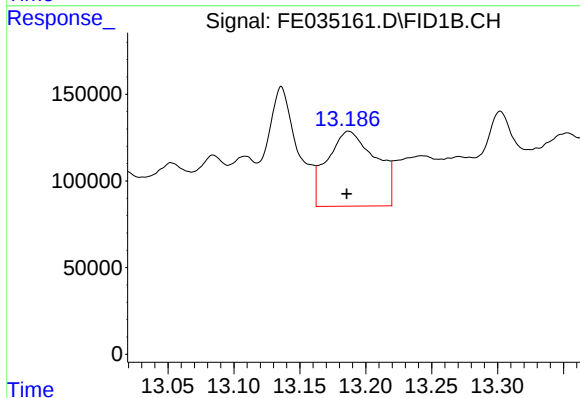


#12 1-chlorooctadecane (SURR)

R.T.: 13.187 min
Delta R.T.: 0.002 min
Response: 1109135
Conc: N.D.

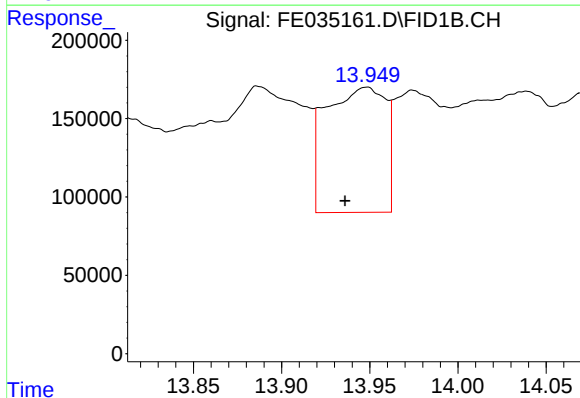


#13 n-Docosane (C22)

R.T.: 13.948 min
Delta R.T.: 0.012 min
Response: 1873941
Conc: 2.09 ug/ml

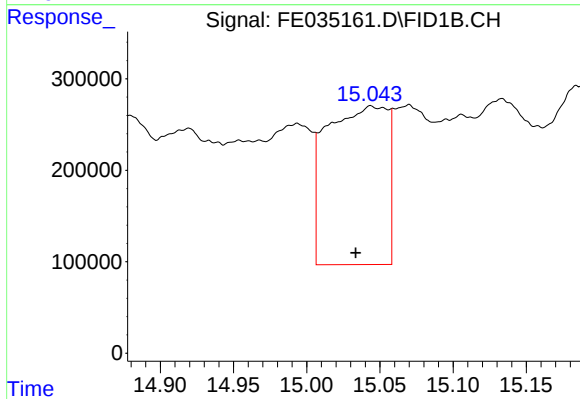

#14 n-Tetracosane (C24)


R.T.: 15.045 min
Delta R.T.: 0.012 min
Response: 5016649
Conc: 5.70 ug/ml

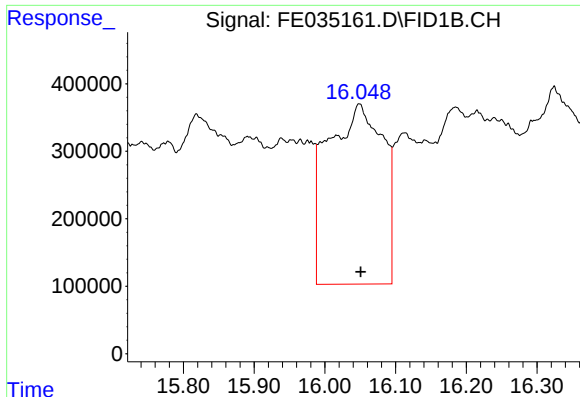

#15 n-Hexacosane (C26)


R.T.: 16.049 min
Delta R.T.: -0.002 min
Response: 14499955
Conc: 17.18 ug/ml

Instrument :
FID_E
ClientSampleId :

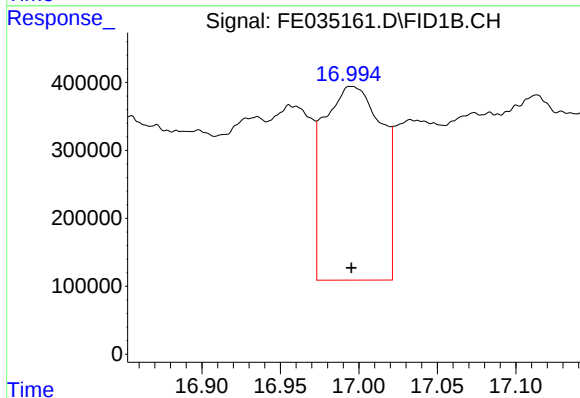


#16 n-Octacosane (C28)

R.T.: 16.996 min
Delta R.T.: 0.000 min
Response: 7381192
Conc: 9.40 ug/ml

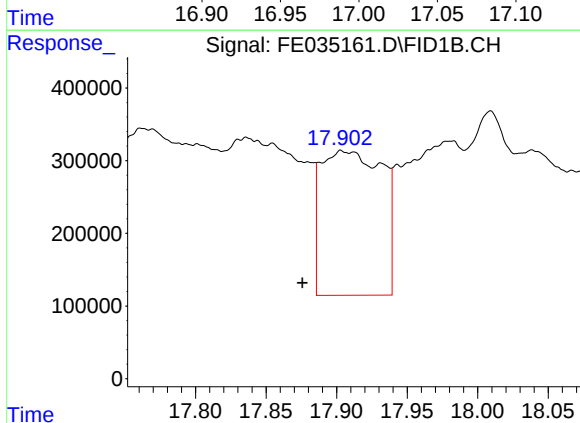


#17 n-Tricontane (C30)

R.T.: 17.905 min
Delta R.T.: 0.029 min
Response: 5999111
Conc: 8.61 ug/ml

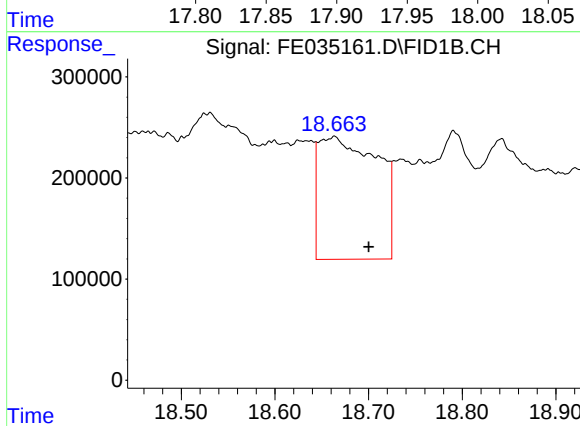

#18 n-Dotriacontane (C32)

R.T.: 18.663 min
Delta R.T.: -0.037 min
Response: 5280593
Conc: 9.36 ug/ml

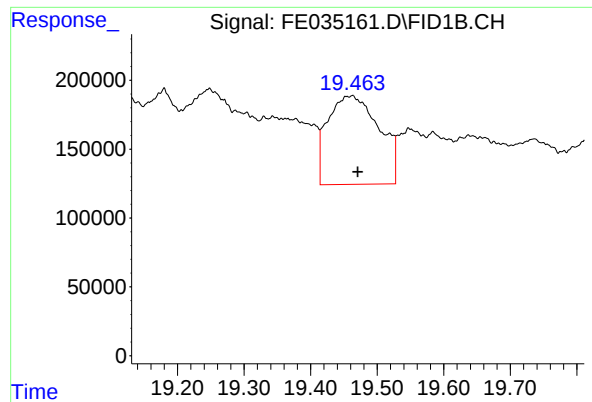

#19 n-Tetratriacontane (C34)

R.T.: 19.461 min
Delta R.T.: -0.010 min
Response: 3440503
Conc: 8.26 ug/ml

Instrument :

FID_E

ClientSampleId :