

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022322AL\
 Data File : FE035140.D
 Signal(s) : FID1B.CH
 Acq On : 22 Feb 2022 12:09
 Operator : YP\AJ
 Sample : N1594-01DL 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 RO-CONCRETE-COMPDL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/23/2022
 Supervised By :Ankita Jodhani 02/23/2022

Integration File: autoint1.e
 Quant Time: Feb 22 13:01:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022222.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 22 01:24:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.723	3240496	3.248 ug/mlm
Spiked Amount 50.000		Recovery =	6.50%
12) S 1-chlorooctadecane (S...	13.141	2398861	3.089 ug/mlm
Spiked Amount 50.000		Recovery =	6.18%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022322AL\
Data File : FE035140.D
Signal(s) : FID1B.CH
Acq On : 22 Feb 2022 12:09
Operator : YP\AJ
Sample : N1594-01DL 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
RO-CONCRETE-COMPDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/23/2022
Supervised By :Ankita Jodhani 02/23/2022

Integration File: autoint1.e
Quant Time: Feb 22 13:01:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022222.M
Quant Title : GC Extractables
QLast Update : Tue Feb 22 01:24:23 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

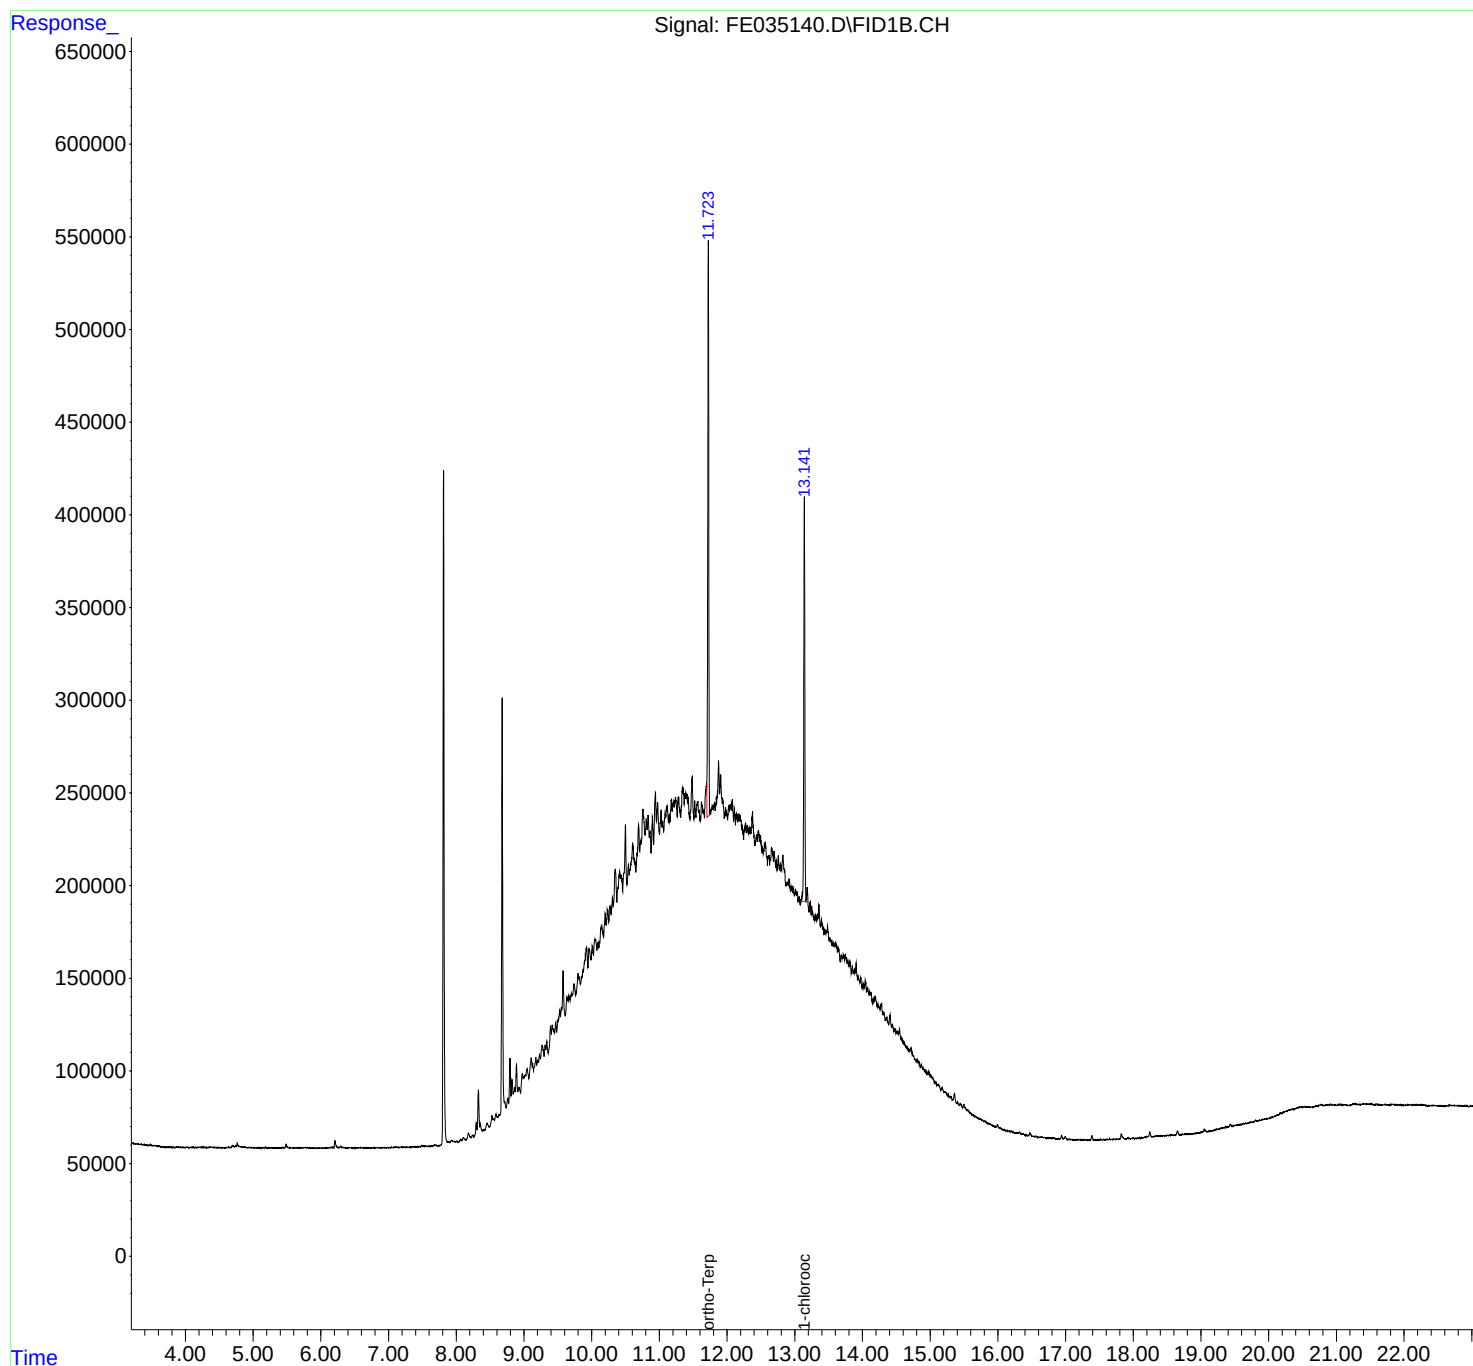

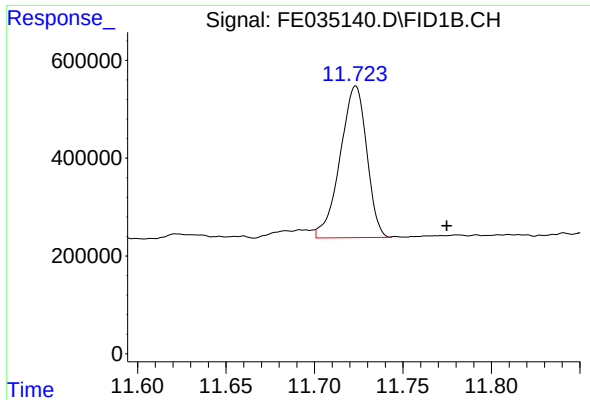


#9 ortho-Terphenyl (SURR)

R.T.: 11.723 min
Delta R.T.: -0.052 min
Response: 3240496
Conc: 3.25 ug/ml

Instrument :
FID_E
ClientSampleId :
RO-CONCRETE-COMPD

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/23/2022
Supervised By :Ankita Jodhani 02/23/2022

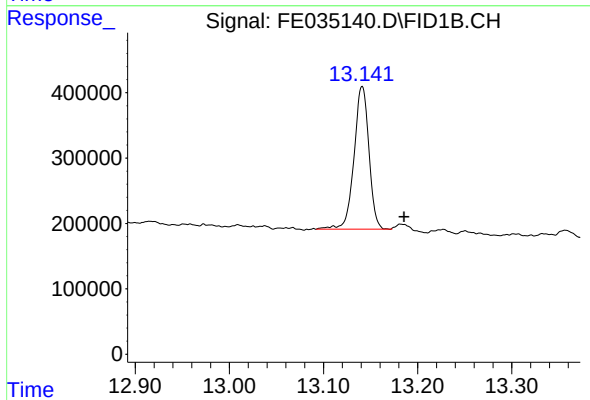

#12 1-chlorooctadecane (SURR)

R.T.: 13.141 min
Delta R.T.: -0.045 min
Response: 2398861
Conc: 3.09 ug/ml m