

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022322AL\
 Data File : FE035154.D
 Signal(s) : FID1B.CH
 Acq On : 22 Feb 2022 19:59
 Operator : YP\AJ
 Sample : N1626-08DL 20X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 CC-B4DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/23/2022
 Supervised By :Ankita Jodhani 02/23/2022

Integration File: autoint1.e
 Quant Time: Feb 23 01:03:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022222.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 22 01:24:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.715	1740528	1.744 ug/mlm
Spiked Amount	50.000	Recovery =	3.49%
12) S 1-chlorooctadecane (S...	13.136	1321547	1.702 ug/mlm
Spiked Amount	50.000	Recovery =	3.40%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022322AL\
Data File : FE035154.D
Signal(s) : FID1B.CH
Acq On : 22 Feb 2022 19:59
Operator : YP\AJ
Sample : N1626-08DL 20X
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
CC-B4DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/23/2022
Supervised By :Ankita Jodhani 02/23/2022

Integration File: autoint1.e
Quant Time: Feb 23 01:03:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022222.M
Quant Title : GC Extractables
QLast Update : Tue Feb 22 01:24:23 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

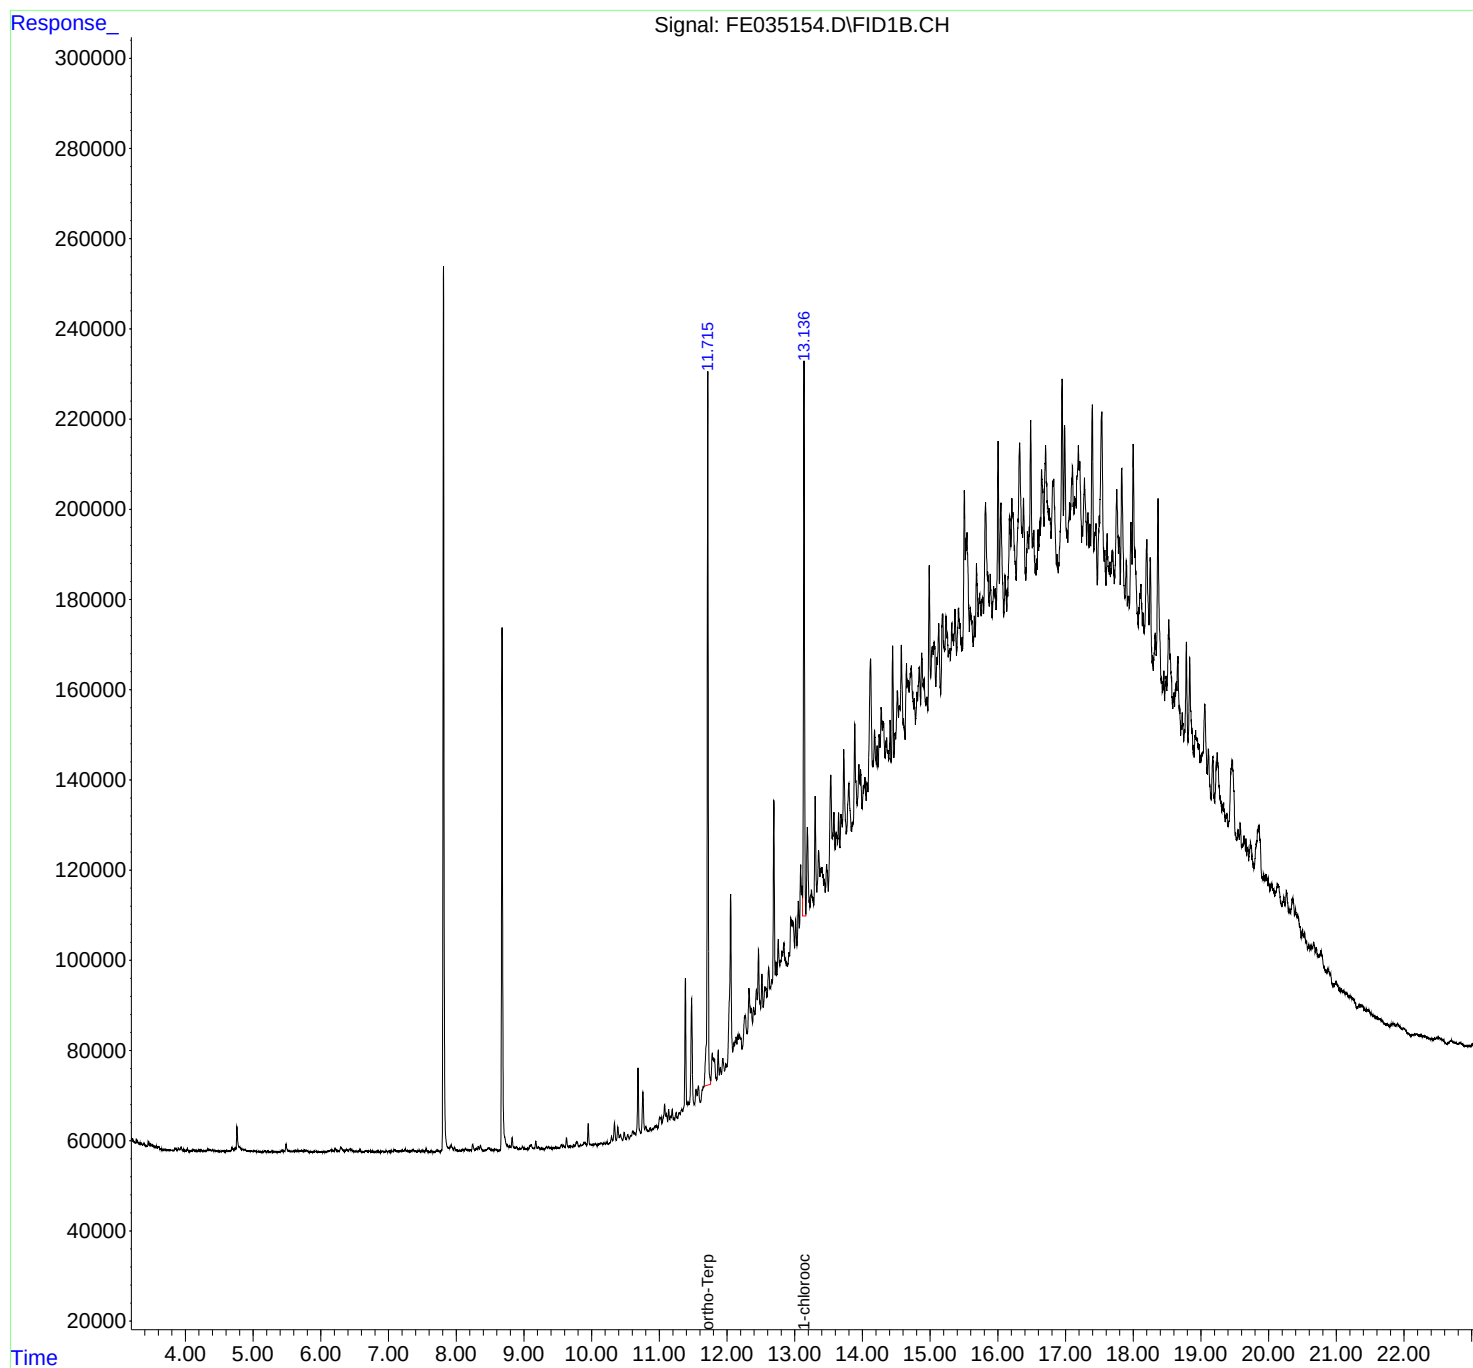

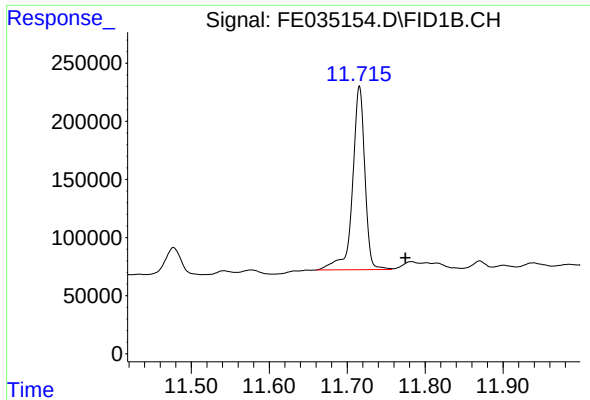


#9 ortho-Terphenyl (SURR)

R.T.: 11.715 min
Delta R.T.: -0.059 min
Response: 1740528
Conc: 1.74 ug/ml

Instrument :
FID_E
ClientSampleId :
CC-B4DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/23/2022
Supervised By :Ankita Jodhani 02/23/2022

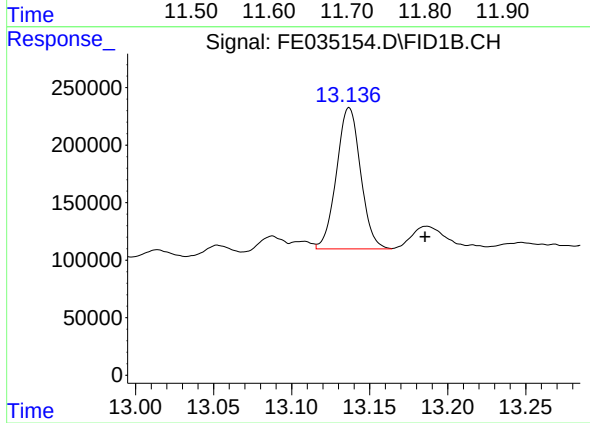

#12 1-chlorooctadecane (SURR)

R.T.: 13.136 min
Delta R.T.: -0.049 min
Response: 1321547
Conc: 1.70 ug/ml m