

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022323AL\
 Data File : FE040524.D
 Signal(s) : FID1B.ch
 Acq On : 23 Feb 2023 19:41
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 24 04:48:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 020223.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 02 04:52:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
17) T n-Tricontane (C30)	18.040	53269	0.361 ug/ml
18) T n-Dotriacontane (C32)	18.873	75900	0.518 ug/ml
19) T n-Tetratriacontane (C34)	19.657	87867	0.639 ug/ml
20) T n-Hexatriacontane (C36)	20.397	163653	1.234 ug/ml
21) T n-Octatriacontane (C38)	21.128	147468	1.137 ug/ml
22) T n-Tetracontane (C40)	22.023	195573	1.473 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022323AL\
Data File : FE040524.D
Signal(s) : FID1B.ch
Acq On : 23 Feb 2023 19:41
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 24 04:48:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 020223.M
Quant Title : GC Extractables
QLast Update : Thu Feb 02 04:52:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

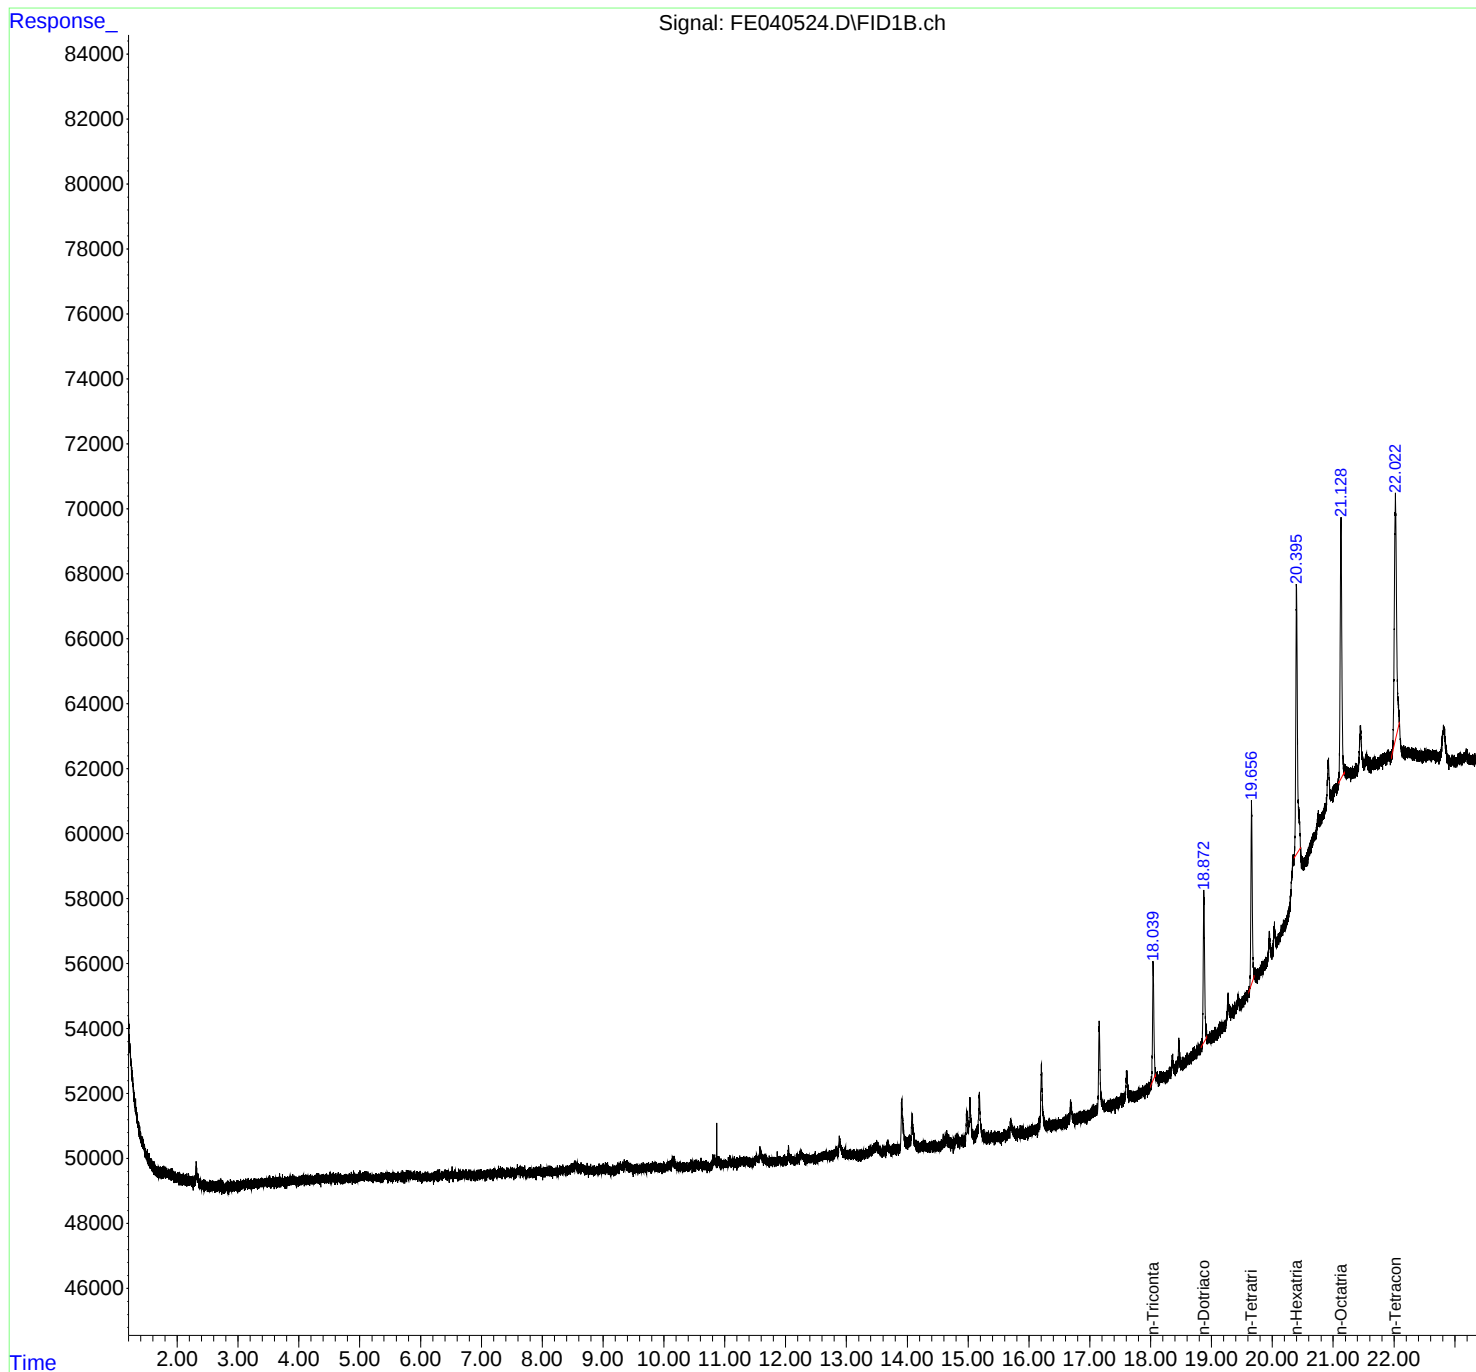


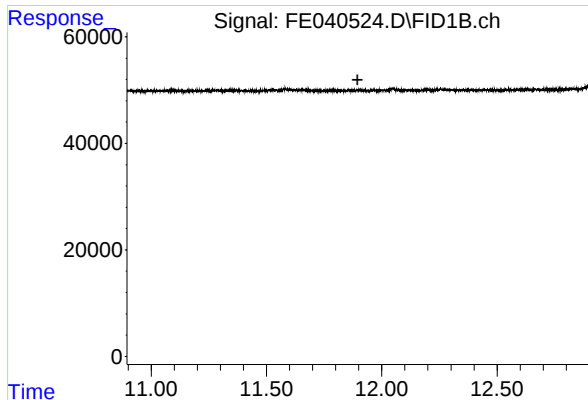

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.895 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

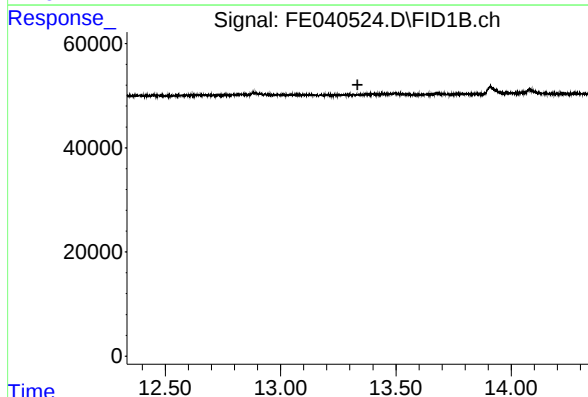


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.333 min
Response: 0
Conc: N.D.

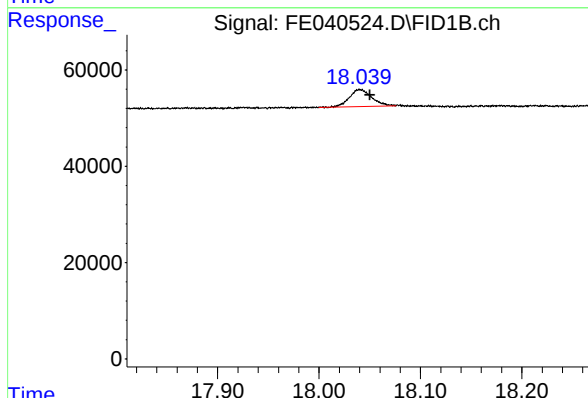


#17 n-Tricontane (C30)

R.T.: 18.040 min
Delta R.T.: -0.010 min
Response: 53269
Conc: 0.36 ug/ml

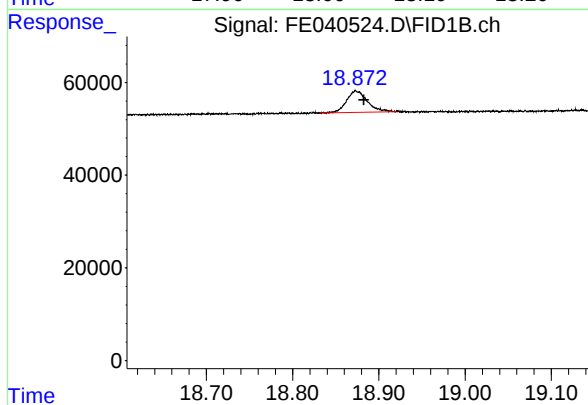

#18 n-Dotriacontane (C32)


R.T.: 18.873 min
Delta R.T.: -0.009 min
Response: 75900
Conc: 0.52 ug/ml

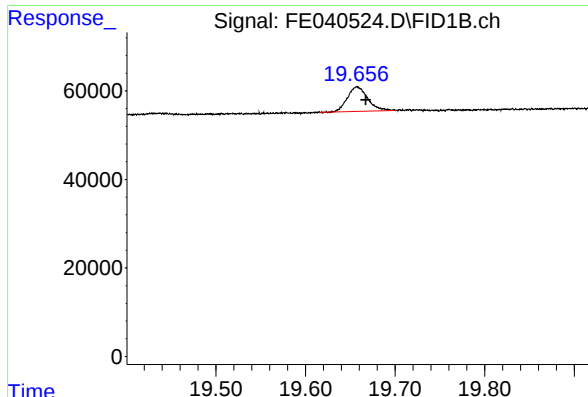

#19 n-Tetratriacontane (C34)


R.T.: 19.657 min
Delta R.T.: -0.010 min
Response: 87867
Conc: 0.64 ug/ml

Instrument :
FID_E
ClientSampleId :

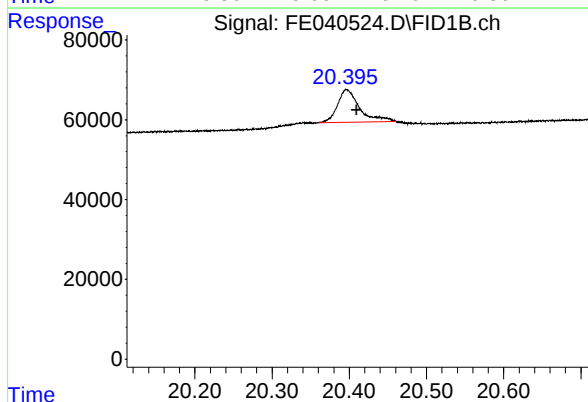


#20 n-Hexatriacontane (C36)

R.T.: 20.397 min
Delta R.T.: -0.013 min
Response: 163653
Conc: 1.23 ug/ml

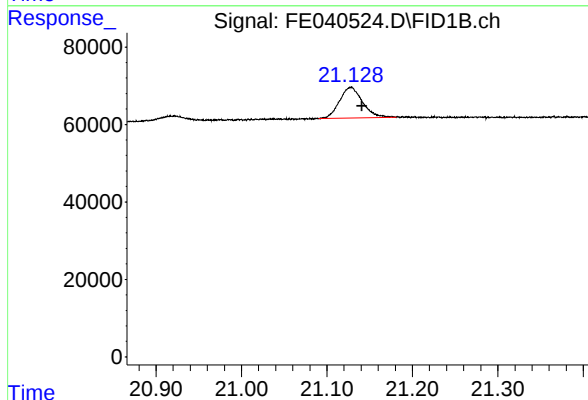

#21 n-Octatriacontane (C38)

R.T.: 21.128 min
Delta R.T.: -0.013 min
Response: 147468
Conc: 1.14 ug/ml

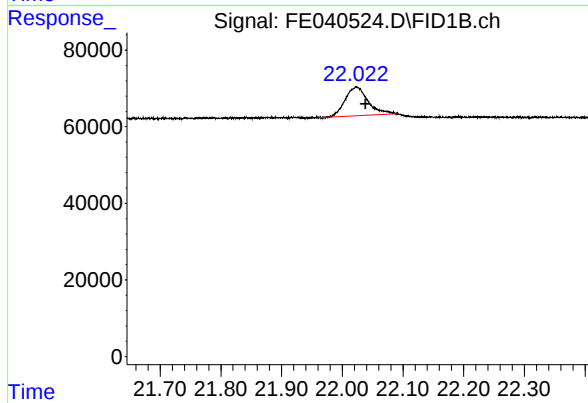

#22 n-Tetracontane (C40)

R.T.: 22.023 min
Delta R.T.: -0.015 min
Response: 195573
Conc: 1.47 ug/ml