

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022521\
 Data File : FE033301.D
 Signal(s) : FID1B.CH
 Acq On : 25 Feb 2021 9:04
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Feb 25 13:42:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022221.M
 Quant Title :
 QLast Update : Tue Feb 23 10:21:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.567	17665050	51.429 ug/ml
Target Compounds			
2) N-DECANE	4.321	18915330	56.907 ug/ml
3) N-DODECANE	6.327	19175600	56.183 ug/ml
4) N-TETRADECANE	8.119	19781570	54.307 ug/ml
5) N-HEXADECANE	9.719	19763943	53.842 ug/ml
6) N-OCTADECANE	11.161	20100944	53.162 ug/ml
7) N-EICOSANE	12.470	20013743	52.348 ug/ml
8) N-DOCOSANE	13.669	20053265	51.817 ug/ml
10) N-TETRACOSANE	14.773	20095983	51.584 ug/ml
11) N-HEXACOSANE	15.794	19924372	51.357 ug/ml
12) N-OCTACOSANE	16.744	20014432	51.069 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE022521\
Data File : FE033301.D
Signal(s) : FID1B.CH
Acq On : 25 Feb 2021 9:04
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Feb 25 13:42:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022221.M
Quant Title :
QLast Update : Tue Feb 23 10:21:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

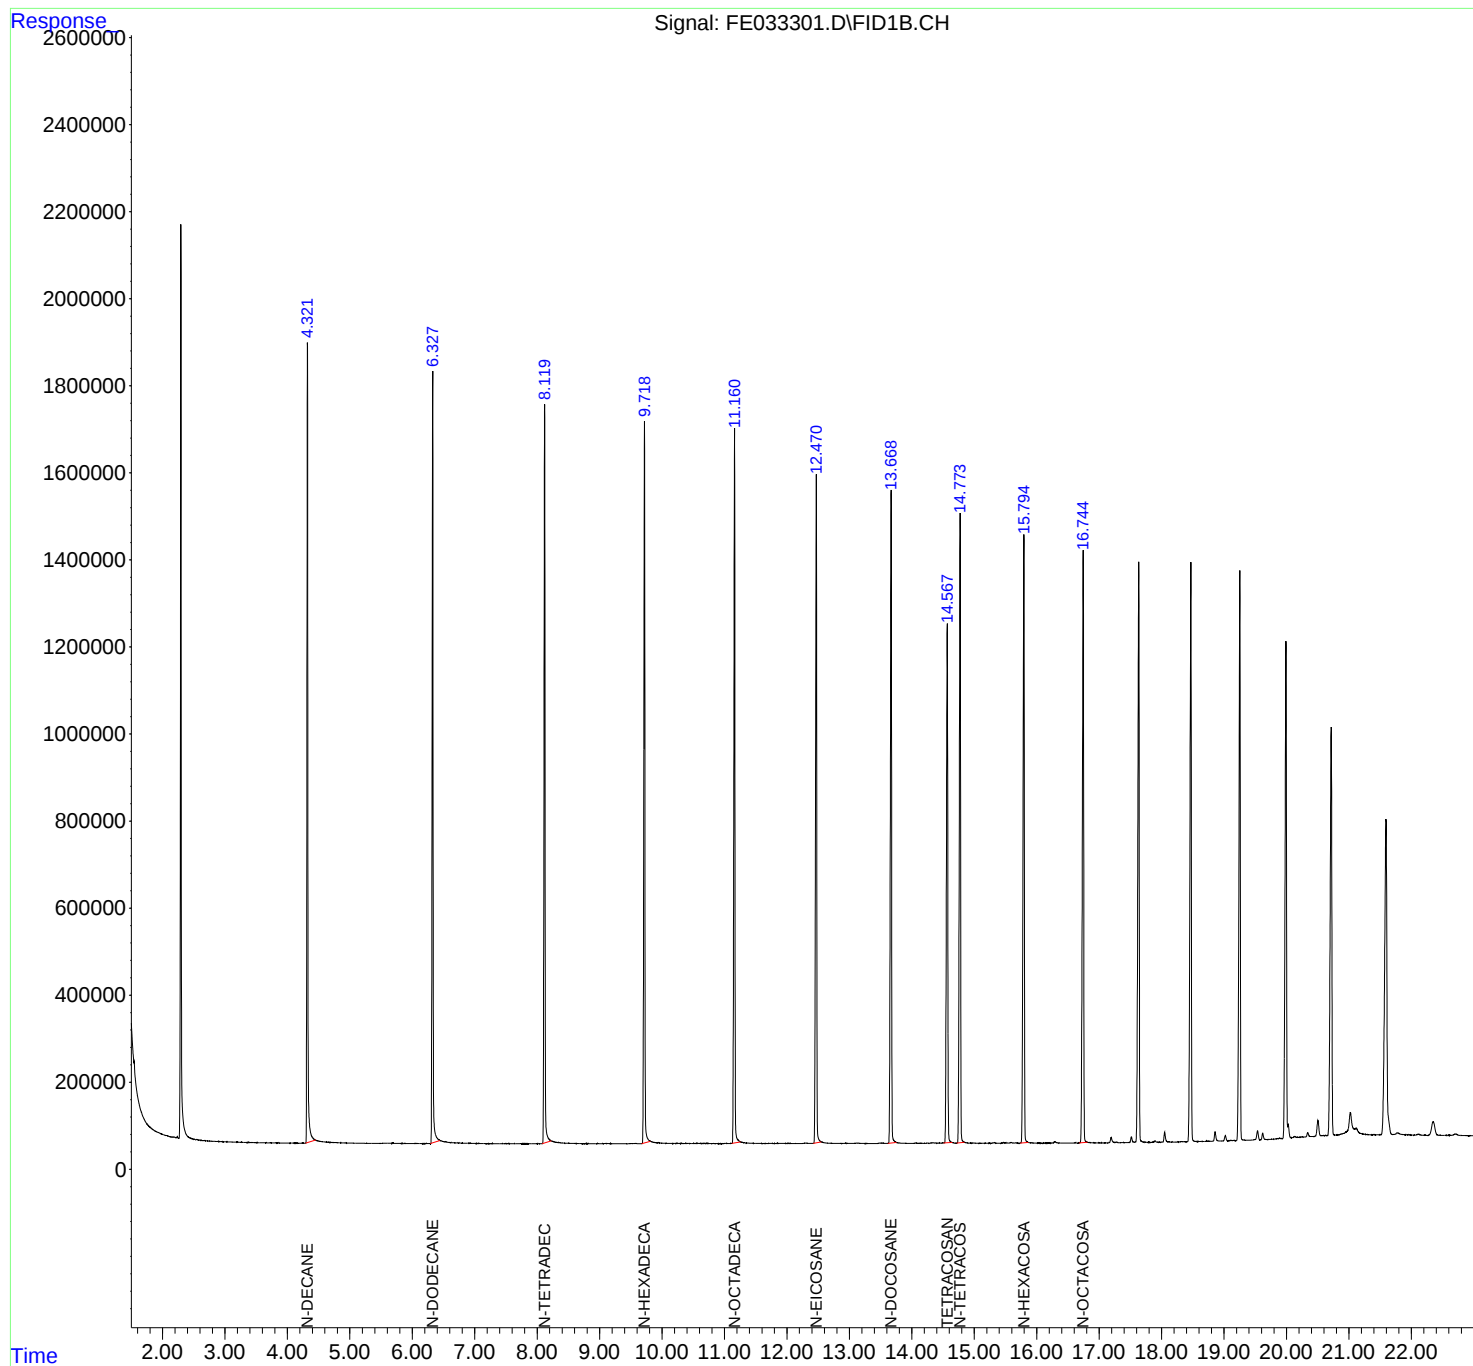


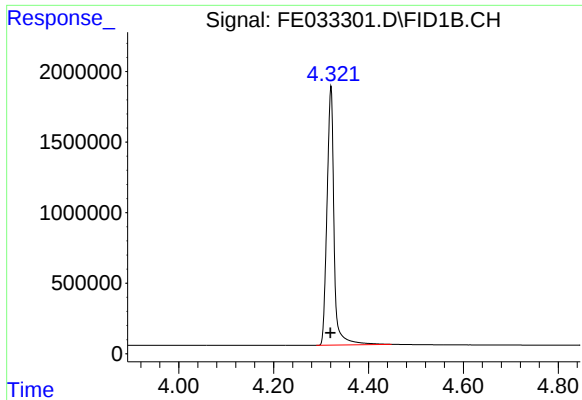

#2 N-DECANE


R.T.: 4.321 min
Delta R.T.: 0.000 min
Response: 18915330
Conc: 56.91 ug/ml

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

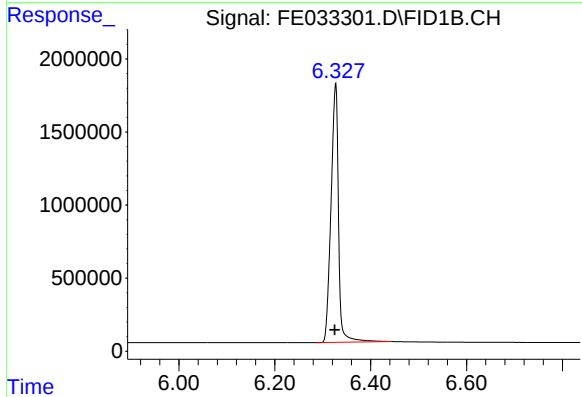


#3 N-DODECANE

R.T.: 6.327 min
Delta R.T.: 0.002 min
Response: 19175600
Conc: 56.18 ug/ml

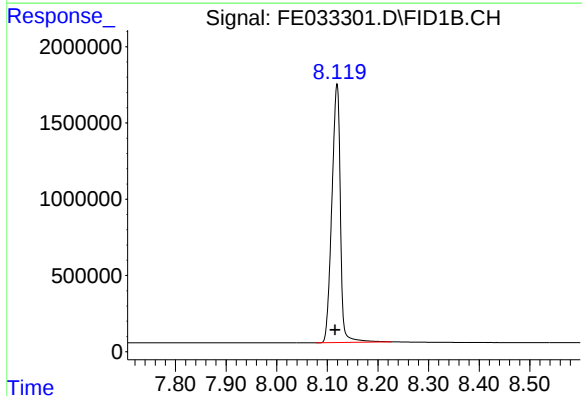


#4 N-TETRADECANE

R.T.: 8.119 min
Delta R.T.: 0.004 min
Response: 19781570
Conc: 54.31 ug/ml

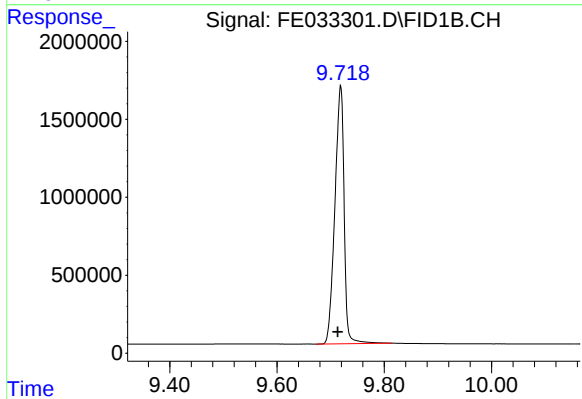

#5 N-HEXADECANE


R.T.: 9.719 min
Delta R.T.: 0.005 min
Response: 19763943
Conc: 53.84 ug/ml

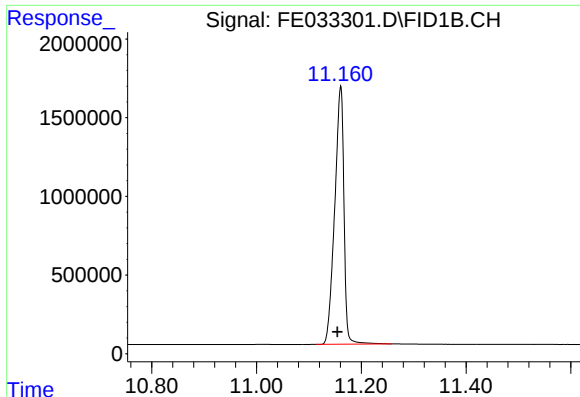

#6 N-OCTADECANE


R.T.: 11.161 min
Delta R.T.: 0.007 min
Response: 20100944
Conc: 53.16 ug/ml

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

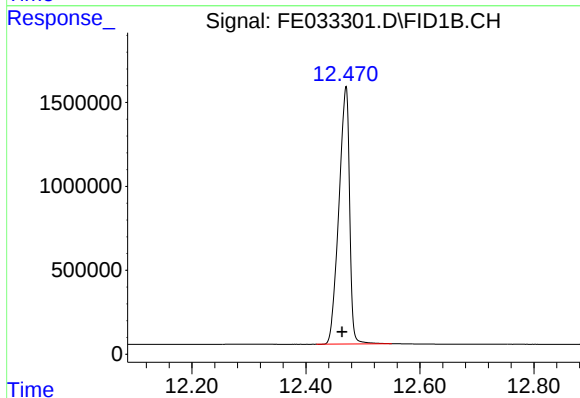


#7 N-EICOSANE

R.T.: 12.470 min
Delta R.T.: 0.007 min
Response: 20013743
Conc: 52.35 ug/ml

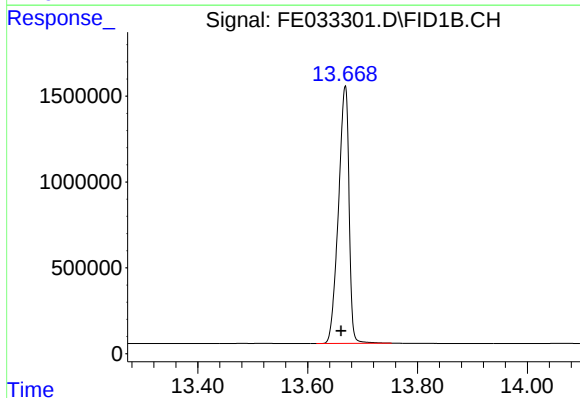


#8 N-DOCOSANE

R.T.: 13.669 min
Delta R.T.: 0.008 min
Response: 20053265
Conc: 51.82 ug/ml

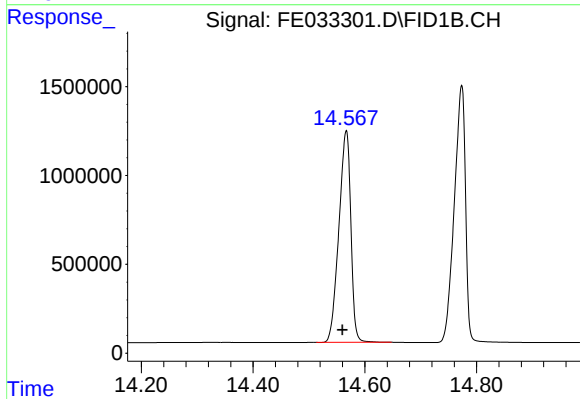

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.567 min
Delta R.T.: 0.007 min
Response: 17665050
Conc: 51.43 ug/ml

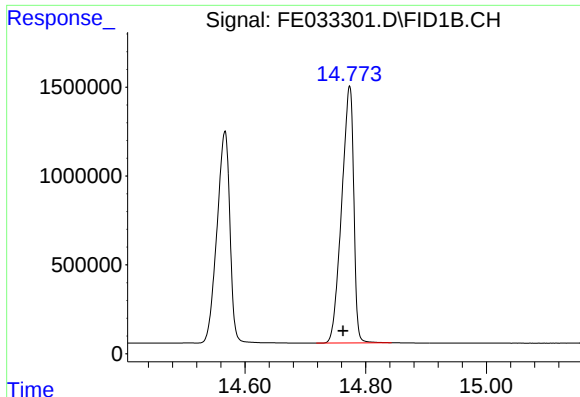

#10 N-TETRACOSANE


R.T.: 14.773 min
Delta R.T.: 0.011 min
Response: 20095983
Conc: 51.58 ug/ml

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

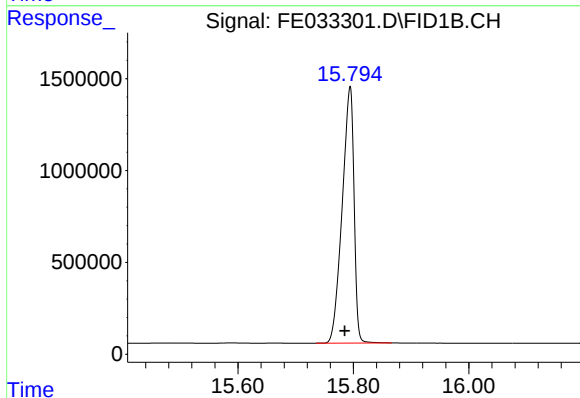

#11 N-HEXACOSANE

R.T.: 15.794 min
Delta R.T.: 0.009 min
Response: 19924372
Conc: 51.36 ug/ml

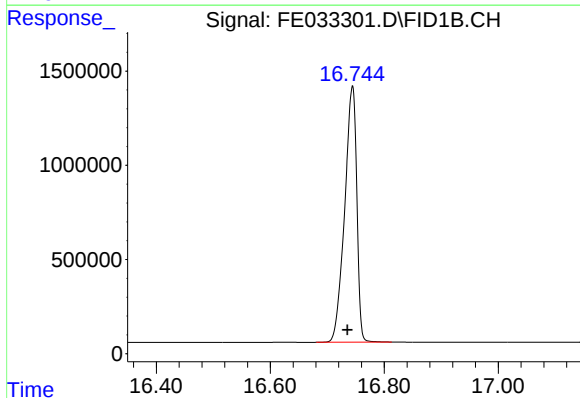

#12 N-OCTACOSANE

R.T.: 16.744 min
Delta R.T.: 0.009 min
Response: 20014432
Conc: 51.07 ug/ml