

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030123AL\
Data File : FE040593.D
Signal(s) : FID1B.ch
Acq On : 28 Feb 2023 11:35
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 01 02:55:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022823.M
Quant Title : GC Extractables
QLast Update : Tue Feb 28 03:05:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.888	82756	0.484 ug/ml
20) T	n-Hexatriacontane (C36)	20.442	135718	0.934 ug/ml
22) T	n-Tetracontane (C40)	22.068	334750	2.166 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030123AL\
Data File : FE040593.D
Signal(s) : FID1B.ch
Acq On : 28 Feb 2023 11:35
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 01 02:55:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022823.M
Quant Title : GC Extractables
QLast Update : Tue Feb 28 03:05:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

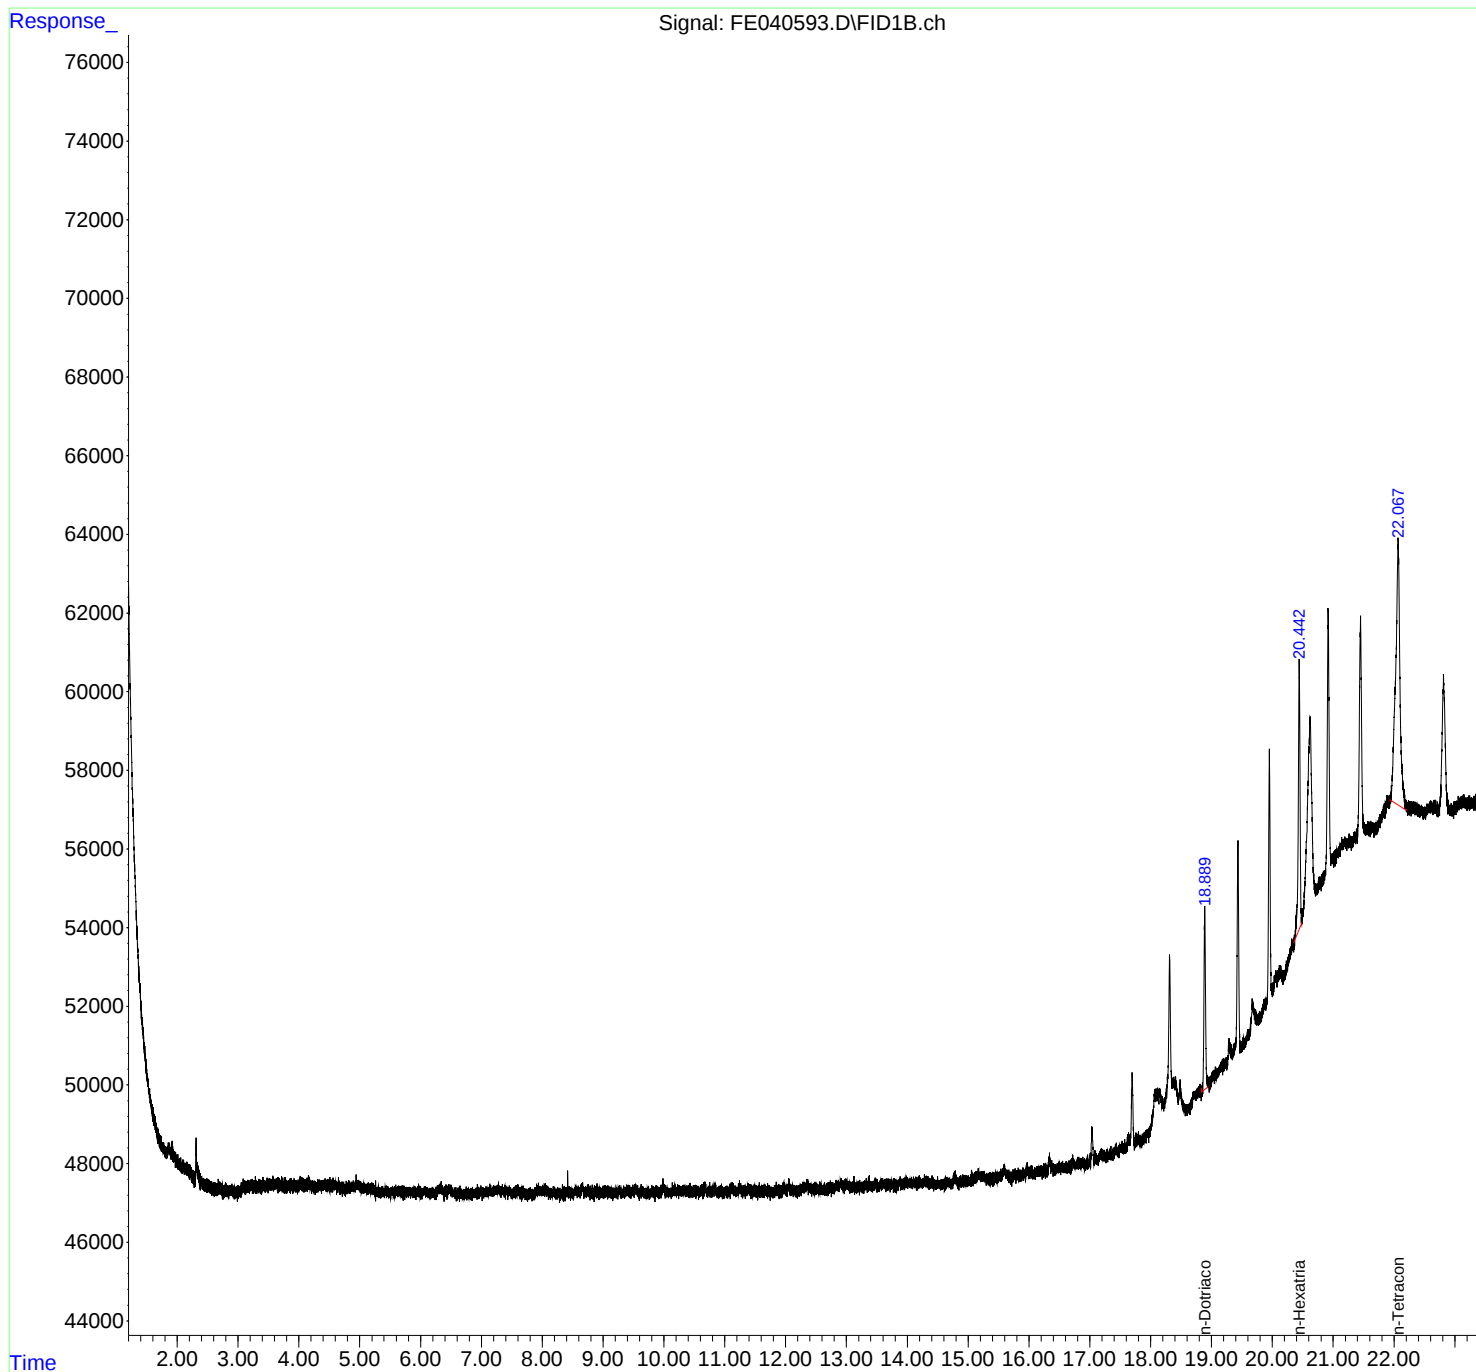


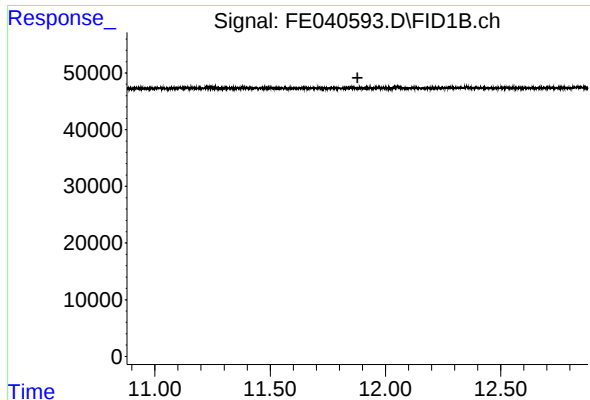

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.879 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

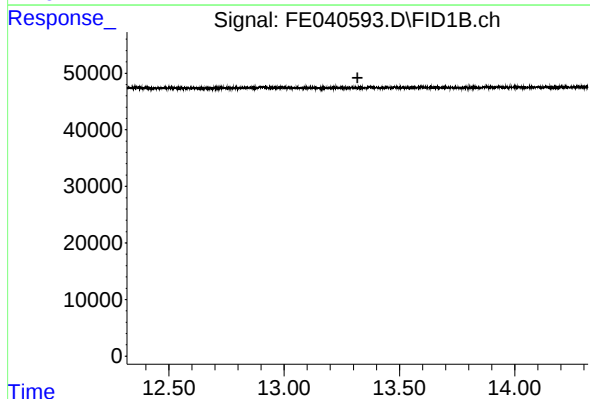


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.318 min
Response: 0
Conc: N.D.

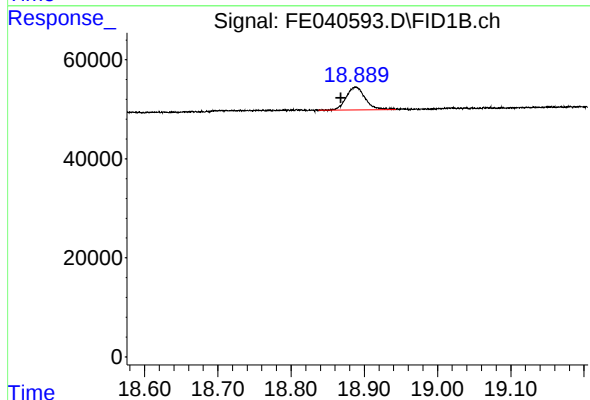


#18 n-Dotriacontane (C32)

R.T.: 18.888 min
Delta R.T.: 0.020 min
Response: 82756
Conc: 0.48 ug/ml

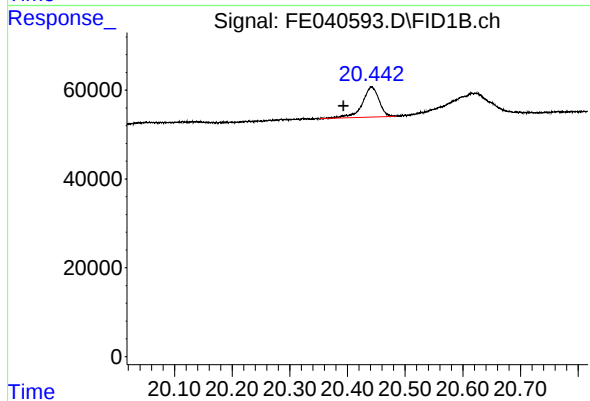

#20 n-Hexatriacontane (C36)

R.T.: 20.442 min
Delta R.T.: 0.049 min
Response: 135718
Conc: 0.93 ug/ml

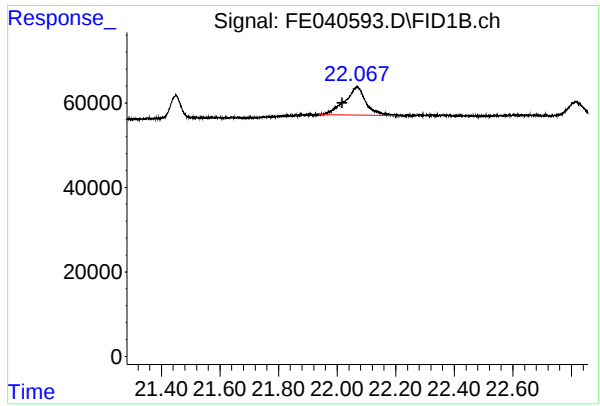

#22 n-Tetracontane (C40)

R.T.: 22.068 min
Delta R.T.: 0.050 min
Response: 334750
Conc: 2.17 ug/ml

Instrument :

FID_E

ClientSampleId :