

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030123AL\
 Data File : FE040611.D
 Signal(s) : FID1B.ch
 Acq On : 01 Mar 2023 01:12
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 01 02:57:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022823.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 28 03:05:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
16) T n-Octacosane (C28)	17.159	43367	0.259 ug/ml
18) T n-Dotriacontane (C32)	18.890	756997	4.423 ug/ml
19) T n-Tetratriacontane (C34)	19.658	107749	0.697 ug/ml
20) T n-Hexatriacontane (C36)	20.397	46260	0.318 ug/ml
21) T n-Octatriacontane (C38)	21.127	136438	0.993 ug/ml
22) T n-Tetracontane (C40)	22.015	521890	3.377 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030123AL\
Data File : FE040611.D
Signal(s) : FID1B.ch
Acq On : 01 Mar 2023 01:12
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 01 02:57:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022823.M
Quant Title : GC Extractables
QLast Update : Tue Feb 28 03:05:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

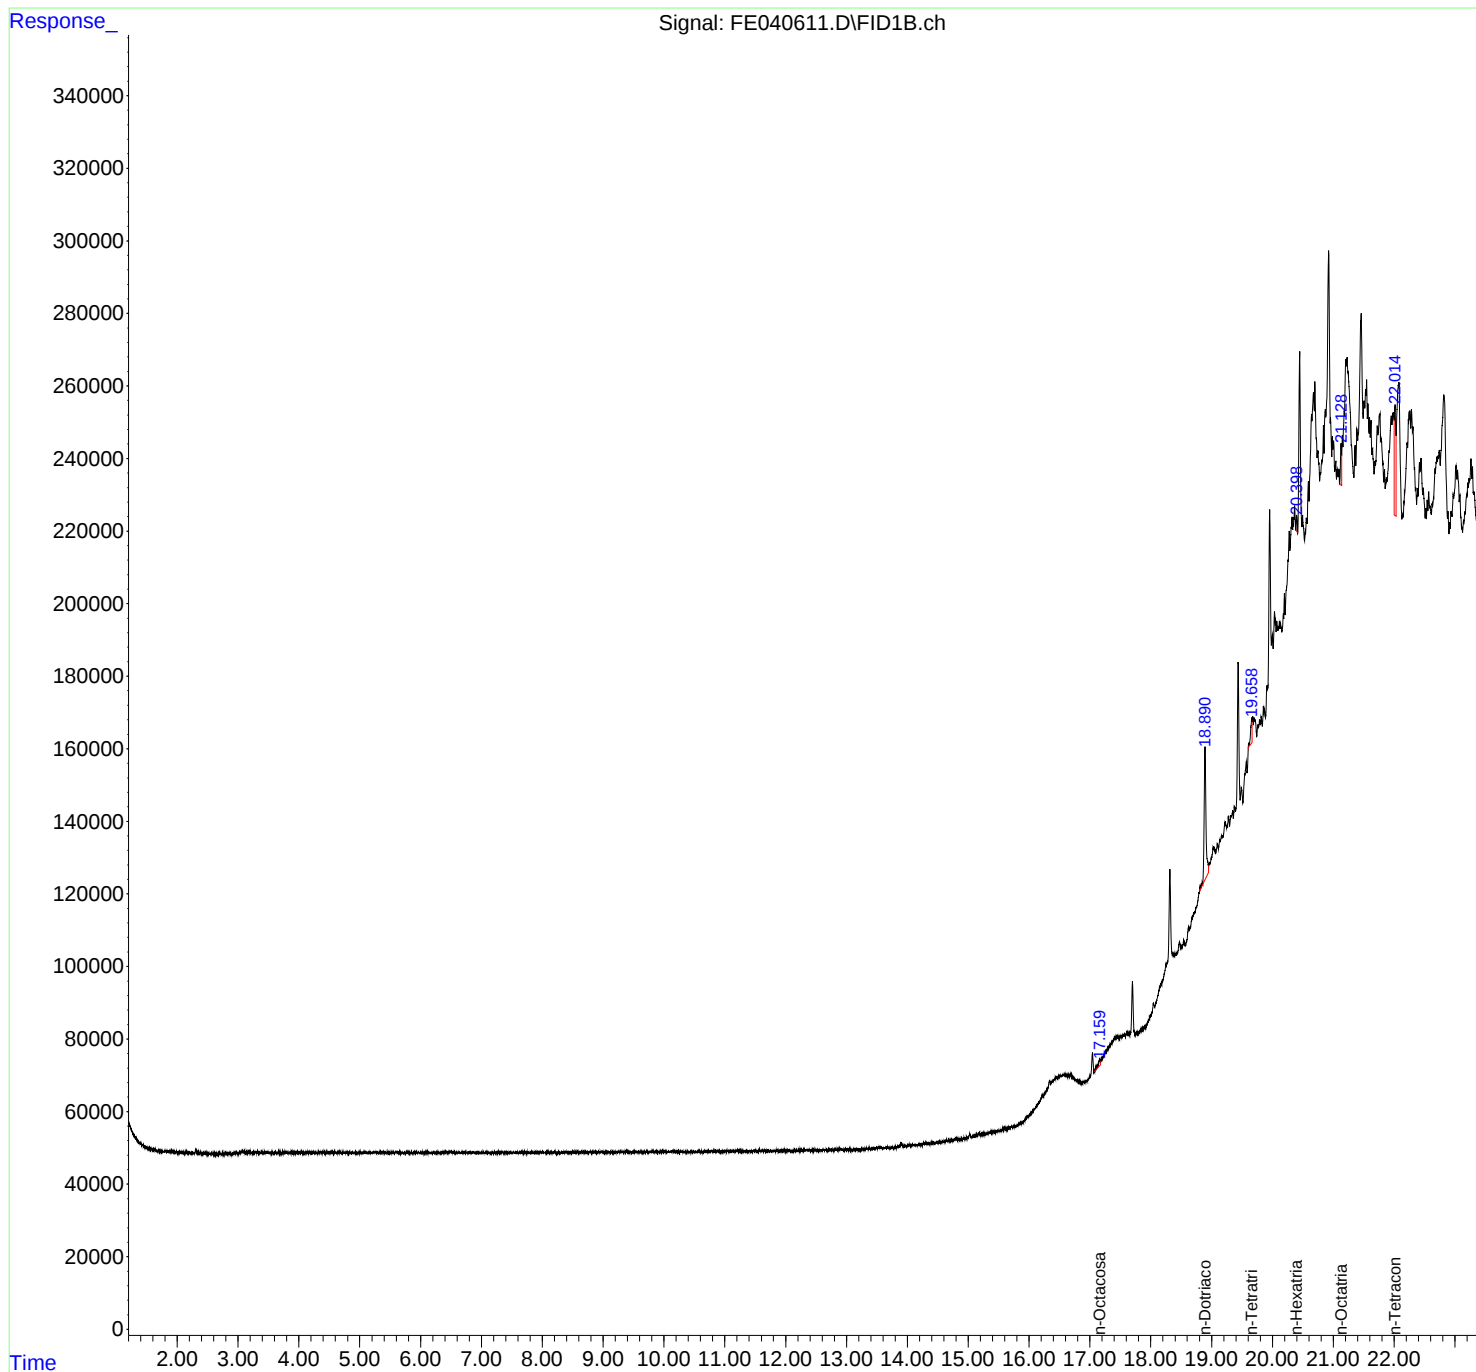


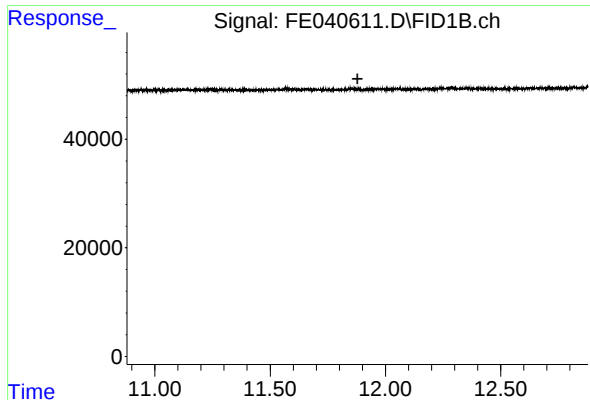

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.879 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

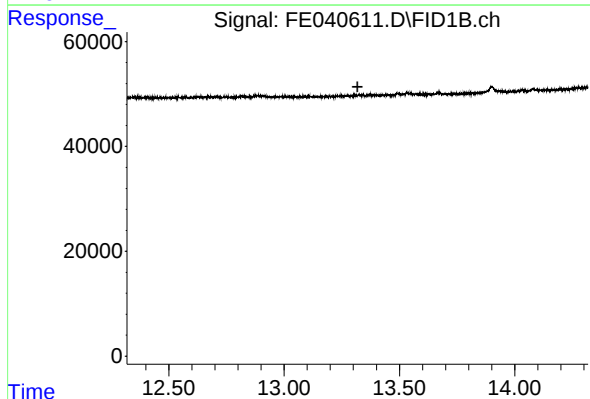


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.318 min
Response: 0
Conc: N.D.

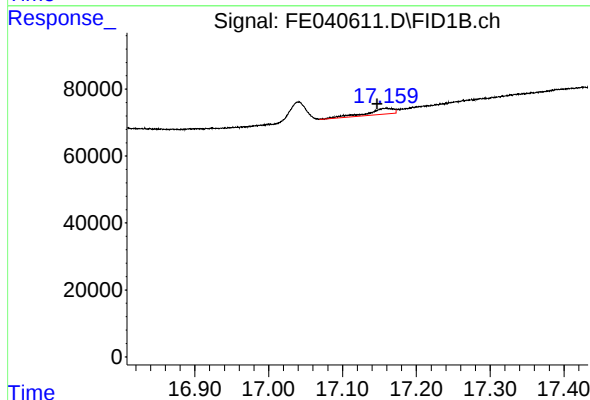


#16 n-Octacosane (C28)

R.T.: 17.159 min
Delta R.T.: 0.012 min
Response: 43367
Conc: 0.26 ug/ml

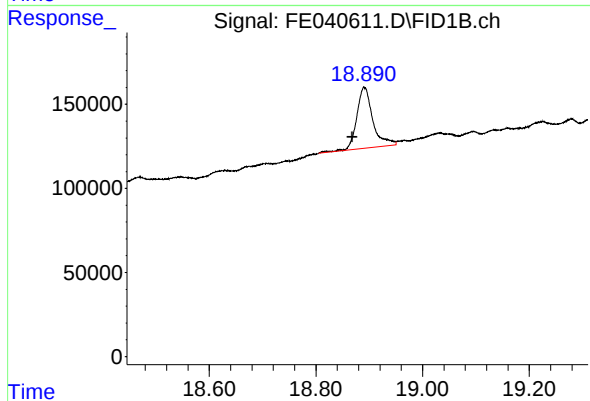

#18 n-Dotriacontane (C32)


R.T.: 18.890 min
Delta R.T.: 0.022 min
Response: 756997
Conc: 4.42 ug/ml

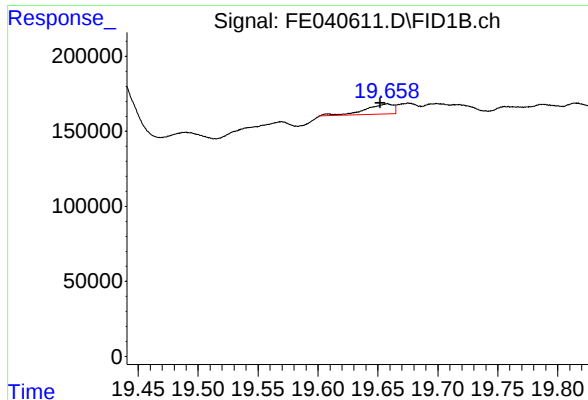

#19 n-Tetratriacontane (C34)


R.T.: 19.658 min
Delta R.T.: 0.006 min
Response: 107749
Conc: 0.70 ug/ml

Instrument :
FID_E
ClientSampleId :

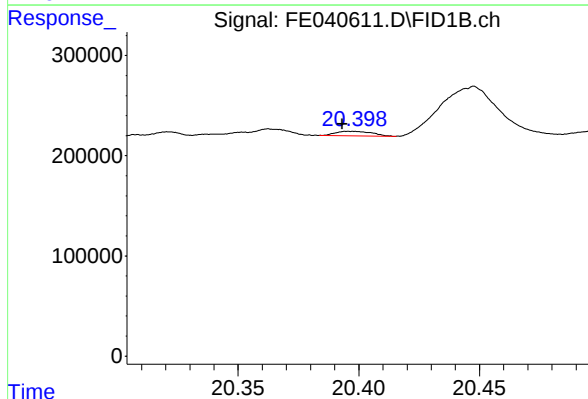


#20 n-Hexatriacontane (C36)

R.T.: 20.397 min
Delta R.T.: 0.004 min
Response: 46260
Conc: 0.32 ug/ml

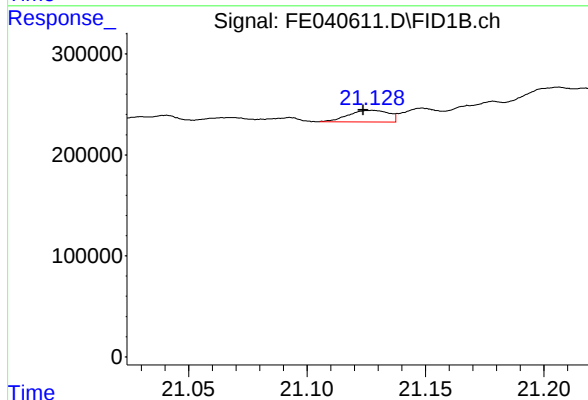

#21 n-Octatriacontane (C38)

R.T.: 21.127 min
Delta R.T.: 0.004 min
Response: 136438
Conc: 0.99 ug/ml

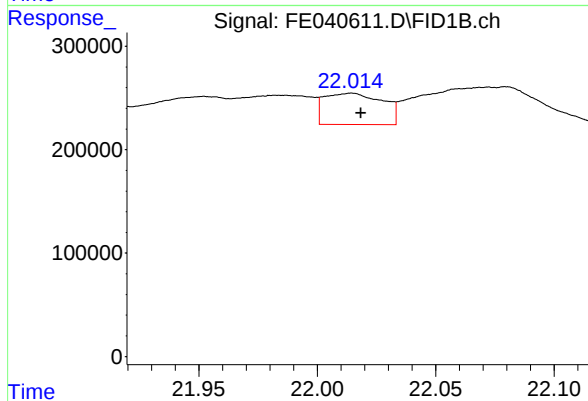

#22 n-Tetracontane (C40)

R.T.: 22.015 min
Delta R.T.: -0.004 min
Response: 521890
Conc: 3.38 ug/ml