

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030220\
 Data File : FE031380.D
 Signal(s) : FID1B.CH
 Acq On : 02 Mar 2020 18:17
 Operator : DD\AJ
 Sample : L1743-08 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 03 00:27:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE021120.M
 Quant Title :
 QLast Update : Tue Feb 11 12:55:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.605	779983	2.510 ug/ml
Target Compounds			
7) N-EICOSANE	12.568f	6076088	17.441 ug/ml
8) N-DOCOSANE	13.733	575909	1.632 ug/ml
10) N-TETRACOSANE	14.797	3108900	8.716 ug/ml
12) N-OCTACOSANE	16.809	812677	2.243 ug/ml
13) N-TRIACONTANE	17.672	386130	1.051 ug/ml
14) N-DOTRIACONTANE	18.499	1278147	3.623 ug/ml
15) N-TETRATRIACONTANE	19.312	1192371	3.904 ug/ml
16) N-HEXATRIACONTANE	20.046	2872688	11.577 ug/ml
18) N-TETRACONTANE	21.671	1611704	8.771 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030220\
Data File : FE031380.D
Signal(s) : FID1B.CH
Acq On : 02 Mar 2020 18:17
Operator : DD\AJ
Sample : L1743-08 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 03 00:27:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE021120.M
Quant Title :
QLast Update : Tue Feb 11 12:55:11 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

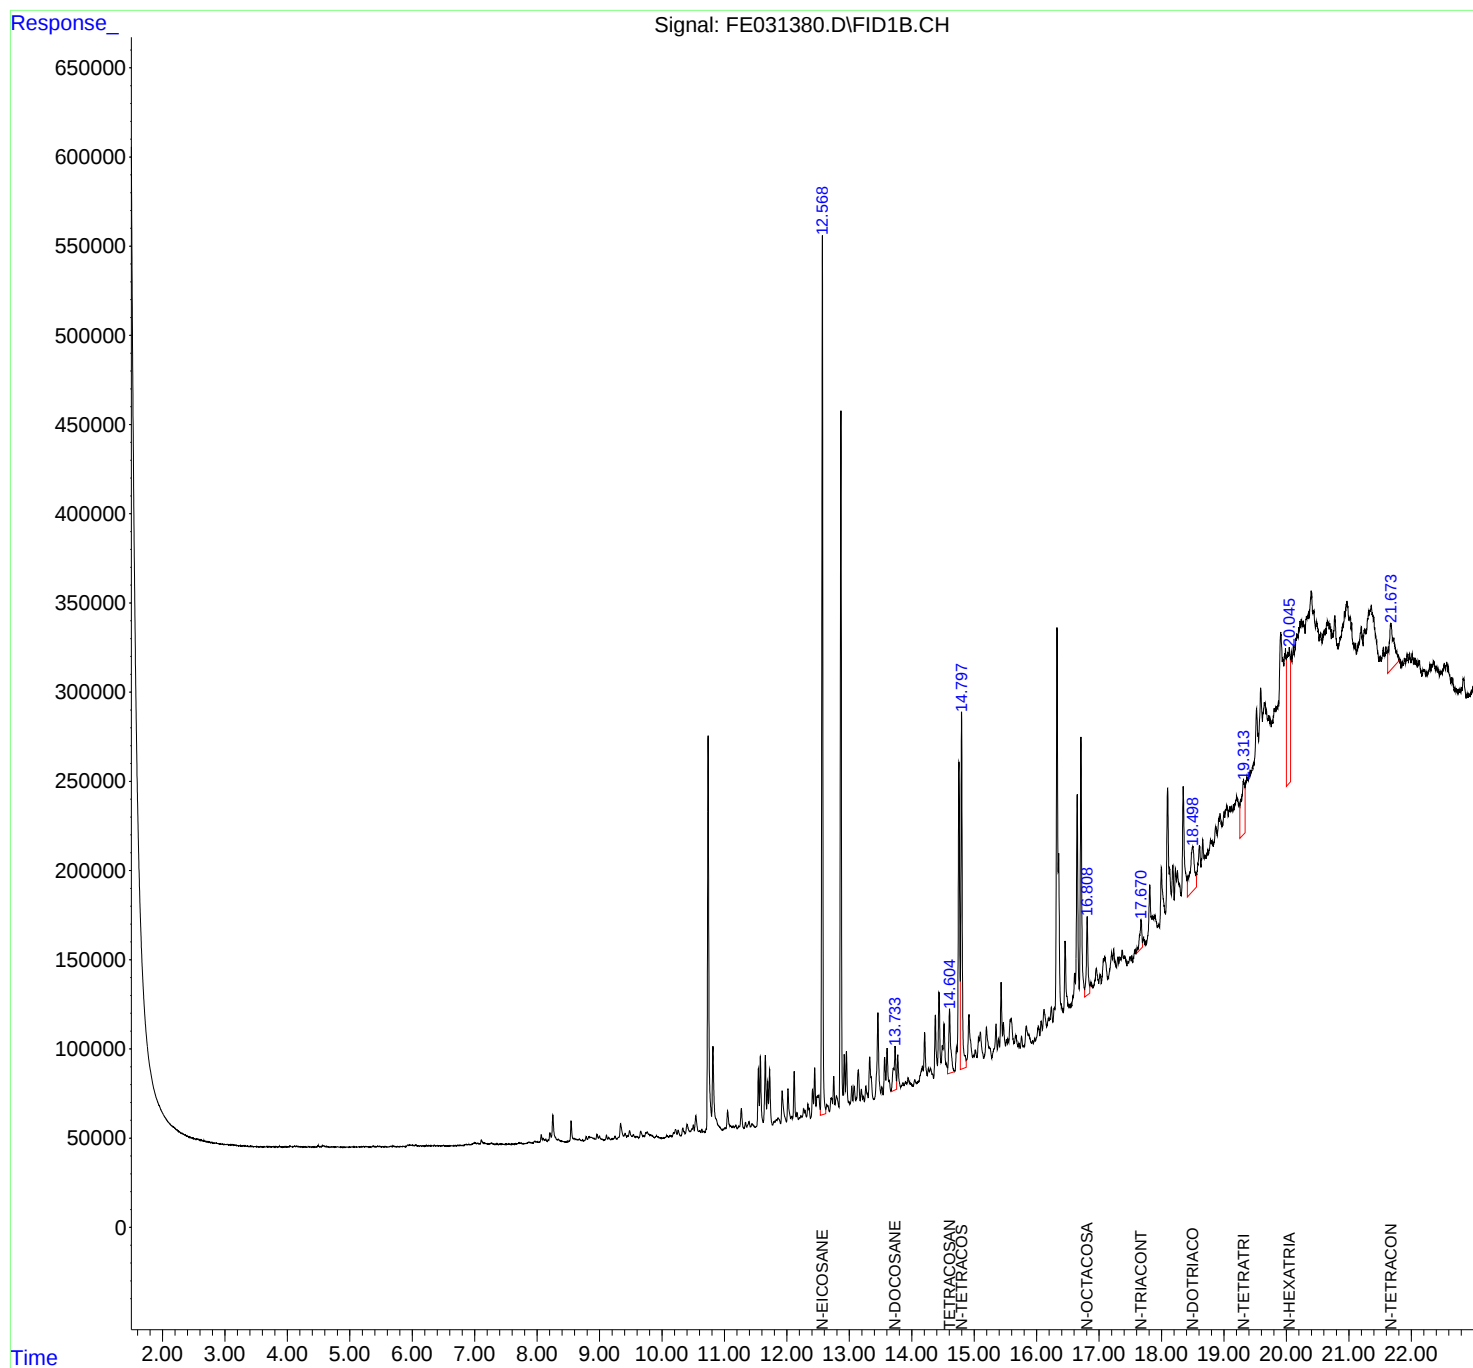


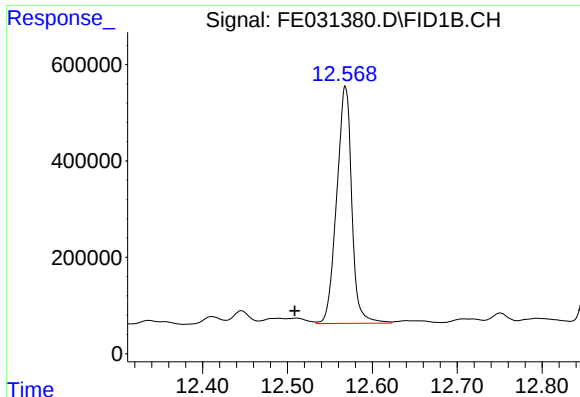

#7 N-EICOSANE


R.T.: 12.568 min
Delta R.T.: 0.059 min
Response: 6076088
Conc: 17.44 ug/ml

Instrument :
FID_E
ClientSampleId :

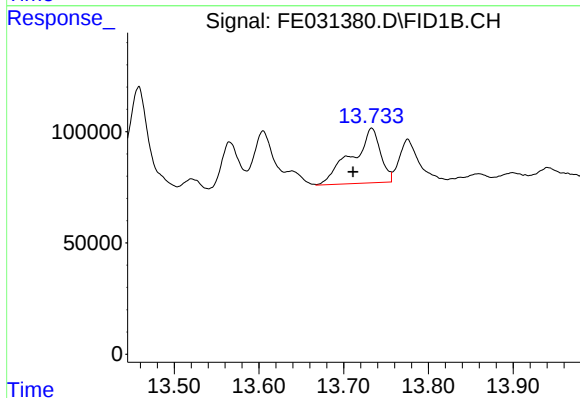


#8 N-DOCOSANE

R.T.: 13.733 min
Delta R.T.: 0.022 min
Response: 575909
Conc: 1.63 ug/ml

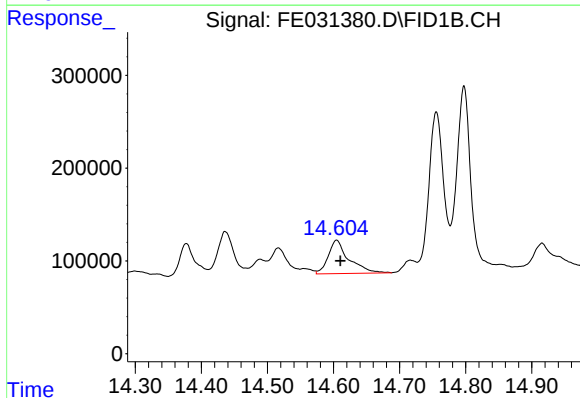


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.605 min
Delta R.T.: -0.006 min
Response: 779983
Conc: 2.51 ug/ml

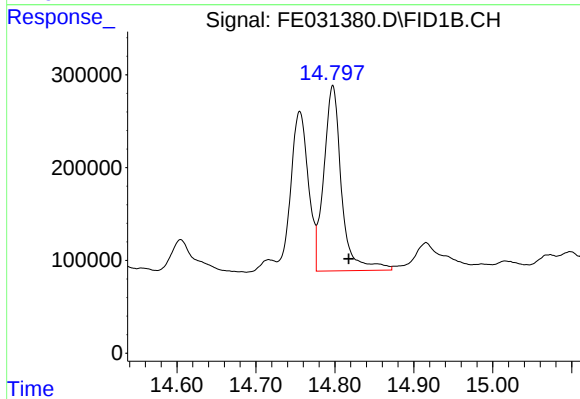

#10 N-TETRACOSANE


R.T.: 14.797 min
Delta R.T.: -0.020 min
Response: 3108900
Conc: 8.72 ug/ml

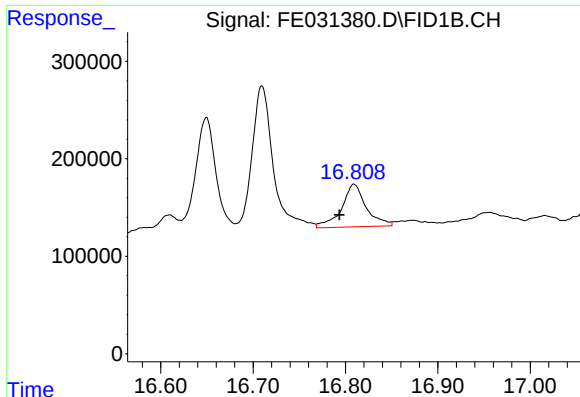

#12 N-OCTACOSANE


R.T.: 16.809 min
Delta R.T.: 0.016 min
Response: 812677
Conc: 2.24 ug/ml

Instrument :
FID_E
ClientSampleId :

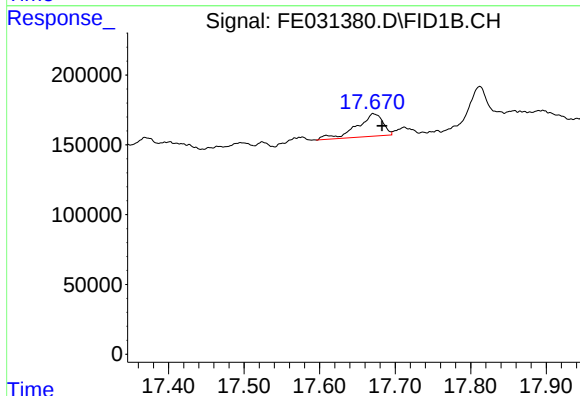


#13 N-TRIACONTANE

R.T.: 17.672 min
Delta R.T.: -0.011 min
Response: 386130
Conc: 1.05 ug/ml

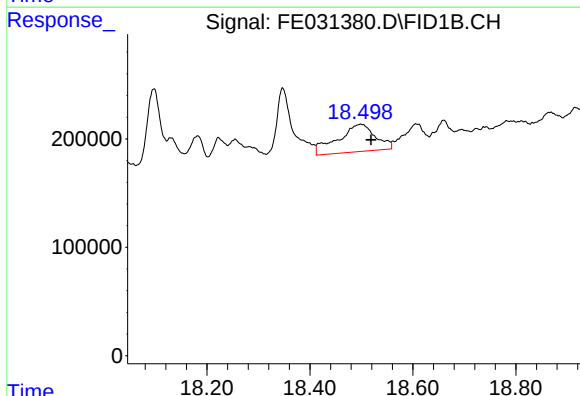


#14 N-DOTRIACONTANE

R.T.: 18.499 min
Delta R.T.: -0.020 min
Response: 1278147
Conc: 3.62 ug/ml

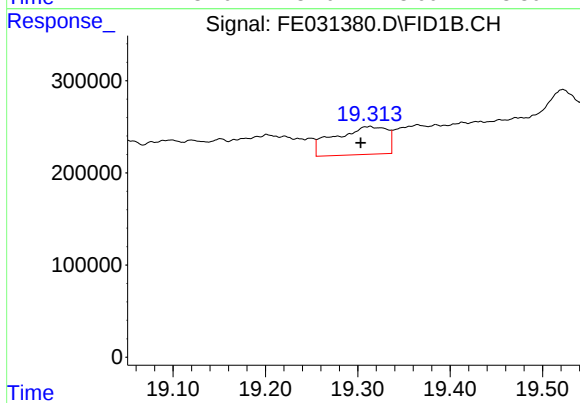

#15 N-TETRATRIACONTANE


R.T.: 19.312 min
Delta R.T.: 0.009 min
Response: 1192371
Conc: 3.90 ug/ml

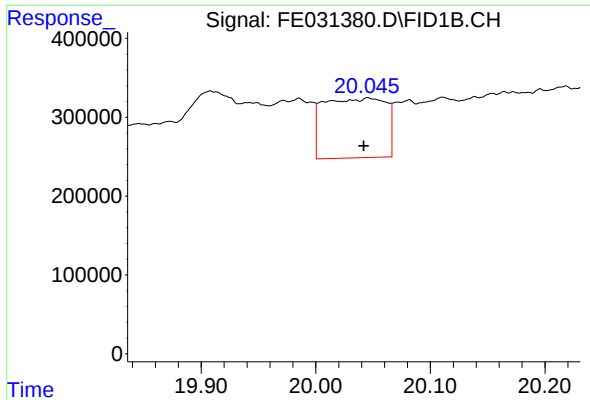

#16 N-HEXATRIACONTANE

R.T.: 20.046 min
Delta R.T.: 0.004 min
Response: 2872688
Conc: 11.58 ug/ml

Instrument :
FID_E
ClientSampleId :

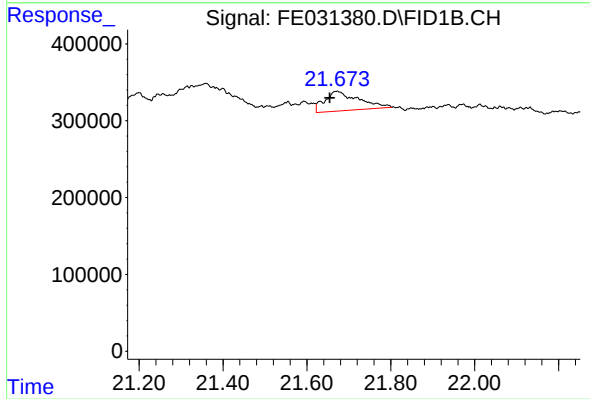

#18 N-TETRACONTANE

R.T.: 21.671 min
Delta R.T.: 0.016 min
Response: 1611704
Conc: 8.77 ug/ml