

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030221\
Data File : FE033316.D
Signal(s) : FID1B.CH
Acq On : 02 Mar 2021 10:36
Operator : DD\AJ
Sample : M1503-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
SEDGWICK-AVE

Manual Integrations
APPROVED

Ankita
3/3/2021 11:17:57 AM

Integration File: autoint1.e
Quant Time: Mar 03 02:09:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022221.M
Quant Title :
QLast Update : Tue Feb 23 10:21:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.568	9705192	28.255 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030221\
Data File : FE033316.D
Signal(s) : FID1B.CH
Acq On : 02 Mar 2021 10:36
Operator : DD\AJ
Sample : M1503-01
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
SEDGWICK-AVE


Manual Integrations
APPROVED

Ankita
3/3/2021 11:17:57 AM

Integration File: autoint1.e
Quant Time: Mar 03 02:09:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022221.M
Quant Title :
QLast Update : Tue Feb 23 10:21:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

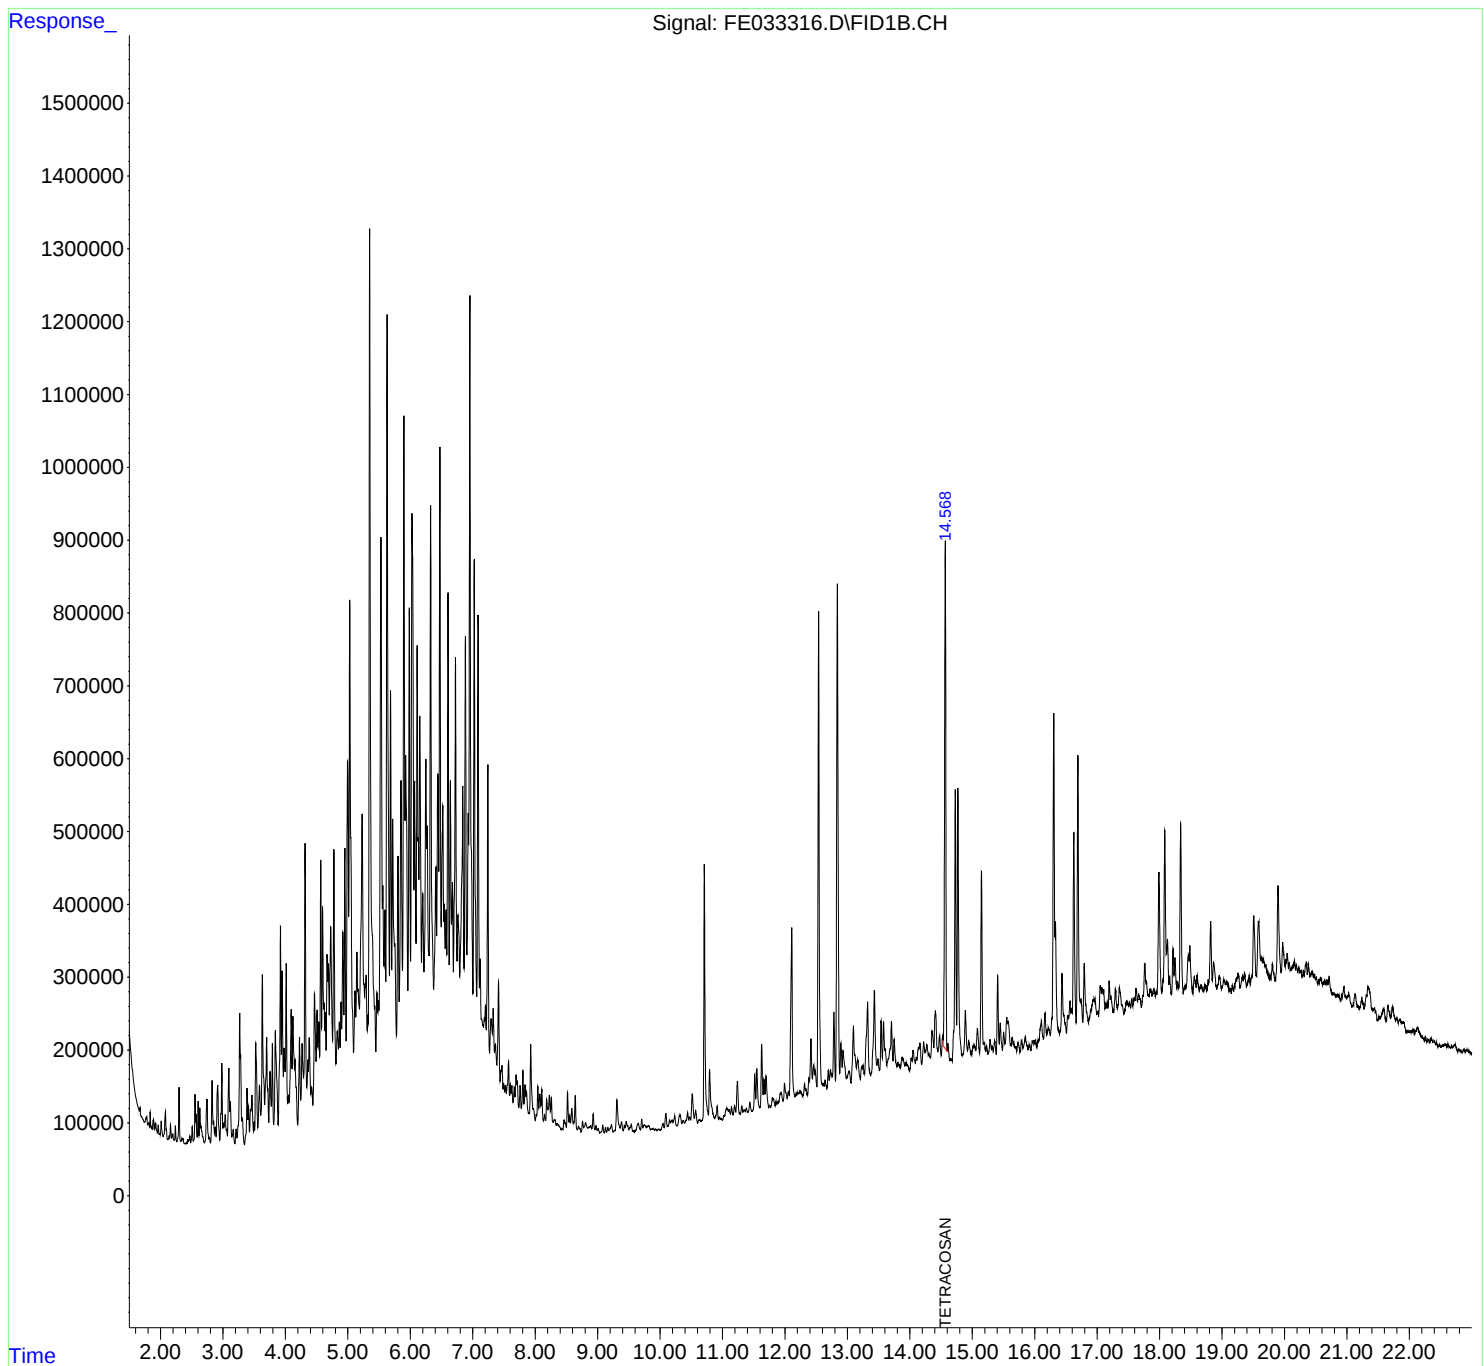

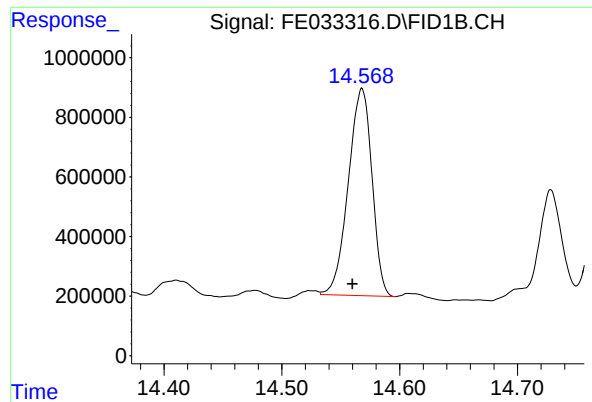

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.568 min
Delta R.T.: 0.008 min
Response: 9705192
Conc: 28.26 ug/ml m

Instrument :
FID_E
ClientSampleId :
SEDGWICK-AVE

Manual Integrations
APPROVED

Ankita
3/3/2021 11:17:57 AM