

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030320\
 Data File : FE031391.D
 Signal(s) : FID1B.CH
 Acq On : 03 Mar 2020 14:43
 Operator : DD\AJ
 Sample : L1762-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 04 00:31:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE021120.M
 Quant Title :
 QLast Update : Tue Feb 11 12:55:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.602	3901948	12.554 ug/ml
Target Compounds			
4) N-TETRADECANE	8.198f	519576	1.537 ug/ml
7) N-EICOSANE	12.559f	1238445	3.555 ug/ml
10) N-TETRACOSANE	14.792	785002	2.201 ug/ml
11) N-HEXACOSANE	15.830	150997	0.424 ug/ml
12) N-OCTACOSANE	16.783	583114	1.609 ug/ml
13) N-TRIACONTANE	17.675	842809	2.294 ug/ml
14) N-DOTRIACONTANE	18.508	734313	2.081 ug/ml
15) N-TETRATRIACONTANE	19.306	378639	1.240 ug/ml
16) N-HEXATRIACONTANE	20.043	1005487	4.052 ug/ml
17) N-OCTATRIACONTANE	20.700f	139329	0.718 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030320\
Data File : FE031391.D
Signal(s) : FID1B.CH
Acq On : 03 Mar 2020 14:43
Operator : DD\AJ
Sample : L1762-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 04 00:31:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE021120.M
Quant Title :
QLast Update : Tue Feb 11 12:55:11 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

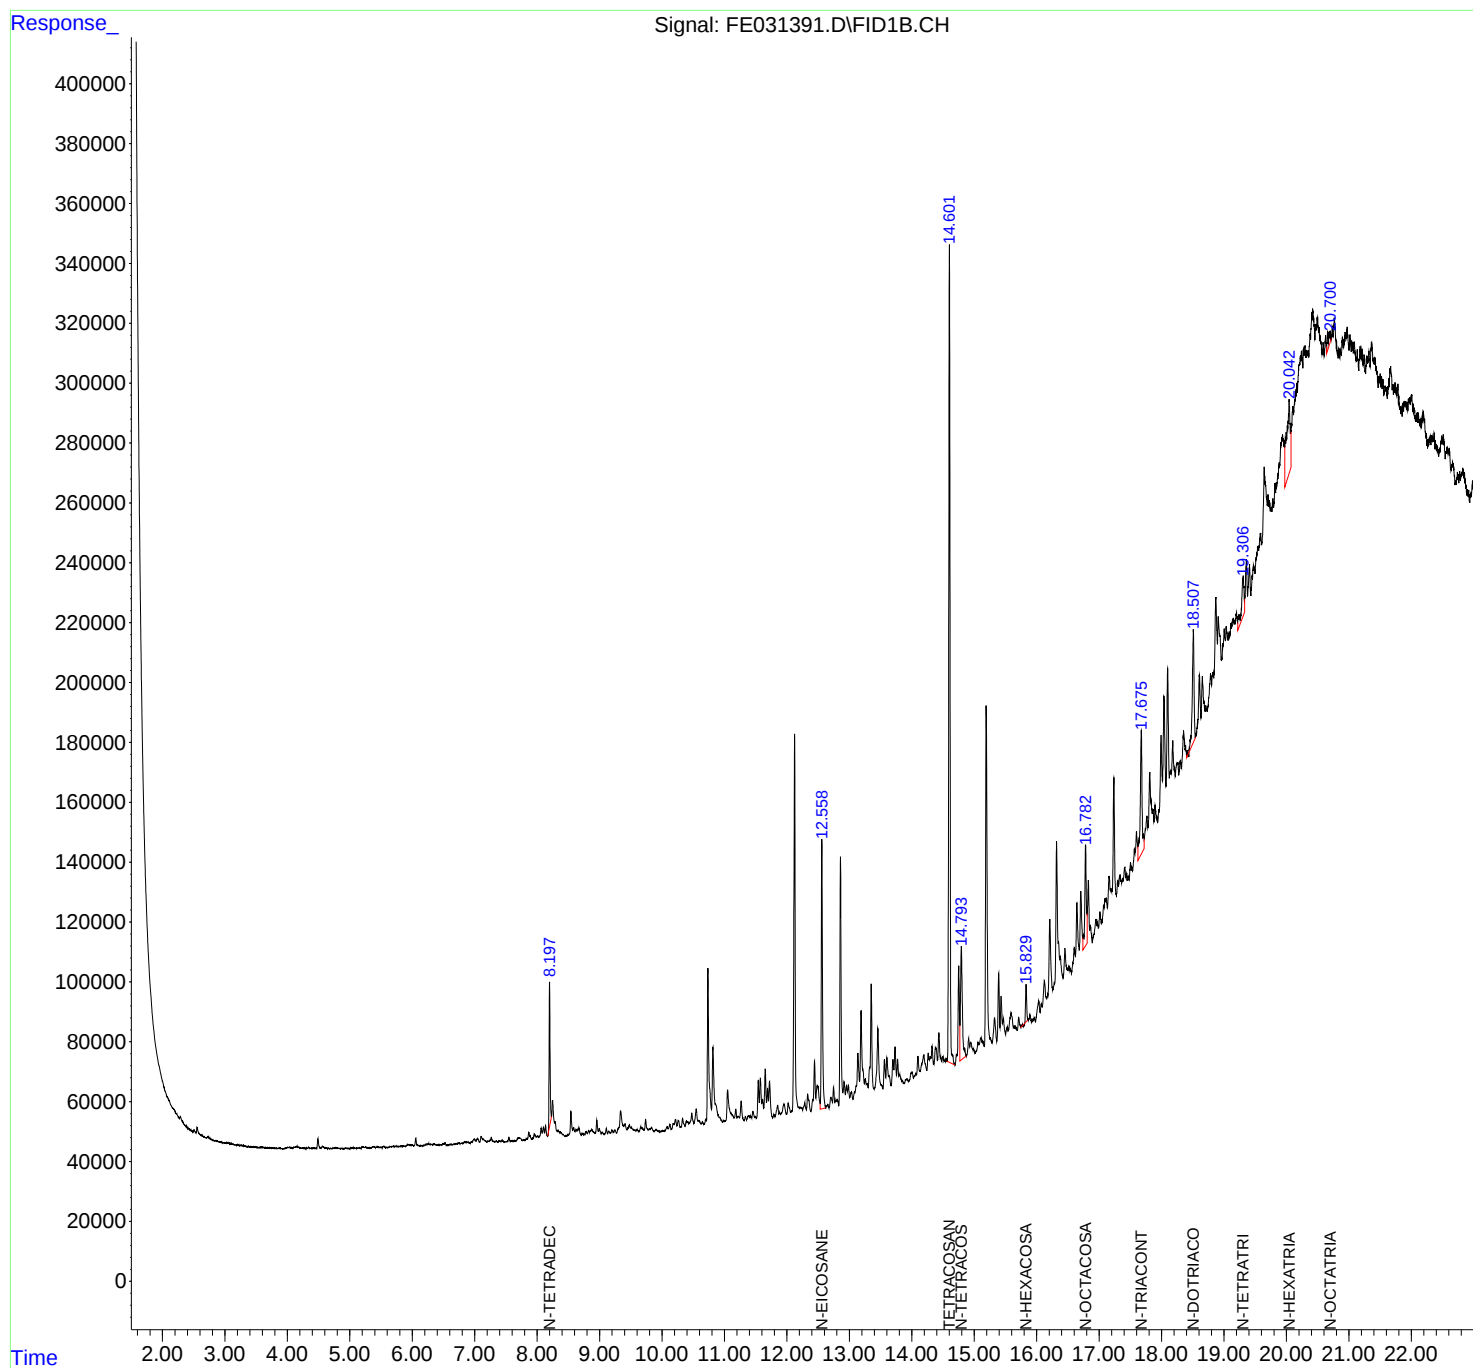

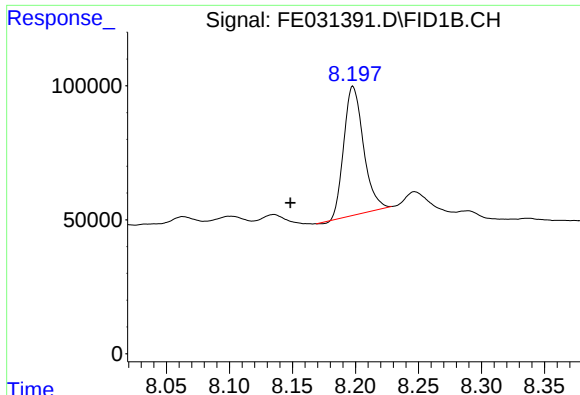


#4 N-TETRADECANE

R.T.: 8.198 min
Delta R.T.: 0.050 min
Response: 519576
Conc: 1.54 ug/ml

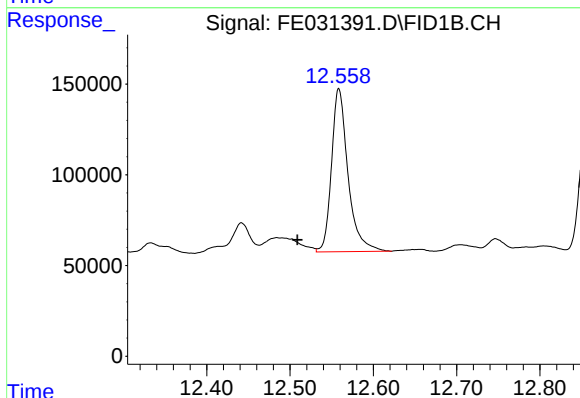


#7 N-EICOSANE

R.T.: 12.559 min
Delta R.T.: 0.050 min
Response: 1238445
Conc: 3.55 ug/ml

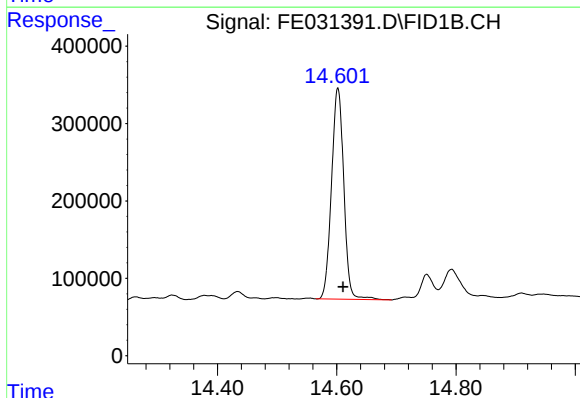


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.602 min
Delta R.T.: -0.009 min
Response: 3901948
Conc: 12.55 ug/ml

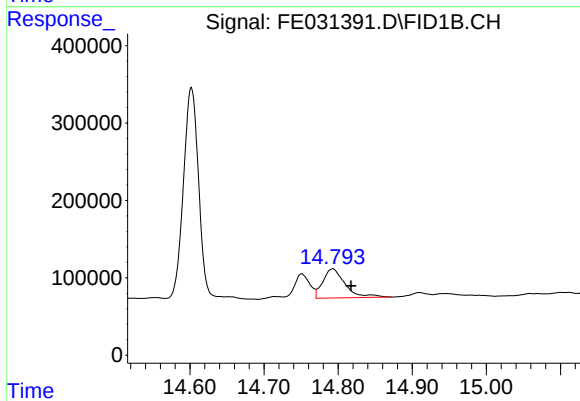


#10 N-TETRACOSANE

R.T.: 14.792 min
Delta R.T.: -0.025 min
Response: 785002
Conc: 2.20 ug/ml

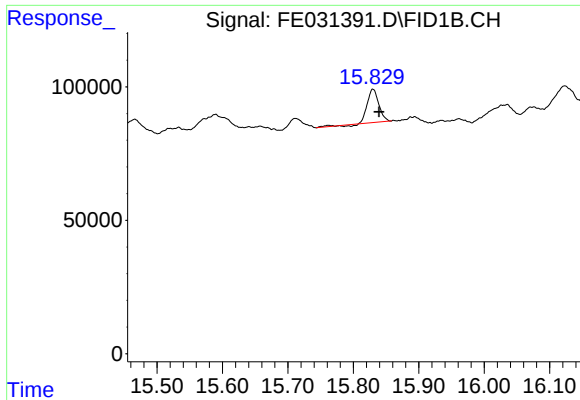


#11 N-HEXACOSANE

R.T.: 15.830 min
Delta R.T.: -0.009 min
Response: 150997
Conc: 0.42 ug/ml

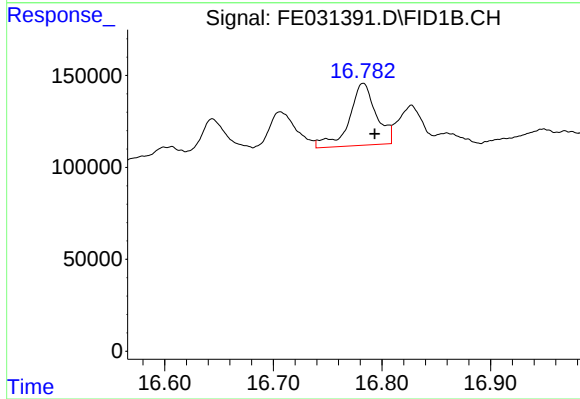


#12 N-OCTACOSANE

R.T.: 16.783 min
Delta R.T.: -0.011 min
Response: 583114
Conc: 1.61 ug/ml

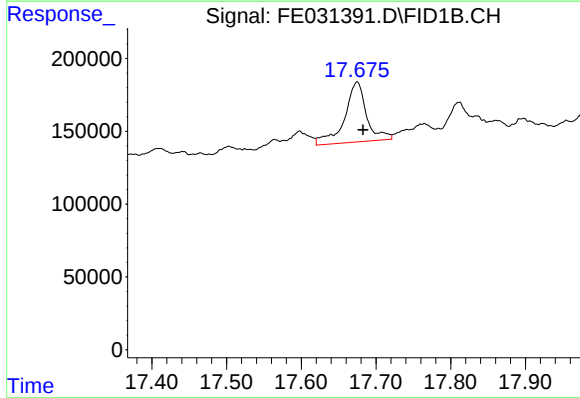


#13 N-TRIACONTANE

R.T.: 17.675 min
Delta R.T.: -0.008 min
Response: 842809
Conc: 2.29 ug/ml

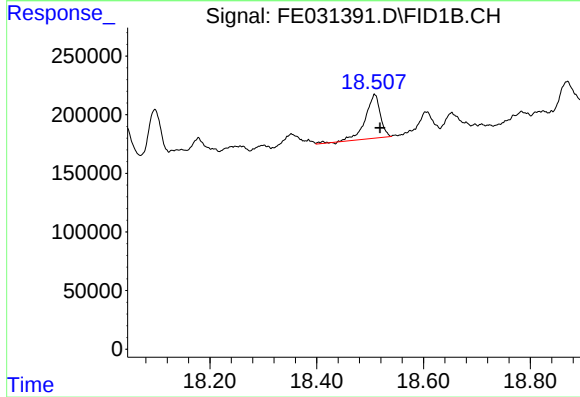


#14 N-DOTRIACONTANE

R.T.: 18.508 min
Delta R.T.: -0.010 min
Response: 734313
Conc: 2.08 ug/ml

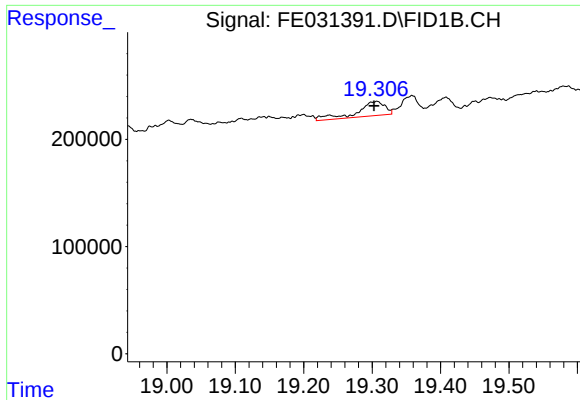


#15 N-TETRATRIACONTANE

R.T.: 19.306 min
Delta R.T.: 0.003 min
Response: 378639
Conc: 1.24 ug/ml

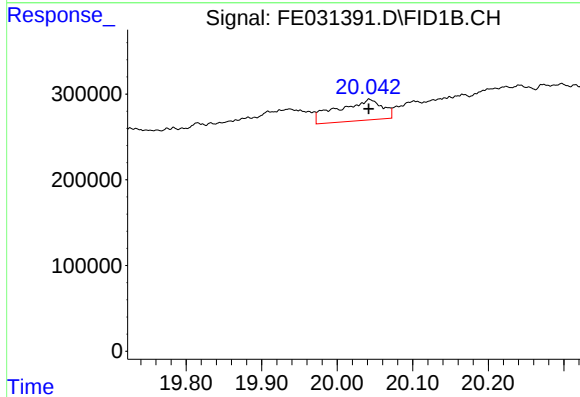

#16 N-HEXATRIACONTANE

R.T.: 20.043 min
Delta R.T.: 0.001 min
Response: 1005487
Conc: 4.05 ug/ml

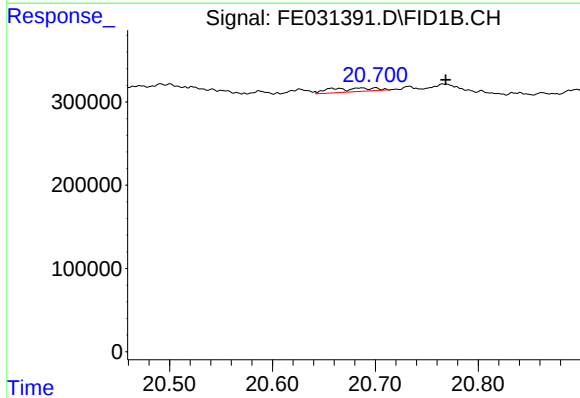

#17 N-OCTATRIACONTANE

R.T.: 20.700 min
Delta R.T.: -0.069 min
Response: 139329
Conc: 0.72 ug/ml