

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030322AL\
 Data File : FE035211.D
 Signal(s) : FID1B.CH
 Acq On : 03 Mar 2022 16:02
 Operator : YP\AJ
 Sample : N1756-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 33567-33569

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/04/2022
 Supervised By :Ankita Jodhani 03/04/2022

Integration File: autoint1.e
 Quant Time: Mar 04 00:37:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022822.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 02:07:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.362	3714239	26.817 ug/mlm
Spiked Amount 50.000		Recovery =	53.63%
12) S 1-chlorooctadecane (S...	12.796	2126853	19.635 ug/ml
Spiked Amount 50.000		Recovery =	39.27%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030322AL\
Data File : FE035211.D
Signal(s) : FID1B.CH
Acq On : 03 Mar 2022 16:02
Operator : YP\AJ
Sample : N1756-03
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
33567-33569


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/04/2022
Supervised By :Ankita Jodhani 03/04/2022

Integration File: autoint1.e
Quant Time: Mar 04 00:37:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022822.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 02:07:56 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

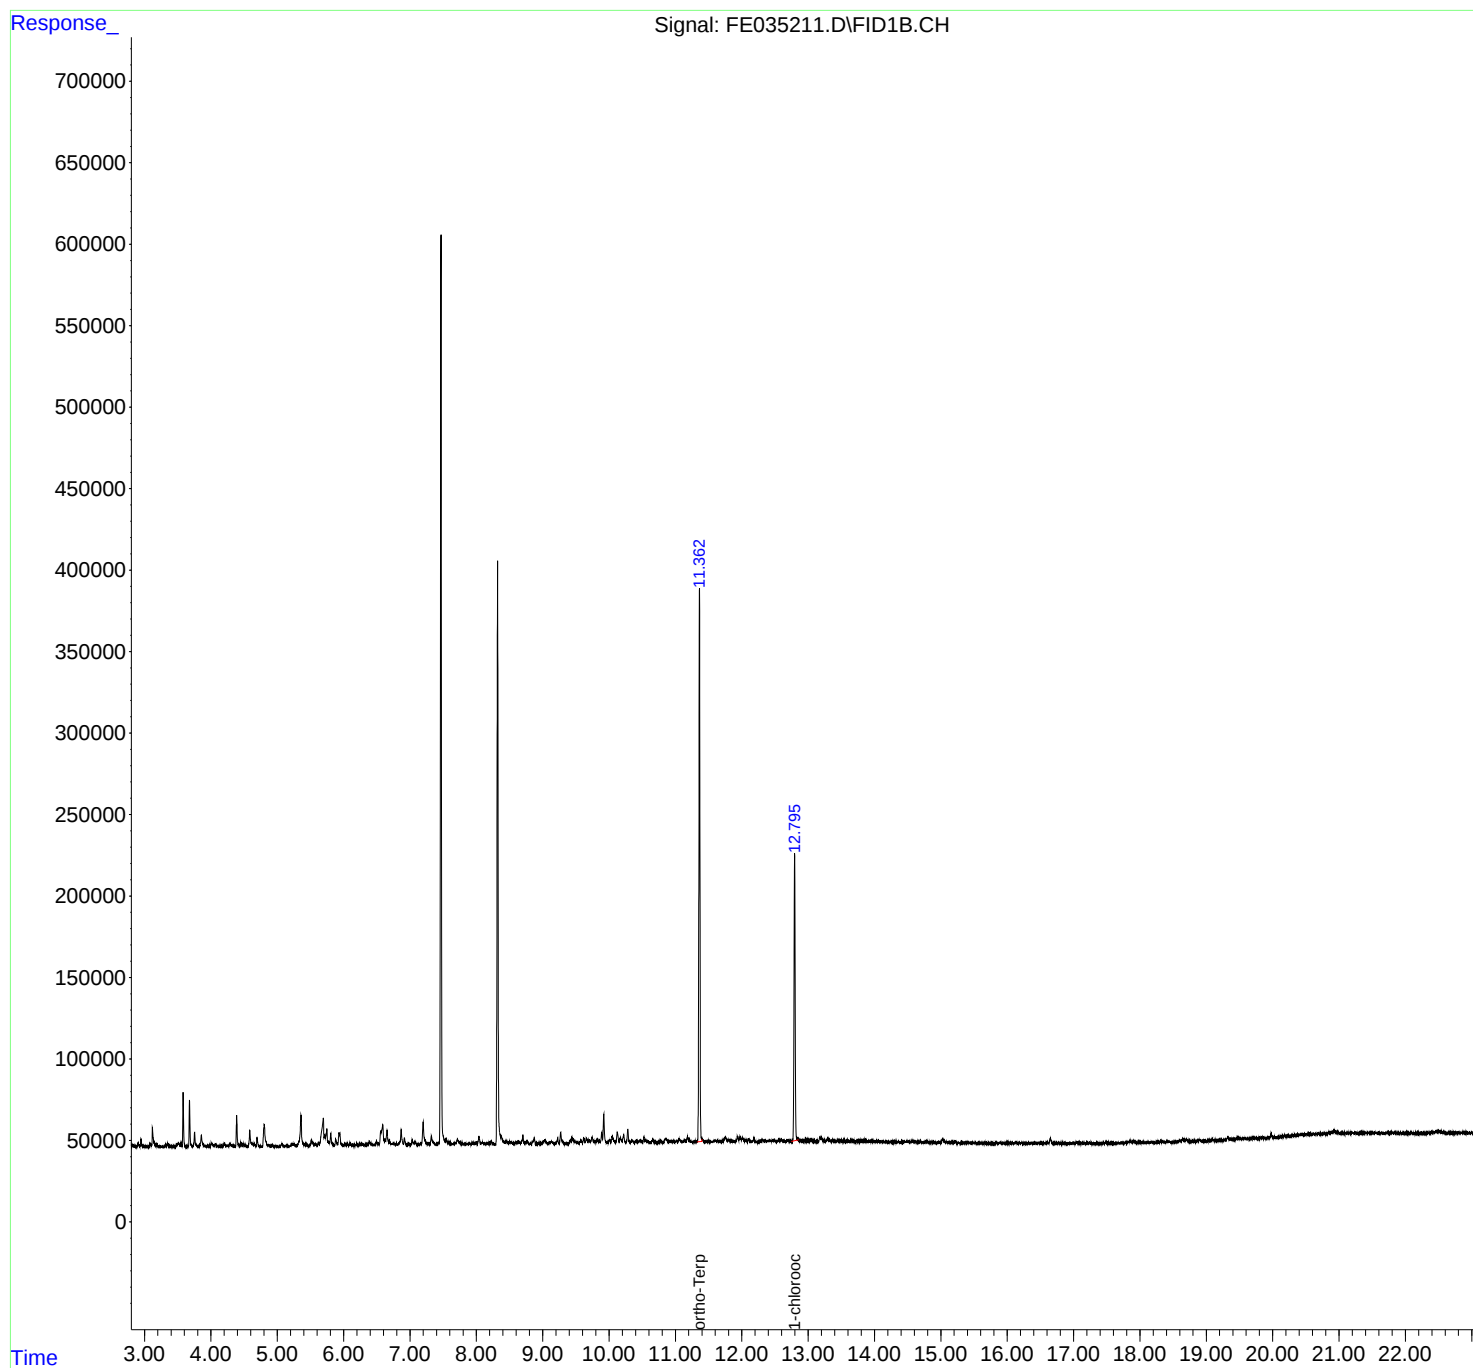

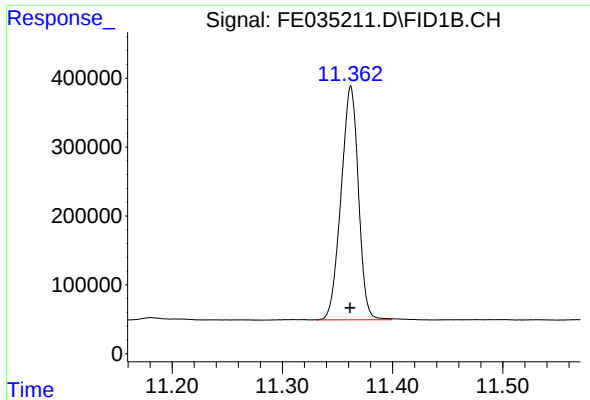

#9 ortho-Terphenyl (SURR)

R.T.: 11.362 min
Delta R.T.: 0.000 min
Response: 3714239
Conc: 26.82 ug/ml


Instrument :

FID_E

ClientSampleId :
33567-33569

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/04/2022
Supervised By :Ankita Jodhani 03/04/2022

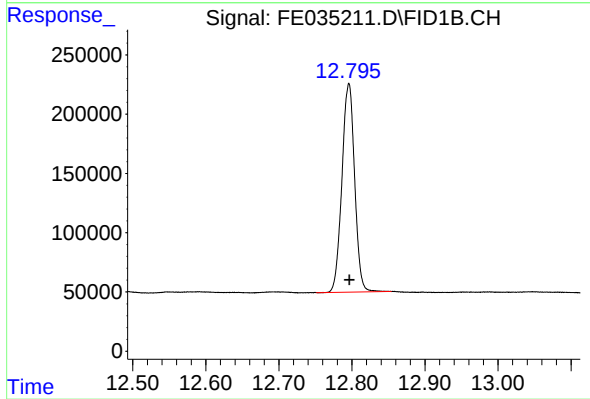

#12 1-chlorooctadecane (SURR)

R.T.: 12.796 min
Delta R.T.: 0.000 min
Response: 2126853
Conc: 19.64 ug/ml