

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030323AL\
 Data File : FE040649.D
 Signal(s) : FID1B.ch
 Acq On : 03 Mar 2023 02:54
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 03 04:05:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022823.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 28 03:05:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) T n-Dotriacontane (C32)	18.879	189480	1.107 ug/ml
19) T n-Tetratriacontane (C34)	19.667	75119	0.486 ug/ml
20) T n-Hexatriacontane (C36)	20.442	40578	0.279 ug/ml
21) T n-Octatriacontane (C38)	21.129	32073	0.233 ug/ml
22) T n-Tetracontane (C40)	21.970	721002	4.666 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030323AL\
Data File : FE040649.D
Signal(s) : FID1B.ch
Acq On : 03 Mar 2023 02:54
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 03 04:05:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022823.M
Quant Title : GC Extractables
QLast Update : Tue Feb 28 03:05:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

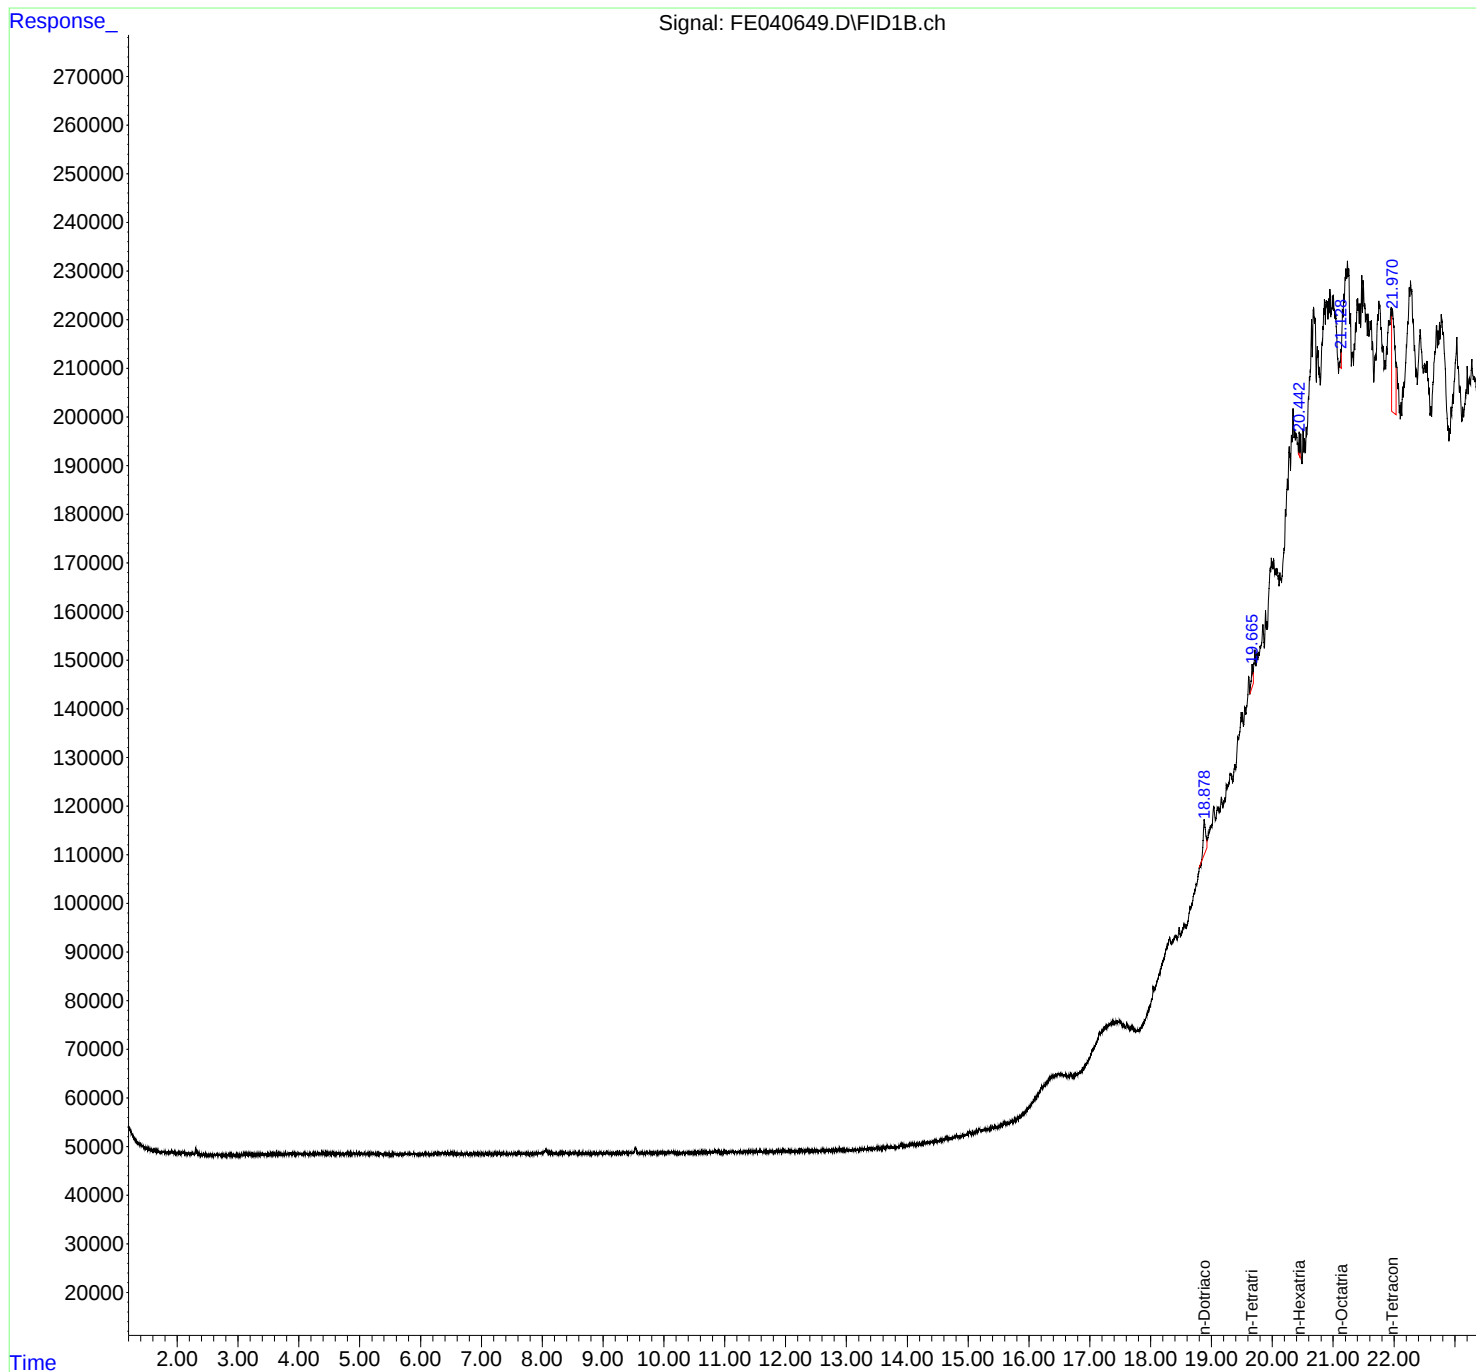


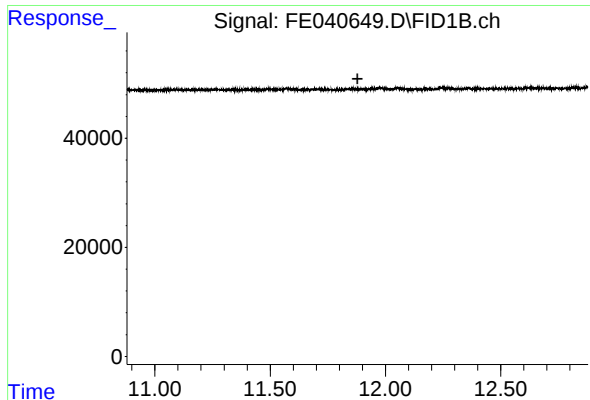

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.879 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

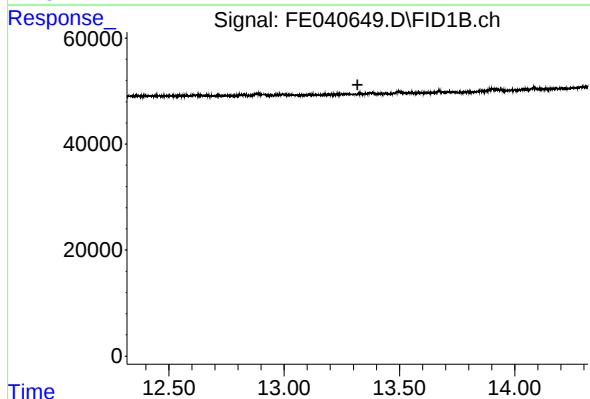


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.318 min
Response: 0
Conc: N.D.

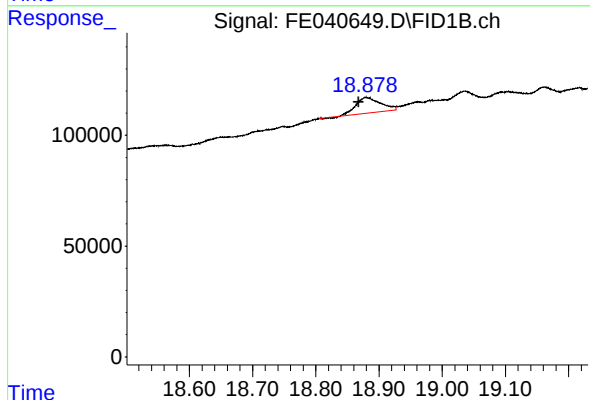


#18 n-Dotriacontane (C32)

R.T.: 18.879 min
Delta R.T.: 0.011 min
Response: 189480
Conc: 1.11 ug/ml

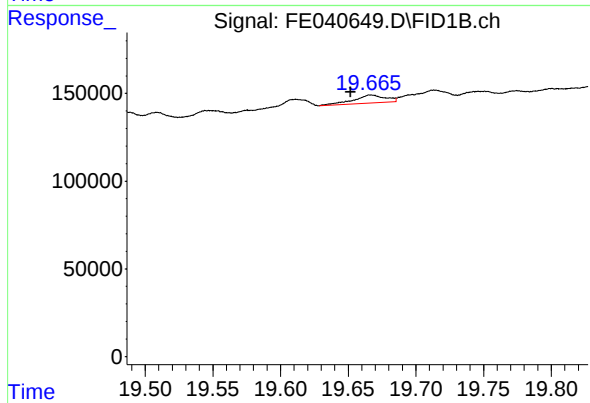

#19 n-Tetratriacontane (C34)

R.T.: 19.667 min
Delta R.T.: 0.015 min
Response: 75119
Conc: 0.49 ug/ml

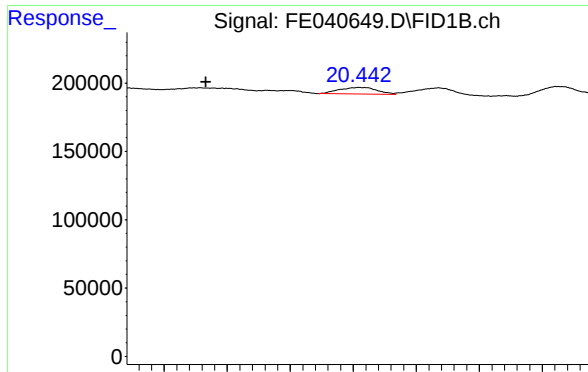


#20 n-Hexatriacontane (C36)

R.T.: 20.442 min
Delta R.T.: 0.049 min
Response: 40578
Conc: 0.28 ug/ml

Instrument :


FID_E

ClientSampleId :

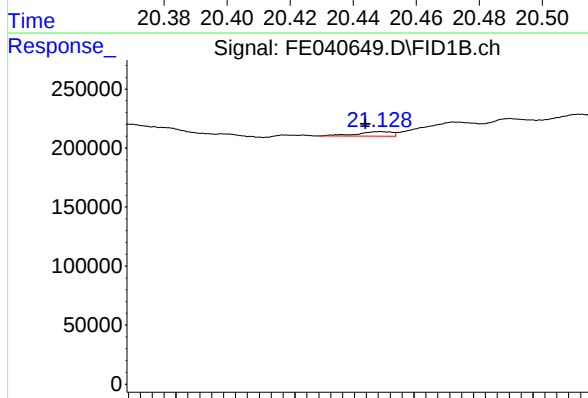

#21 n-Octatriacontane (C38)

R.T.: 21.129 min
Delta R.T.: 0.005 min
Response: 32073
Conc: 0.23 ug/ml

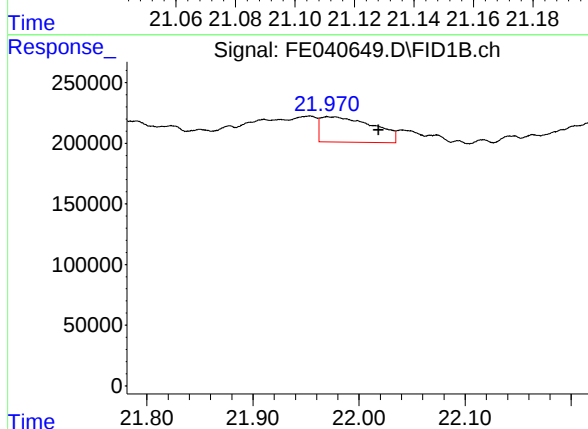

#22 n-Tetracontane (C40)

R.T.: 21.970 min
Delta R.T.: -0.048 min
Response: 721002
Conc: 4.67 ug/ml