

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030519\
Data File : FE029608.D
Signal(s) : FID1B.CH
Acq On : 05 Mar 2019 12:46
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 06 01:09:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE030419.M
Quant Title :
QLast Update : Tue Mar 05 10:37:48 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
5) N-DODECANE	6.541	3909562	21.151 ug/ml
11) N-OCTACOSANE	16.989	3969838	23.308 ug/ml
12) N-DOTRIACONTANE	18.721	102914	0.643 ug/ml
16) N-TETRTETRACOOCTANE	24.866	283289	3.912 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030519\
Data File : FE029608.D
Signal(s) : FID1B.CH
Acq On : 05 Mar 2019 12:46
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 06 01:09:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE030419.M
Quant Title :
QLast Update : Tue Mar 05 10:37:48 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

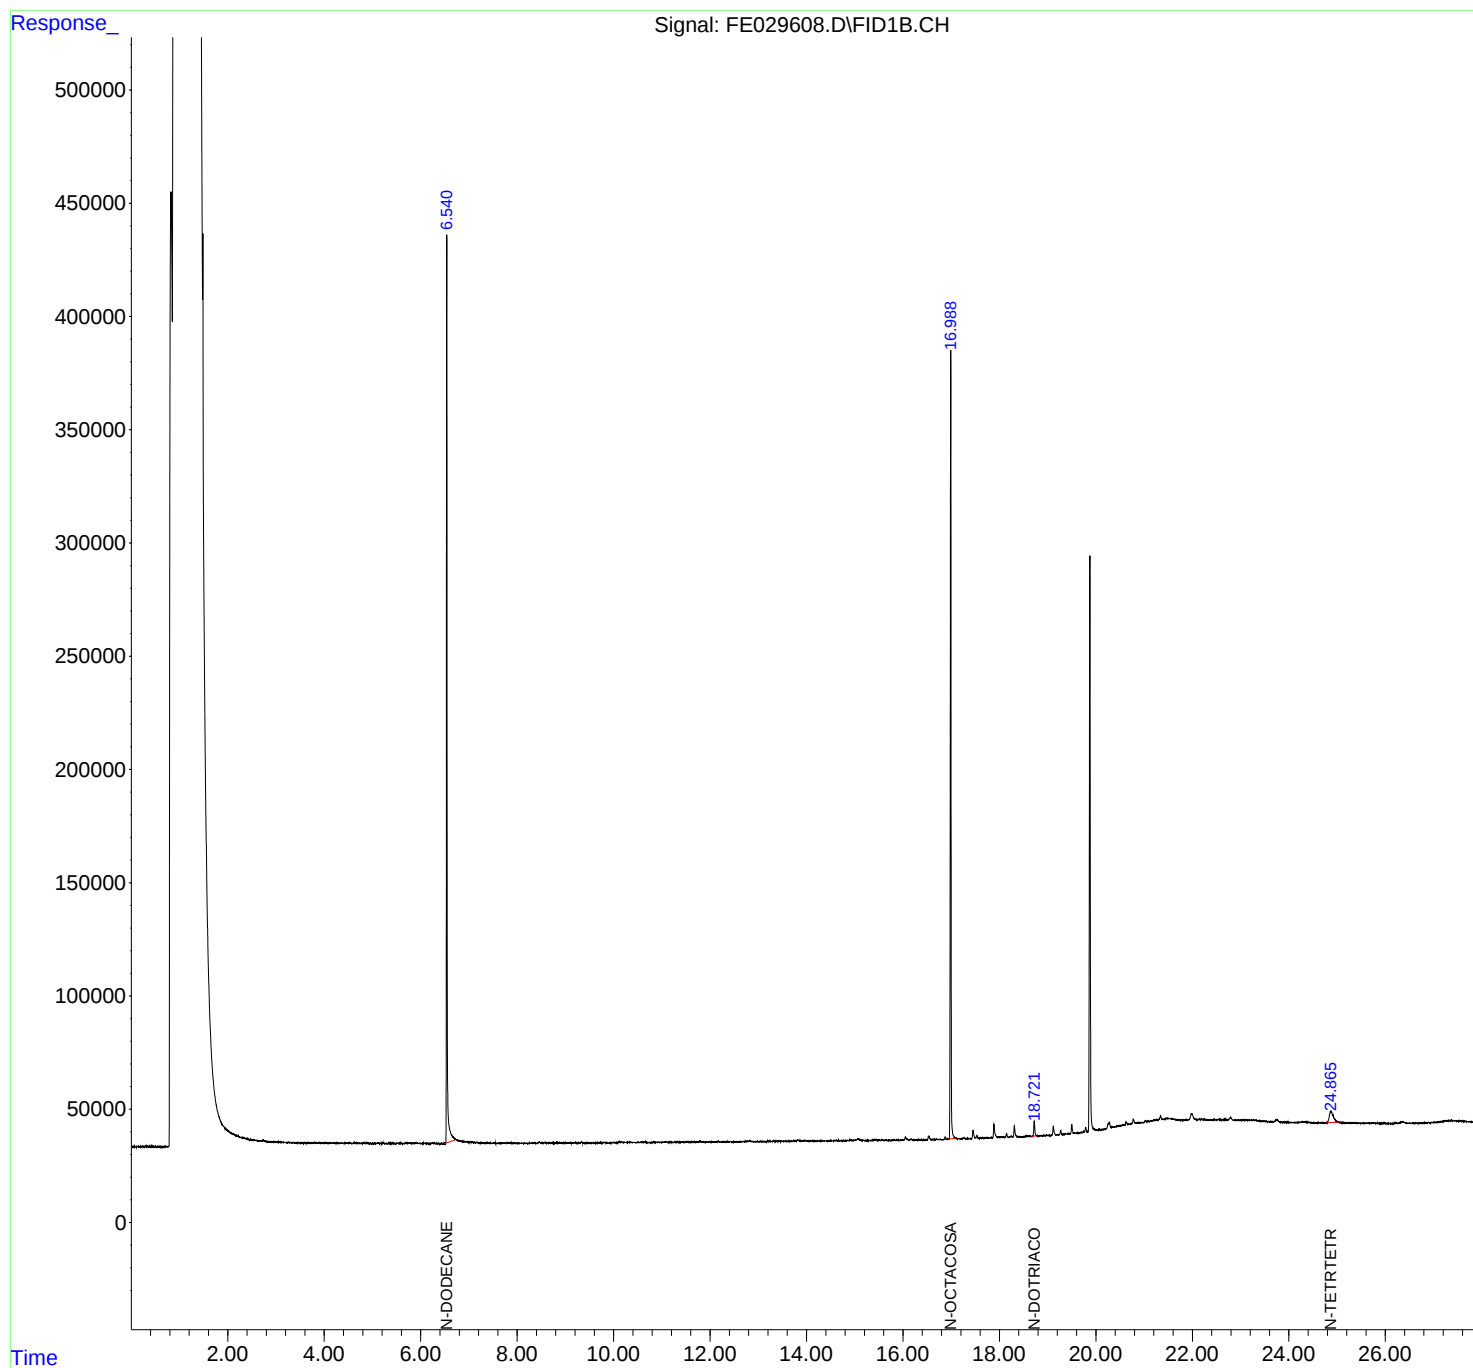

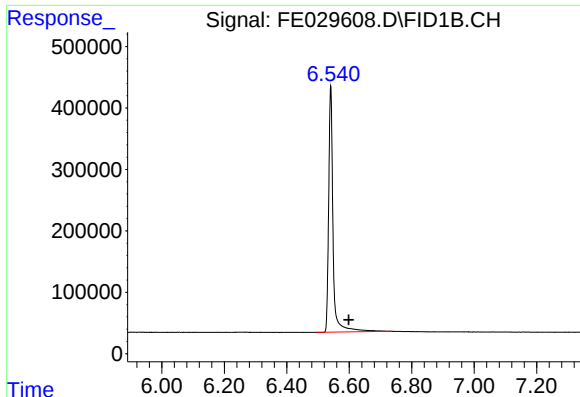


#5 N-DODECANE

R.T.: 6.541 min
Delta R.T.: -0.057 min
Response: 3909562
Conc: 21.15 ug/ml

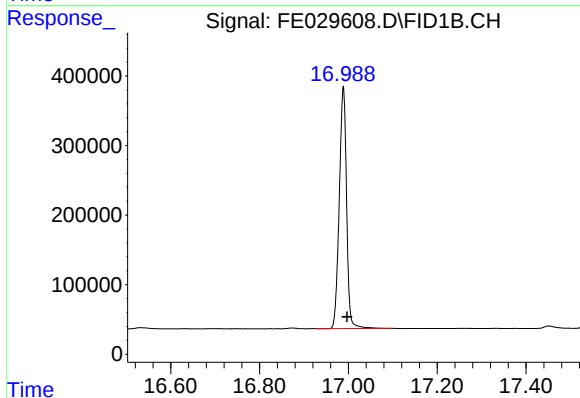


#11 N-OCTACOSANE

R.T.: 16.989 min
Delta R.T.: -0.008 min
Response: 3969838
Conc: 23.31 ug/ml

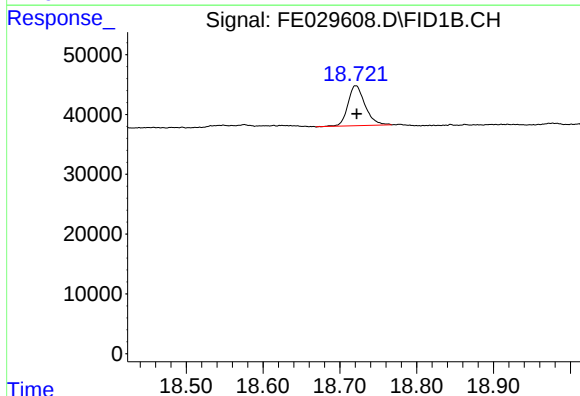


#12 N-DOTRIACONTANE

R.T.: 18.721 min
Delta R.T.: -0.001 min
Response: 102914
Conc: 0.64 ug/ml

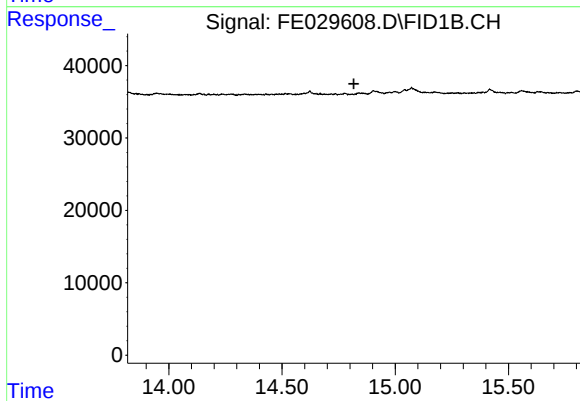

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.817 min
Response: 0
Conc: N.D.

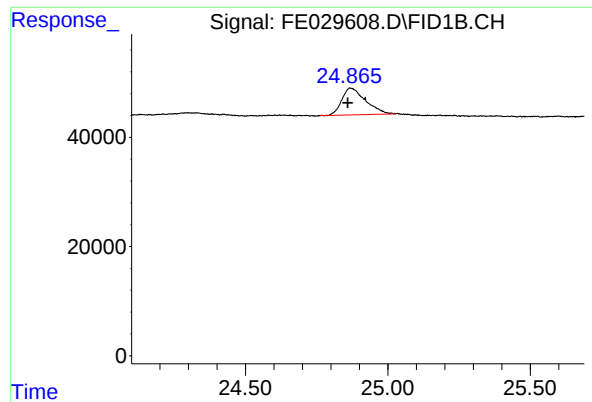

#16 N-TETRTETRACOCTANE

R.T.:	24.866 min
Delta R.T.:	0.007 min
Response:	283289
Conc:	3.91 ug/ml