

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030525AL\
Data File : FE052630.D
Signal(s) : FID1B.ch
Acq On : 05 Mar 2025 13:54
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 06 01:48:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 030325.M
Quant Title : GC Extractables
QLast Update : Mon Mar 03 13:39:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.926	153038	1.054 ug/ml
19) T	n-Tetratriacontane (C34)	19.712	132218	0.981 ug/ml
20) T	n-Hexatriacontane (C36)	20.454	98485	0.829 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030525AL\
Data File : FE052630.D
Signal(s) : FID1B.ch
Acq On : 05 Mar 2025 13:54
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 06 01:48:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 030325.M
Quant Title : GC Extractables
QLast Update : Mon Mar 03 13:39:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

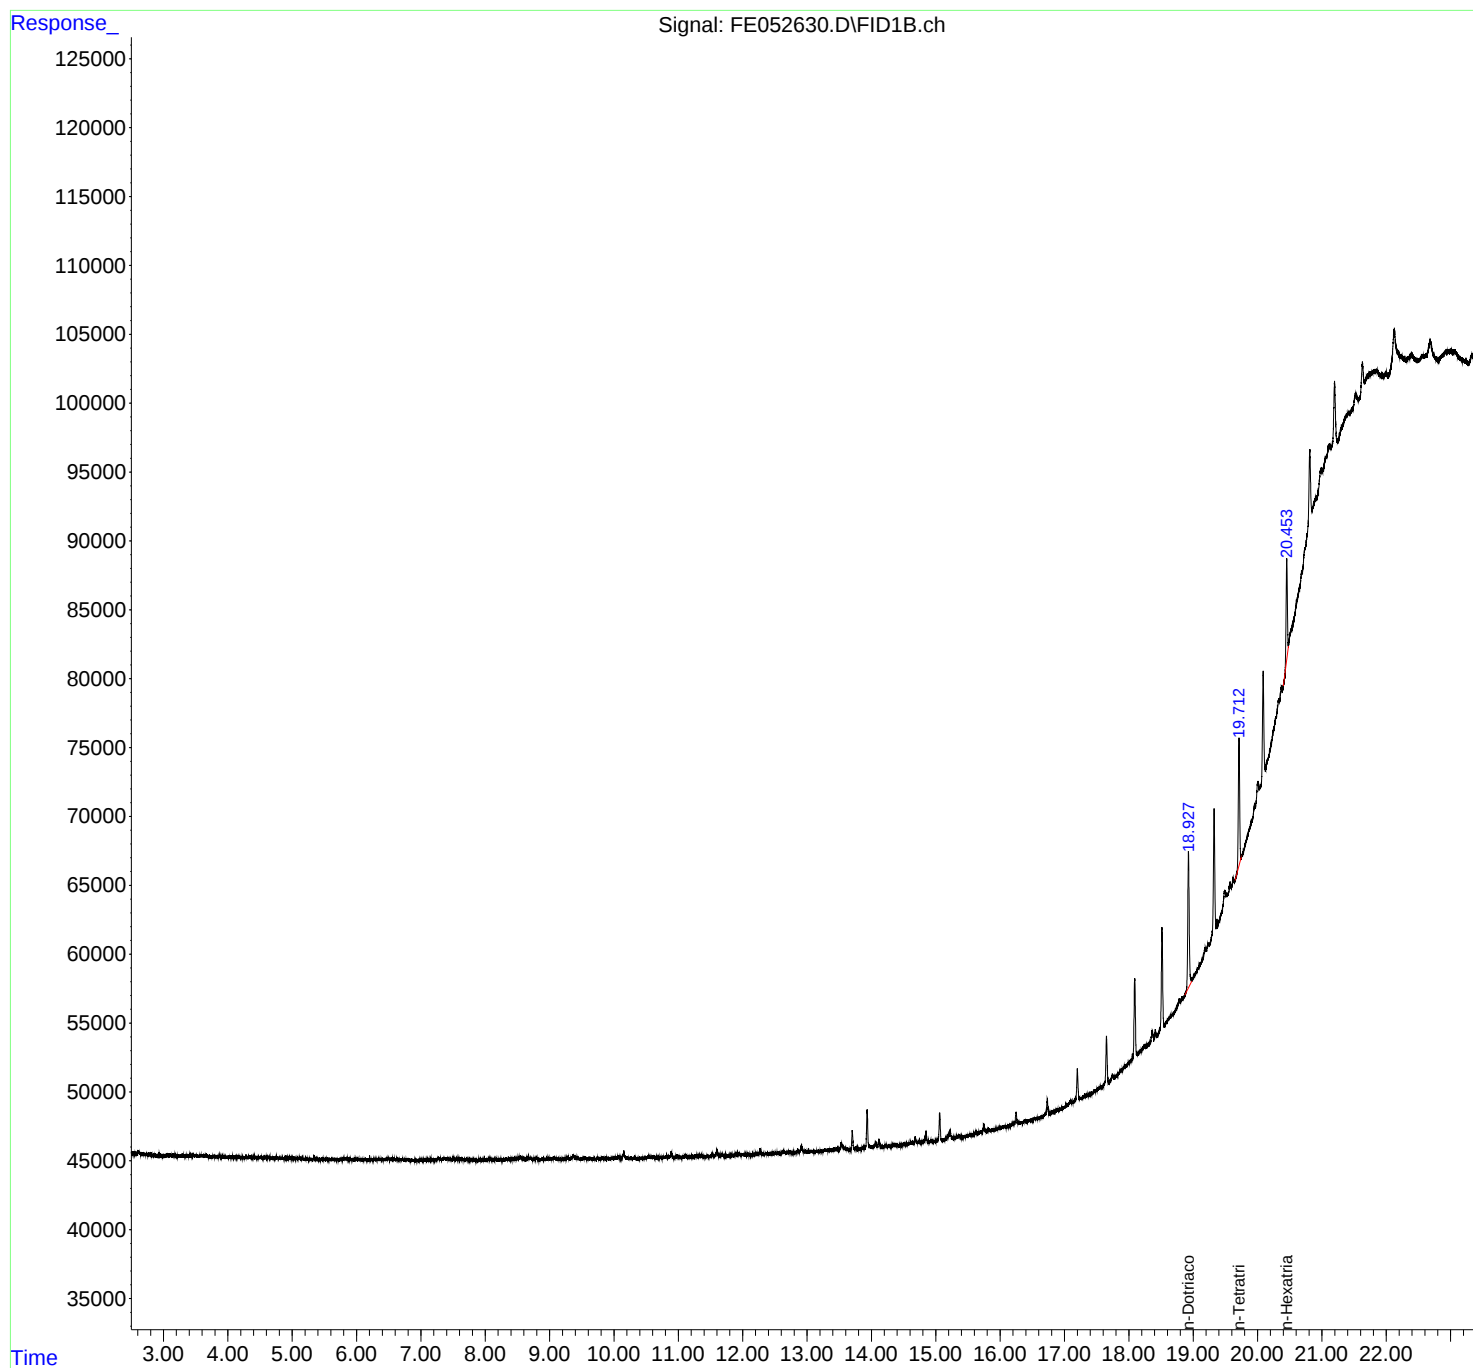


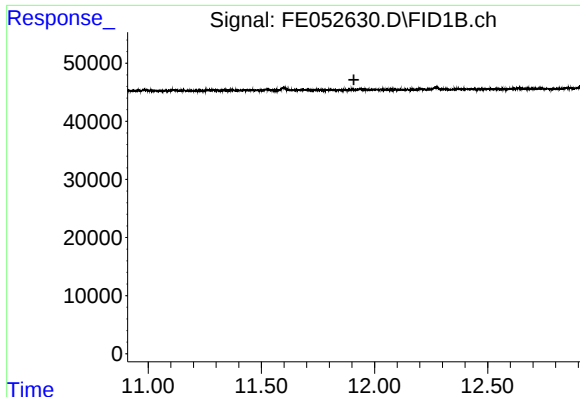

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.909 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

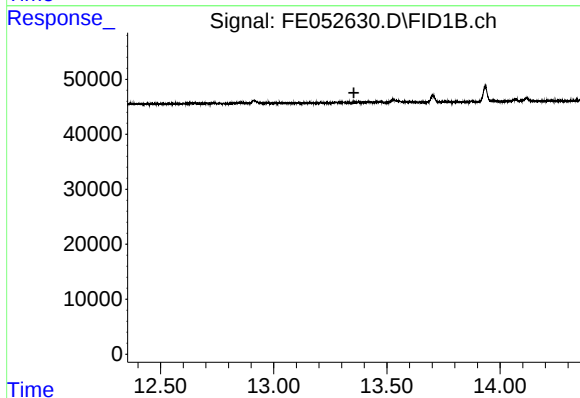


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.354 min
Response: 0
Conc: N.D.

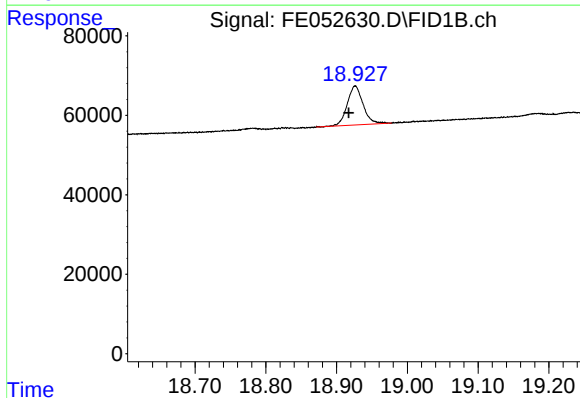


#18 n-Dotriacontane (C32)

R.T.: 18.926 min
Delta R.T.: 0.009 min
Response: 153038
Conc: 1.05 ug/ml

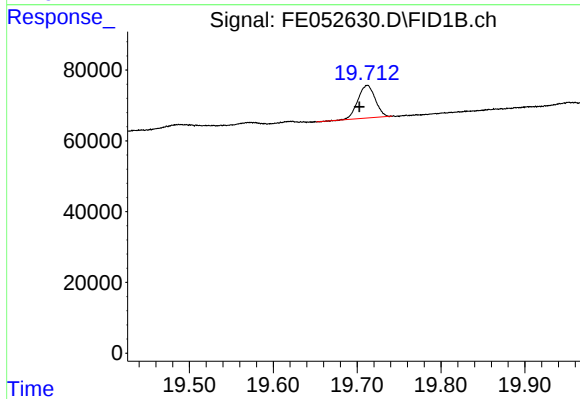

#19 n-Tetratriacontane (C34)

R.T.: 19.712 min
Delta R.T.: 0.009 min
Response: 132218
Conc: 0.98 ug/ml

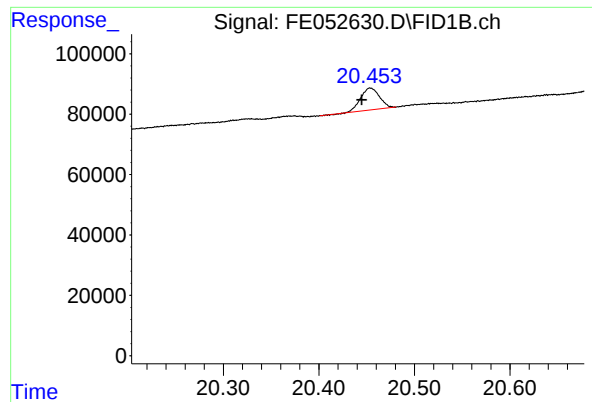

#20 n-Hexatriacontane (C36)

R.T.: 20.454 min
Delta R.T.: 0.009 min
Response: 98485
Conc: 0.83 ug/ml

Instrument :

FID_E

ClientSampleId :