

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030823\
 Data File : FE040711.D
 Signal(s) : FID1B.ch
 Acq On : 08 Mar 2023 13:30
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 08 22:39:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022123.M
 Quant Title :
 QLast Update : Wed Feb 22 06:24:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.685	3027615	21.728 ug/ml
12) N-OCTACOSANE	17.152	2886889	20.396 ug/ml
16) N-HEXATRIACONTANE	20.400	302665	2.567 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030823\
Data File : FE040711.D
Signal(s) : FID1B.ch
Acq On : 08 Mar 2023 13:30
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 08 22:39:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022123.M
Quant Title :
QLast Update : Wed Feb 22 06:24:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

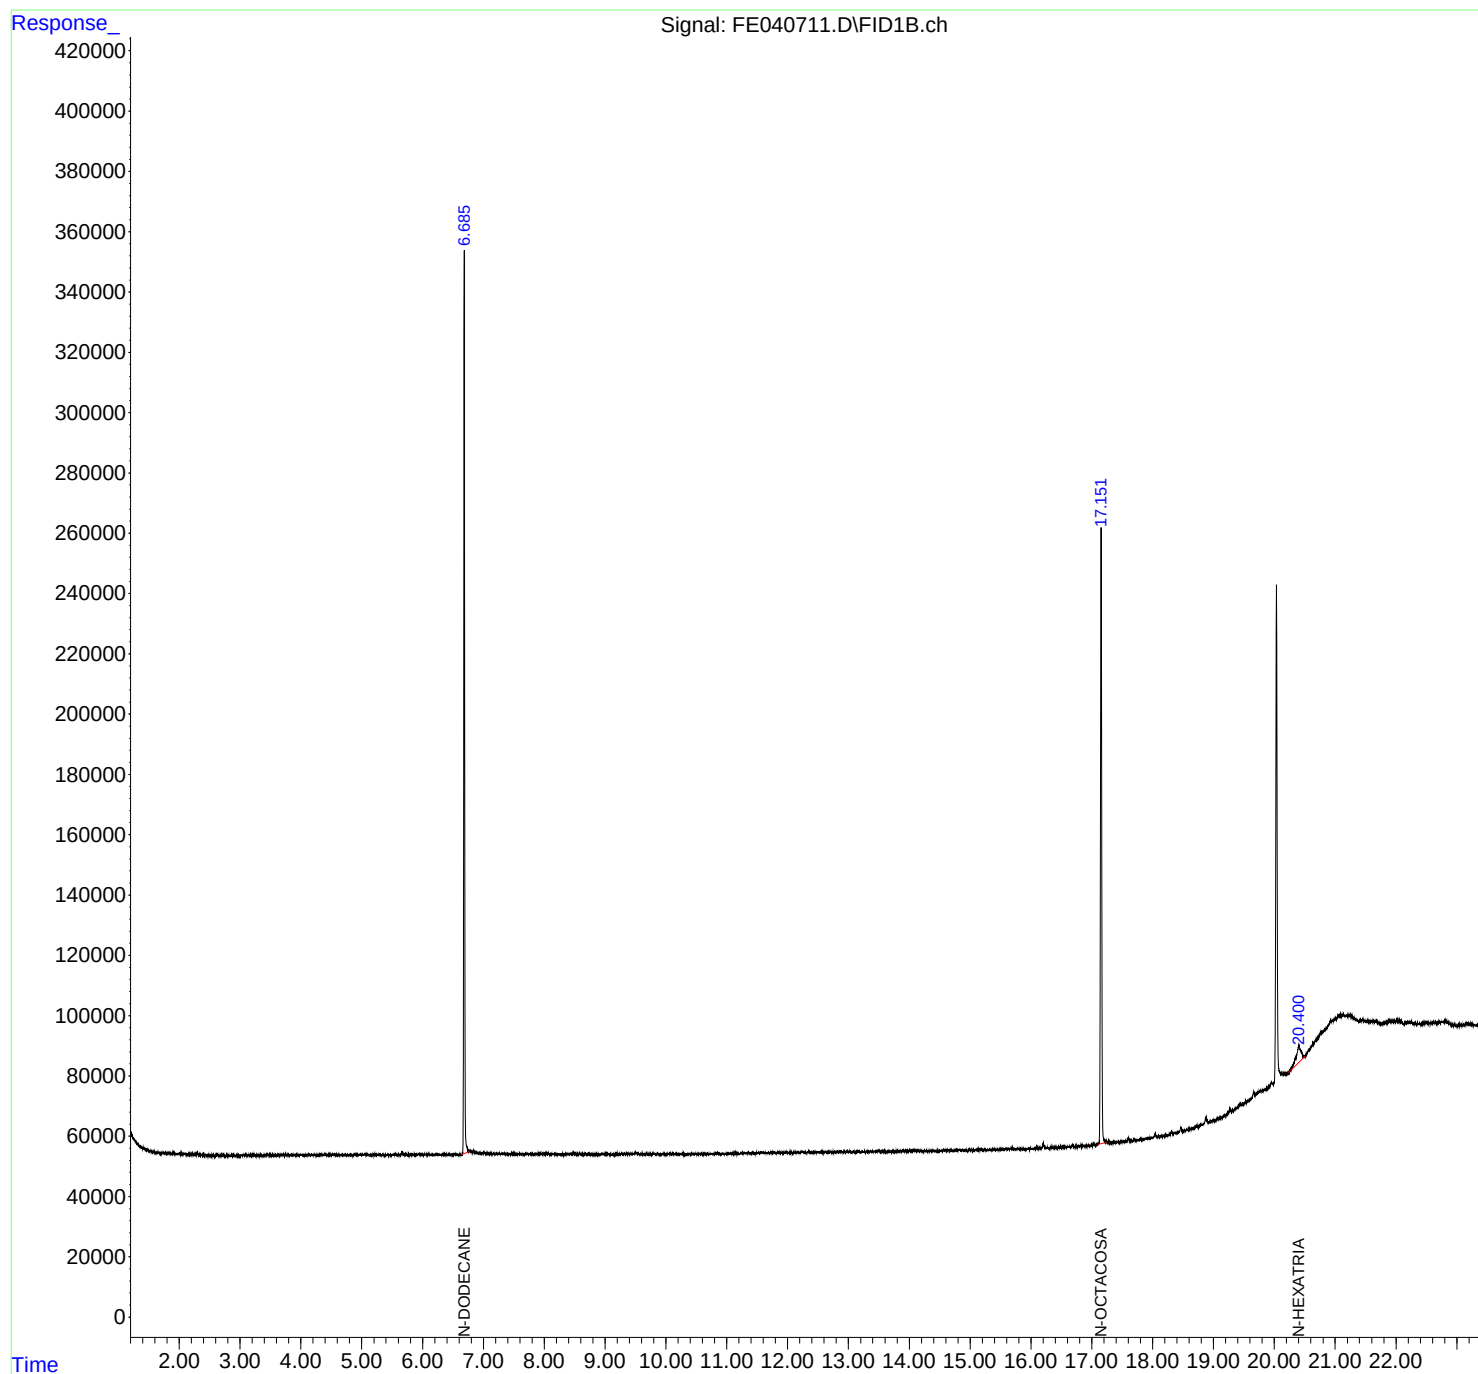


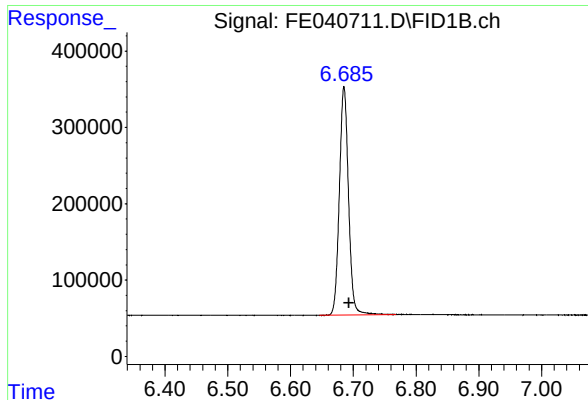

#3 N-DODECANE


R.T.: 6.685 min
Delta R.T.: -0.008 min
Response: 3027615
Conc: 21.73 ug/ml

Instrument :
FID_E
ClientSampleId :

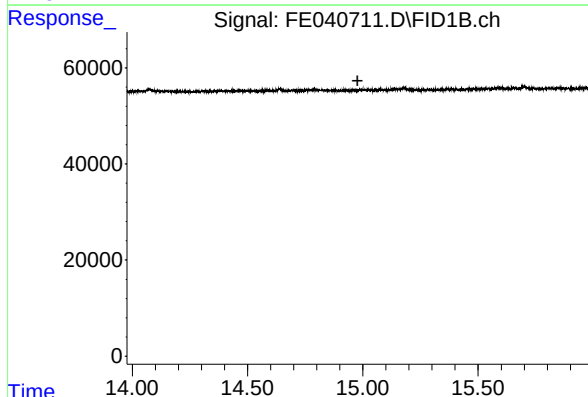


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.977 min
Response: 0
Conc: N.D.

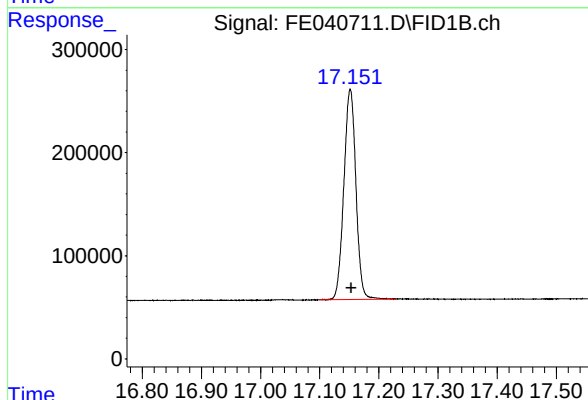

#12 N-OCTACOSANE

R.T.: 17.152 min
Delta R.T.: -0.002 min
Response: 2886889
Conc: 20.40 ug/ml

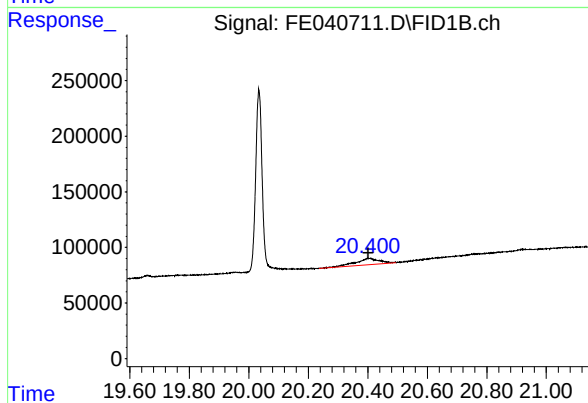

#16 N-HEXATRIACONTANE

R.T.: 20.400 min
Delta R.T.: -0.001 min
Response: 302665
Conc: 2.57 ug/ml