

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030823\
Data File : FE040714.D
Signal(s) : FID1B.ch
Acq On : 08 Mar 2023 15:35
Operator : YP\AJ
Sample : 01821-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
WC-IDW-S-1

Integration File: autoint1.e
Quant Time: Mar 08 22:39:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022123.M
Quant Title :
QLast Update : Wed Feb 22 06:24:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.973	1943414	14.718 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030823\
Data File : FE040714.D
Signal(s) : FID1B.ch
Acq On : 08 Mar 2023 15:35
Operator : YP\AJ
Sample : 01821-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
WC-IDW-S-1

Integration File: autoint1.e
Quant Time: Mar 08 22:39:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022123.M
Quant Title :
QLast Update : Wed Feb 22 06:24:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

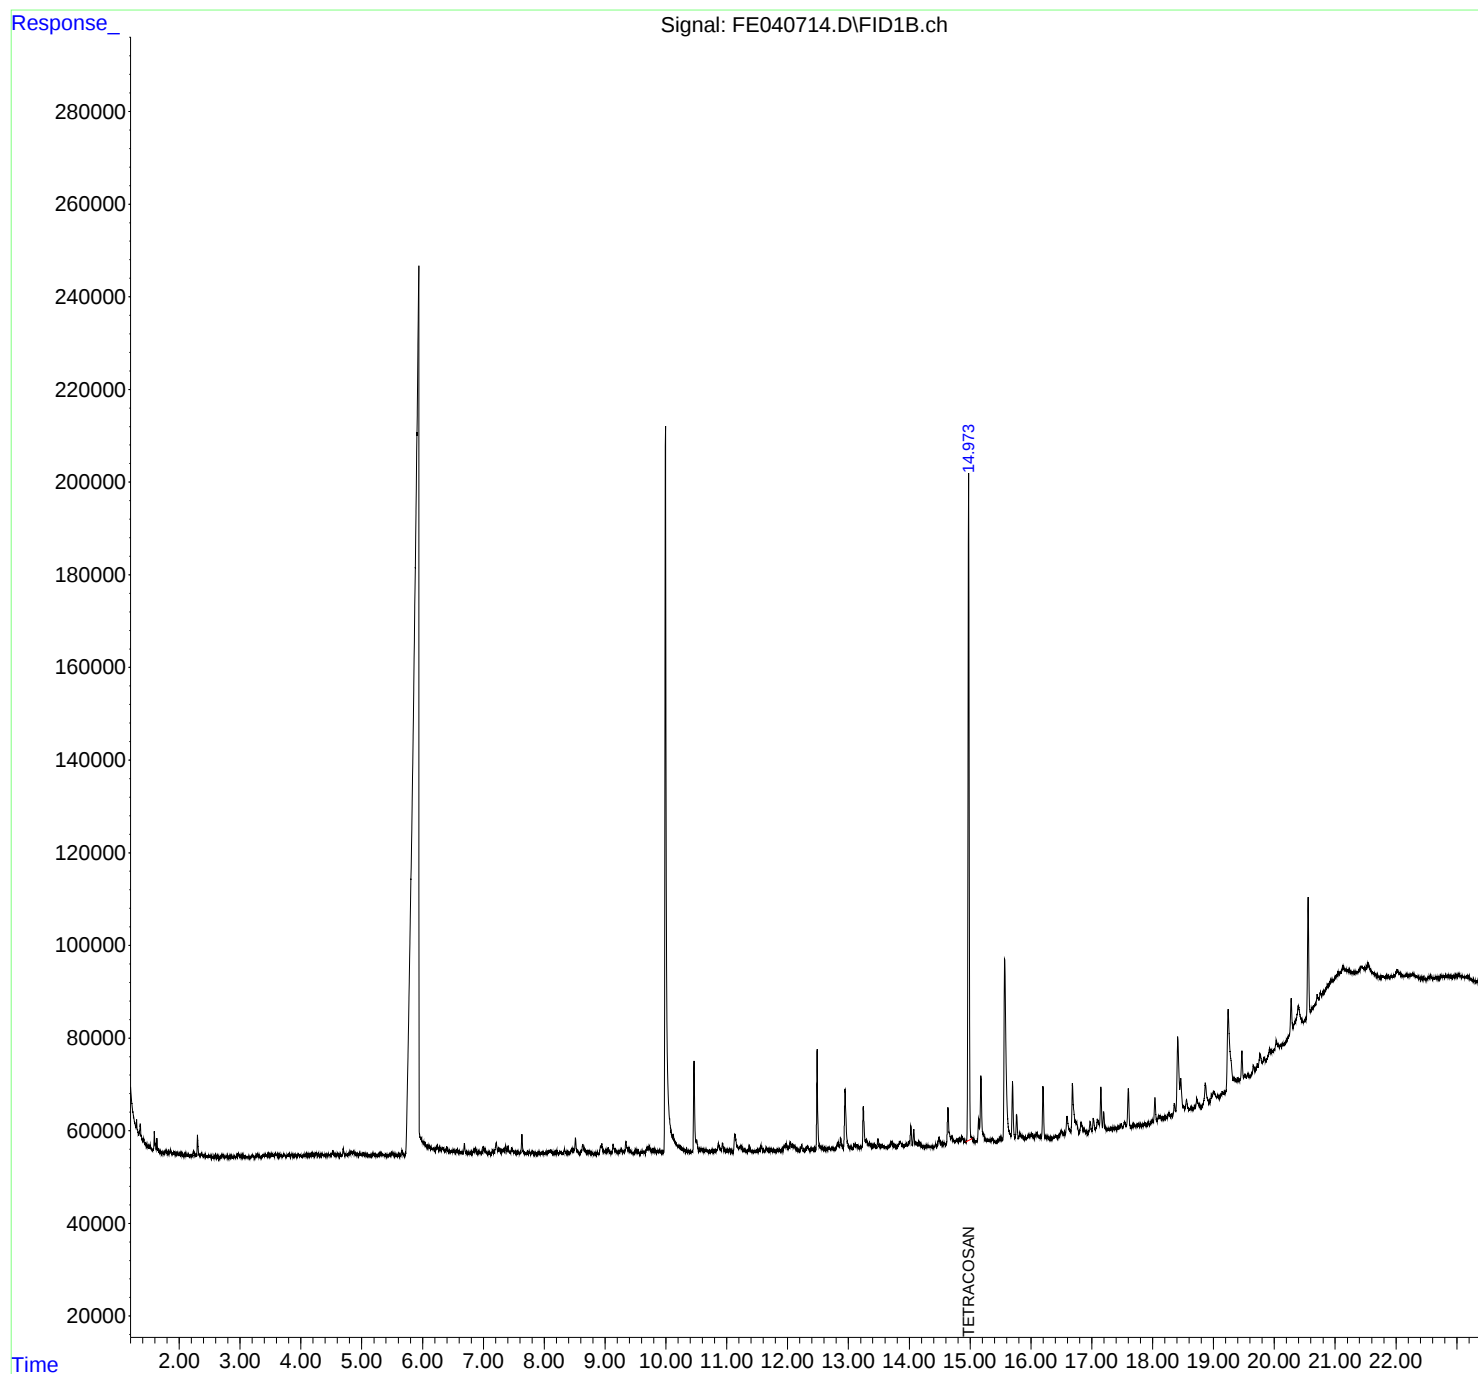

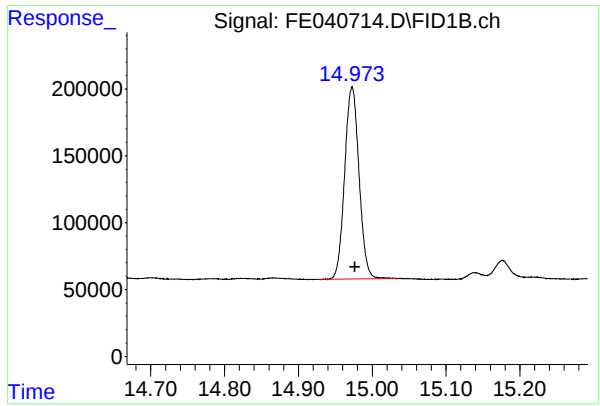

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.973 min
Delta R.T.: -0.004 min
Response: 1943414
Conc: 14.72 ug/ml

Instrument :
FID_E
ClientSampleId :
WC-IDW-S-1