

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030823\
Data File : FE040720.D
Signal(s) : FID1B.ch
Acq On : 08 Mar 2023 18:45
Operator : YP\AJ
Sample : 01829-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
SS-02-20230306

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2023
Supervised By :Ankita Jodhani 03/09/2023

Integration File: autoint1.e
Quant Time: Mar 08 22:40:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022123.M
Quant Title :
QLast Update : Wed Feb 22 06:24:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.973	2246690	17.015 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030823\
Data File : FE040720.D
Signal(s) : FID1B.ch
Acq On : 08 Mar 2023 18:45
Operator : YP\AJ
Sample : 01829-02
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
SS-02-20230306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2023
Supervised By :Ankita Jodhani 03/09/2023

Integration File: autoint1.e
Quant Time: Mar 08 22:40:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022123.M
Quant Title :
QLast Update : Wed Feb 22 06:24:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

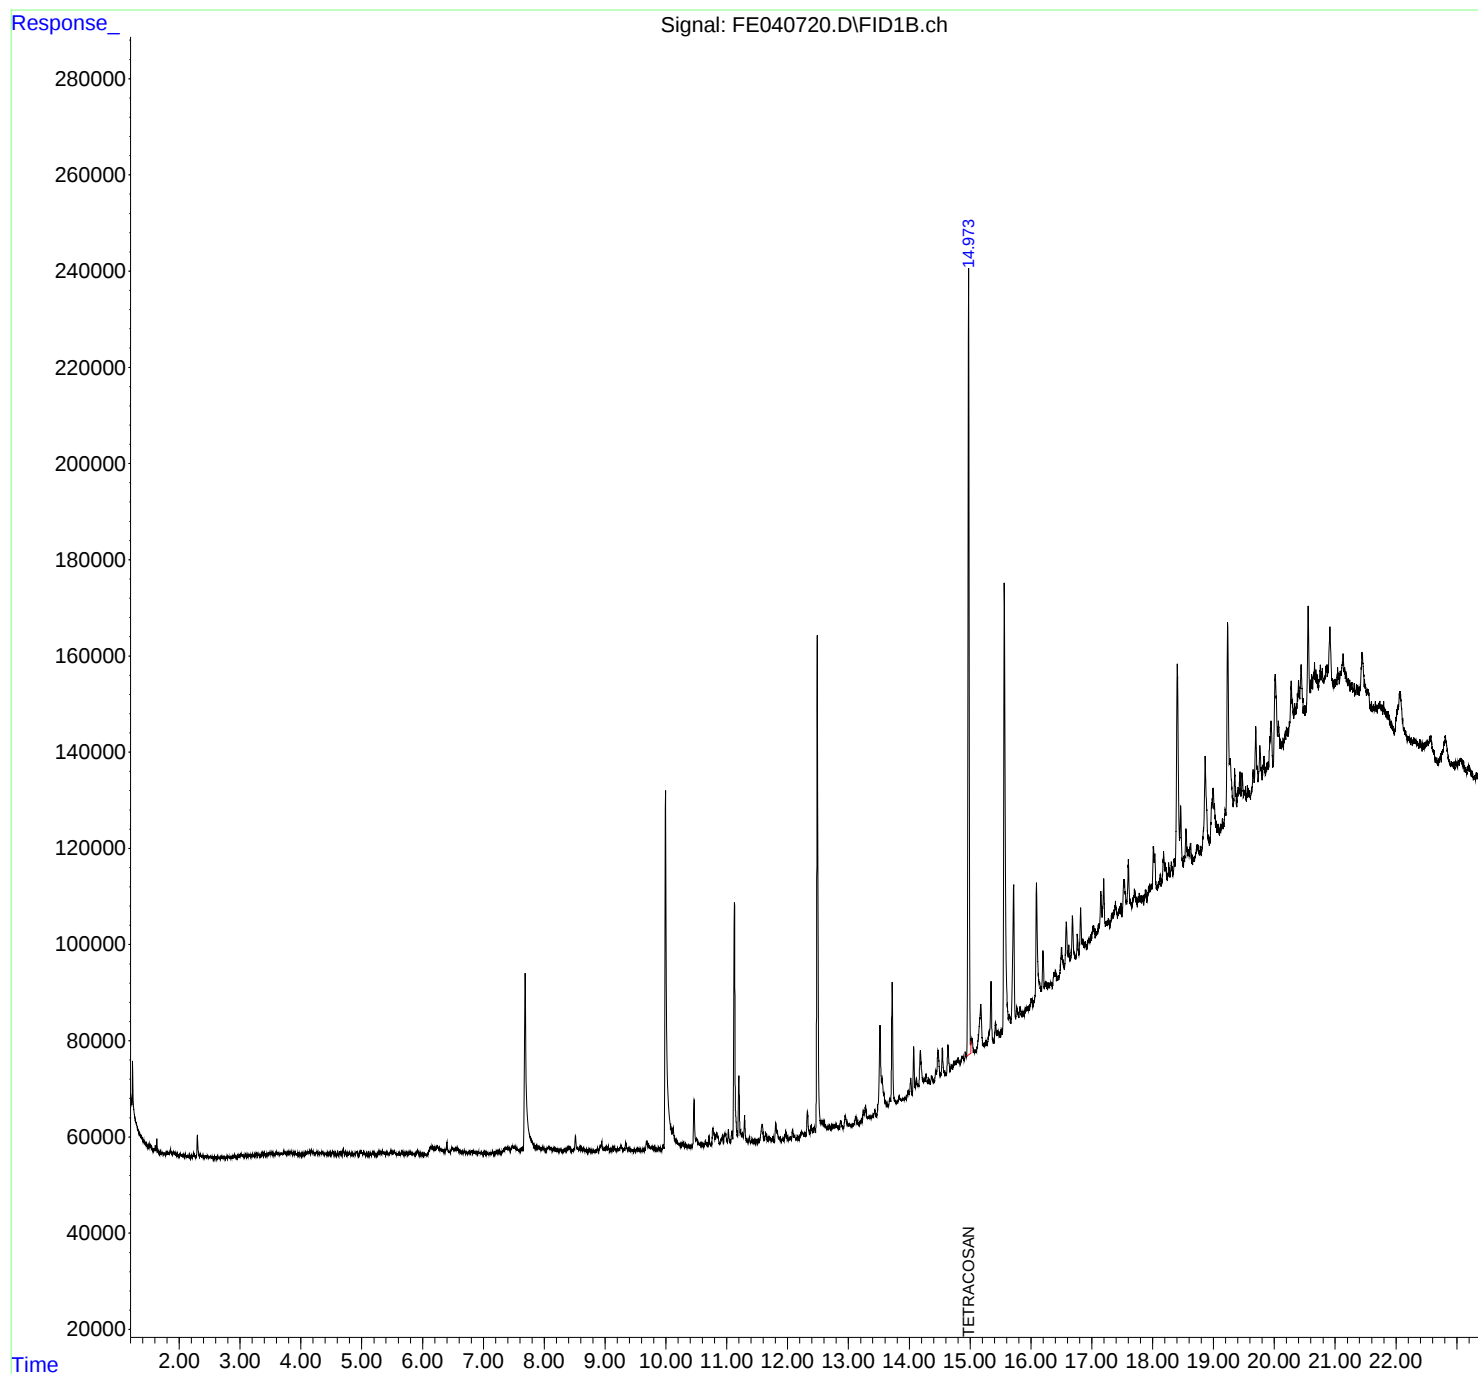

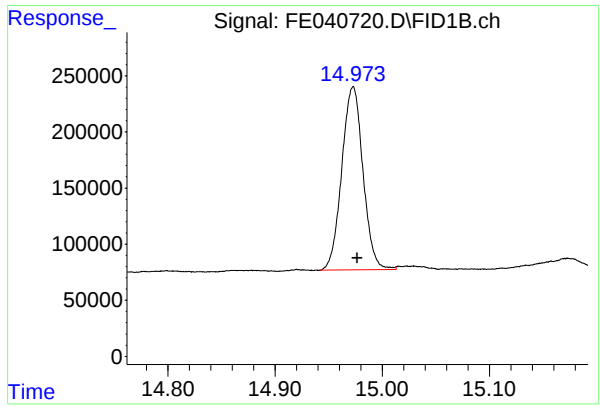

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.973 min
Delta R.T.: -0.004 min
Response: 2246690
Conc: 17.01 ug/ml

Instrument :

FID_E

ClientSampleId :

SS-02-20230306

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 03/09/2023

Supervised By :Ankita Jodhani 03/09/2023