

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030921\
 Data File : FE033358.D
 Signal(s) : FID1B.CH
 Acq On : 09 Mar 2021 16:49
 Operator : DD\AJ
 Sample : M1603-06 50X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 10 00:58:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022221.M
 Quant Title :
 QLast Update : Tue Feb 23 10:21:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

11)	N-HEXACOSANE	15.784	244226	0.630 ug/ml
12)	N-OCTACOSANE	16.736	625519	1.596 ug/ml
13)	N-TRIACONTANE	17.621	365042	0.923 ug/ml
14)	N-DOTRIACONTANE	18.451	432555	1.093 ug/ml
15)	N-TETRATRIACONTANE	19.237	318428	0.819 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030921\
Data File : FE033358.D
Signal(s) : FID1B.CH
Acq On : 09 Mar 2021 16:49
Operator : DD\AJ
Sample : M1603-06 50X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 10 00:58:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022221.M
Quant Title :
QLast Update : Tue Feb 23 10:21:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

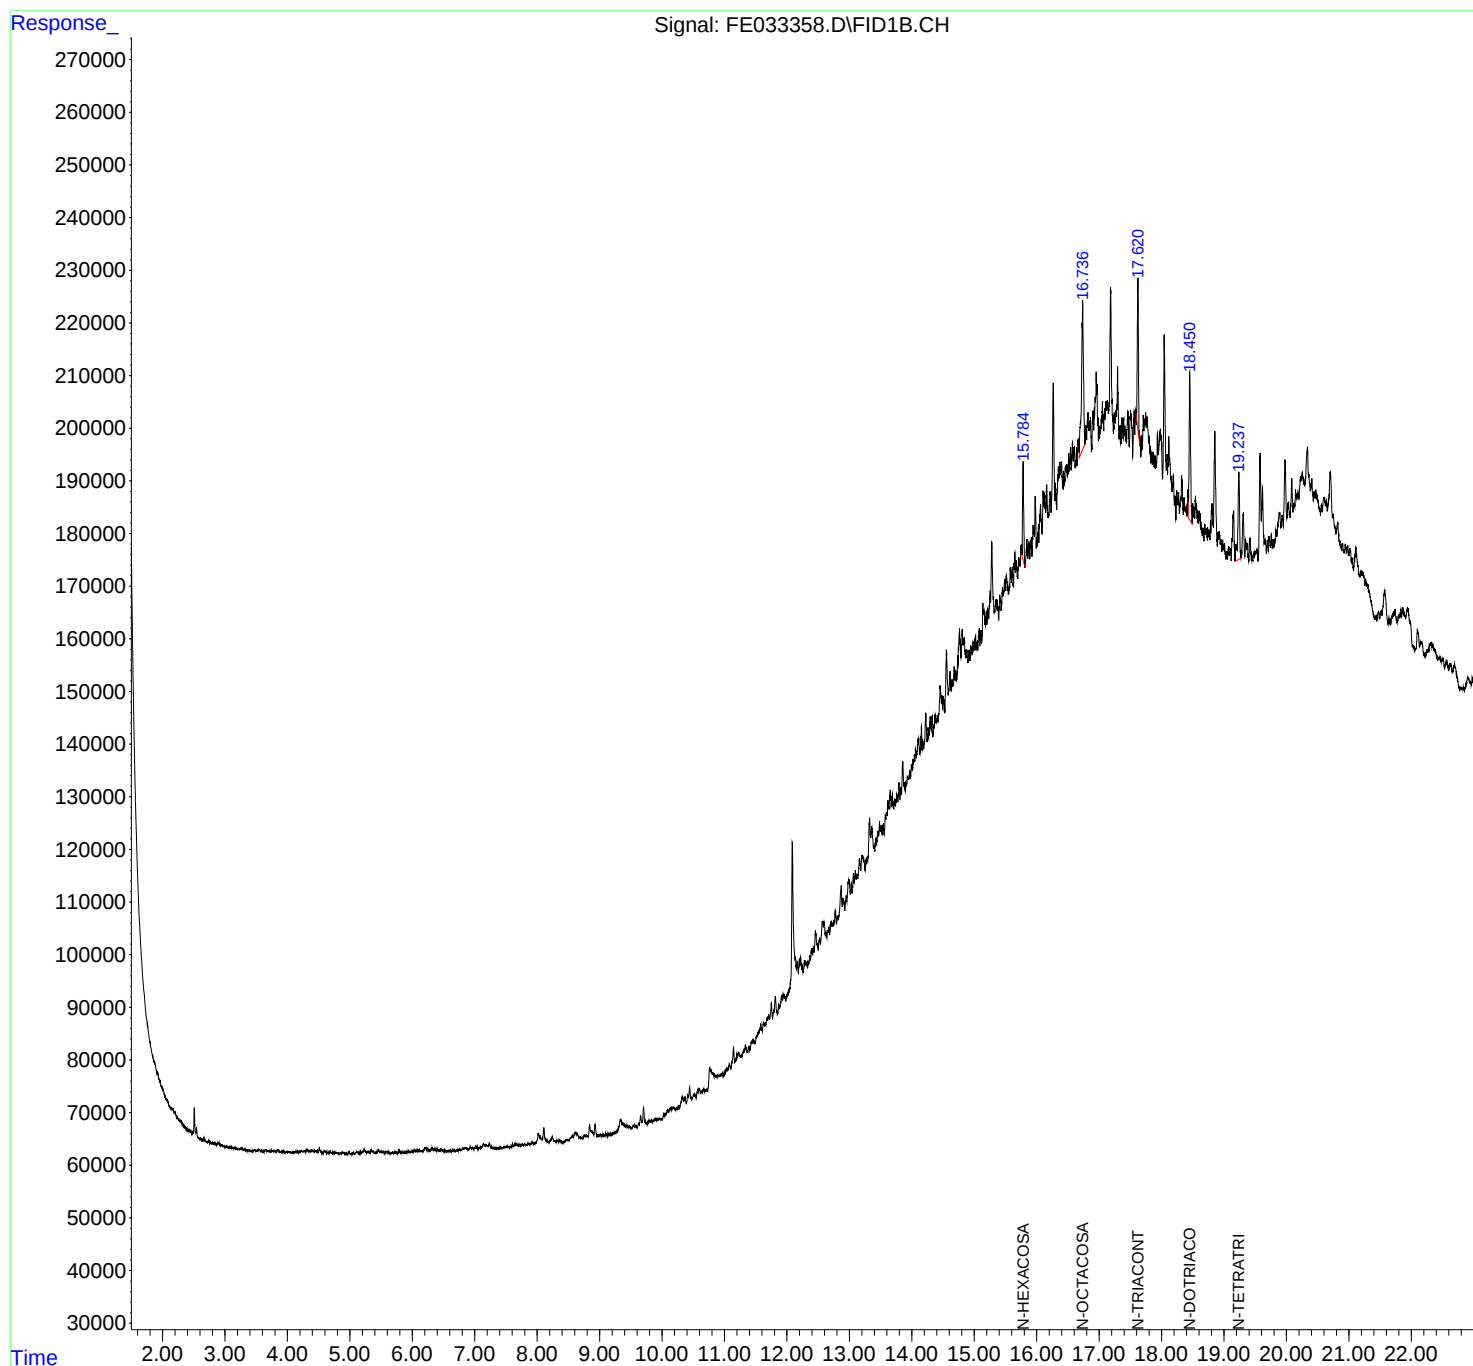


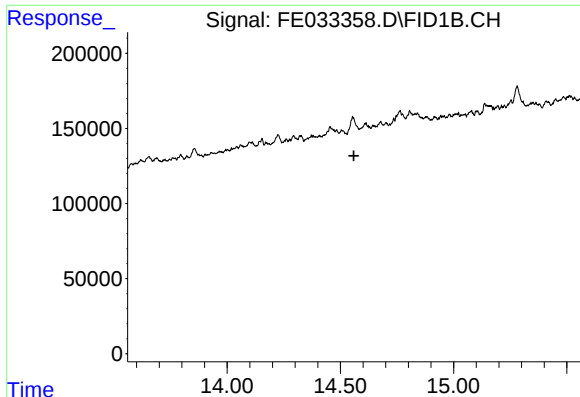

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.560 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

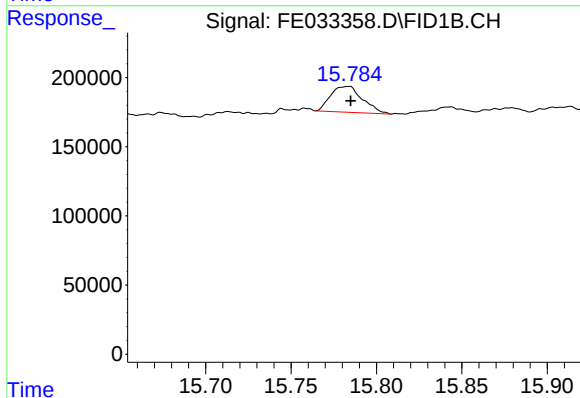


#11 N-HEXACOSANE

R.T.: 15.784 min
Delta R.T.: 0.000 min
Response: 244226
Conc: 0.63 ug/ml

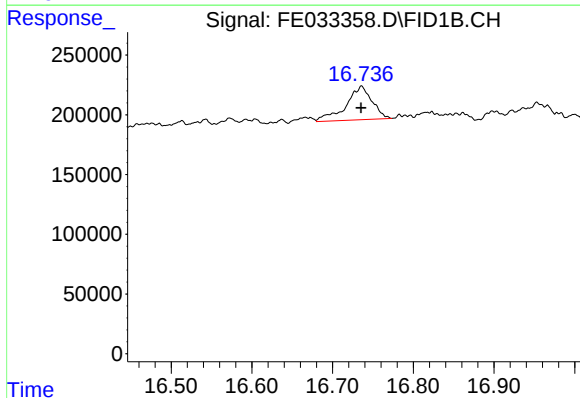


#12 N-OCTACOSANE

R.T.: 16.736 min
Delta R.T.: 0.000 min
Response: 625519
Conc: 1.60 ug/ml

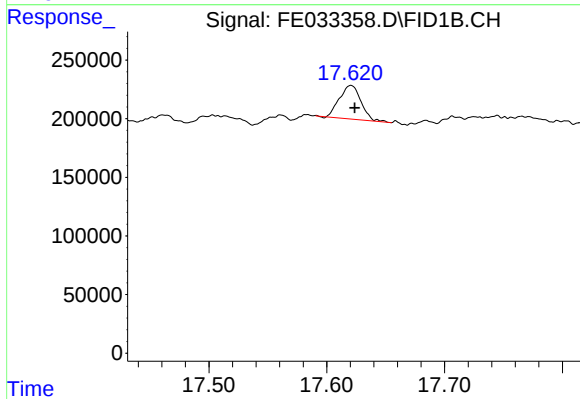

#13 N-TRIACONTANE


R.T.: 17.621 min
Delta R.T.: -0.003 min
Response: 365042
Conc: 0.92 ug/ml

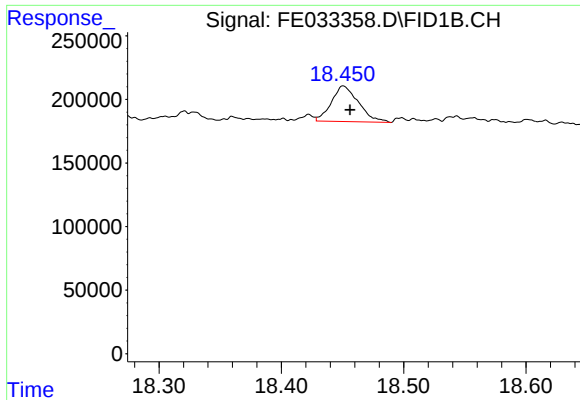

#14 N-DOTRIACONTANE

R.T.: 18.451 min
Delta R.T.: -0.006 min
Response: 432555
Conc: 1.09 ug/ml

Instrument :
FID_E
ClientSampleId :

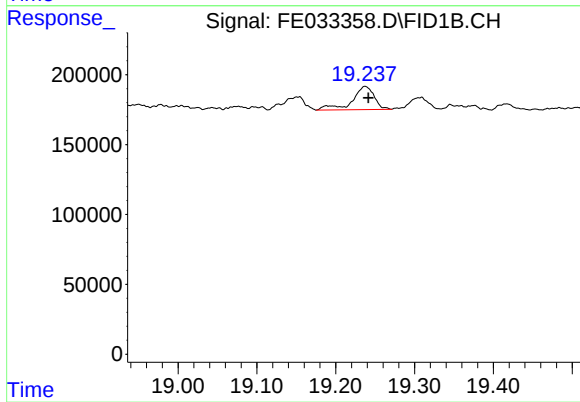

#15 N-TETRATRIACONTANE

R.T.: 19.237 min
Delta R.T.: -0.004 min
Response: 318428
Conc: 0.82 ug/ml