

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030921\
 Data File : FE033360.D
 Signal(s) : FID1B.CH
 Acq On : 09 Mar 2021 18:34
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 10 00:59:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022221.M
 Quant Title :
 QLast Update : Tue Feb 23 10:21:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.554	6376783	18.565 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.615	185698	0.470 ug/ml
14) N-DOTRIACONTANE	18.449	241850	0.611 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030921\
Data File : FE033360.D
Signal(s) : FID1B.CH
Acq On : 09 Mar 2021 18:34
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 10 00:59:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE022221.M
Quant Title :
QLast Update : Tue Feb 23 10:21:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

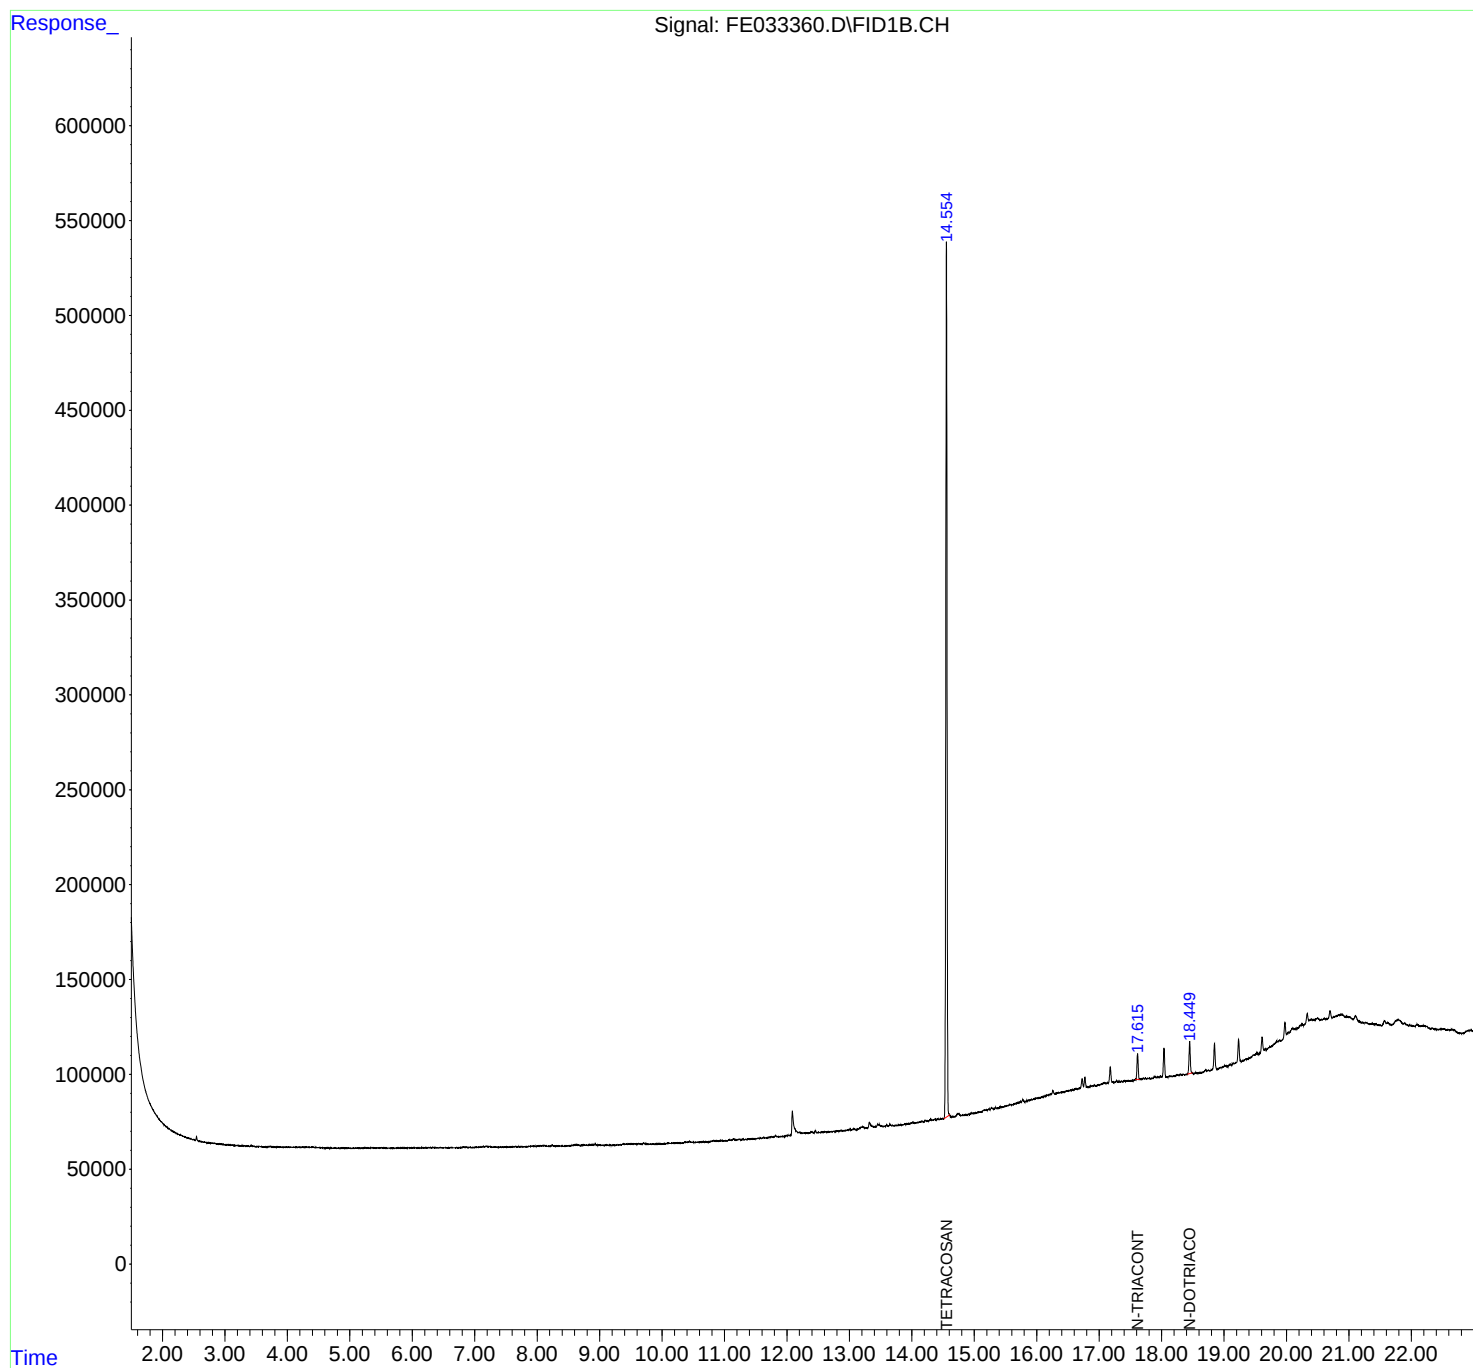


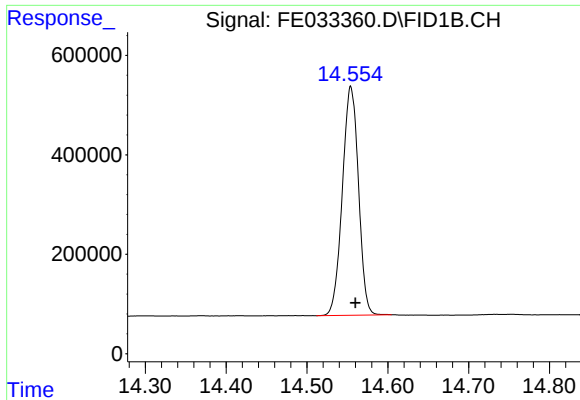

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.554 min
Delta R.T.: -0.006 min
Response: 6376783
Conc: 18.56 ug/ml

Instrument :
FID_E
ClientSampleId :

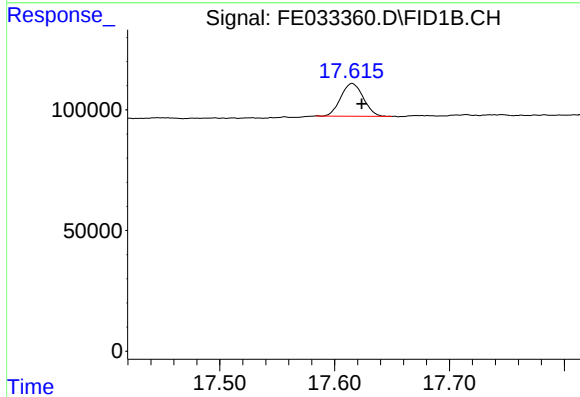

#13 N-TRIACONTANE

R.T.: 17.615 min
Delta R.T.: -0.008 min
Response: 185698
Conc: 0.47 ug/ml

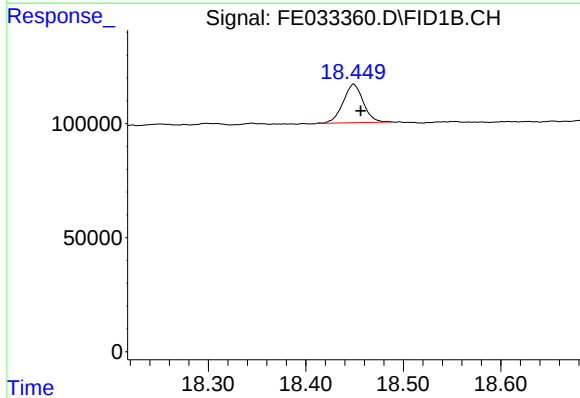

#14 N-DOTRIACONTANE

R.T.: 18.449 min
Delta R.T.: -0.007 min
Response: 241850
Conc: 0.61 ug/ml