

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030923AL\
 Data File : FE040752.D
 Signal(s) : FID1B.ch
 Acq On : 10 Mar 2023 04:20
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 10 04:53:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022823.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 28 03:05:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) T n-Dotriacontane (C32)	18.874	35839	0.209 ug/ml
19) T n-Tetratriacontane (C34)	19.655	19113	0.124 ug/ml
22) T n-Tetracontane (C40)	22.001	12093	0.078 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030923AL\
Data File : FE040752.D
Signal(s) : FID1B.ch
Acq On : 10 Mar 2023 04:20
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 10 04:53:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022823.M
Quant Title : GC Extractables
QLast Update : Tue Feb 28 03:05:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

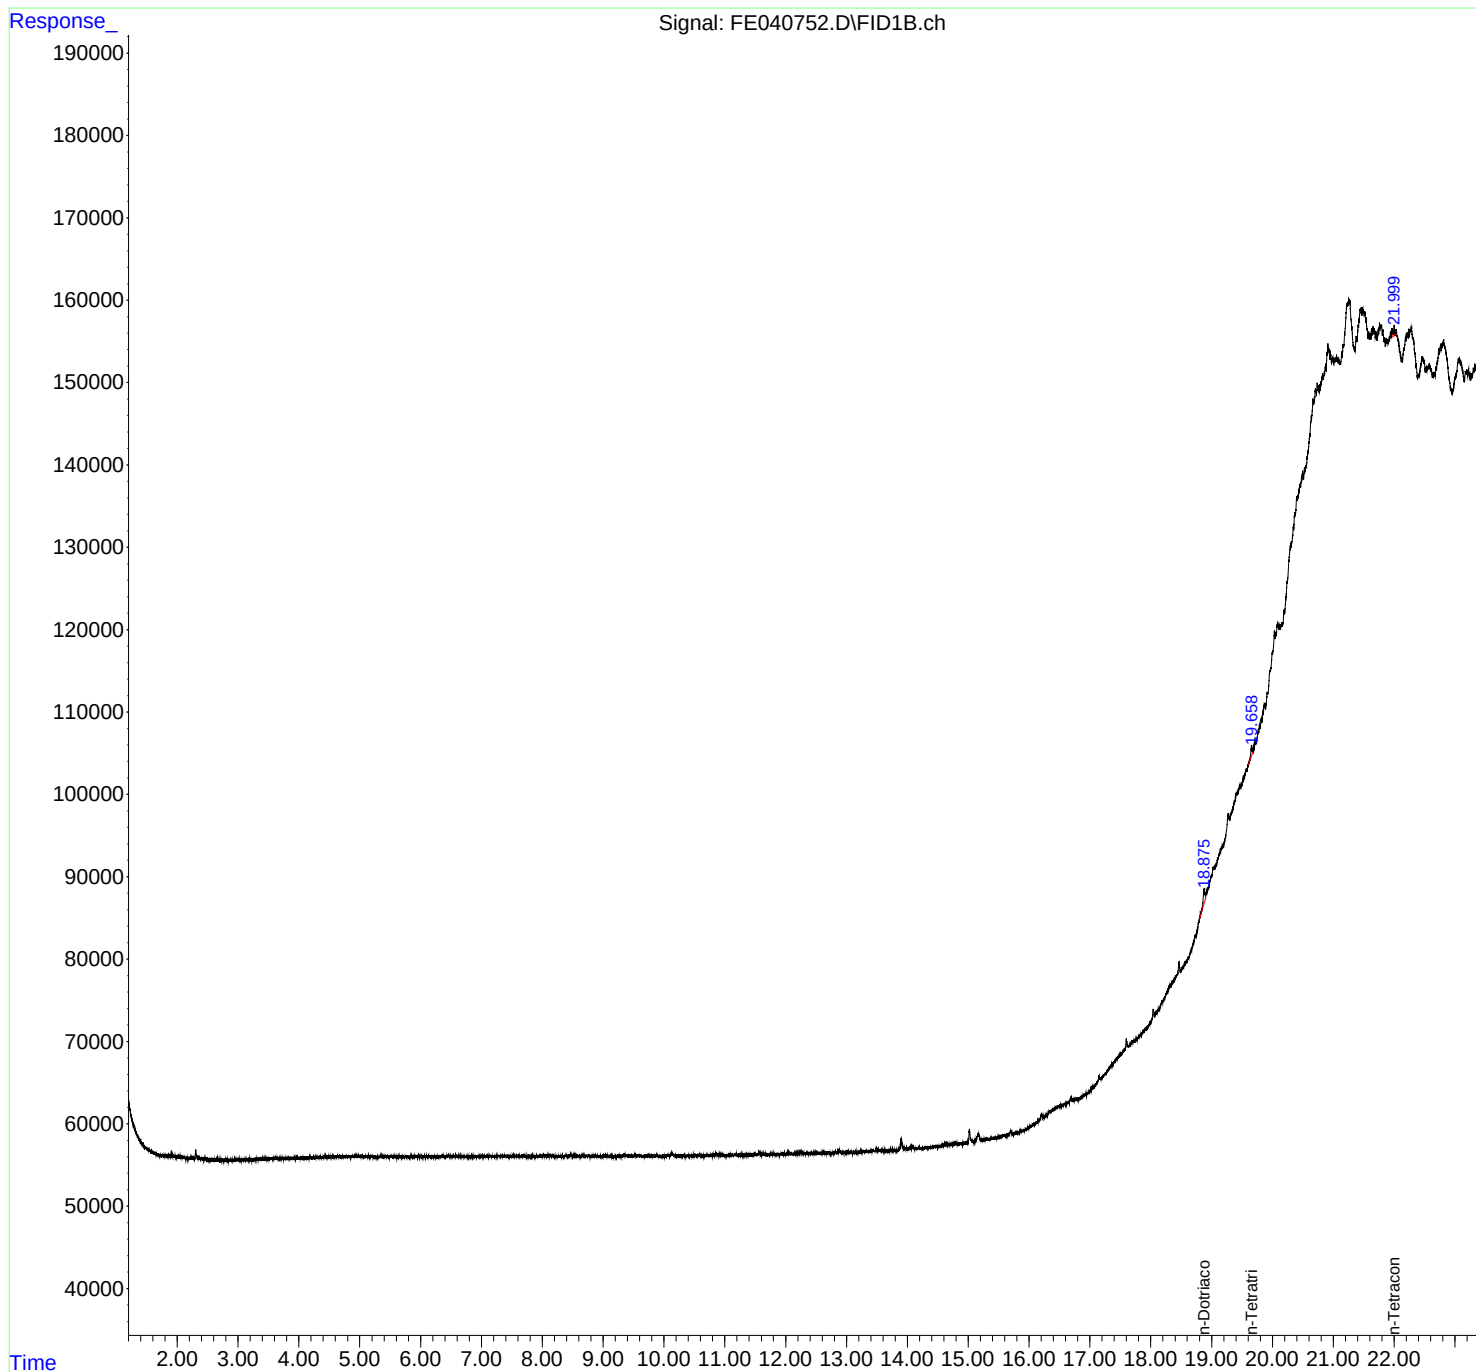


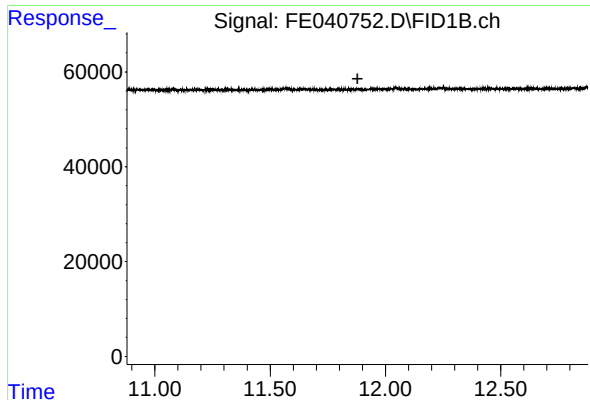

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.879 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

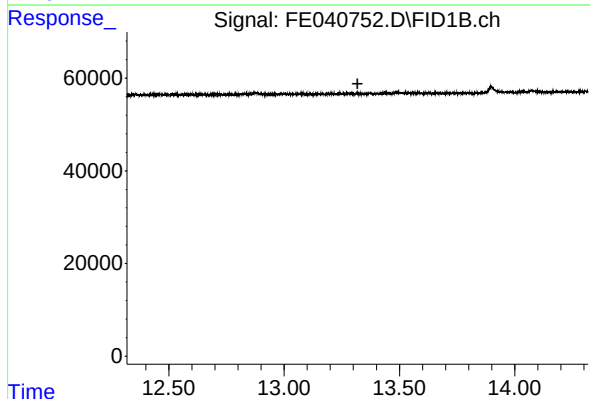


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.318 min
Response: 0
Conc: N.D.

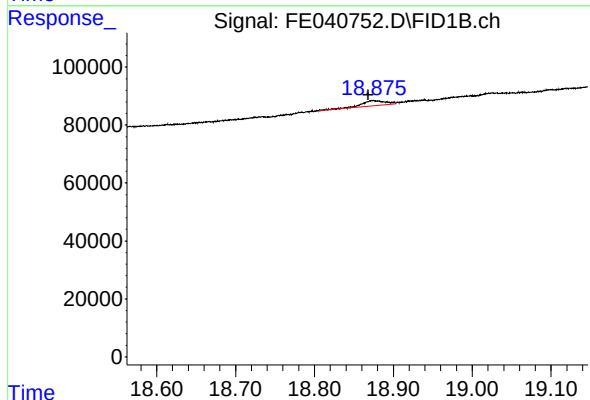


#18 n-Dotriacontane (C32)

R.T.: 18.874 min
Delta R.T.: 0.006 min
Response: 35839
Conc: 0.21 ug/ml

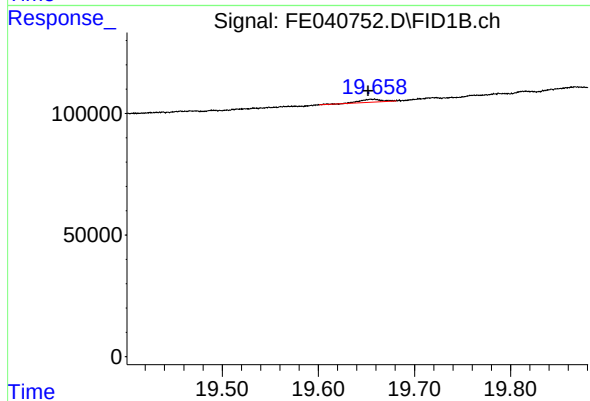

#19 n-Tetratriacontane (C34)

R.T.: 19.655 min
Delta R.T.: 0.003 min
Response: 19113
Conc: 0.12 ug/ml

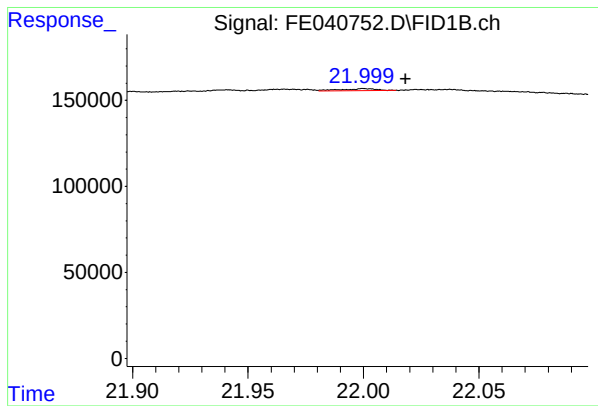

#22 n-Tetracontane (C40)

R.T.: 22.001 min

Delta R.T.: -0.018 min

Response: 12093

Conc: 0.08 ug/ml

Instrument :

FID_E

ClientSampleId :