

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030923AL\
 Data File : FE040749.D
 Signal(s) : FID1B.ch
 Acq On : 10 Mar 2023 02:16
 Operator : YP\AJ
 Sample : 01847-02DL 5X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 TR-05-030823DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/10/2023
 Supervised By :Ankita Jodhani 03/10/2023

Integration File: autoint1.e
 Quant Time: Mar 10 03:00:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022823.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 28 03:05:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.878	1549863	8.296 ug/mlm
Spiked Amount	50.000	Recovery	= 16.59%
12) S 1-chlorooctadecane (S...	13.308	7948609	53.705 ug/ml
Spiked Amount	50.000	Recovery	= 107.41%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE030923AL\
Data File : FE040749.D
Signal(s) : FID1B.ch
Acq On : 10 Mar 2023 02:16
Operator : YP\AJ
Sample : 01847-02DL 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
TR-05-030823DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/10/2023
Supervised By :Ankita Jodhani 03/10/2023

Integration File: autoint1.e
Quant Time: Mar 10 03:00:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 022823.
Quant Title : GC Extractables
QLast Update : Tue Feb 28 03:05:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

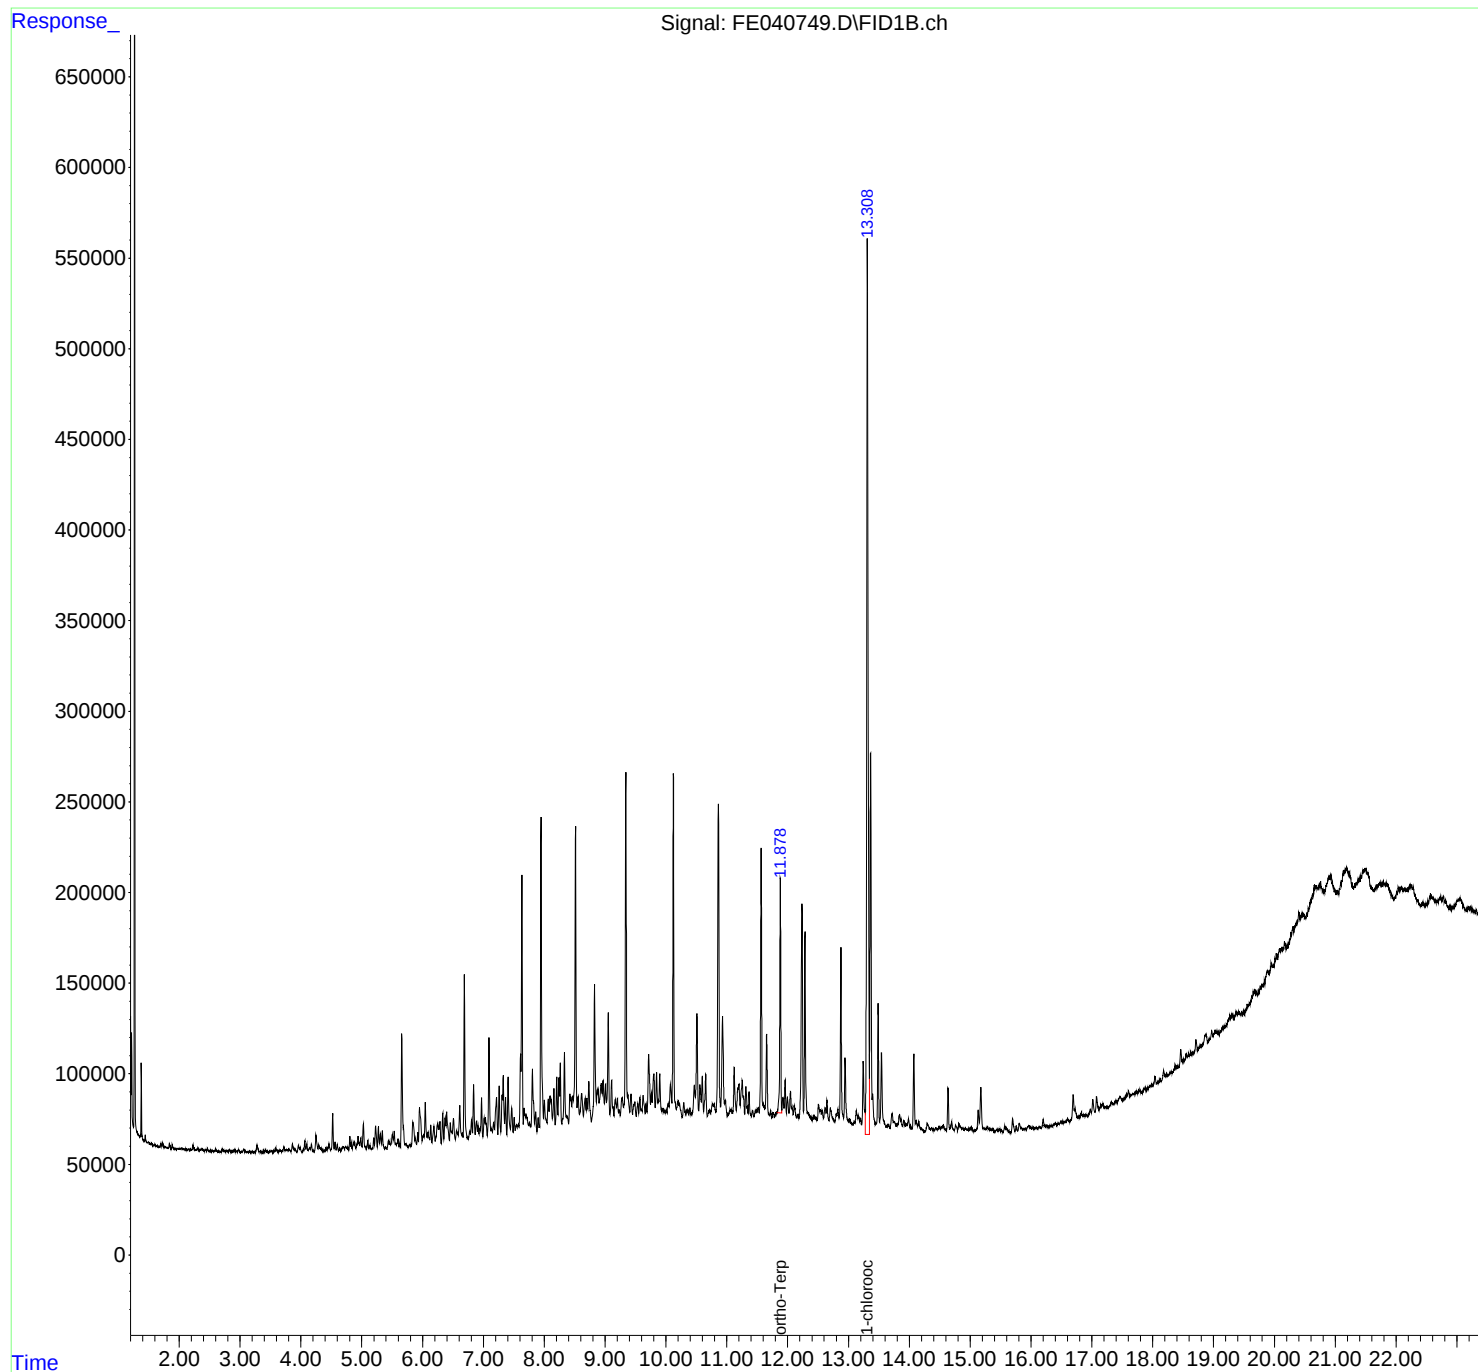

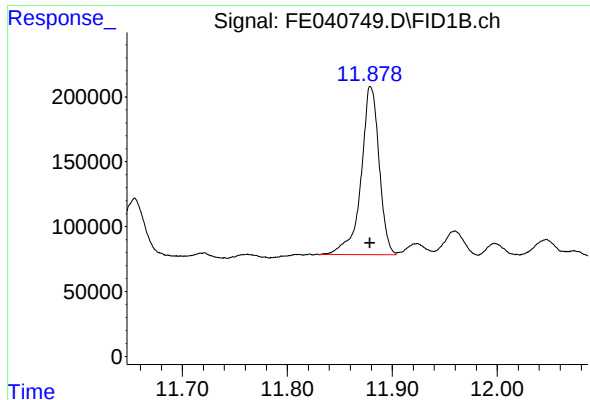


#9 ortho-Terphenyl (SURR)

R.T.: 11.878 min
Delta R.T.: 0.000 min
Response: 1549863
Conc: 8.30 ug/ml

Instrument :
FID_E
ClientSampleId :
TR-05-030823DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/10/2023
Supervised By :Ankita Jodhani 03/10/2023

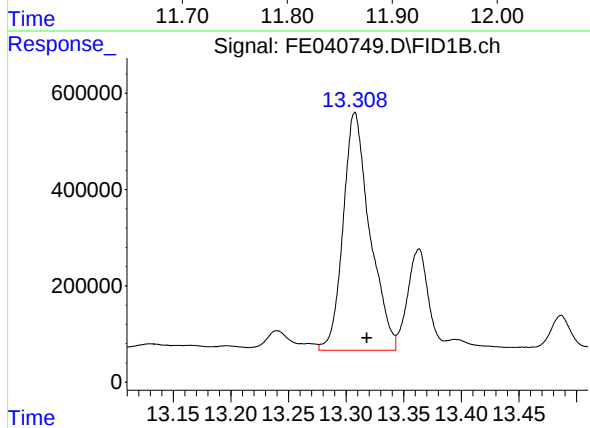

#12 1-chlorooctadecane (SURR)

R.T.: 13.308 min
Delta R.T.: -0.011 min
Response: 7948609
Conc: 53.71 ug/ml