

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031025AL\
 Data File : FE052718.D
 Signal(s) : FID1B.ch
 Acq On : 11 Mar 2025 01:03
 Operator : YP\AJ
 Sample : Q1488-09
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 11 05:26:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 030325.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 03 13:39:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.358	5213495	42.936 ug/ml
Spiked Amount 50.000		Recovery =	85.87%
Target Compounds			
4) T n-Dodecane (C12)	6.692	134980	0.867 ug/ml
6) T n-Tetradecane (C14)	8.529	116104	0.767 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031025AL\
Data File : FE052718.D
Signal(s) : FID1B.ch
Acq On : 11 Mar 2025 01:03
Operator : YP\AJ
Sample : Q1488-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 11 05:26:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 030325.M
Quant Title : GC Extractables
QLast Update : Mon Mar 03 13:39:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

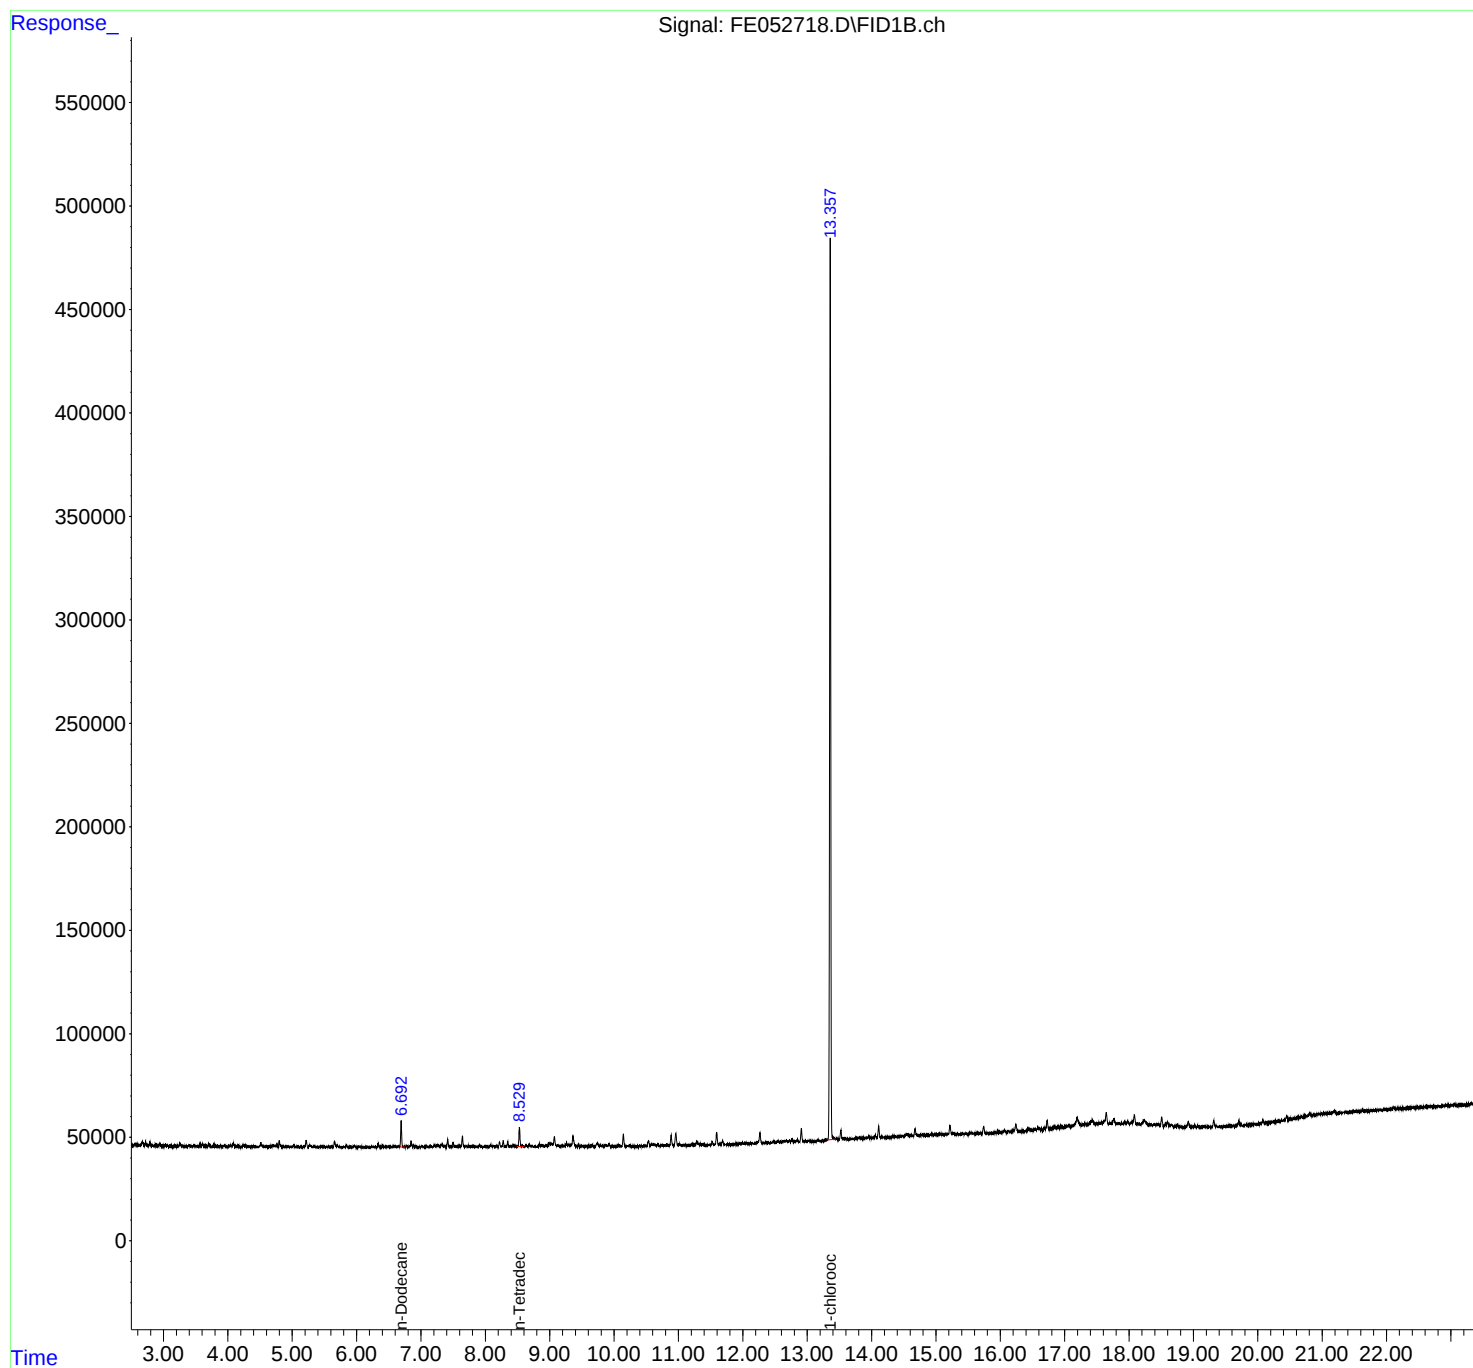


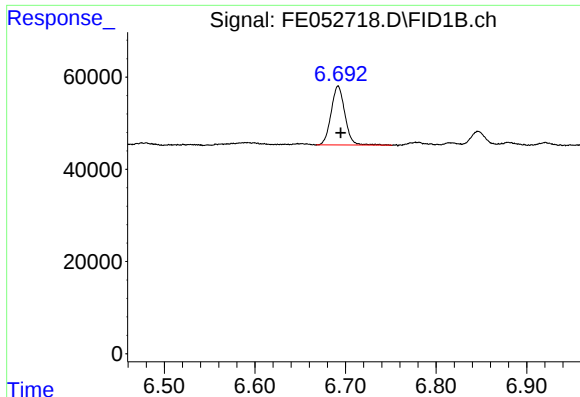

#4 n-Dodecane (C12)


R.T.: 6.692 min
Delta R.T.: -0.003 min
Response: 134980
Conc: 0.87 ug/ml

Instrument :
FID_E
ClientSampleId :

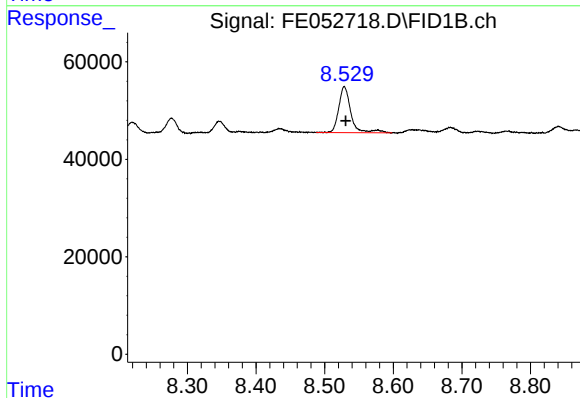


#6 n-Tetradecane (C14)

R.T.: 8.529 min
Delta R.T.: -0.002 min
Response: 116104
Conc: 0.77 ug/ml

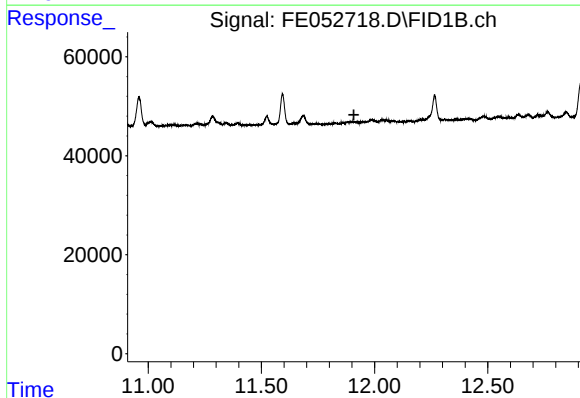

#9 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.909 min
Response: 0
Conc: N.D.

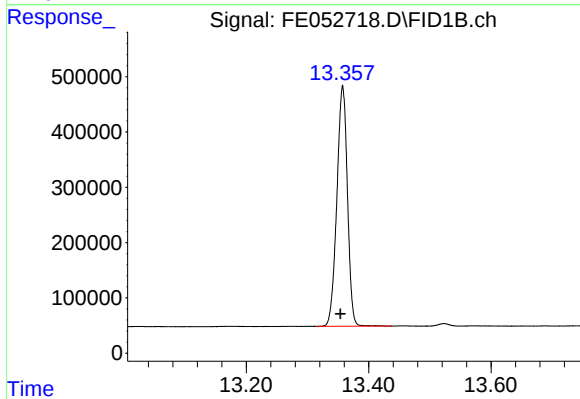

#12 1-chlorooctadecane (SURRE)

R.T.: 13.358 min
Delta R.T.: 0.003 min
Response: 5213495
Conc: 42.94 ug/ml