

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE031025AL\  
 Data File : FE052719.D  
 Signal(s) : FID1B.ch  
 Acq On : 11 Mar 2025 01:34  
 Operator : YP\AJ  
 Sample : Q1488-11  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Mar 11 05:26:31 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 030325.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Mar 03 13:39:39 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 12) S 1-chlorooctadecane (S... | 13.357 | 4009135    | 33.017 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 66.03%       |
|                                |        |            |              |
| Target Compounds               |        |            |              |
| 4) T n-Dodecane (C12)          | 6.692  | 110142     | 0.707 ug/ml  |
| 6) T n-Tetradecane (C14)       | 8.528  | 78988      | 0.522 ug/ml  |
| 18) T n-Dotriacontane (C32)    | 18.919 | 106151     | 0.731 ug/ml  |
| -----                          |        |            |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE031025AL\  
Data File : FE052719.D  
Signal(s) : FID1B.ch  
Acq On : 11 Mar 2025 01:34  
Operator : YP\AJ  
Sample : Q1488-11  
Misc :  
ALS Vial : 30 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Mar 11 05:26:31 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 030325.M  
Quant Title : GC Extractables  
QLast Update : Mon Mar 03 13:39:39 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

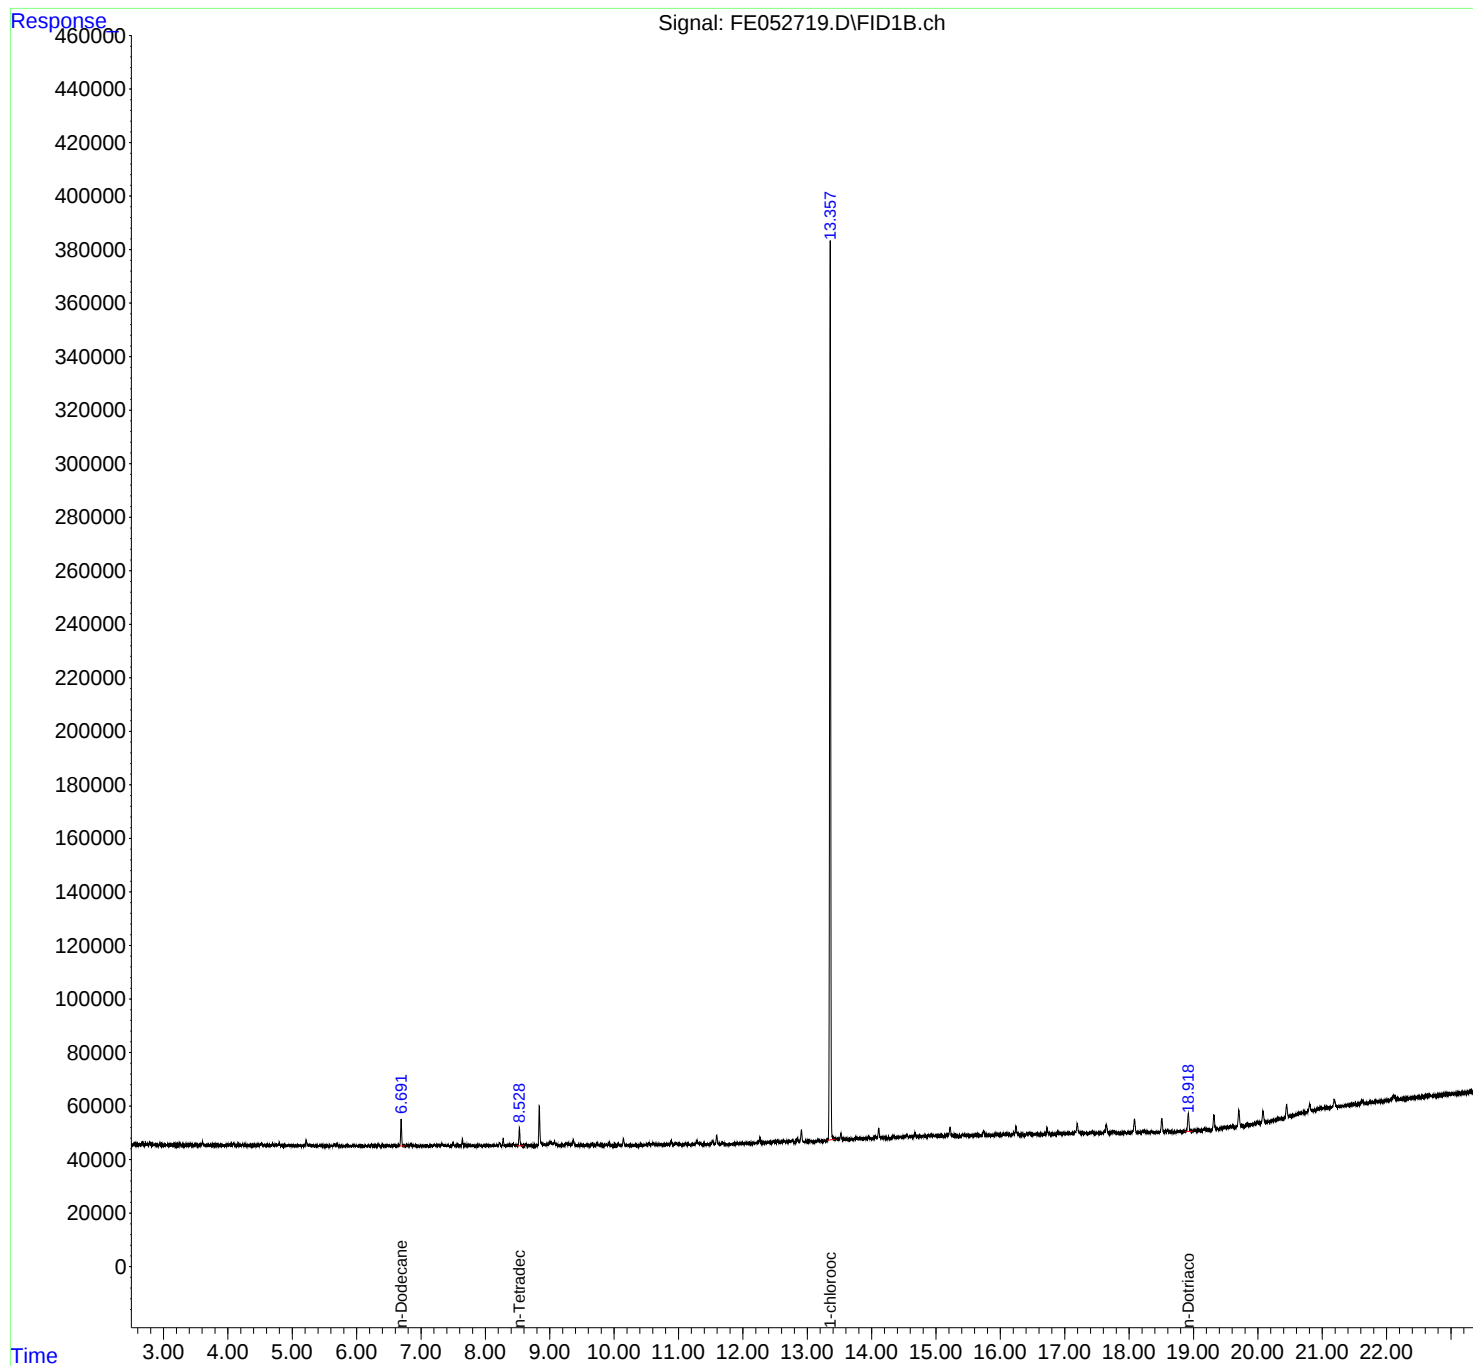


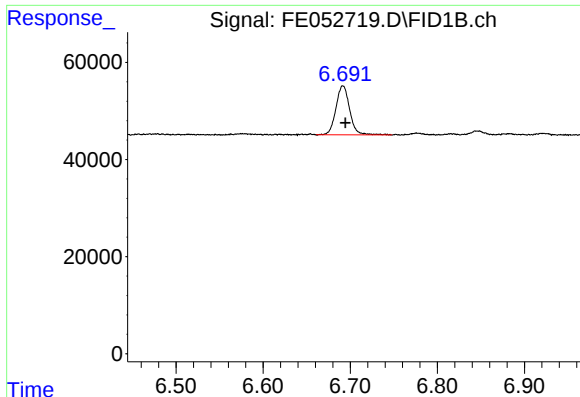

#4 n-Dodecane (C12)


R.T.: 6.692 min  
Delta R.T.: -0.003 min  
Response: 110142  
Conc: 0.71 ug/ml

Instrument :  
FID\_E  
ClientSampleId :

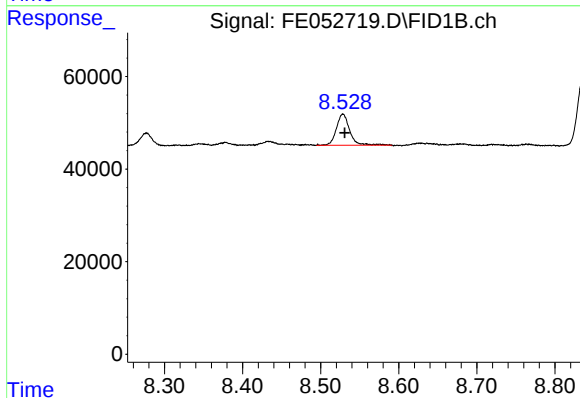


#6 n-Tetradecane (C14)

R.T.: 8.528 min  
Delta R.T.: -0.002 min  
Response: 78988  
Conc: 0.52 ug/ml

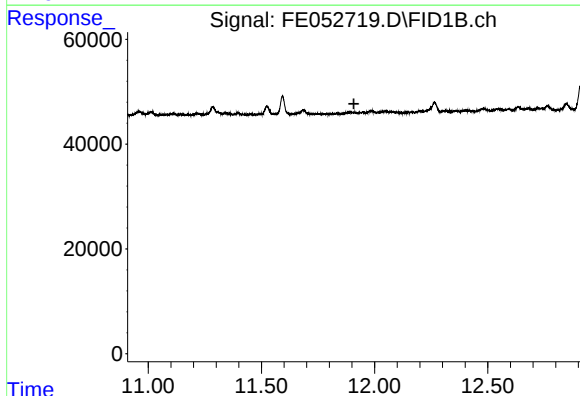


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T. : 11.909 min  
Response: 0  
Conc: N.D.

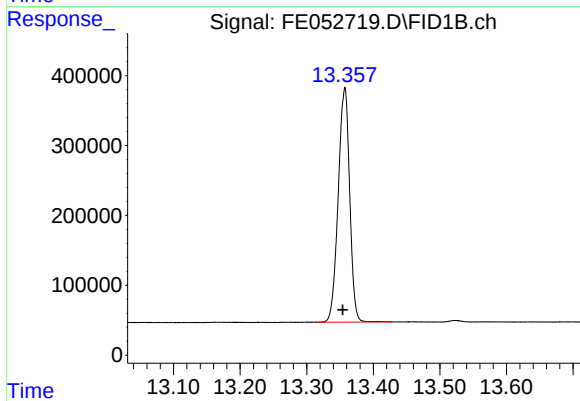

#12 1-chlorooctadecane (SURR)

R.T.: 13.357 min  
Delta R.T.: 0.003 min  
Response: 4009135  
Conc: 33.02 ug/ml

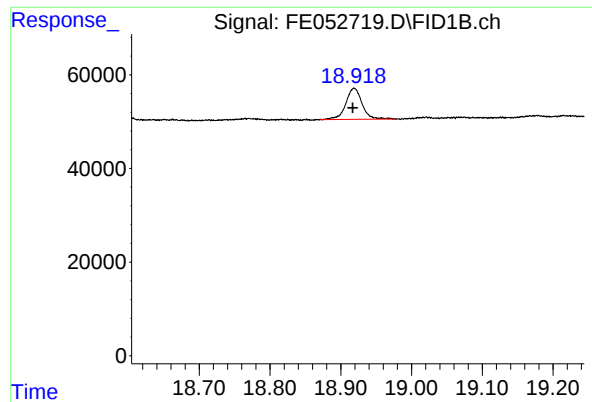

#18 n-Dotriacontane (C32)

R.T.: 18.919 min  
Delta R.T.: 0.002 min  
Response: 106151  
Conc: 0.73 ug/ml

Instrument :

FID\_E

ClientSampleId :