

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031120\
 Data File : FE031468.D
 Signal(s) : FID1B.CH
 Acq On : 12 Mar 2020 6:03
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Mar 12 06:40:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
 Quant Title :
 QLast Update : Wed Mar 11 09:35:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.417	18674918	50.599 ug/ml
Target Compounds			
2) N-DECANE	4.178	21496595	53.950 ug/ml
3) N-DODECANE	6.183	21938823	53.547 ug/ml
4) N-TETRADECANE	7.974	21974173	52.837 ug/ml
5) N-HEXADECANE	9.573	22236157	52.293 ug/ml
6) N-OCTADECANE	11.013	22182028	51.796 ug/ml
7) N-EICOSANE	12.321	21976680	51.411 ug/ml
8) N-DOCOSANE	13.520	21762134	51.007 ug/ml
10) N-TETRACOSANE	14.625	21513770	50.519 ug/ml
11) N-HEXACOSANE	15.645	21076811	50.181 ug/ml
12) N-OCTACOSANE	16.595	20854210	49.689 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031120\
Data File : FE031468.D
Signal(s) : FID1B.CH
Acq On : 12 Mar 2020 6:03
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Mar 12 06:40:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE031020.M
Quant Title :
QLast Update : Wed Mar 11 09:35:11 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

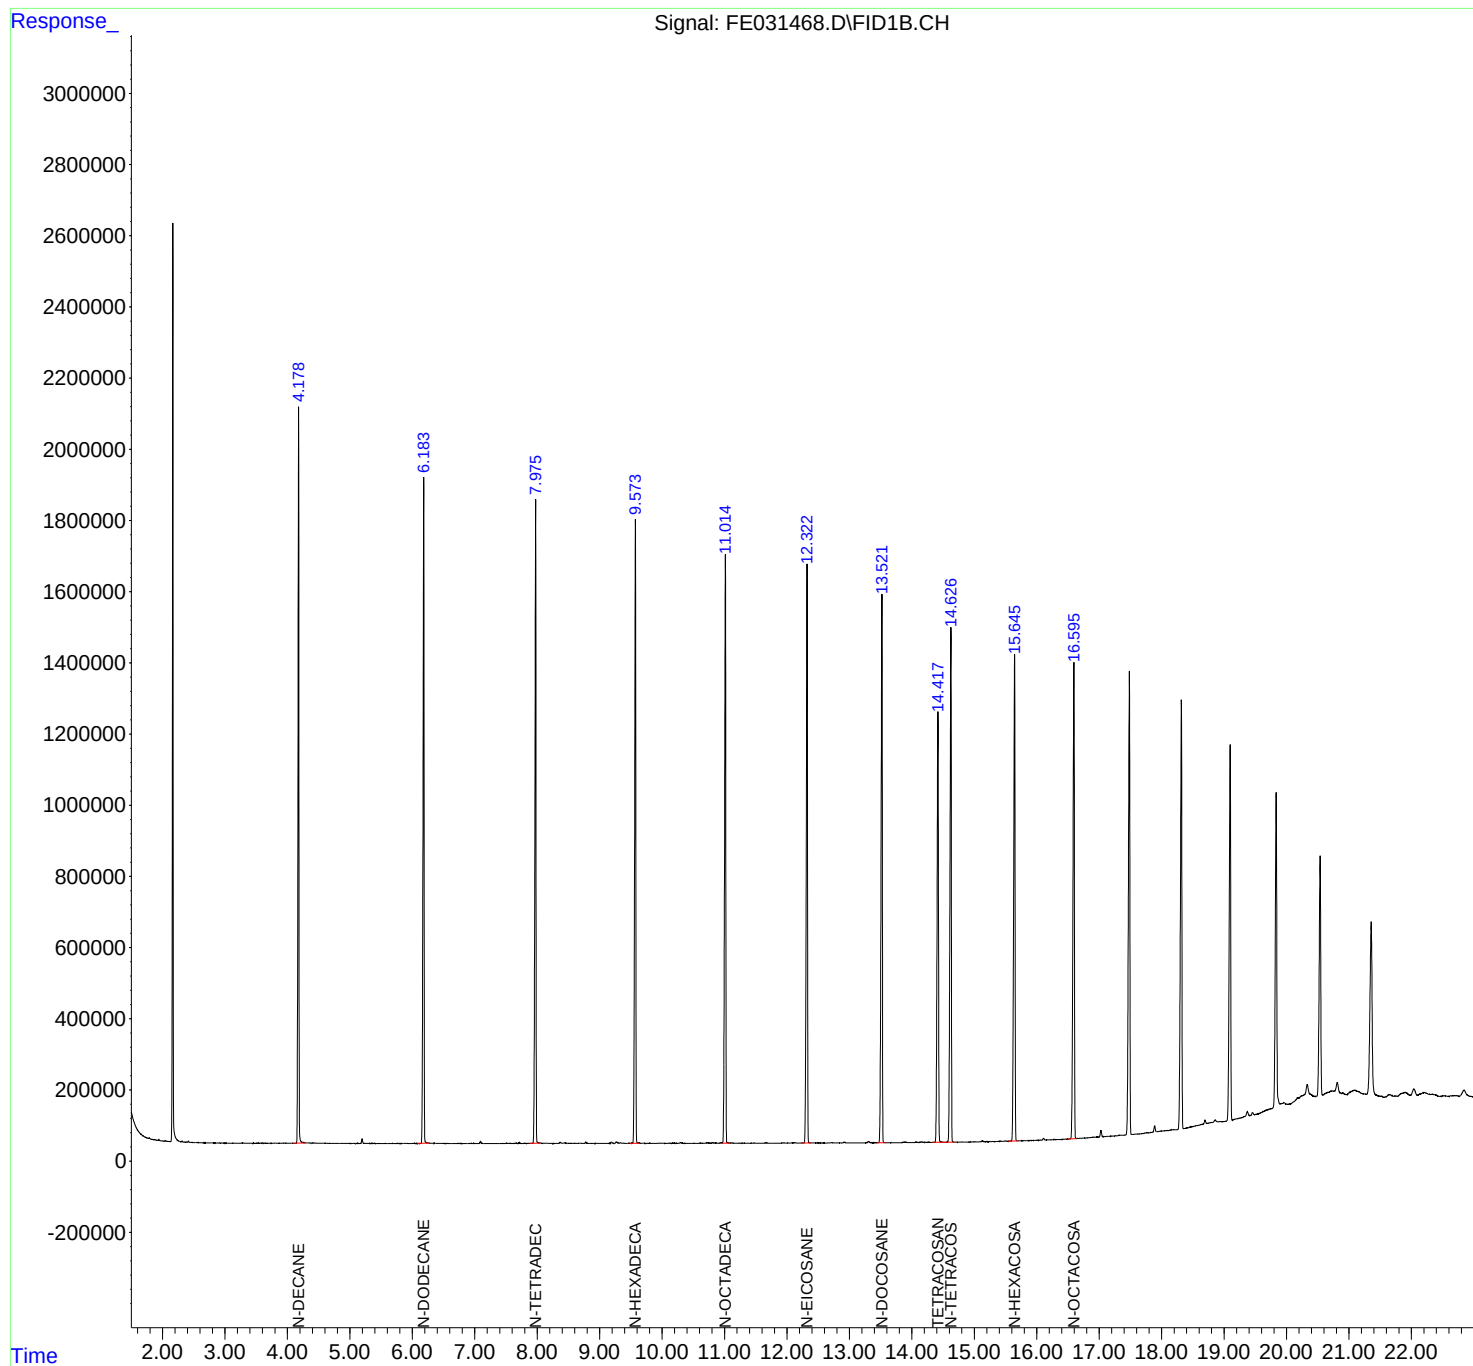


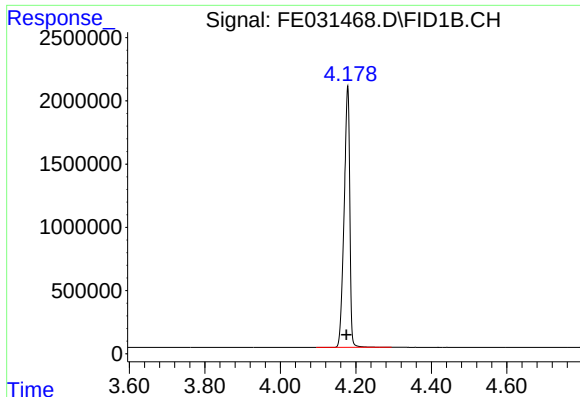

#2 N-DECANE


R.T.: 4.178 min
Delta R.T.: 0.003 min
Response: 21496595
Conc: 53.95 ug/ml

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

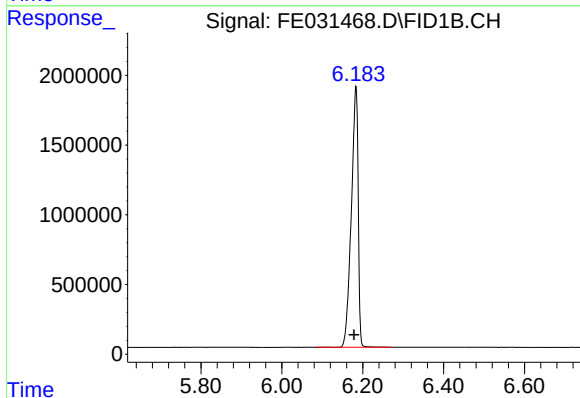


#3 N-DODECANE

R.T.: 6.183 min
Delta R.T.: 0.004 min
Response: 21938823
Conc: 53.55 ug/ml

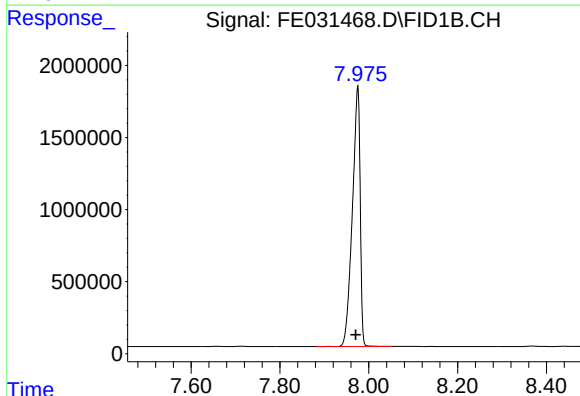


#4 N-TETRADECANE

R.T.: 7.974 min
Delta R.T.: 0.004 min
Response: 21974173
Conc: 52.84 ug/ml

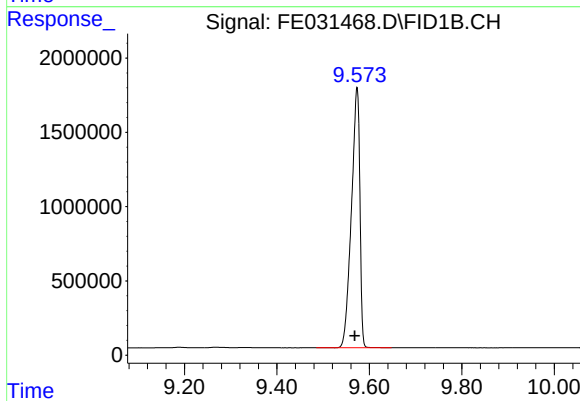

#5 N-HEXADECANE


R.T.: 9.573 min
Delta R.T.: 0.004 min
Response: 22236157
Conc: 52.29 ug/ml

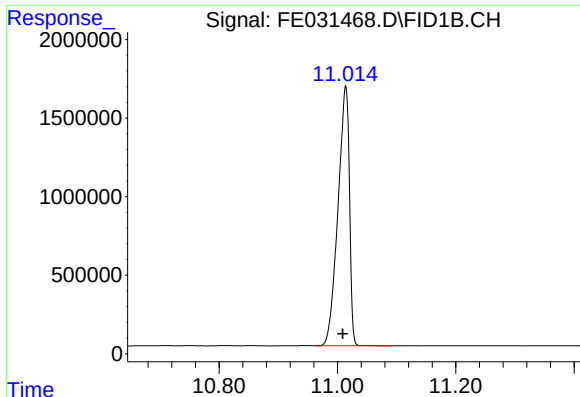

#6 N-OCTADECANE


R.T.: 11.013 min
Delta R.T.: 0.005 min
Response: 22182028
Conc: 51.80 ug/ml

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

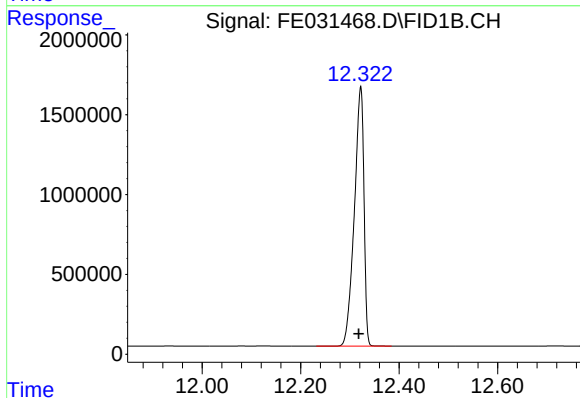


#7 N-EICOSANE

R.T.: 12.321 min
Delta R.T.: 0.004 min
Response: 21976680
Conc: 51.41 ug/ml

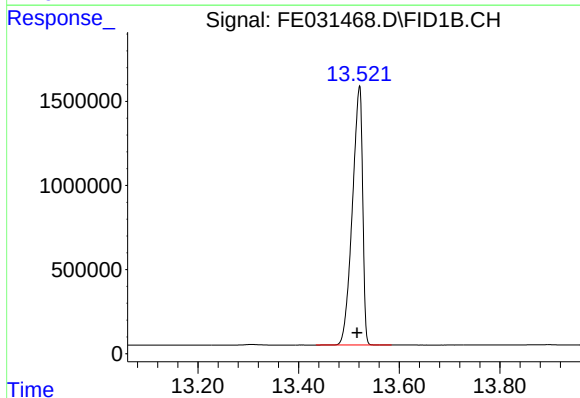


#8 N-DOCOSANE

R.T.: 13.520 min
Delta R.T.: 0.004 min
Response: 21762134
Conc: 51.01 ug/ml

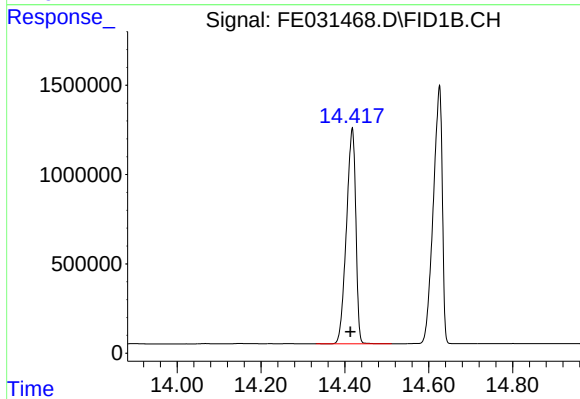

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.417 min
Delta R.T.: 0.004 min
Response: 18674918
Conc: 50.60 ug/ml

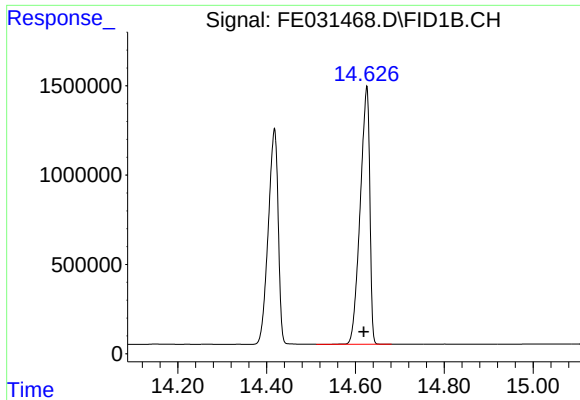

#10 N-TETRACOSANE


R.T.: 14.625 min
Delta R.T.: 0.006 min
Response: 21513770
Conc: 50.52 ug/ml

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

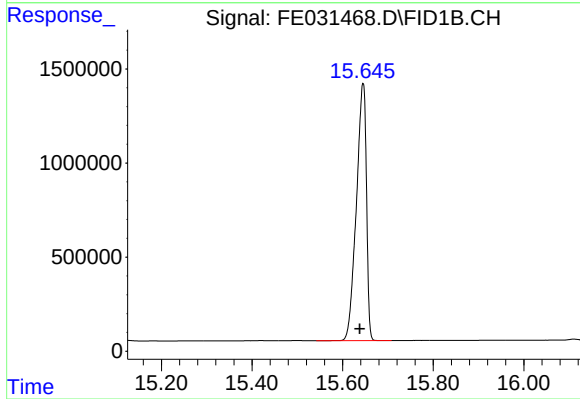

#11 N-HEXACOSANE

R.T.: 15.645 min
Delta R.T.: 0.006 min
Response: 21076811
Conc: 50.18 ug/ml

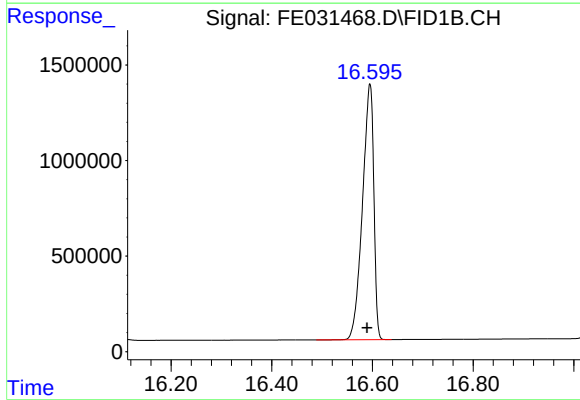

#12 N-OCTACOSANE

R.T.: 16.595 min
Delta R.T.: 0.005 min
Response: 20854210
Conc: 49.69 ug/ml