

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031125AL\
 Data File : FE052735.D
 Signal(s) : FID1B.ch
 Acq On : 11 Mar 2025 15:39
 Operator : YP\AJ
 Sample : Q1534-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 12 02:10:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 030325.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 03 13:39:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.909	4025982	23.881 ug/ml
Spiked Amount 50.000		Recovery =	47.76%
12) S 1-chlorooctadecane (S...	13.354	2939380	24.207 ug/ml
Spiked Amount 50.000		Recovery =	48.41%
Target Compounds			
10) T n-Eicosane (C20)	12.964f	650630	4.482 ug/ml
14) T n-Tetracosane (C24)	15.190	377364	2.637 ug/ml
16) T n-Octacosane (C28)	17.195	95976	0.675 ug/ml
17) T n-Tricontane (C30)	18.081	147711	1.000 ug/ml
18) T n-Dotriacontane (C32)	18.916	102369	0.705 ug/ml
19) T n-Tetratriacontane (C34)	19.703	102264	0.759 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE031125AL\
Data File : FE052735.D
Signal(s) : FID1B.ch
Acq On : 11 Mar 2025 15:39
Operator : YP\AJ
Sample : Q1534-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 12 02:10:16 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 030325.M
Quant Title : GC Extractables
QLast Update : Mon Mar 03 13:39:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

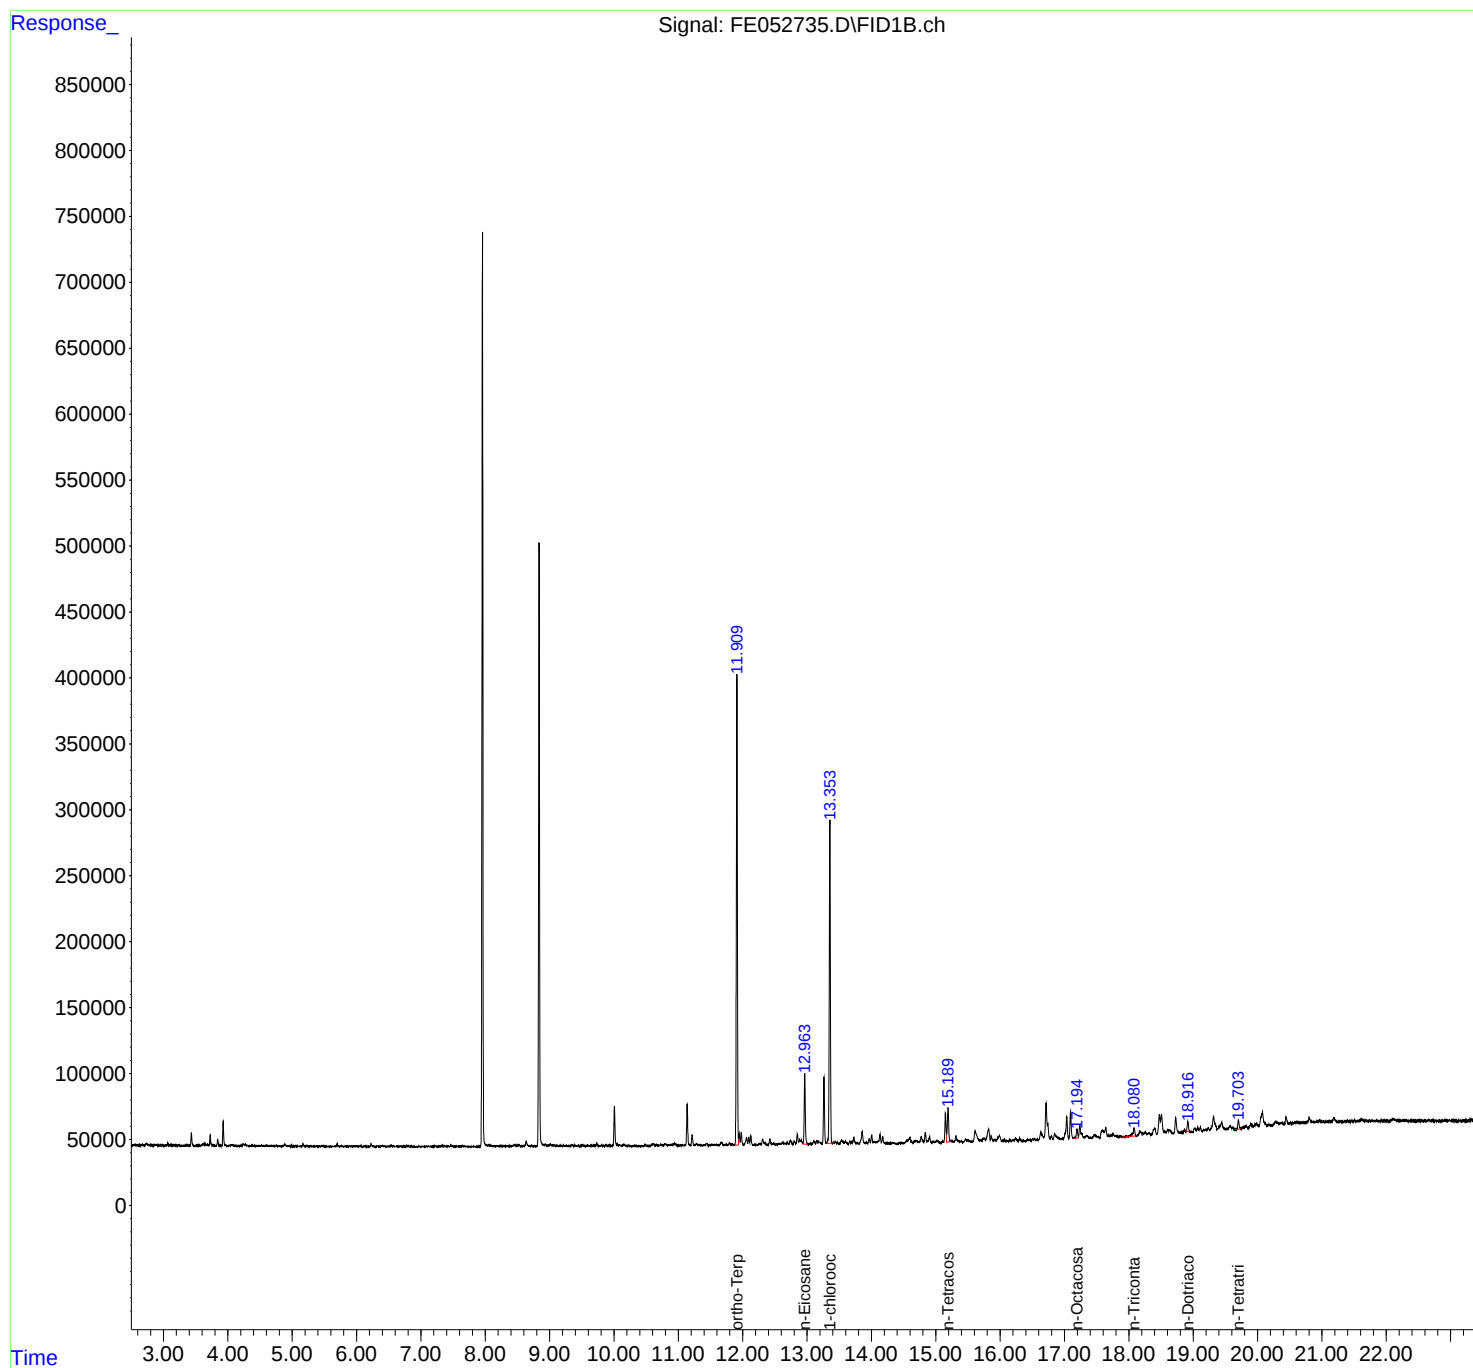


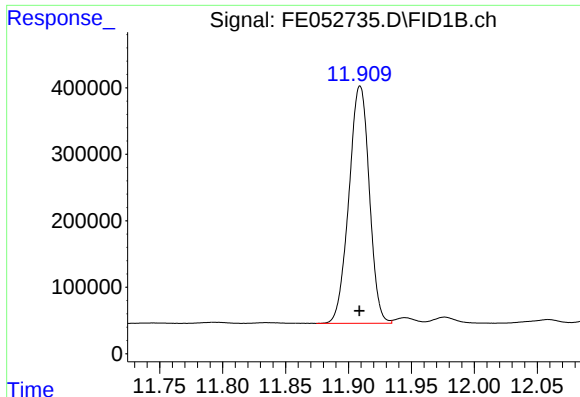

#9 ortho-Terphenyl (SURR)


R.T.: 11.909 min
Delta R.T.: 0.000 min
Response: 4025982
Conc: 23.88 ug/ml

Instrument :
FID_E
ClientSampleId :

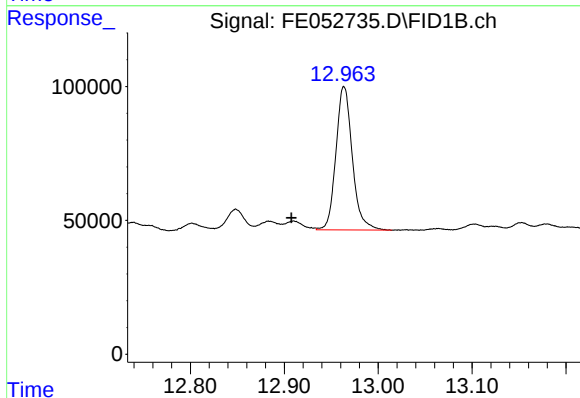


#10 n-Eicosane (C20)

R.T.: 12.964 min
Delta R.T.: 0.056 min
Response: 650630
Conc: 4.48 ug/ml

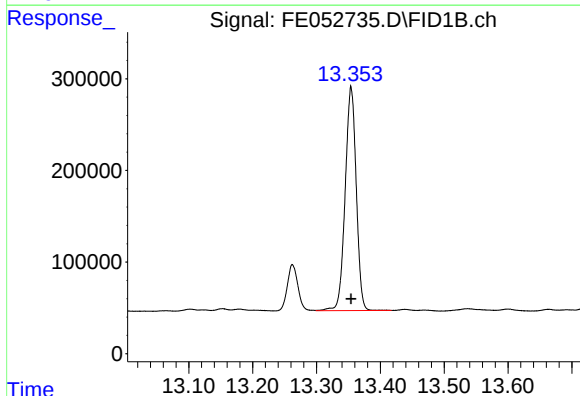


#12 1-chlorooctadecane (SURR)

R.T.: 13.354 min
Delta R.T.: 0.000 min
Response: 2939380
Conc: 24.21 ug/ml

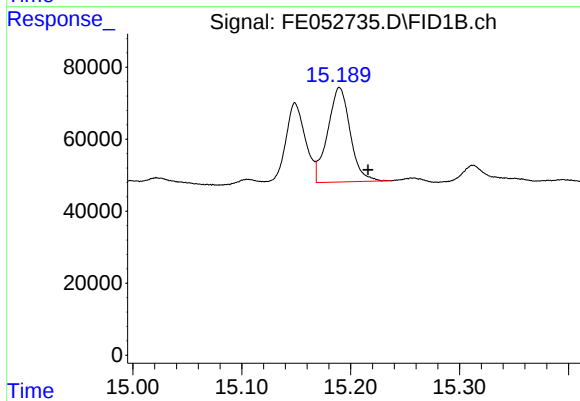

#14 n-Tetracosane (C24)


R.T.: 15.190 min
Delta R.T.: -0.026 min
Response: 377364
Conc: 2.64 ug/ml

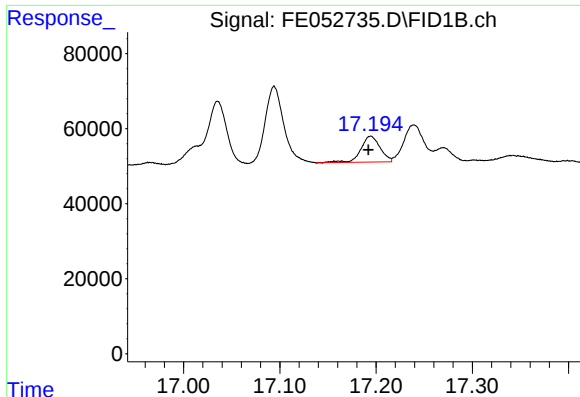

#16 n-Octacosane (C28)


R.T.: 17.195 min
Delta R.T.: 0.002 min
Response: 95976
Conc: 0.67 ug/ml

Instrument :
FID_E
ClientSampleId :

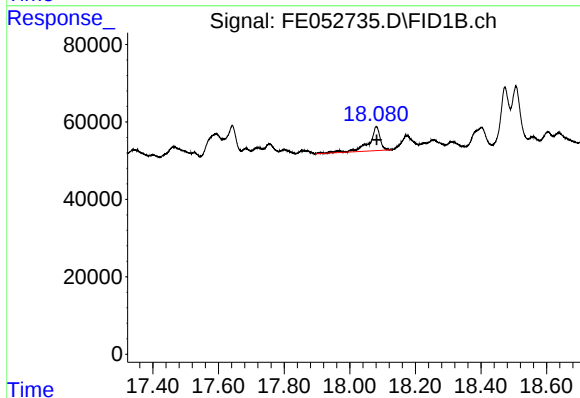


#17 n-Tricontane (C30)

R.T.: 18.081 min
Delta R.T.: -0.001 min
Response: 147711
Conc: 1.00 ug/ml

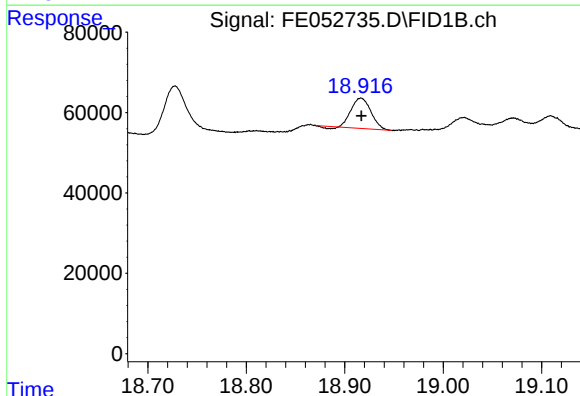

#18 n-Dotriacontane (C32)

R.T.: 18.916 min
Delta R.T.: 0.000 min
Response: 102369
Conc: 0.71 ug/ml

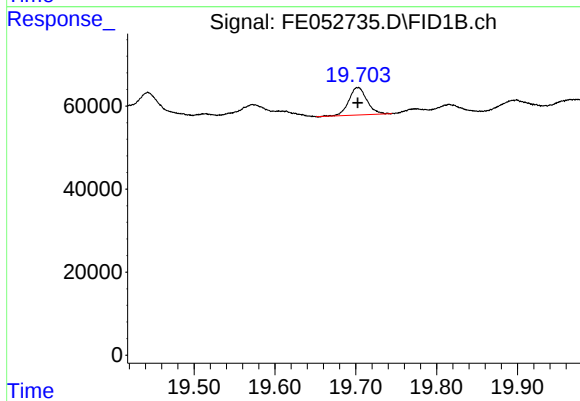

#19 n-Tetratriacontane (C34)

R.T.: 19.703 min
Delta R.T.: 0.000 min
Response: 102264
Conc: 0.76 ug/ml